


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN013009.D
Acq On : 09 Dec 2020 12:39
Operator : CG/JU
Sample : L4862-21DL 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BH4DL

Manual Integrations
APPROVED

mohammad
12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:24:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 07:33:34 2020
Response via : Initial Calibration

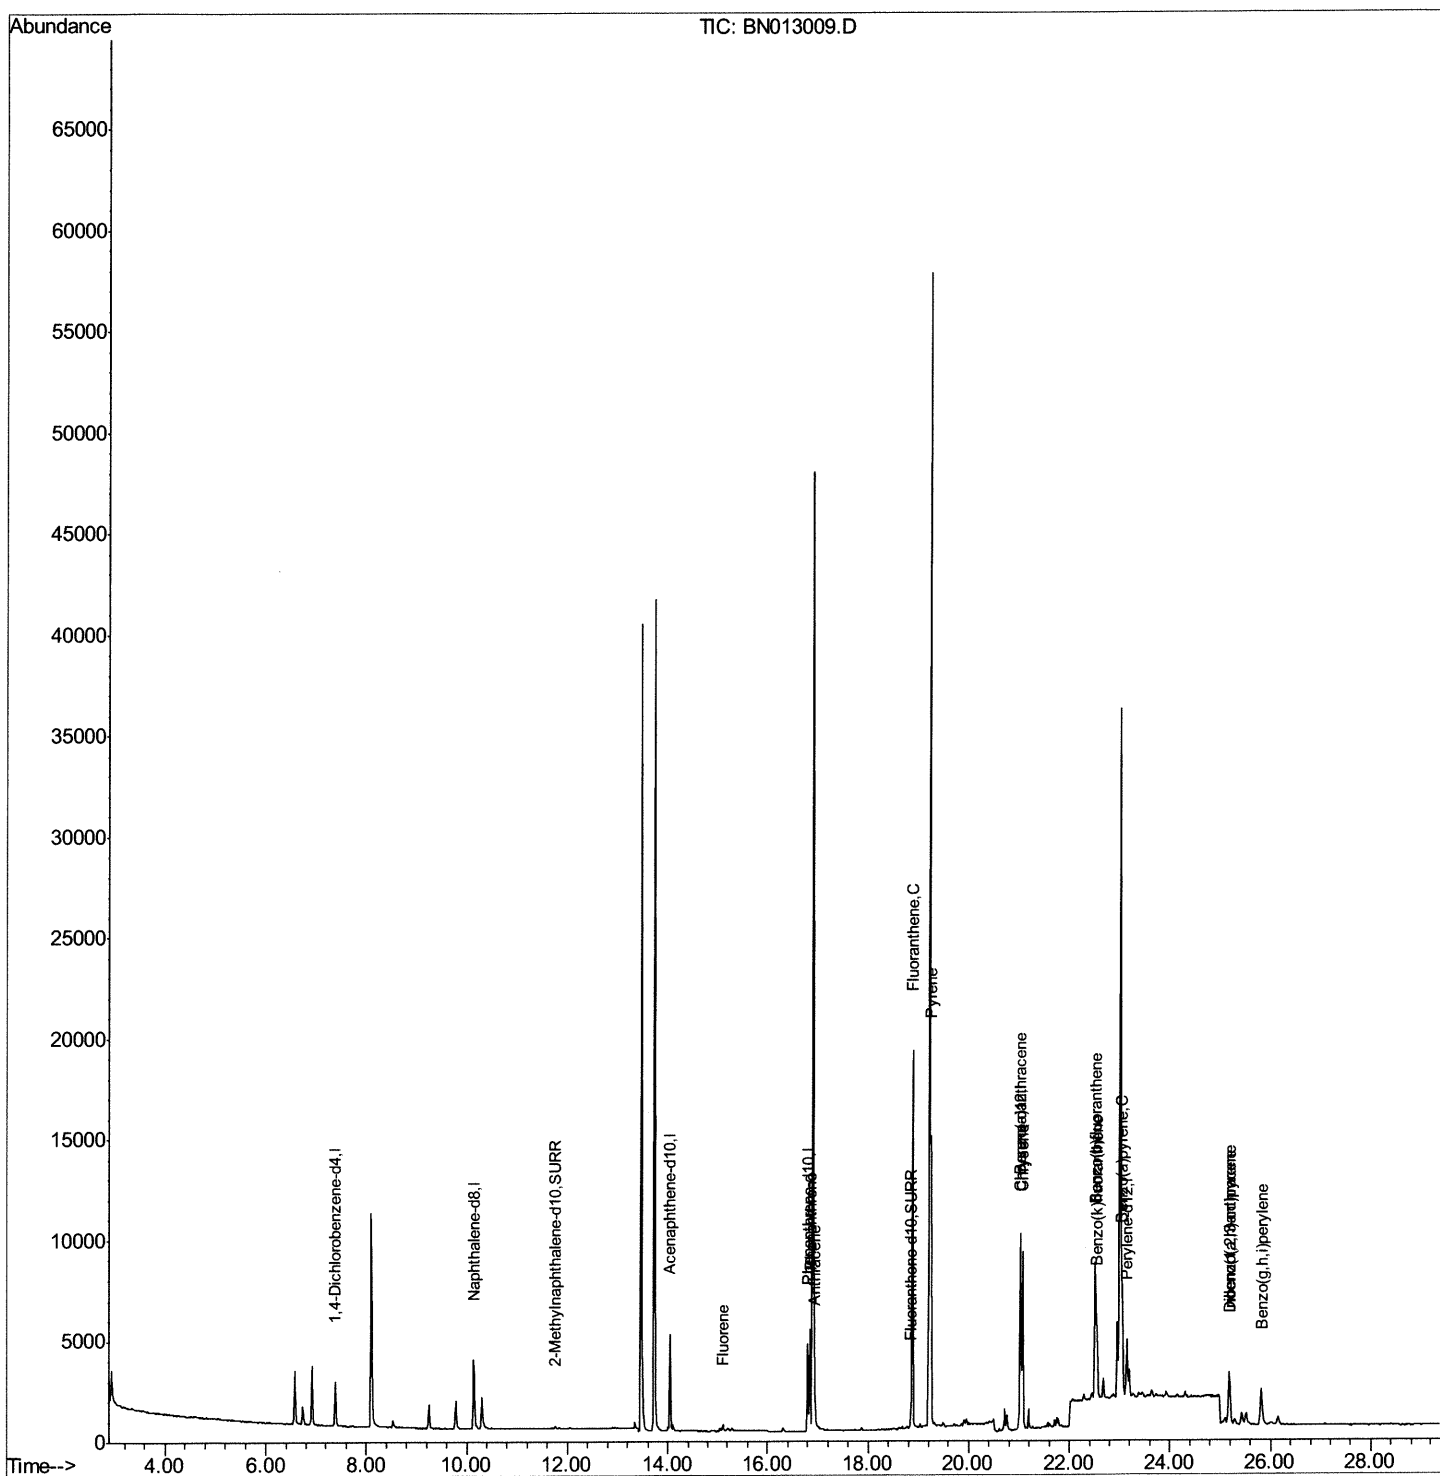

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN013009.D
 Acq On : 09 Dec 2020 12:39
 Operator : CG/JU
 Sample : L4862-21DL 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BH4DL

Manual Integrations
APPROVED

mohammad
 12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:21:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 07:33:34 2020
 Response via : Initial Calibration

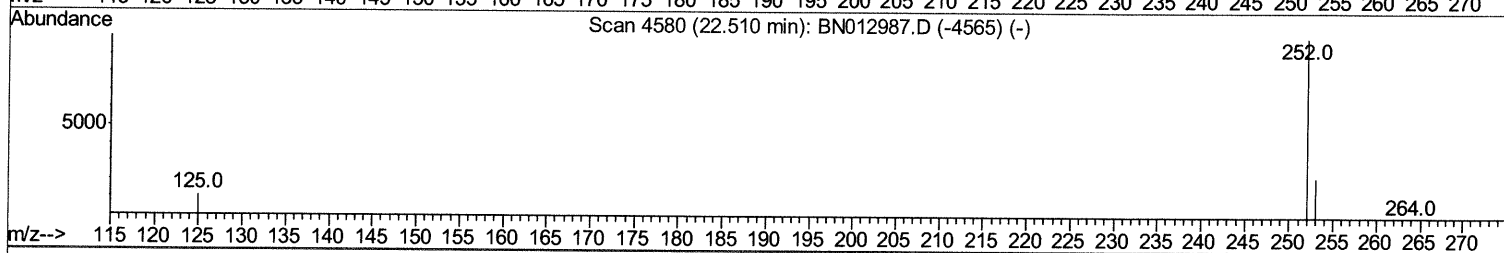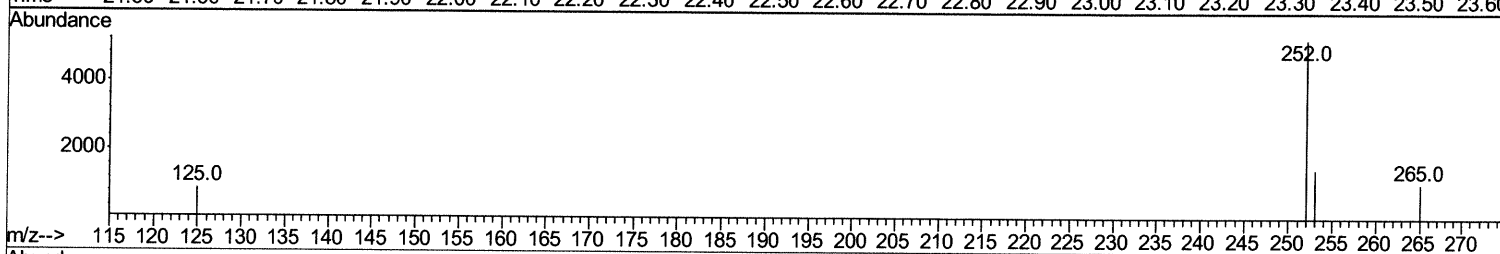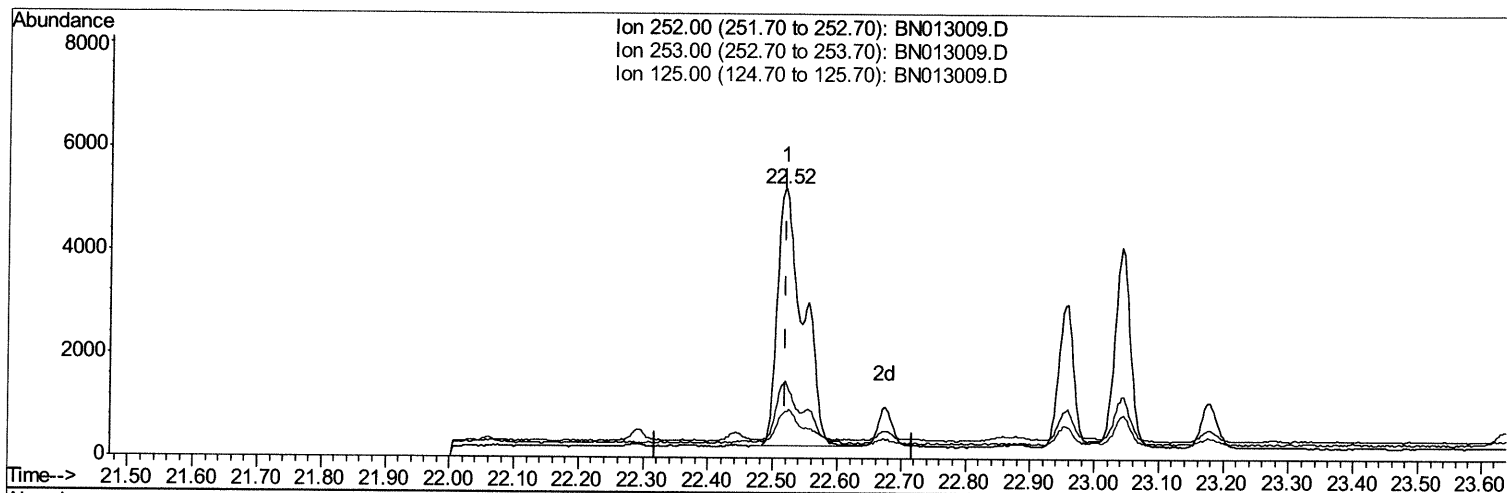

TIC: BN013009.D

(21) Benzo(b)fluoranthene

22.519min (+0.000) 0.92ng/ul

response 13971

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	28.51
125.00	13.00	17.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN013009.D
 Acq On : 09 Dec 2020 12:39
 Operator : CG/JU
 Sample : L4862-21DL 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH4DL

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:21:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 07:33:34 2020
 Response via : Initial Calibration

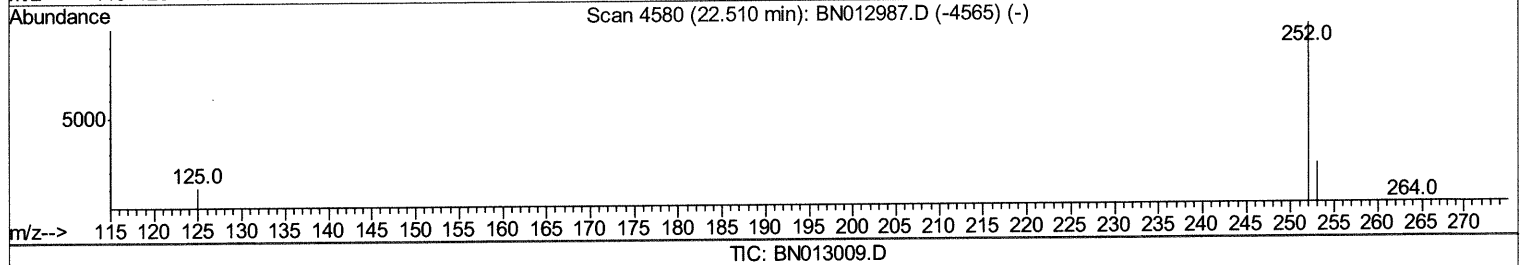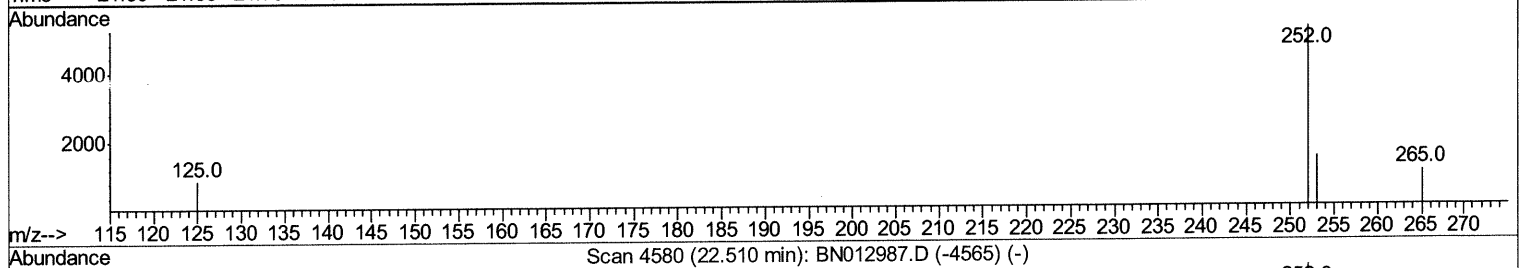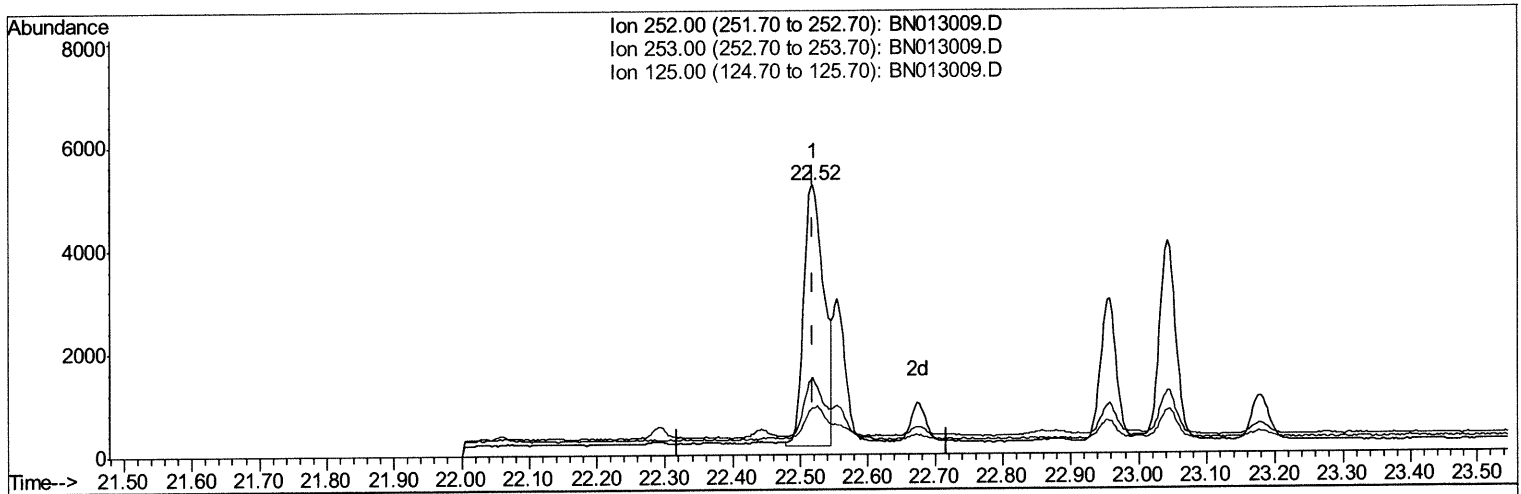

(21) Benzo(b)fluoranthene

22.519min (+0.000) 0.70ng/ul m 12/10/2020

response 10566

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	28.51
125.00	13.00	17.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN013009.D
 Acq On : 09 Dec 2020 12:39
 Operator : CG/JU
 Sample : L4862-21DL 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH4DL

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:21:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 07:33:34 2020
 Response via : Initial Calibration

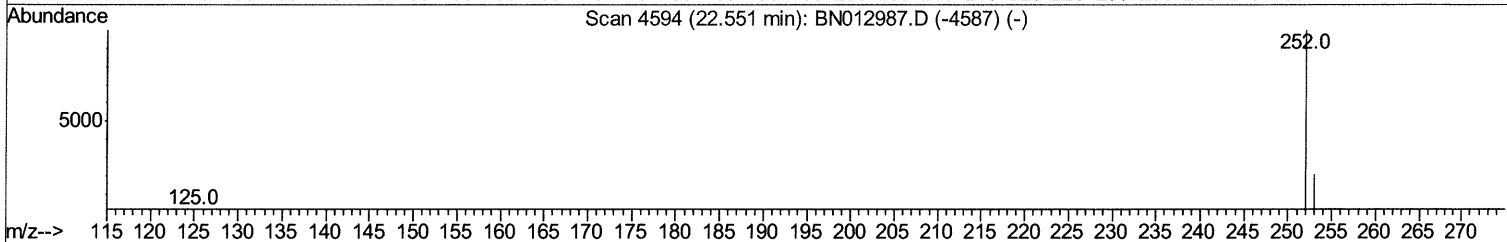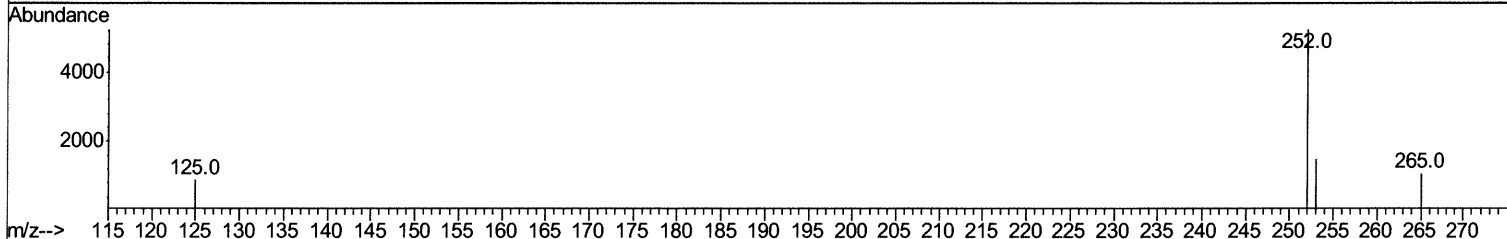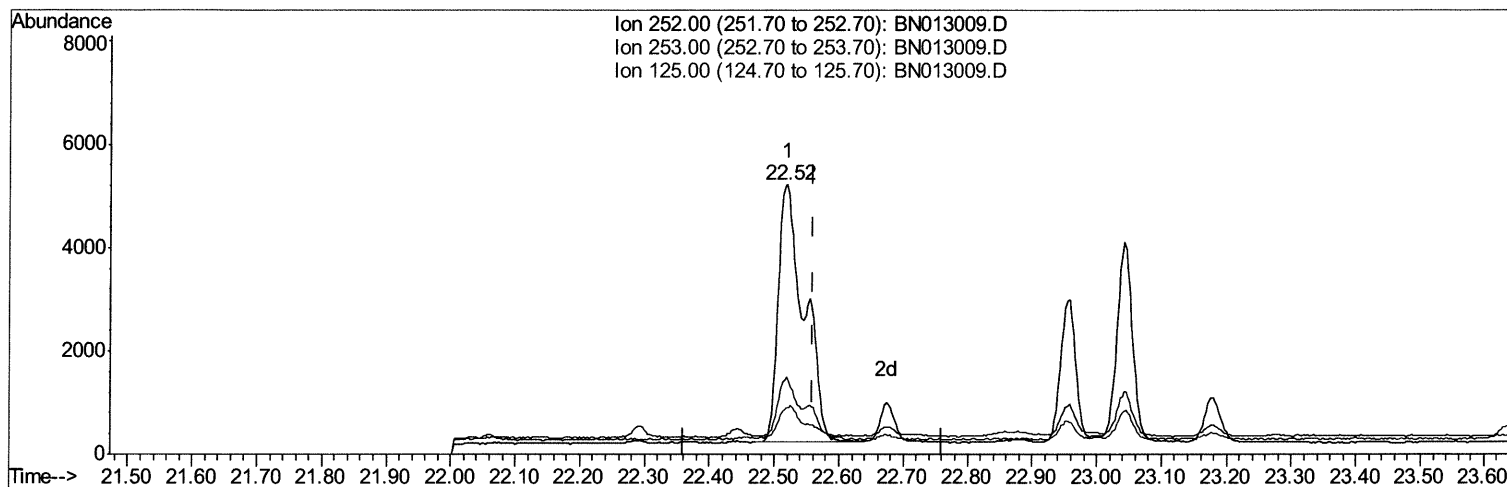

TIC: BN013009.D

(22) Benzo(k)fluoranthene
 22.519min (-0.041) 0.83ng/ul
 response 13971

Ion	Exp%	Act%
252.00	100	100
253.00	29.30	28.51
125.00	13.90	17.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN013009.D
 Acq On : 09 Dec 2020 12:39
 Operator : CG/JU
 Sample : L4862-21DL 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH4DL

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:21:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 07:33:34 2020
 Response via : Initial Calibration

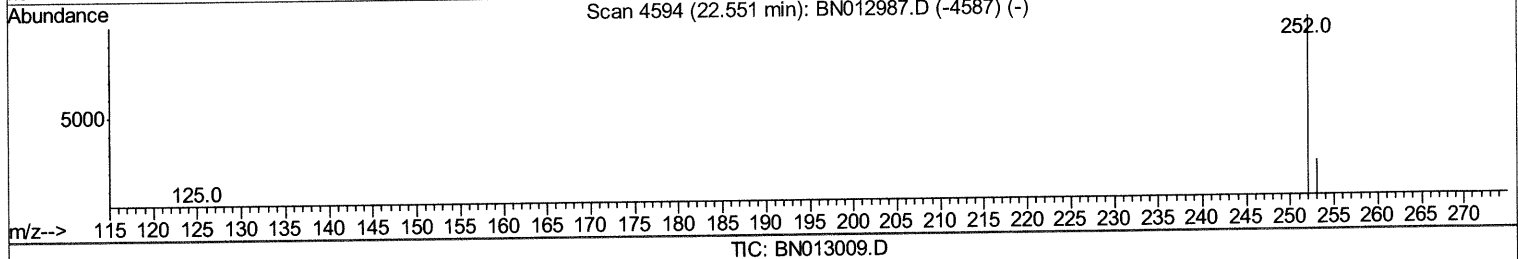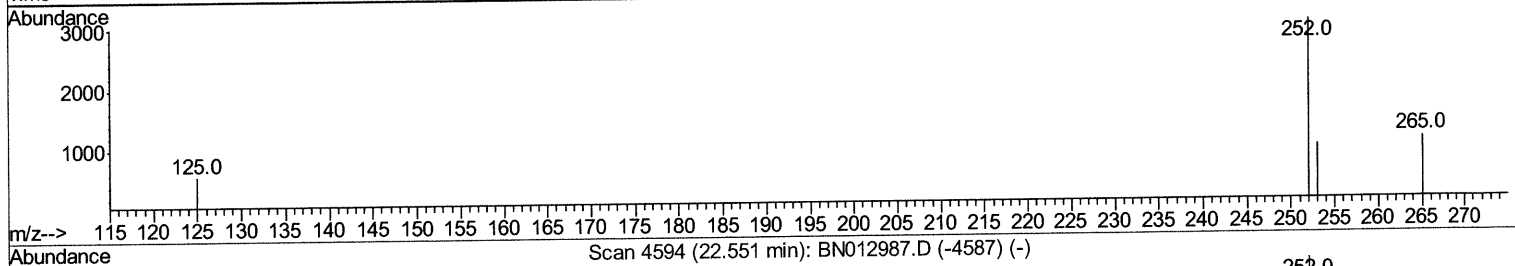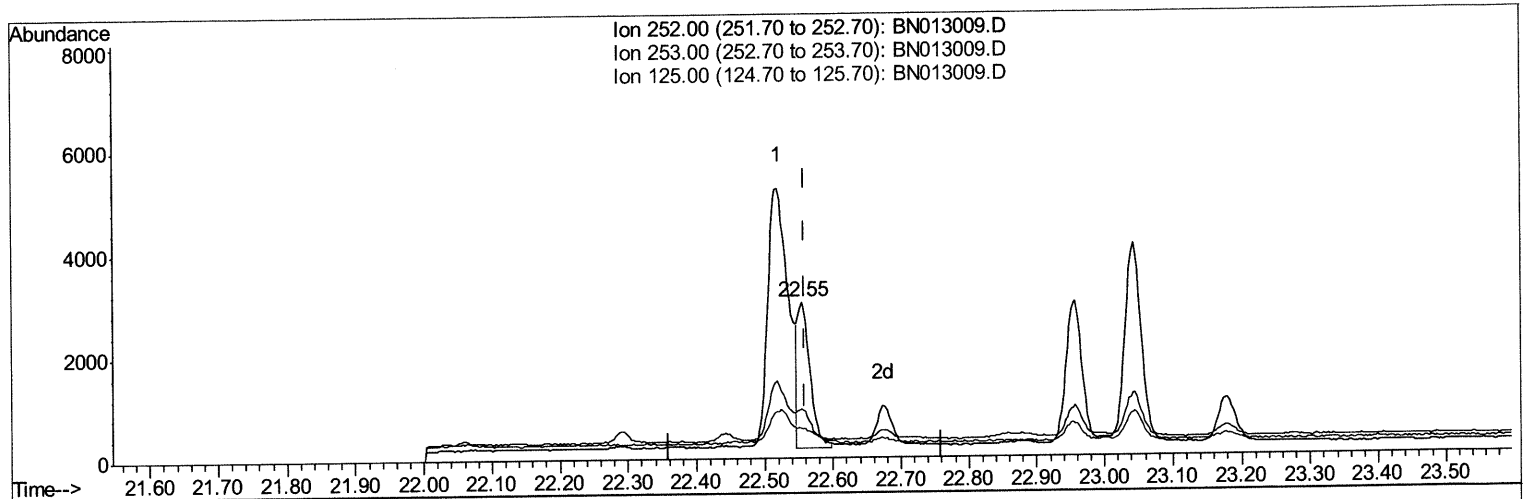

(22) Benzo(k)fluoranthene

22.554min (-0.006) 0.22ng/ul m 12/16/2024

response 3697

Ion	Exp%	Act%
252.00	100	100
253.00	29.30	31.51
125.00	13.90	18.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
 Data File : BN013009.D
 Acq On : 09 Dec 2020 12:39
 Operator : CG/JU
 Sample : L4862-21DL 10X
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH4DL

Manual Integrations
 APPROVED

mohammad
 12/9/2020 5:39:30 PM

Quant Time: Dec 09 13:24:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 07:33:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1140	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	4690	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2528	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	5043	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	3562	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	3280	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	281	0.04	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	519	0.04	ng/ul	0.00

Target Compounds				Ovalue		
9) Fluorene	15.11	166	227	0.020	ng/ul#	87
12) Phenanthrene	16.85	178	5308	0.314	ng/ul	99
13) Anthracene	16.94	178	1114	0.077	ng/ul#	92
15) Fluoranthene	18.88	202	15548	0.774	ng/ul	99
17) Pyrene	19.25	202	14128	0.840	ng/ul	98
18) Benzo(a)anthracene	21.02	228	7530	0.511	ng/ul	99
19) Chrysene	21.07	228	8581	0.527	ng/ul	98
21) Benzo(b)fluoranthene	22.52	252	10566m	0.696	ng/ul	} 12/16/2020
22) Benzo(k)fluoranthene	22.55	252	3697m	0.220	ng/ul	
23) Benzo(a)pyrene	23.04	252	6559	0.466	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.19	276	3791	0.205	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.20	278	1081	0.074	ng/ul#	58
26) Benzo(a,h,i)perylene	25.81	276	3581	0.214	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed