


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN013015.D
Acq On : 09 Dec 2020 17:04
Operator : CG/JU
Sample : PB133393BL
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK93

Manual Integrations
APPROVED

mohammad
12/9/2020 10:01:34 PM

Quant Time: Dec 09 17:42:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 07:33:34 2020
Response via : Initial Calibration

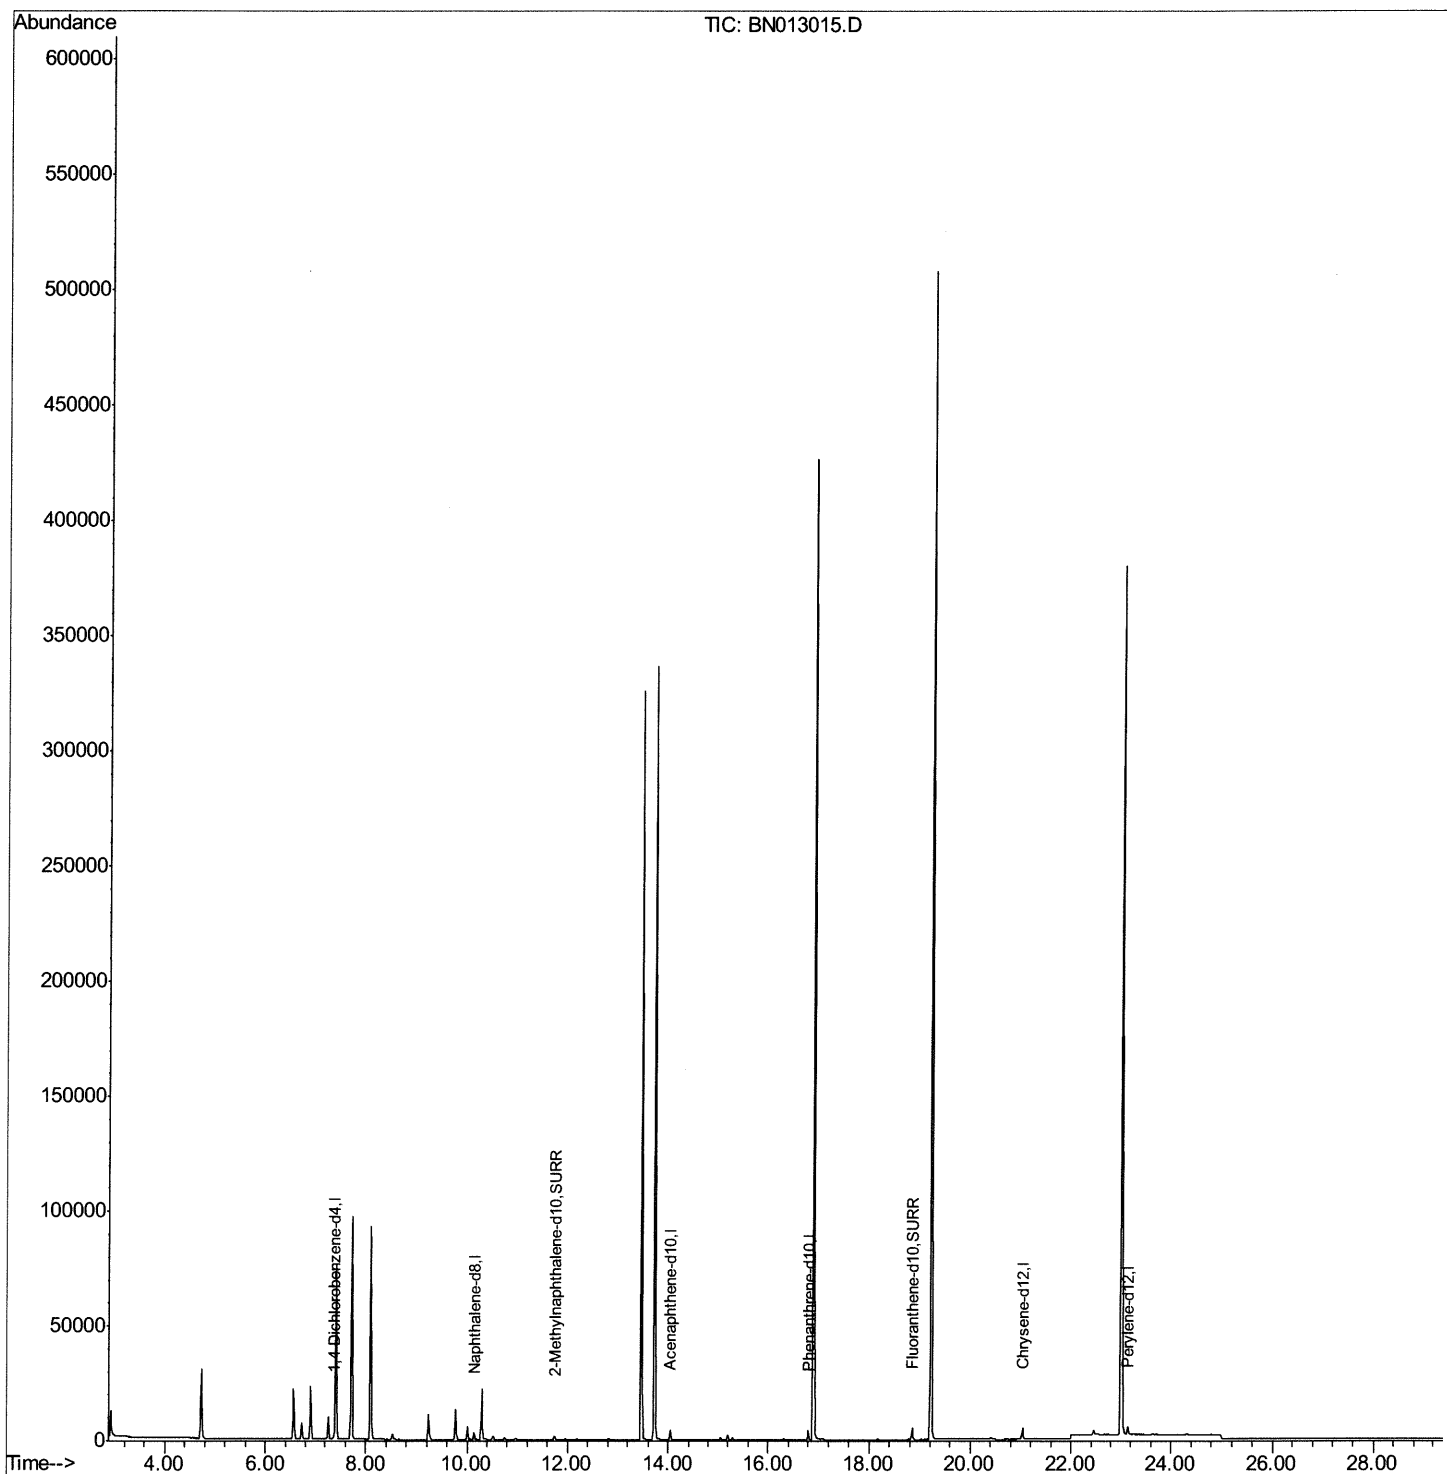

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN013015.D
Acq On : 09 Dec 2020 17:04
Operator : CG/JU
Sample : PB133393BL
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK93

Manual Integrations
APPROVED

mohammad
12/9/2020 10:01:34 PM

Quant Time: Dec 09 17:41:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 07:33:34 2020
Response via : Initial Calibration

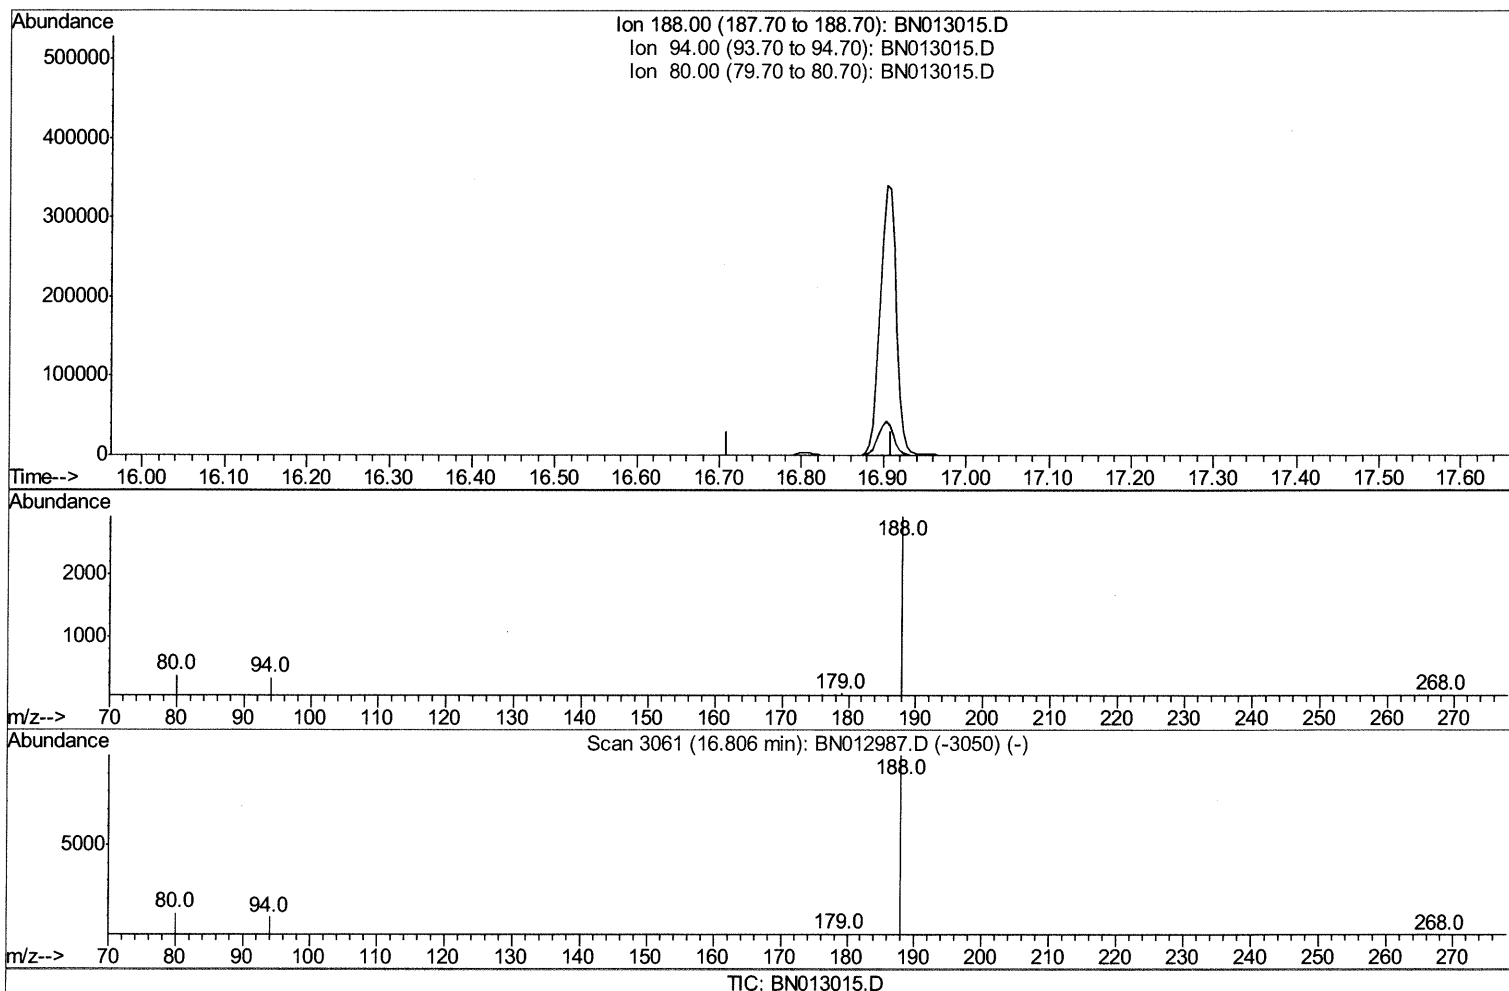

(10) Phenanthrene-d10 (I)

16.810min (-16.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.40	0.00#
80.00	12.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN013015.D
Acq On : 09 Dec 2020 17:04
Operator : CG/JU
Sample : PB133393BL
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK93

Manual Integrations
APPROVED

mohammad
12/9/2020 10:01:34 PM

Quant Time: Dec 09 17:41:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 07:33:34 2020
Response via : Initial Calibration

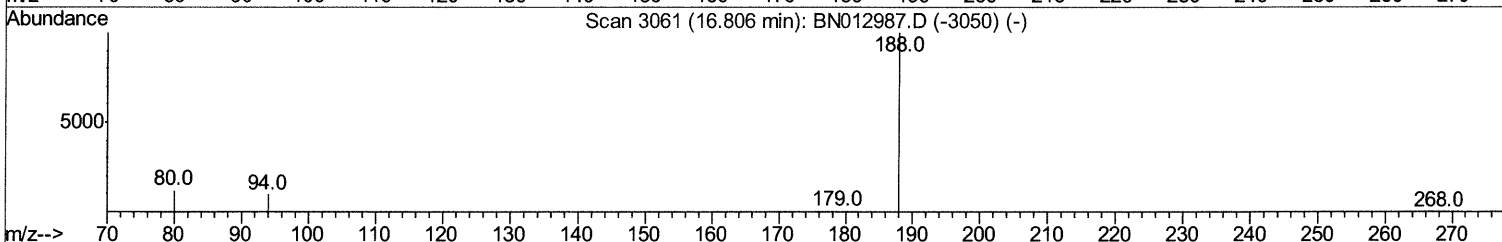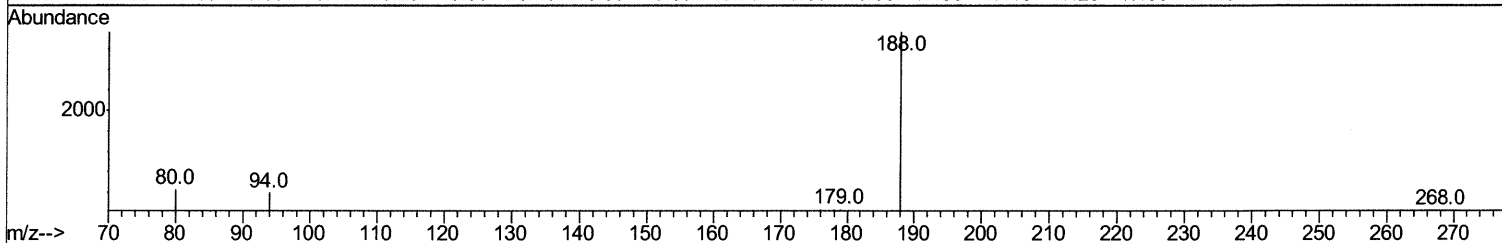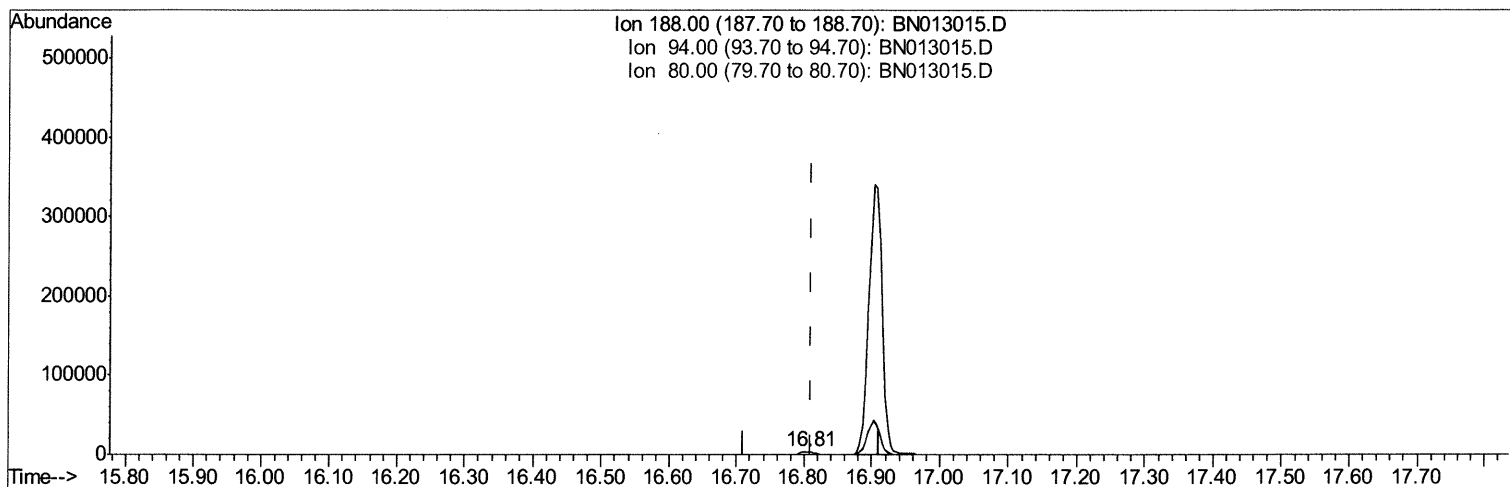

TIC: BN013015.D

(10) Phenanthrene-d10 (I)

16.806min (-0.004) 0.40ng/ul m 12/11/2020

response 4827

Ion	Exp%	Act%
188.00	100	100
94.00	11.40	11.48
80.00	12.40	13.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120720\
Data File : BN013015.D
Acq On : 09 Dec 2020 17:04
Operator : CG/JU
Sample : PB133393BL
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK93

Manual Integrations
APPROVED

mohammad
12/9/2020 10:01:34 PM

Quant Time: Dec 09 17:42:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 07:33:34 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	1123	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.14	136	3799	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.05	164	2286	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4827m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.04	240	4133	0.40	ng/ul	0.00
20) Perylene-d12	23.14	264	4108	0.40	ng/ul	0.00

12/11/2020

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.74	152	2317	0.41	ng/ul	-0.02
14) Fluoranthene-d10	18.85	212	5191	0.40	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed