

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
 Data File : BN012957.D
 Acq On : 08 Dec 2020 01:56
 Operator : CG/JU
 Sample : L4862-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BH3

Manual Integrations
 APPROVED

mohammad
 12/9/2020 12:23:13 PM

Quant Time: Dec 08 02:35:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 08 00:15:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	852	0.40	ng/ul	0.00
2) Naphthalene-d8	10.15	136	3454	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.05	164	2135	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.81	188	4434m	0.40	ng/ul	0.00
16) Chrysene-d12	21.03	240	3682	0.40	ng/ul	0.00
20) Perylene-d12	23.13	264	3815	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.76	152	2678	0.52	ng/ul	0.00
14) Fluoranthene-d10	18.85	212	5751	0.48	ng/ul	0.00
Target Compounds						
12) Phenanthrene	16.85	178	327	0.022	ng/ul#	Ovalue 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120720\
Data File : BN012957.D
Acq On : 08 Dec 2020 01:56
Operator : CG/JU
Sample : L4862-20
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
C0BH3

Quant Time: Dec 08 02:35:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN120320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 08 00:15:39 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
12/9/2020 12:23:13 PM

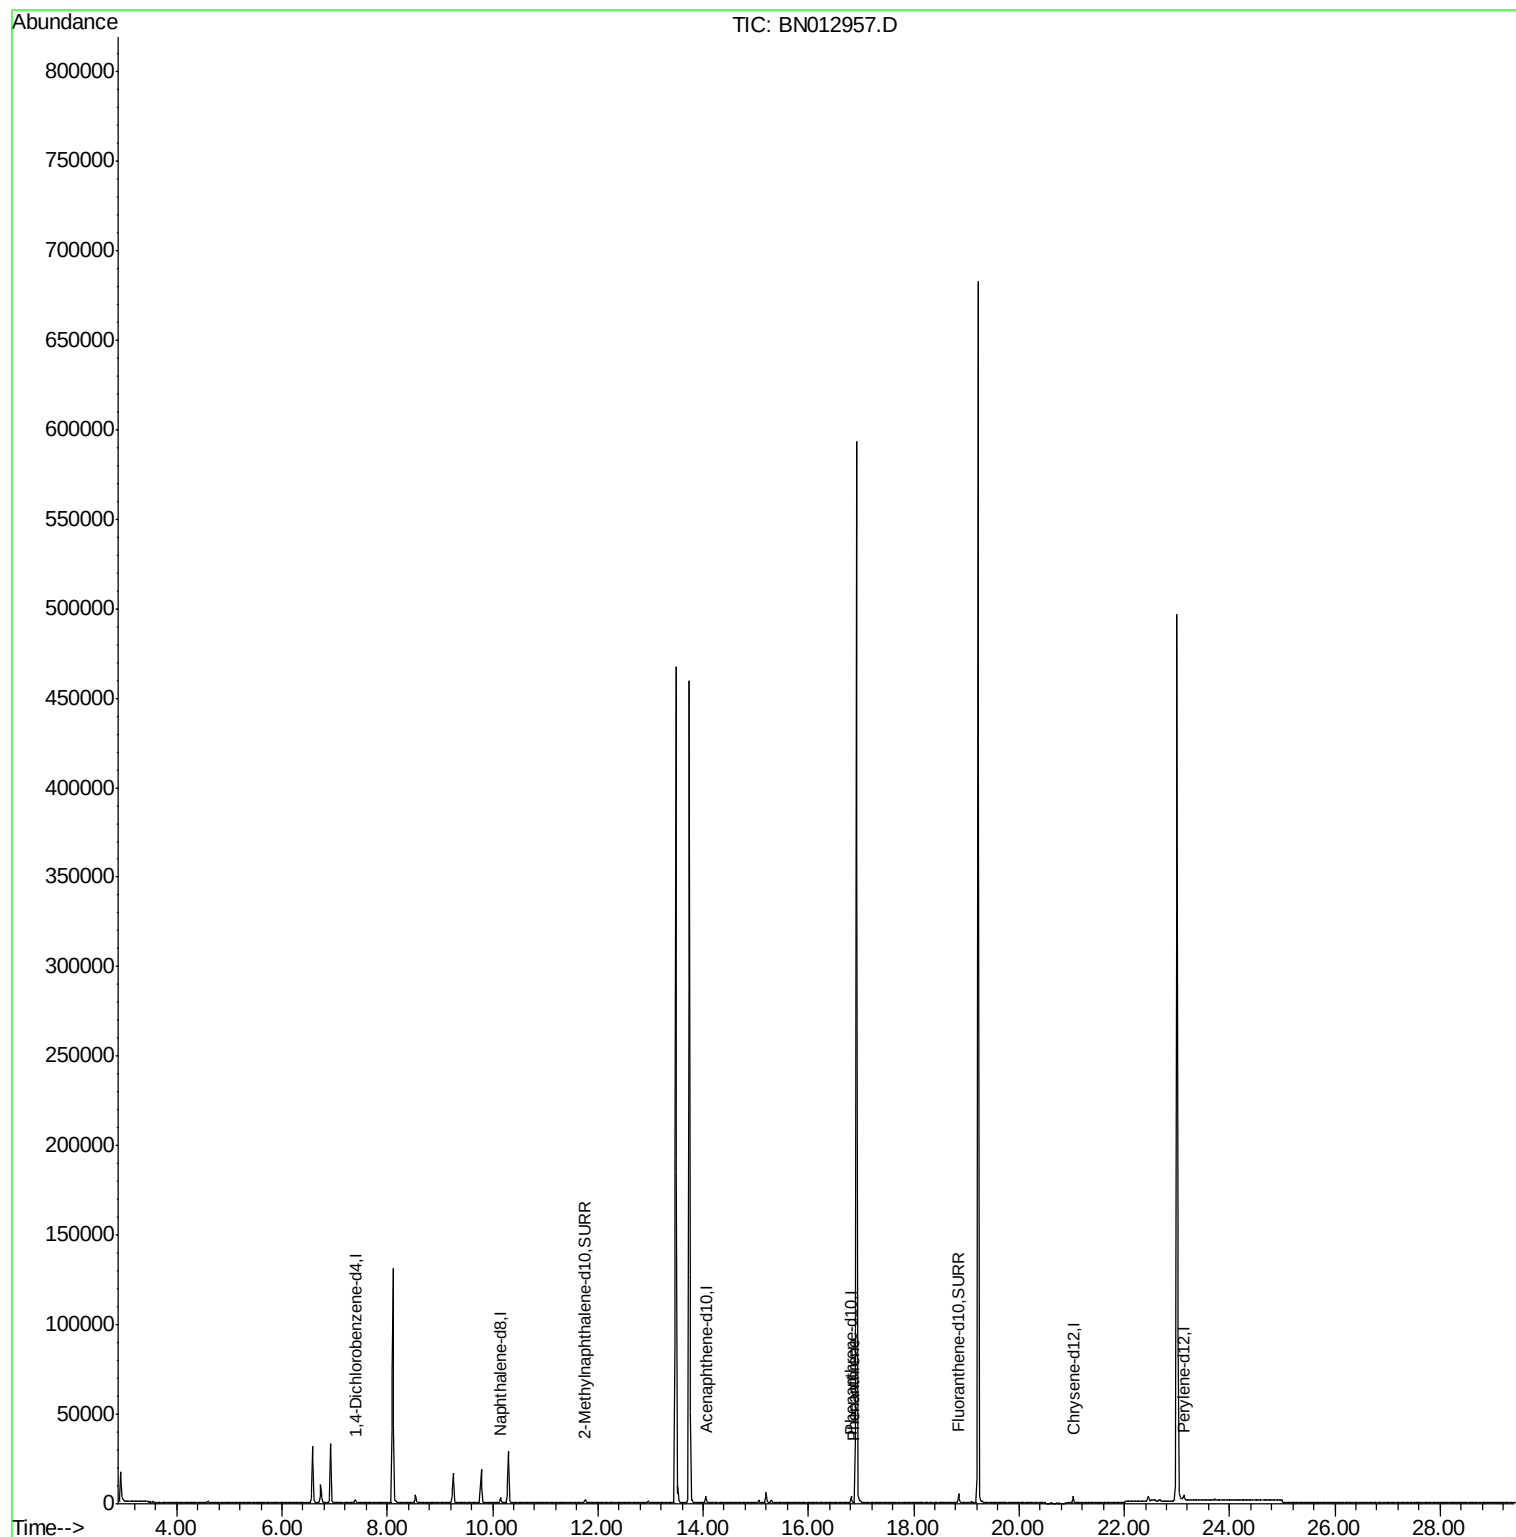

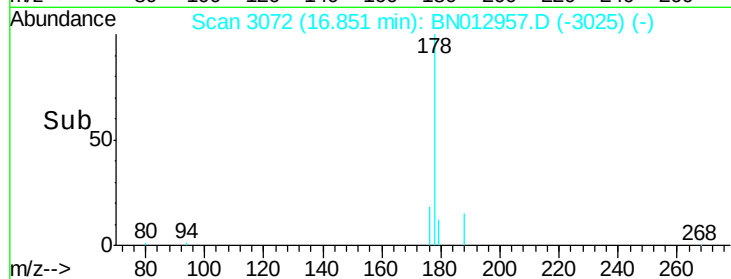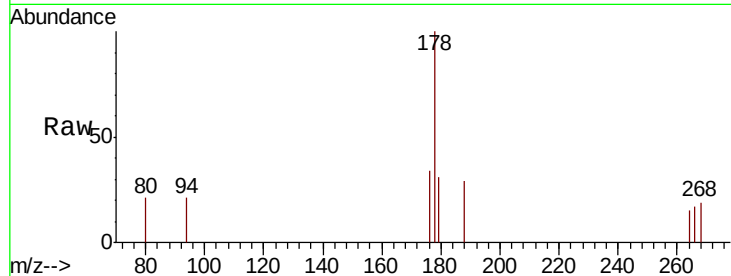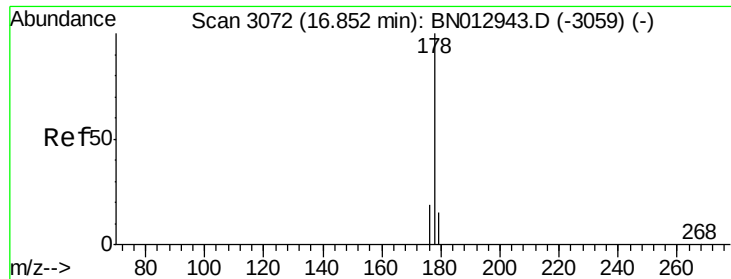

#12

Phenanthrene

Concen: 0.022 ng/ul

RT: 16.85 min Scan# 3072

Delta R.T. -0.00 min

Lab File: BN012957.D

Acq: 08 Dec 2020 01:56

Instrument :

BNA_N

ClientSampleId :

C0BH3

Tot Ion:	178	Resp:	327
Ion Ratio	Lower	Upper	
178	100		
179	31.3	13.6	20.4#
176	34.4	16.4	24.6#

Manual Integrations
APPROVED

mohammad
12/9/2020 12:23:13 PM

