
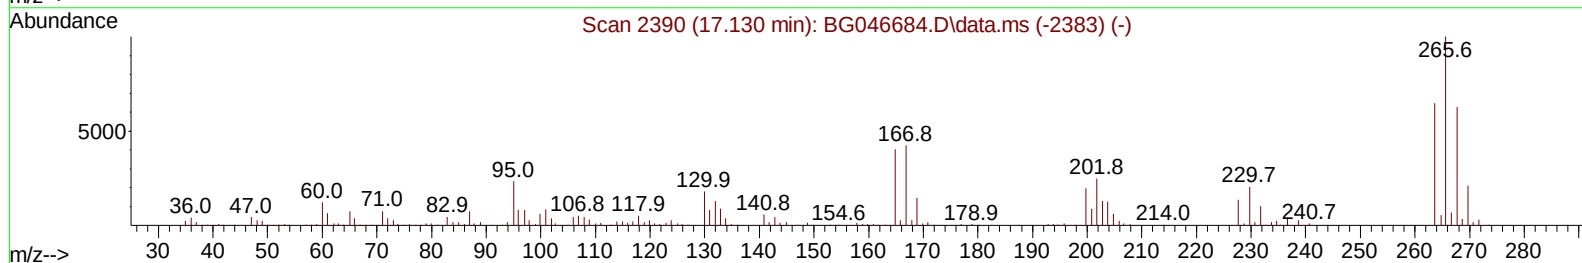
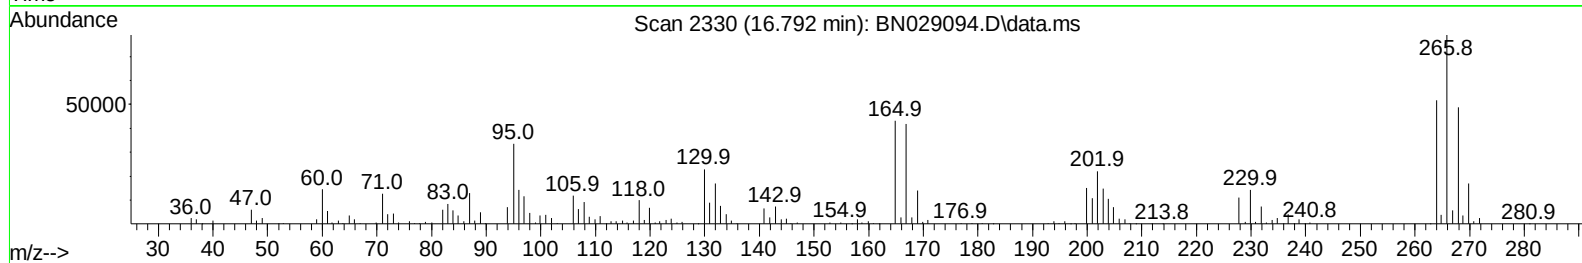


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029094.D
Acq On : 07 Dec 2023 17:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 23:51:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

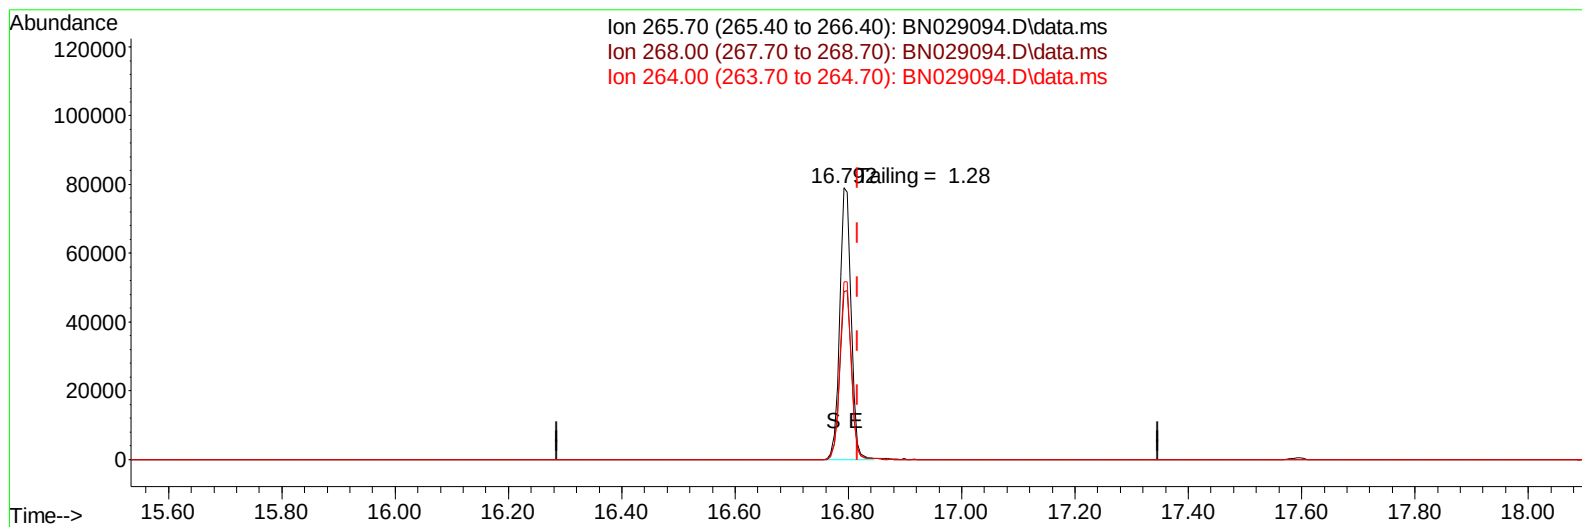

TIC: BN029094.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.024) 14688.15 ng

response 109736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.94
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029094.D
Acq On : 07 Dec 2023 17:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 07 23:51:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

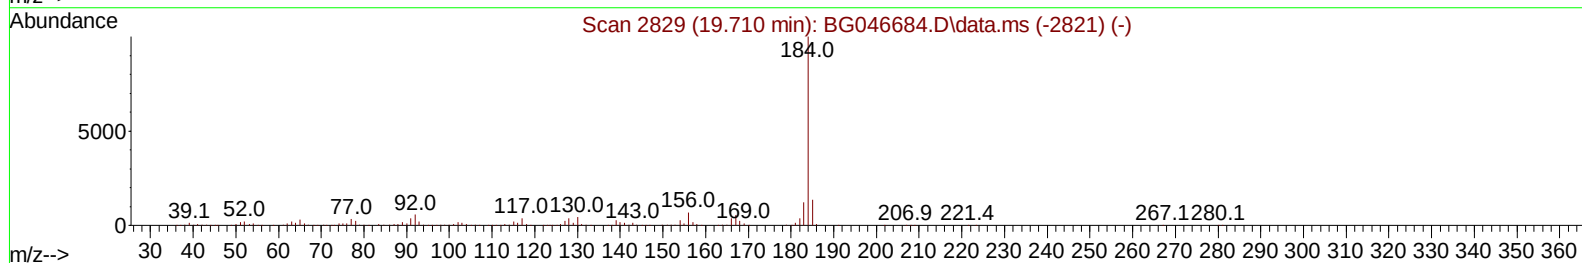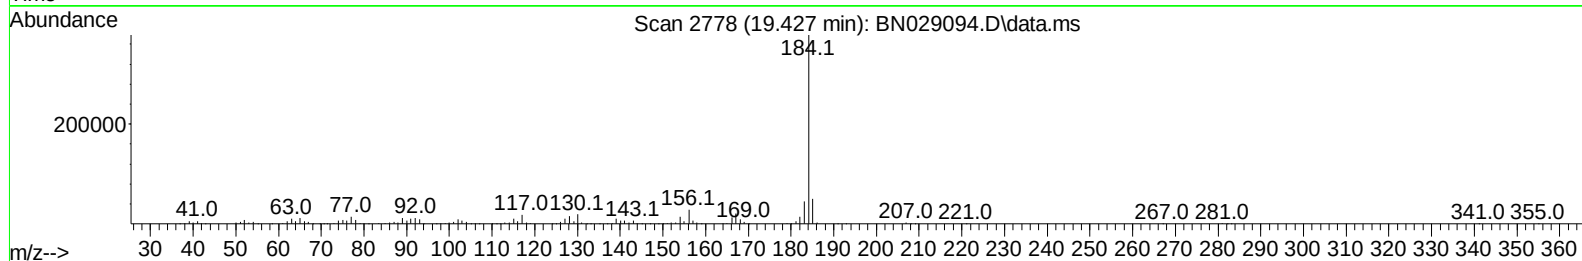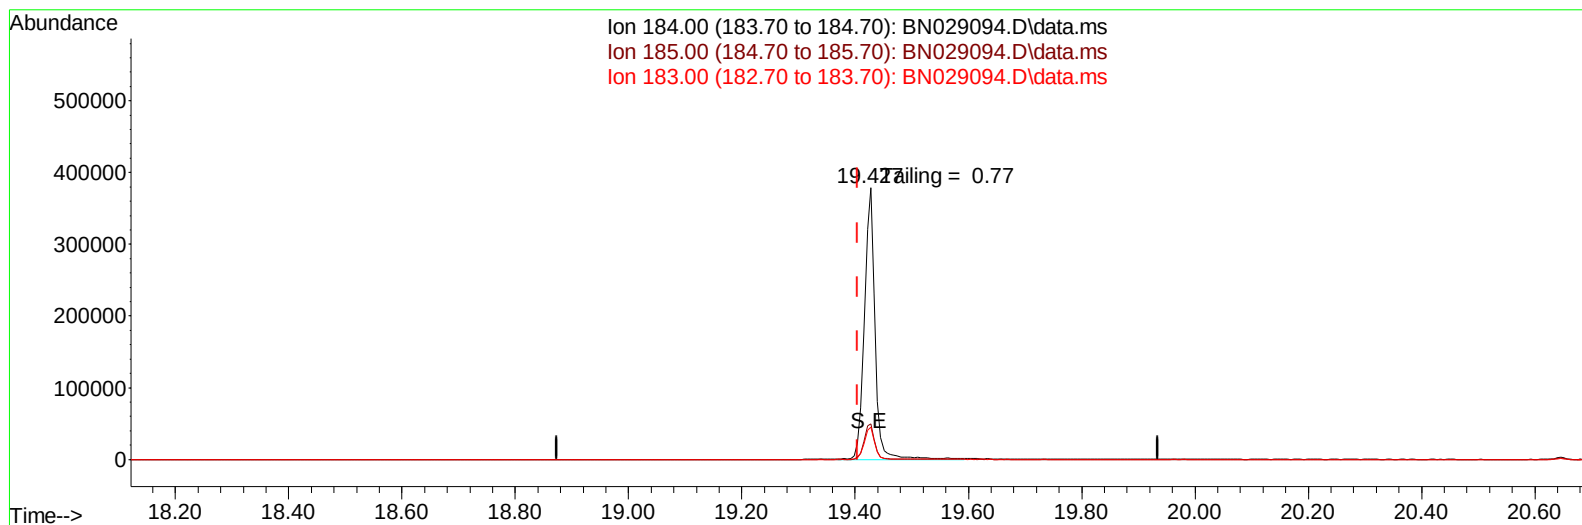

TIC: BN029094.D\data.ms

(77) Benzidine

19.427min (+ 0.023) 0.00 ng

response 489191

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.99
0.00	0.00	0.00