
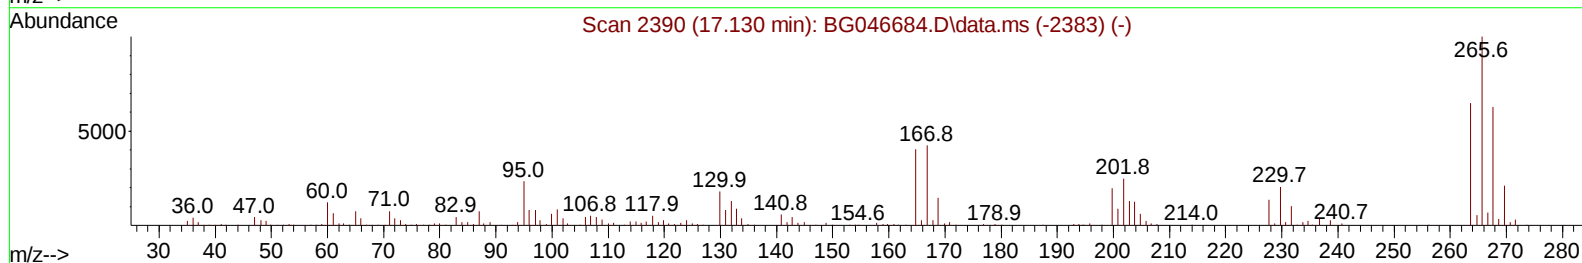
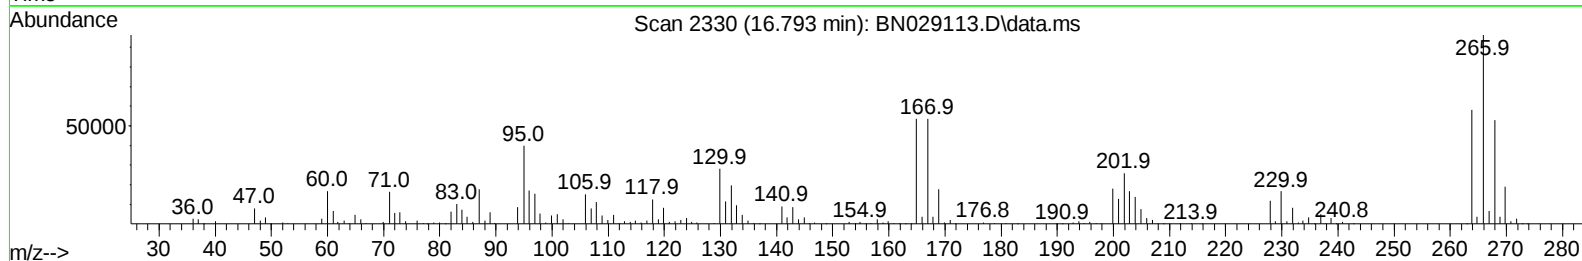


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029113.D
Acq On : 08 Dec 2023 05:41
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 08 06:13:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

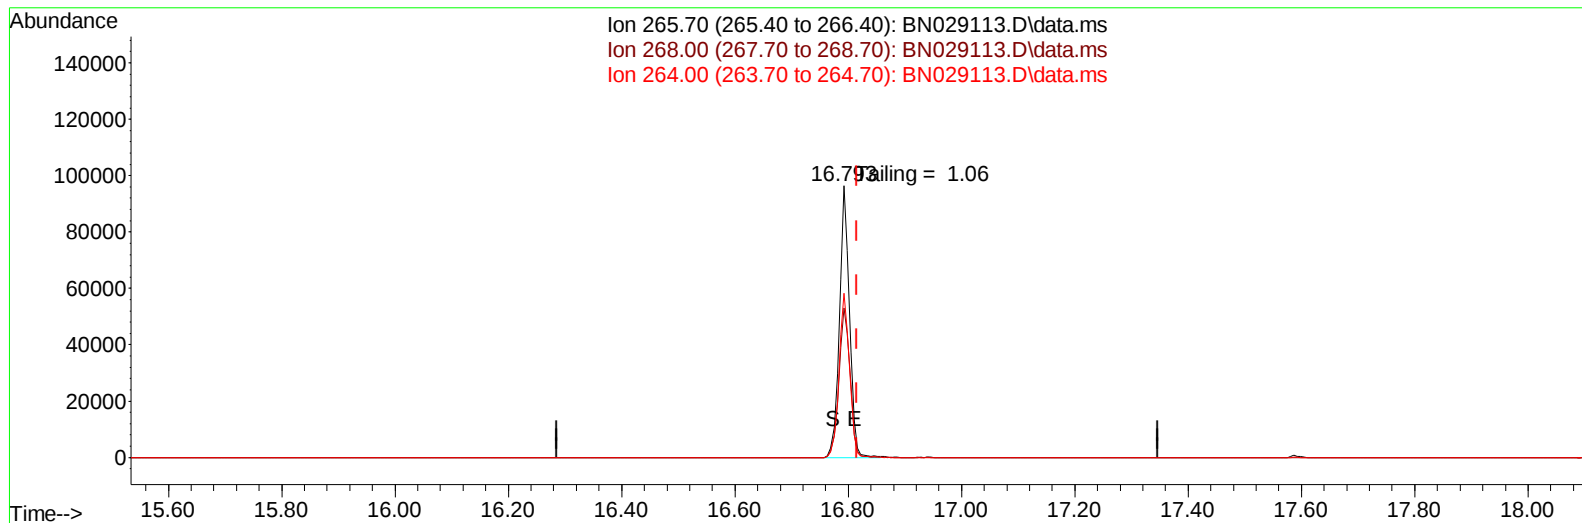

TIC: BN029113.D\data.ms

(70) Pentachlorophenol (C)




16.793min (-0.023) 12735.60 ng

response 117936

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	55.06
264.00	61.60	60.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029113.D
Acq On : 08 Dec 2023 05:41
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 08 06:13:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

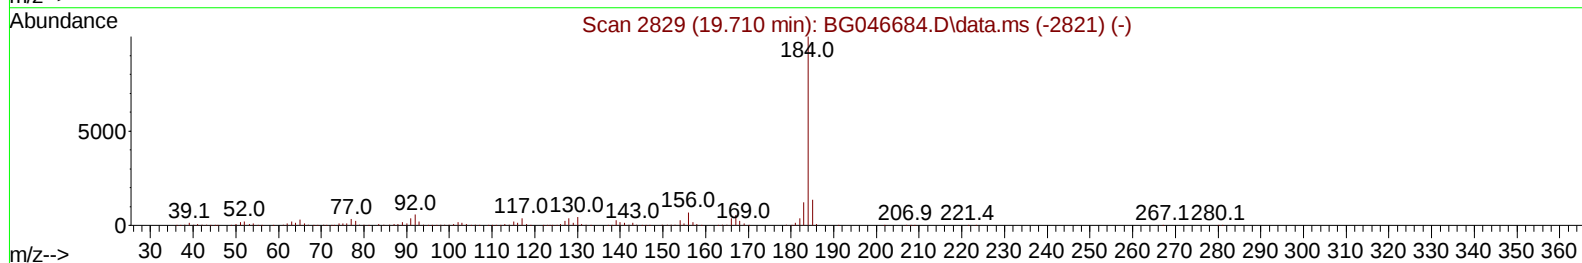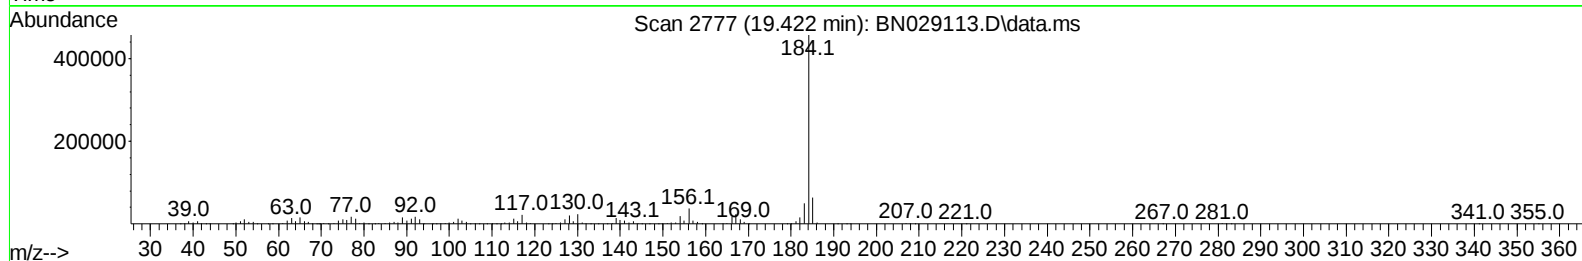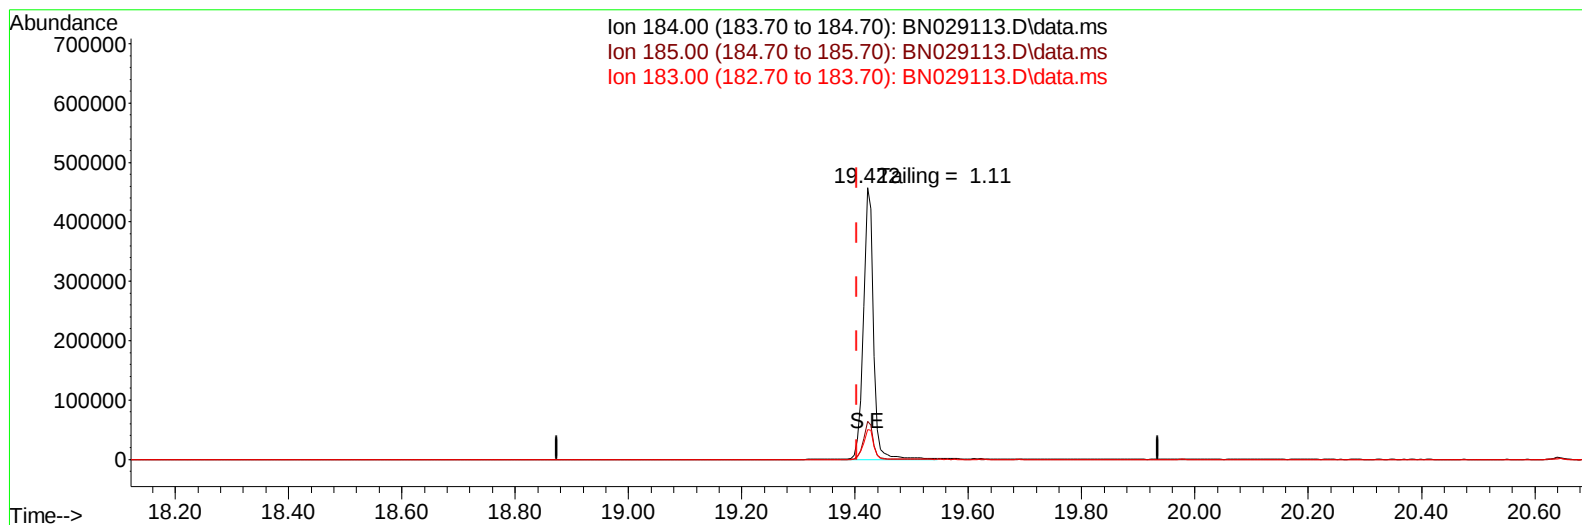

TIC: BN029113.D\data.ms

(77) Benzidine**19.422min (+ 0.018) 0.00 ng****response 559605**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.04
0.00	0.00	0.00