


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029094.D
Acq On : 07 Dec 2023 17:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120523.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 06 00:49:47 2023

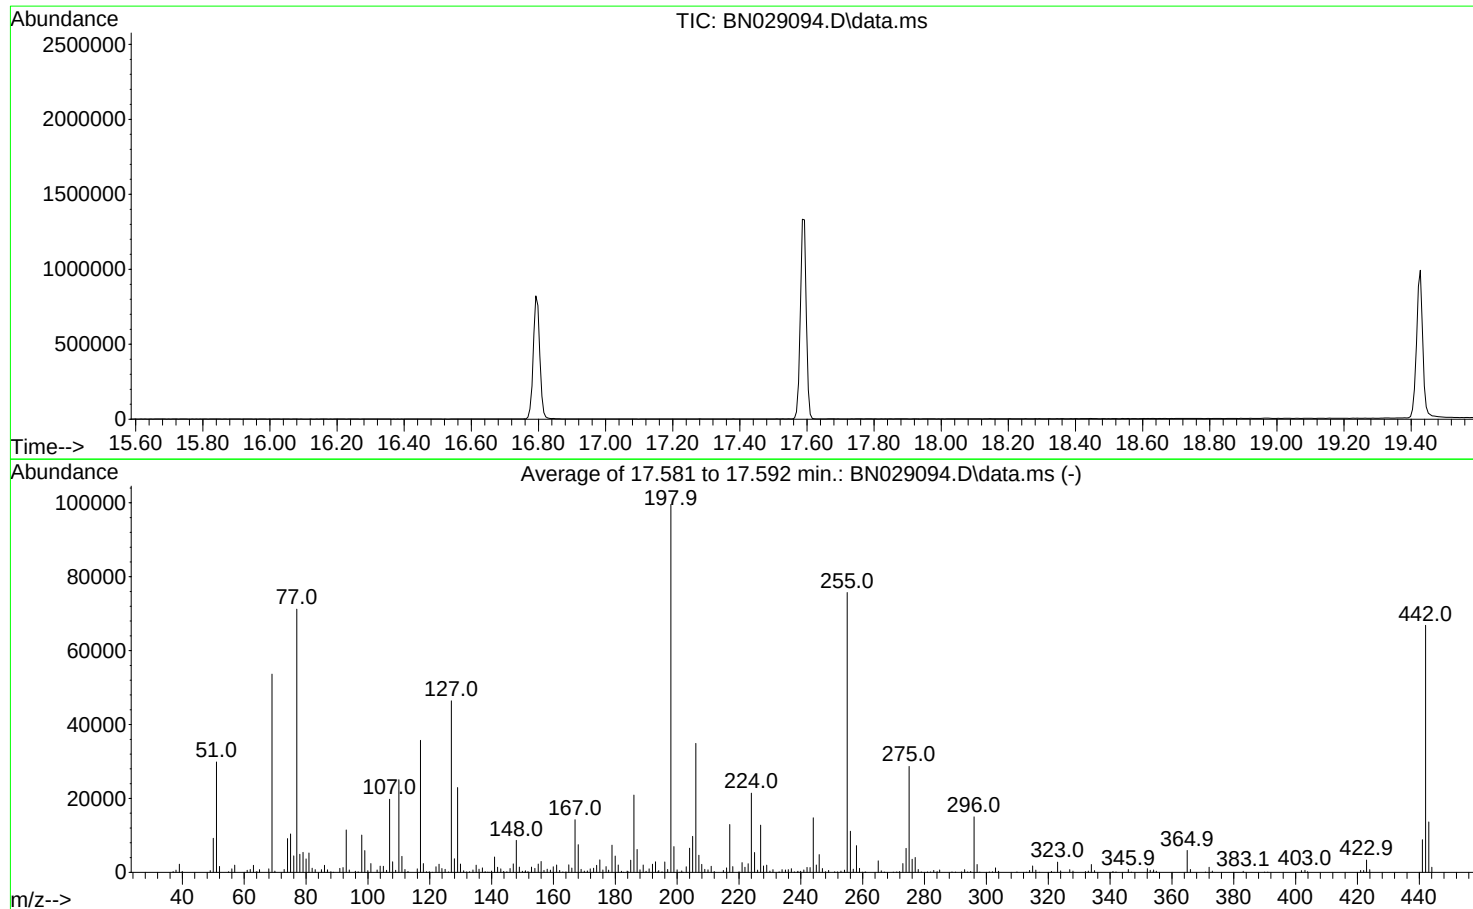




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	29880	PASS
68	69	0.00	2	1.8	962	PASS
69	198	0.00	100	53.9	53651	PASS
70	69	0.00	2	0.7	350	PASS
127	198	10	80	46.6	46413	PASS
197	198	0.00	2	0.8	760	PASS
198	198	100	100	100.0	99541	PASS
199	198	5	9	7.0	6978	PASS
275	198	10	60	28.8	28672	PASS
365	198	1	100	6.0	5928	PASS
441	198	0.01	100	8.9	8832	PASS
442	442	50	100	100.0	66837	PASS
443	442	15	24	20.4	13633	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029094.D
Acq On : 07 Dec 2023 17:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 23:51:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

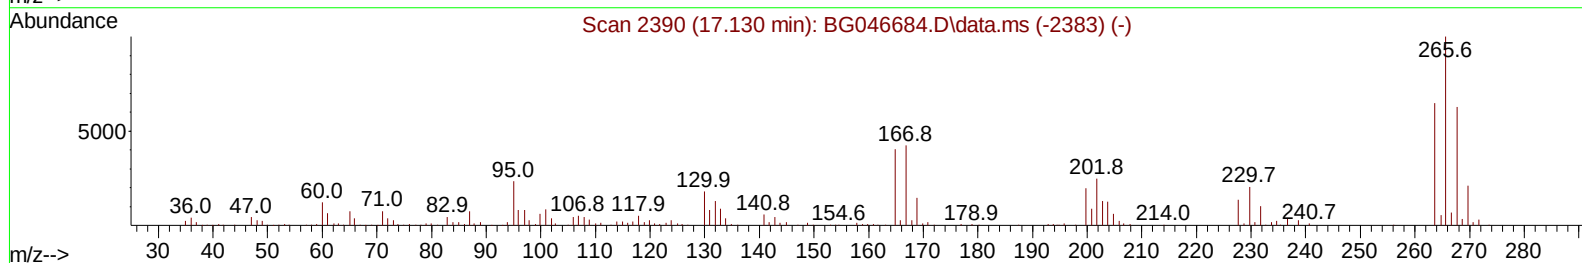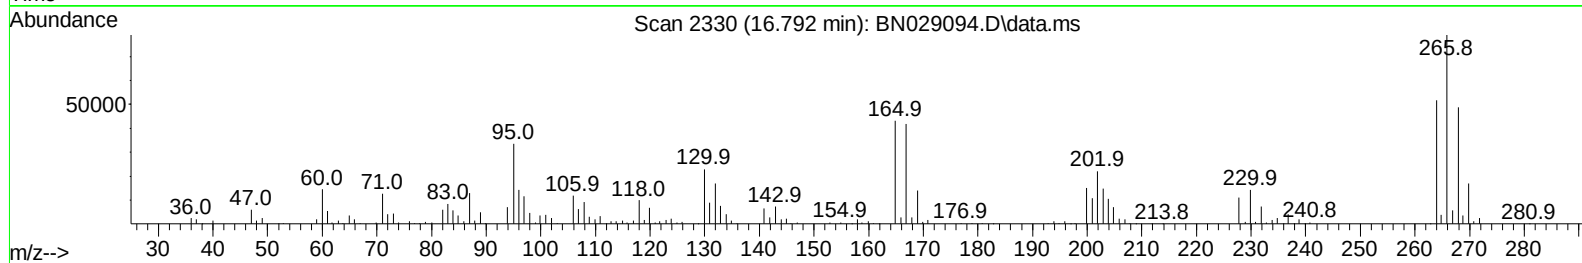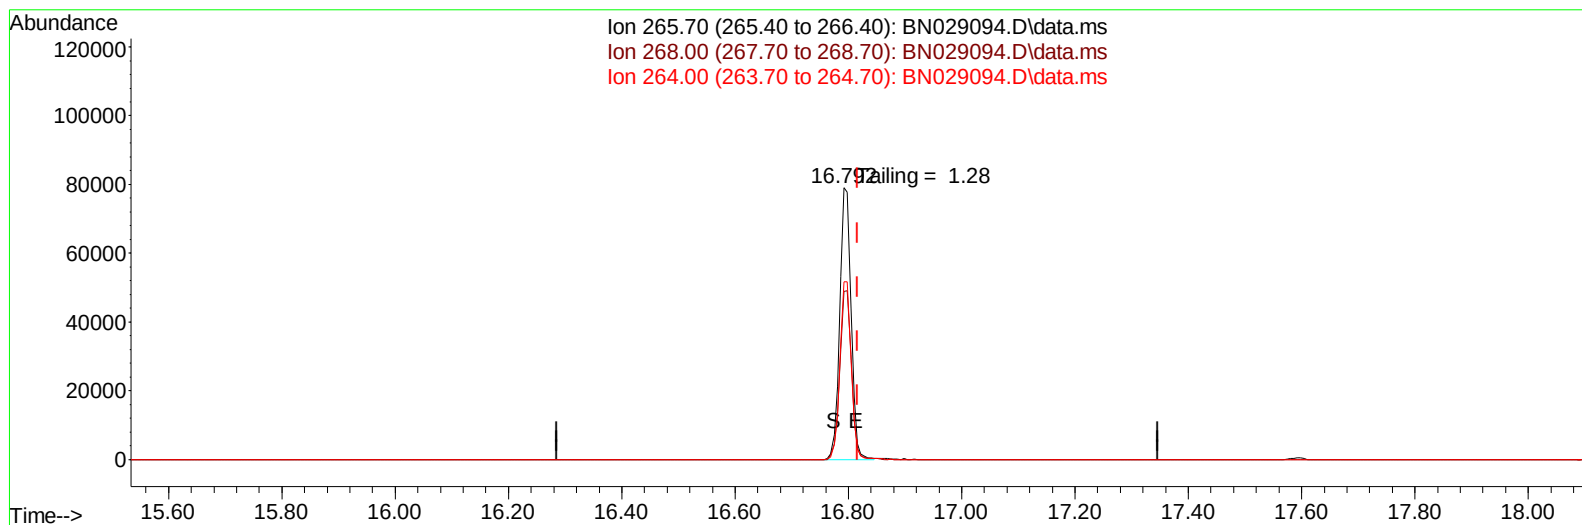

TIC: BN029094.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.024) 14688.15 ng




response 109736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.94
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120723\
Data File : BN029094.D
Acq On : 07 Dec 2023 17:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 07 23:51:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

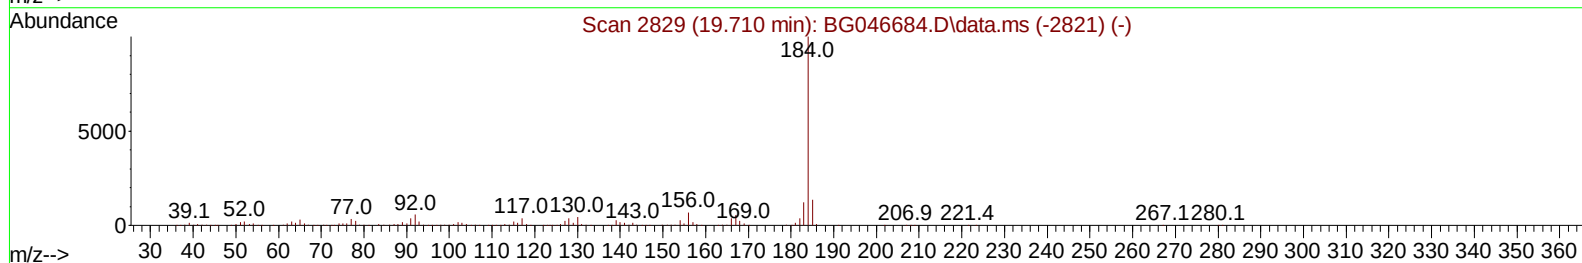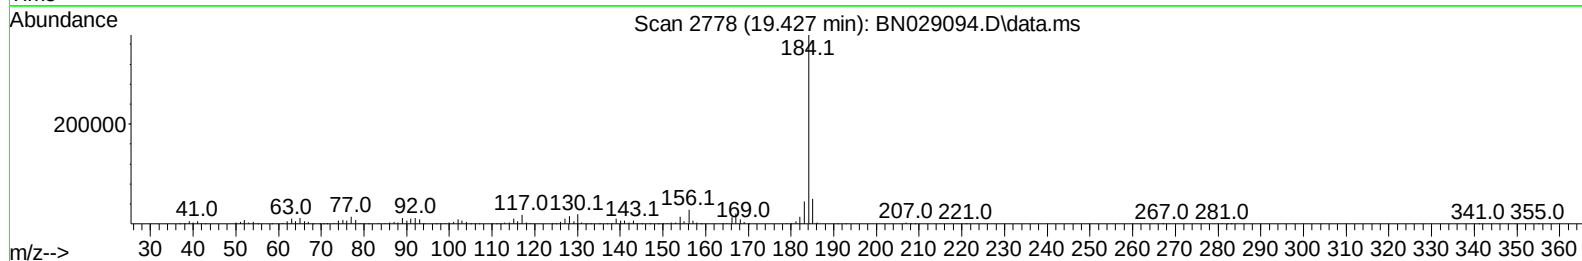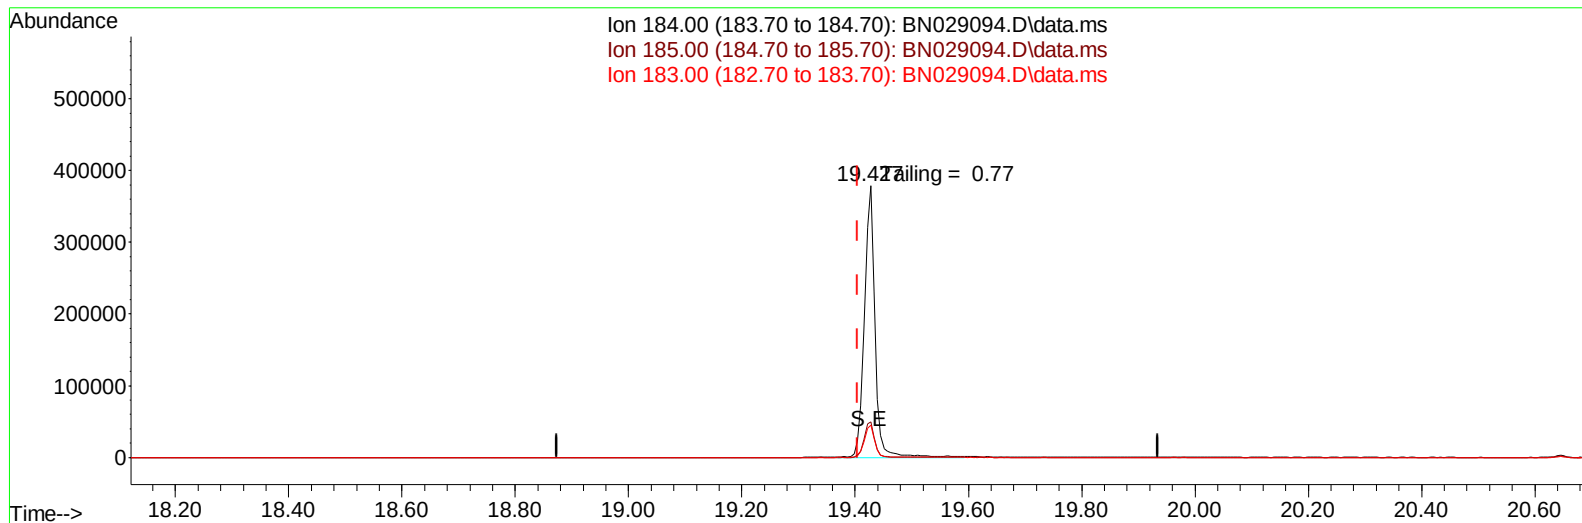

TIC: BN029094.D\data.ms

(77) Benzidine

19.427min (+ 0.023) 0.00 ng

response 489191

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.17
183.00	13.20	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2023	BNA_N	<u>BN029094.D</u>
Compound Name	Response	Retention Time
DDT	388885	20.645
DDD	10078	20.204
DDE	346	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10424	399309	2.61

Instrument :
BNA_N
ClientSampleId :
DFTPP