
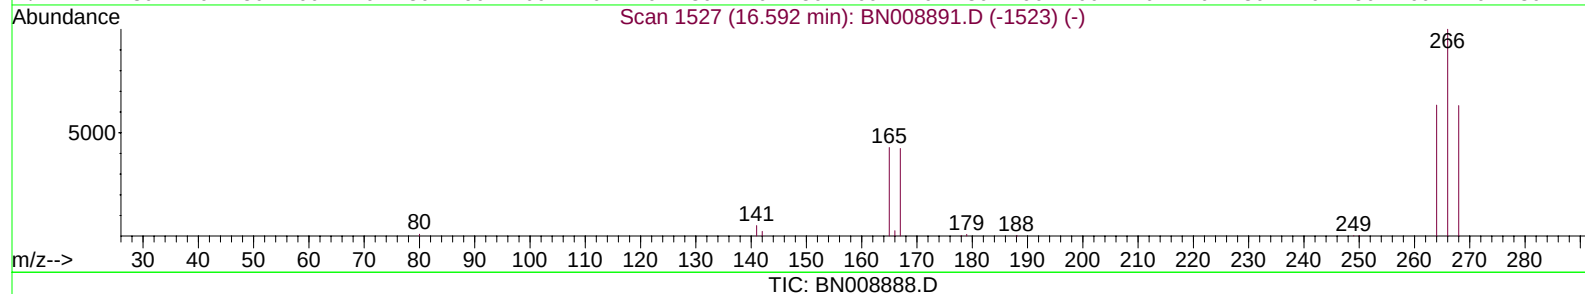
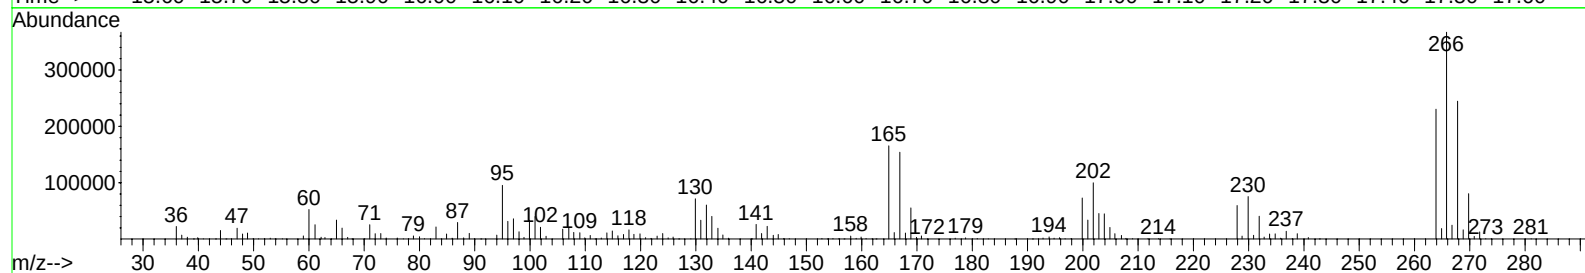


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120919\
Data File : BN008888.D
Acq On : 09 Dec 2019 10:39
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 17:03:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN120919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 09 17:02:53 2019
Response via : Initial Calibration

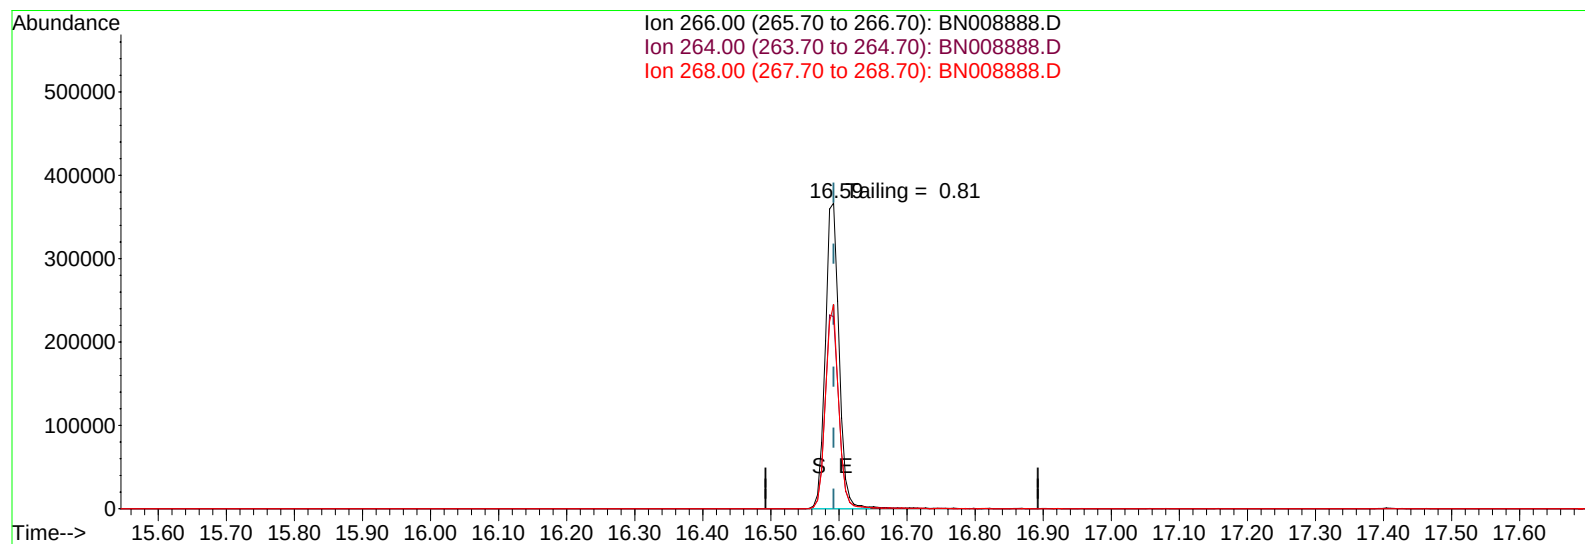

(22) Pentachlorophenol

16.592min (-0.000) 0.00ng

response 516187

Ion	Exp%	Act%
266.00	100	100
264.00	64.40	62.82
268.00	66.40	66.70
0.00	0.00	0.00