


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN120919\
 Data File : BN008888.D
 Acq On : 09 Dec 2019 10:39
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 09 17:02:53 2019

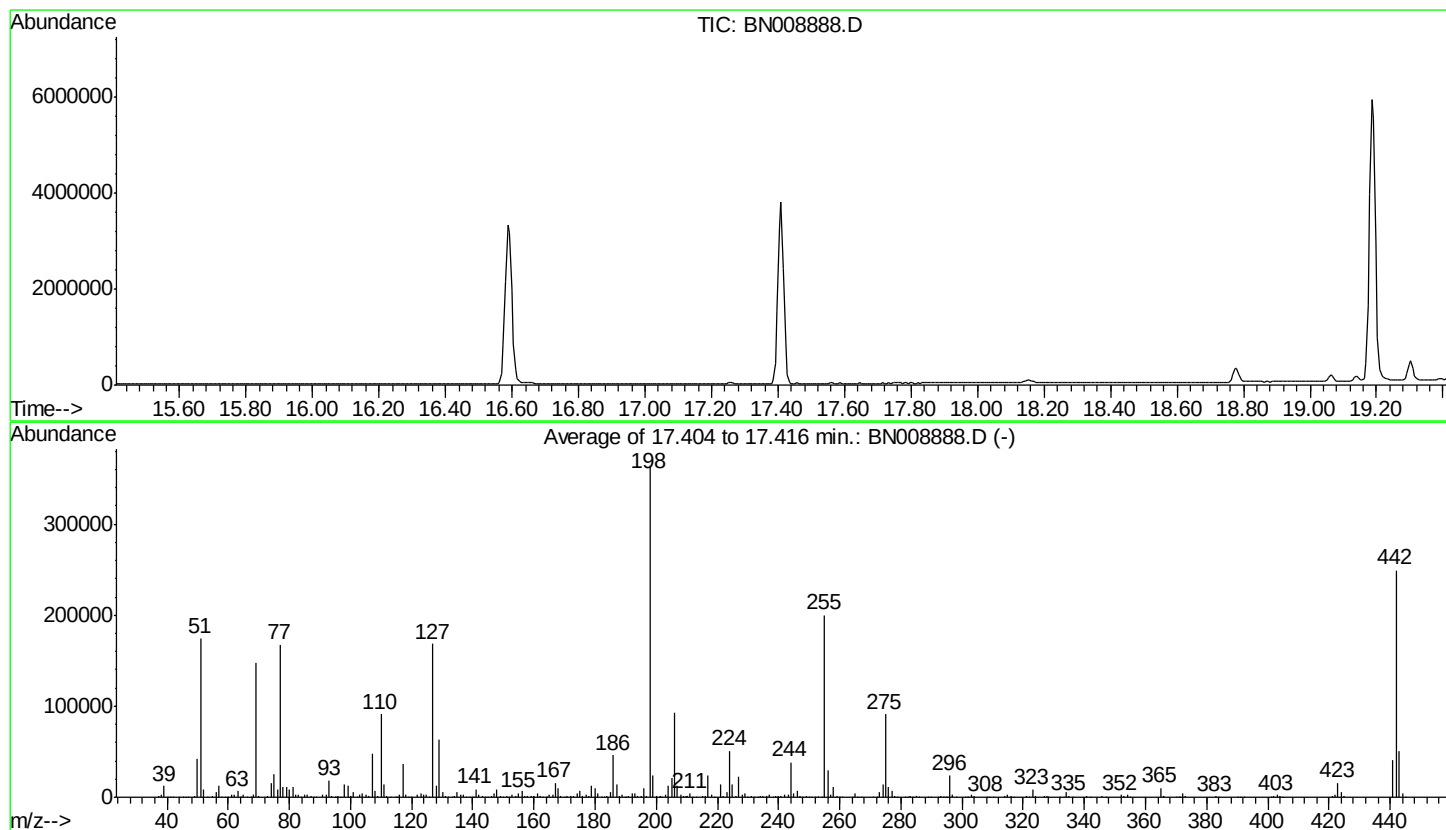

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	174144	PASS
68	69	0.00	2	1.9	2737	PASS
69	198	0.00	100	40.4	147085	PASS
70	69	0.00	2	0.6	856	PASS
127	198	10	80	46.2	168090	PASS
197	198	0.00	2	0.4	1359	PASS
198	198	100	100	100.0	364181	PASS
199	198	5	9	6.6	24008	PASS
275	198	10	60	25.1	91306	PASS
365	198	1	100	2.9	10547	PASS
441	198	0.01	100	11.1	40245	PASS
442	198	50	100	68.5	249557	PASS
443	442	15	24	20.2	50301	PASS