


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121019\
 Data File : BN008897.D
 Acq On : 10 Dec 2019 09:38
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN120919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 09 17:02:53 2019

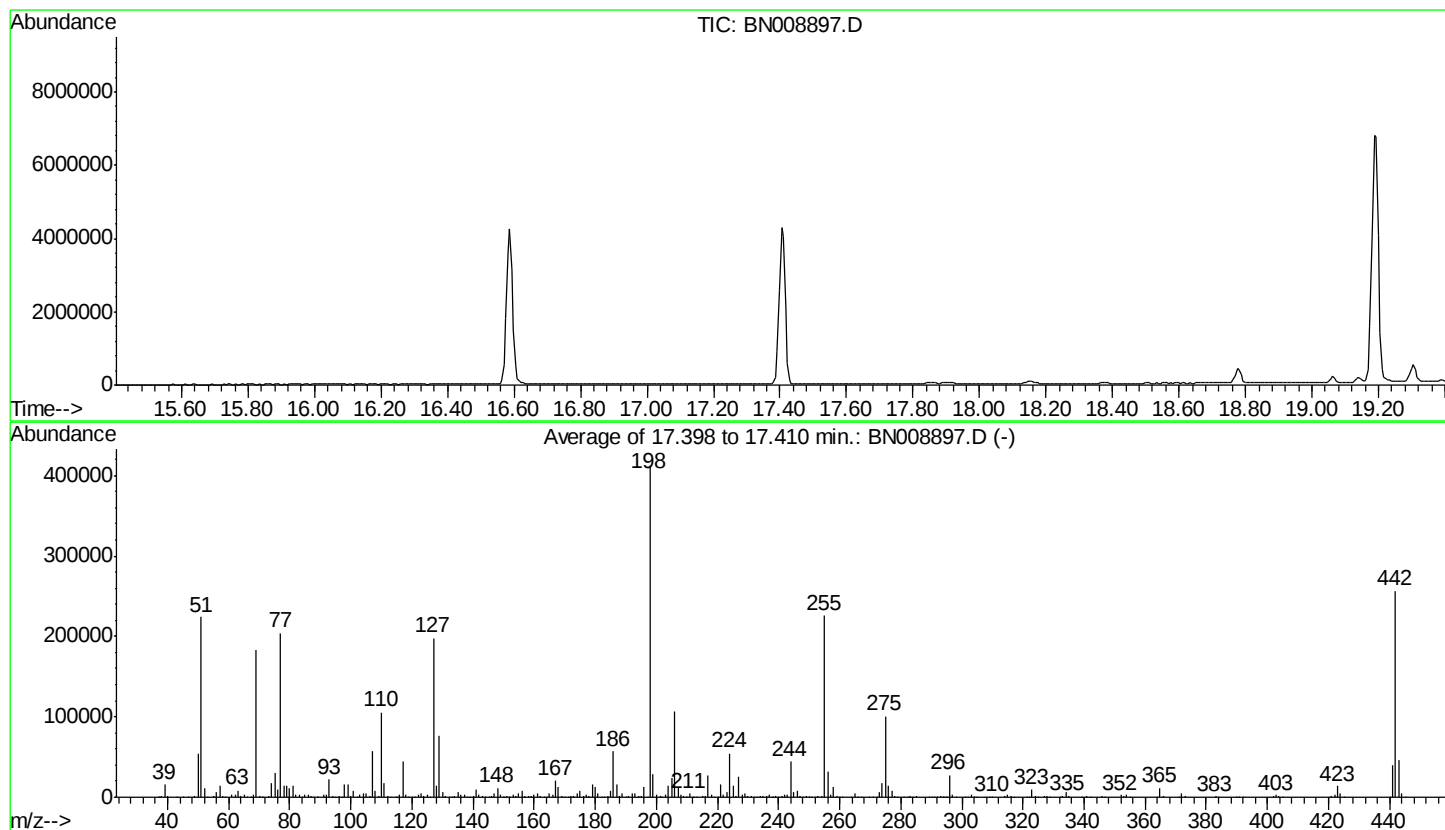

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	224354	PASS
68	69	0.00	2	1.9	3395	PASS
69	198	0.00	100	44.4	183125	PASS
70	69	0.00	2	0.6	1066	PASS
127	198	10	80	48.0	197781	PASS
197	198	0.00	2	0.2	694	PASS
198	198	100	100	100.0	412224	PASS
199	198	5	9	7.0	28690	PASS
275	198	10	60	24.4	100402	PASS
365	198	1	100	2.9	11900	PASS
441	198	0.01	100	9.8	40272	PASS
442	198	50	100	62.2	256413	PASS
443	442	15	24	18.0	46032	PASS