
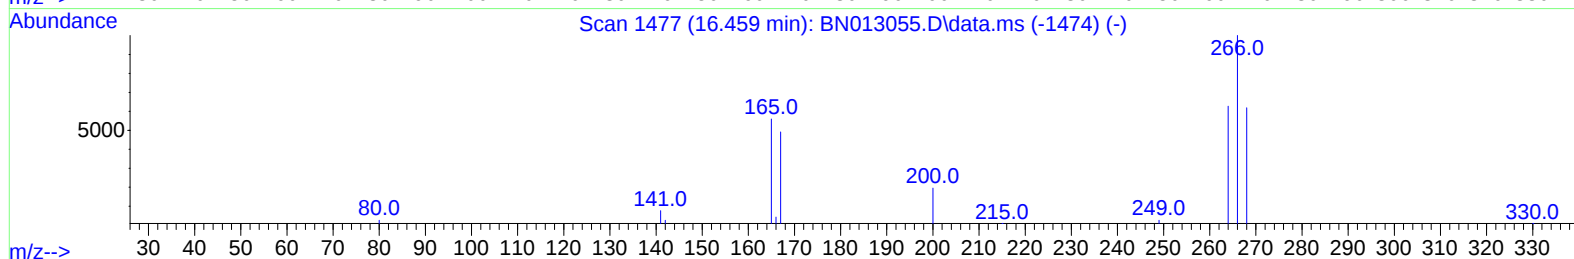
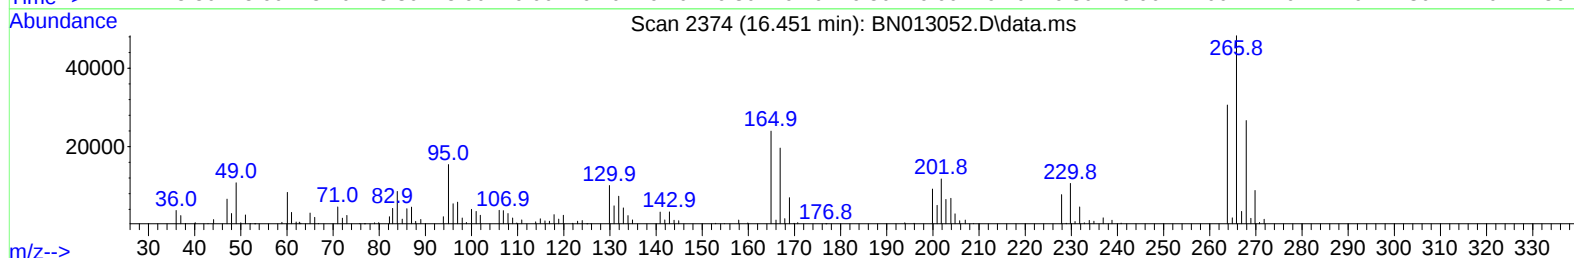


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121020\
Data File : BN013052.D
Acq On : 10 Dec 2020 20:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 04:22:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 01:53:51 2020
Response via : Initial Calibration

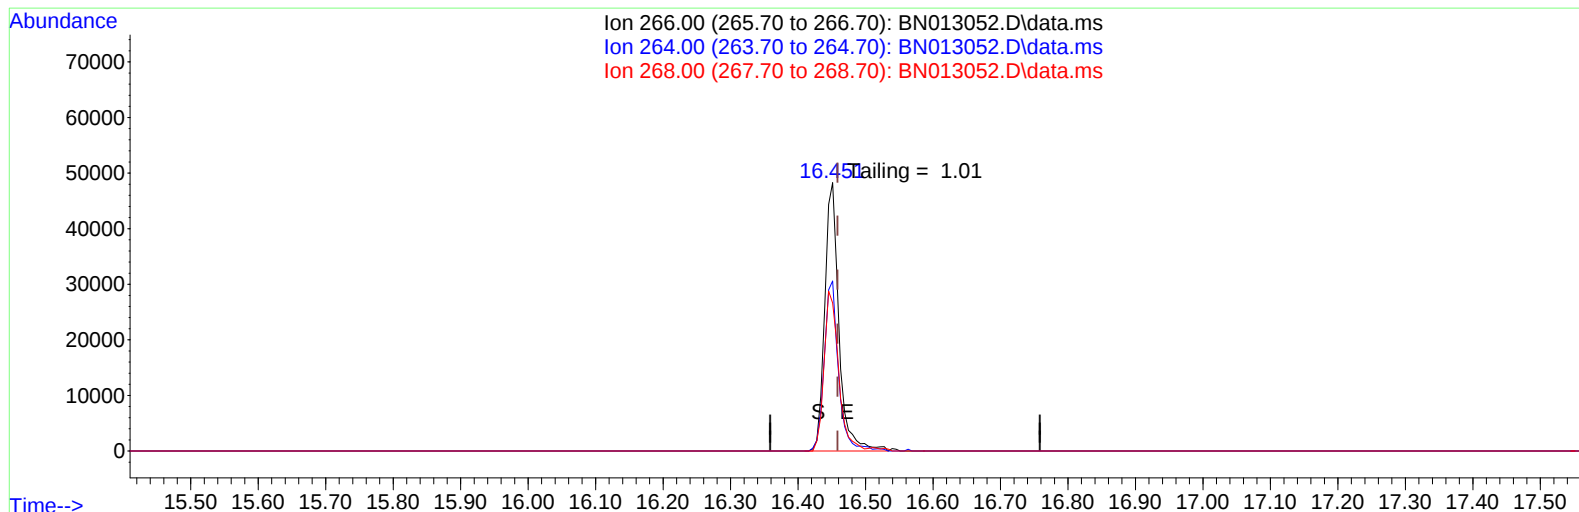

TIC: BN013052.D\data.ms

(24) Pentachlorophenol

16.451min (-0.007) 0.00 ng

response 70976

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	63.60
268.00	64.40	60.94
0.00	0.00	0.00