


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121020\
 Data File : BN013052.D
 Acq On : 10 Dec 2020 20:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 11 01:53:51 2020

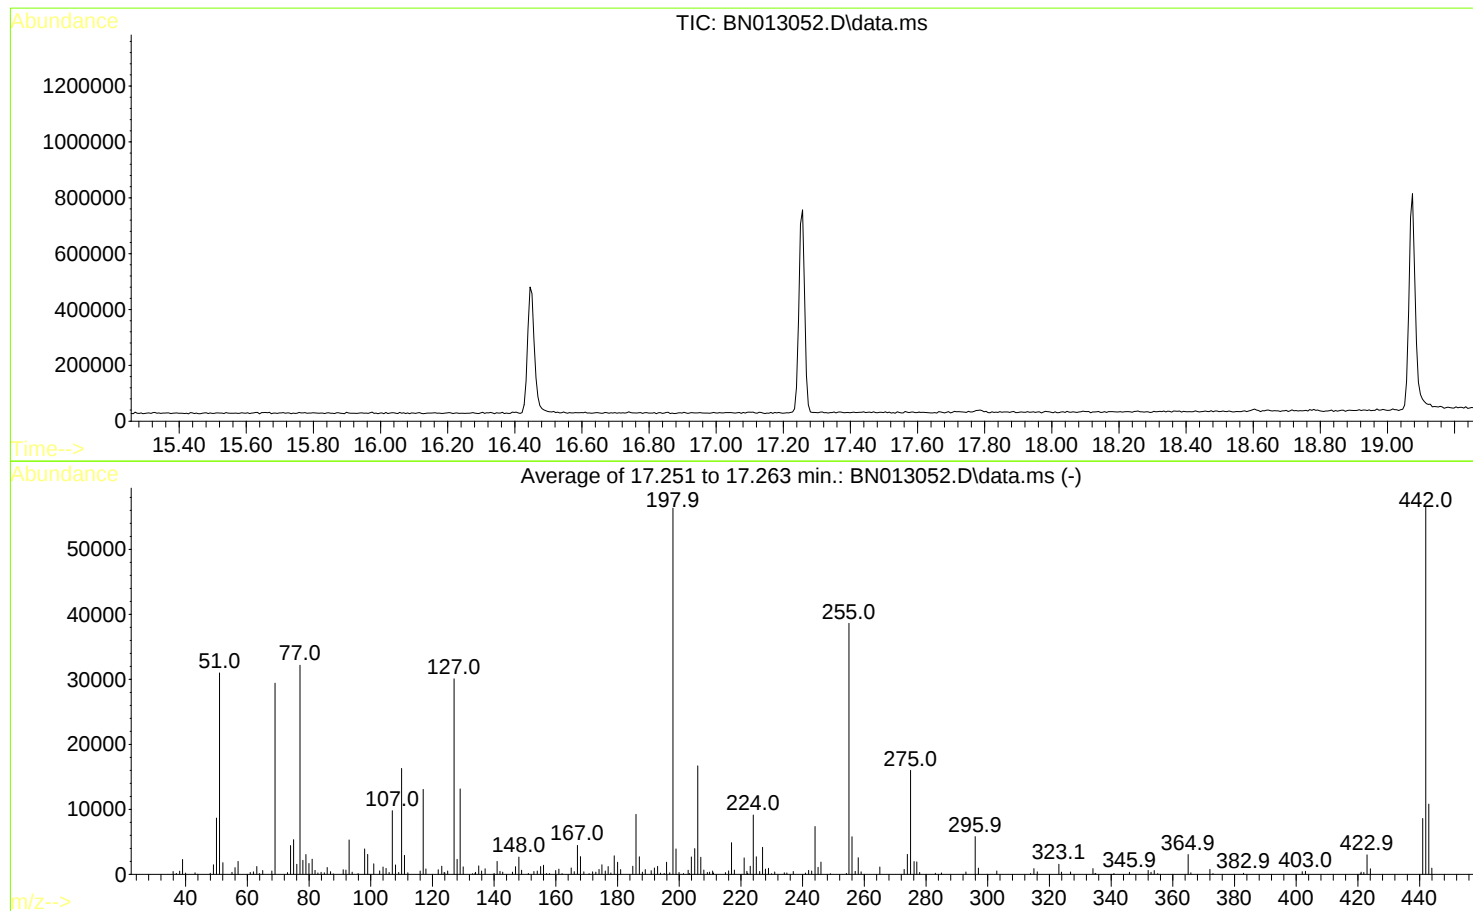

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	31003	PASS
68	69	0.00	2	1.7	510	PASS
69	198	0.00	100	52.2	29411	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	30083	PASS
197	198	0.00	2	0.4	239	PASS
198	198	100	100	100.0	56352	PASS
199	198	5	9	6.9	3908	PASS
275	198	10	60	28.4	15990	PASS
365	198	1	100	5.4	3056	PASS
441	198	0.01	100	15.2	8585	PASS
442	442	50	100	100.0	56595	PASS
443	442	15	24	19.1	10802	PASS