


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121025\
Data File : BN038297.D
Acq On : 10 Dec 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

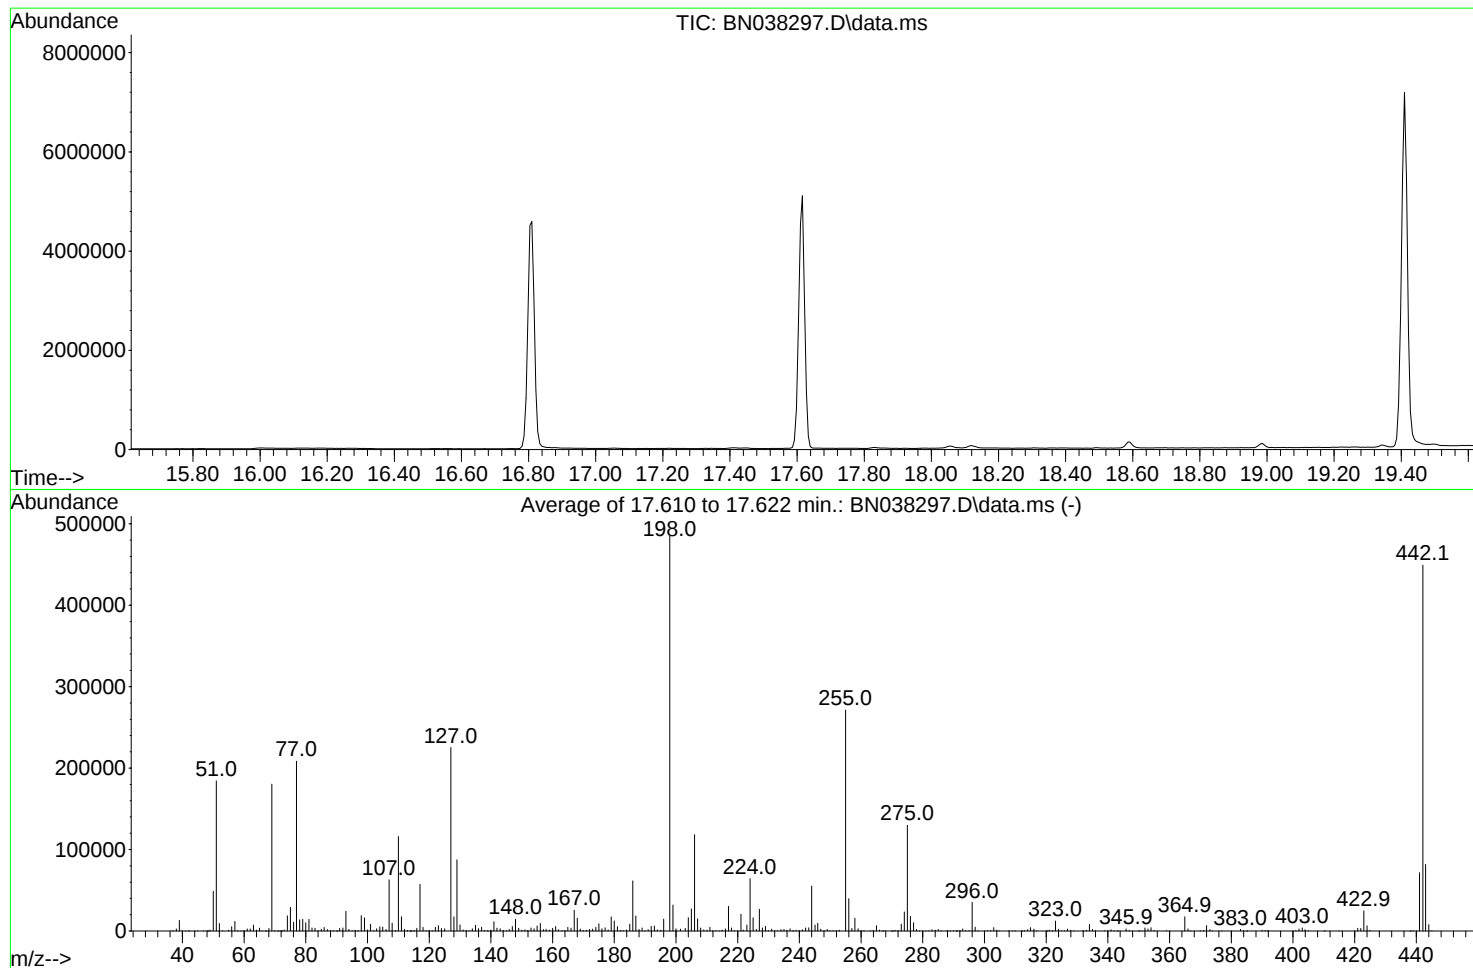




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2461

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3142	PASS
69	69	100	100	100.0	180342	PASS
70	69	0.00	2	0.5	866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	484821	PASS
199	198	5	9	6.6	31797	PASS
365	198	1	100	3.6	17415	PASS
441	443	0.01	150	87.6	71624	PASS
442	442	100	100	100.0	449131	PASS
443	442	15	24	18.2	81797	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121025\
Data File : BN038297.D
Acq On : 10 Dec 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 10:07:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 10:07:34 2025
Response via : Initial Calibration

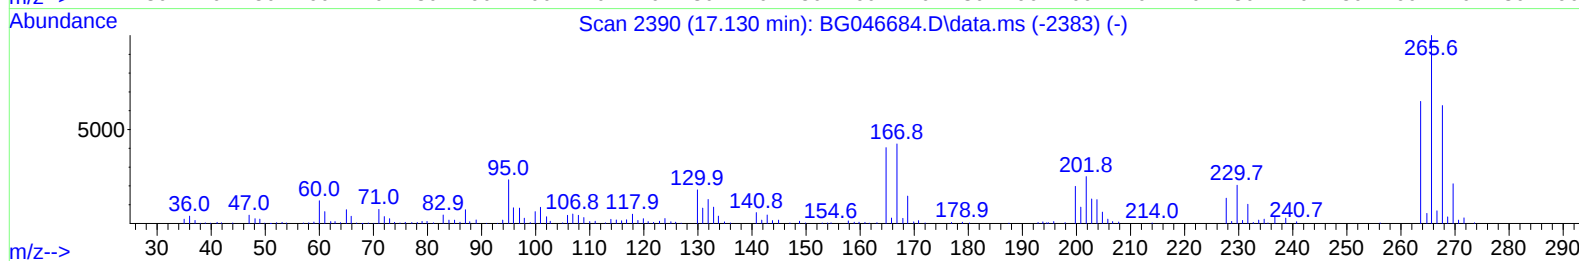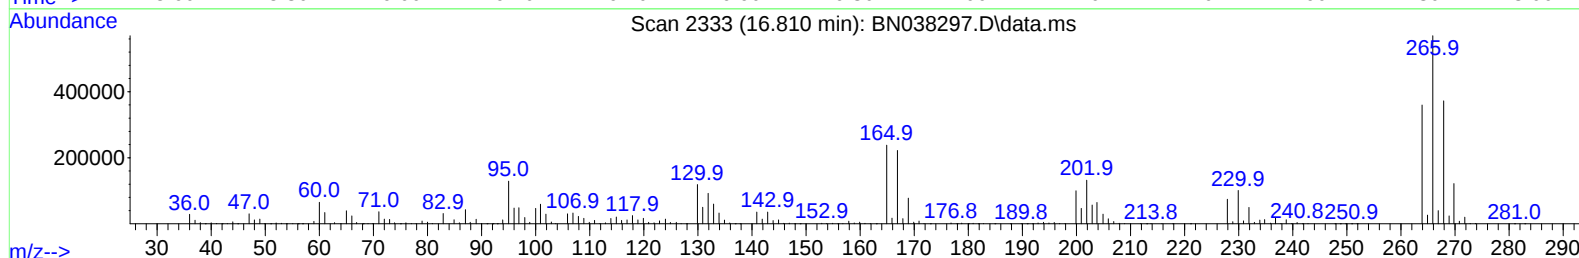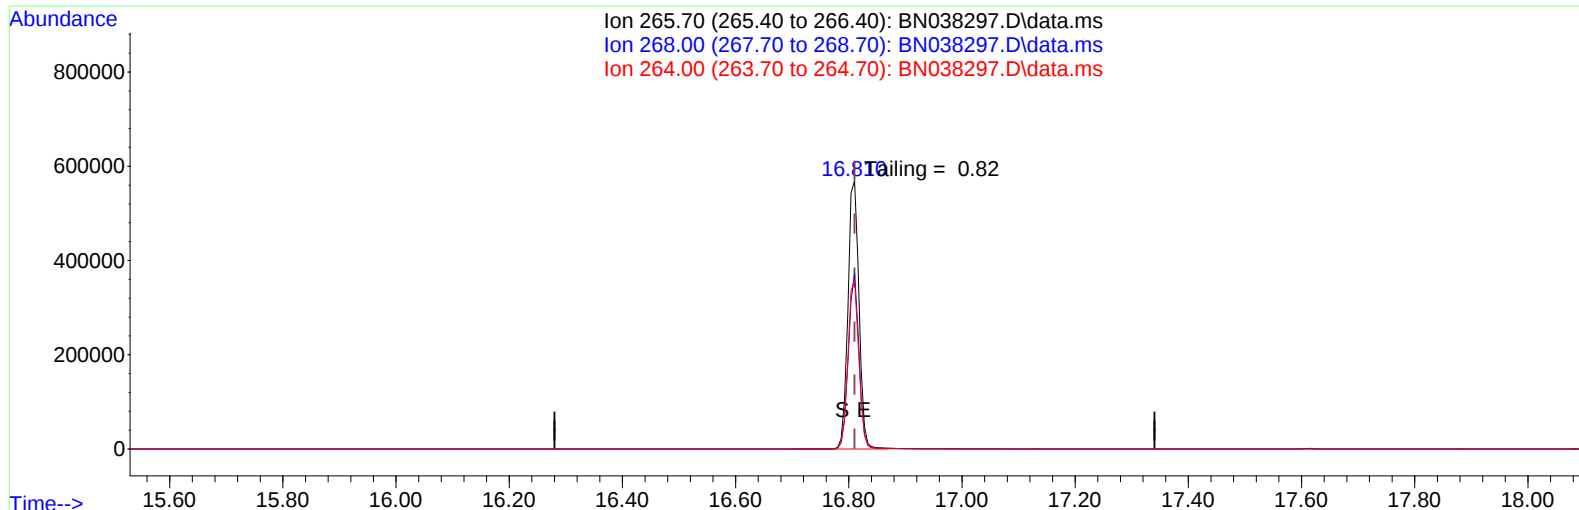

TIC: BN038297.D\data.ms

(70) Pentachlorophenol (C)

16.810min (0.000) 31792.54 ng




response 775196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.41
264.00	61.60	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121025\
Data File : BN038297.D
Acq On : 10 Dec 2025 09:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 10 10:07:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 10:07:34 2025
Response via : Initial Calibration

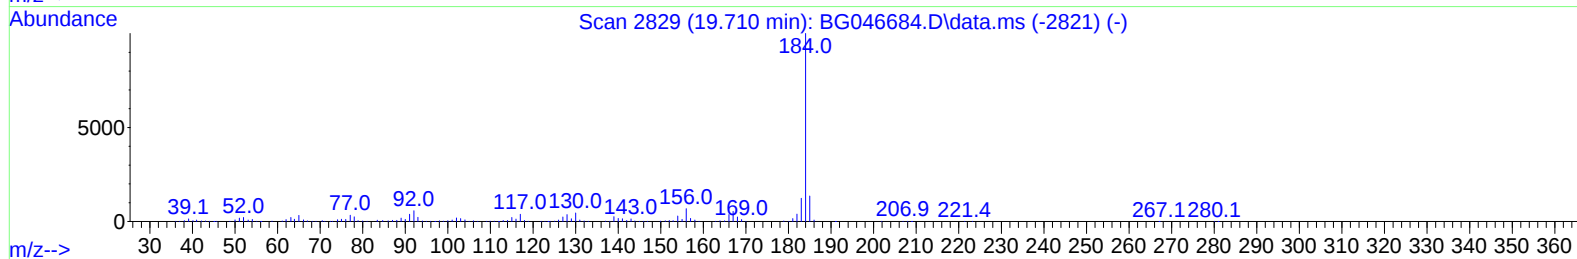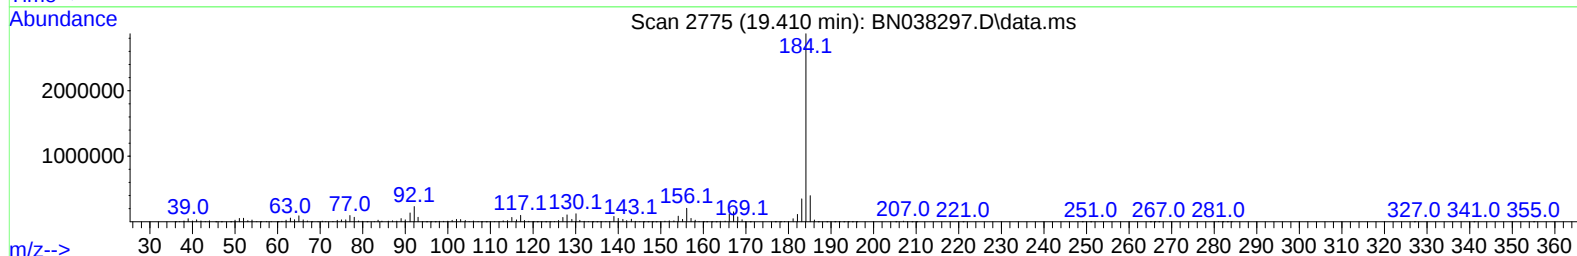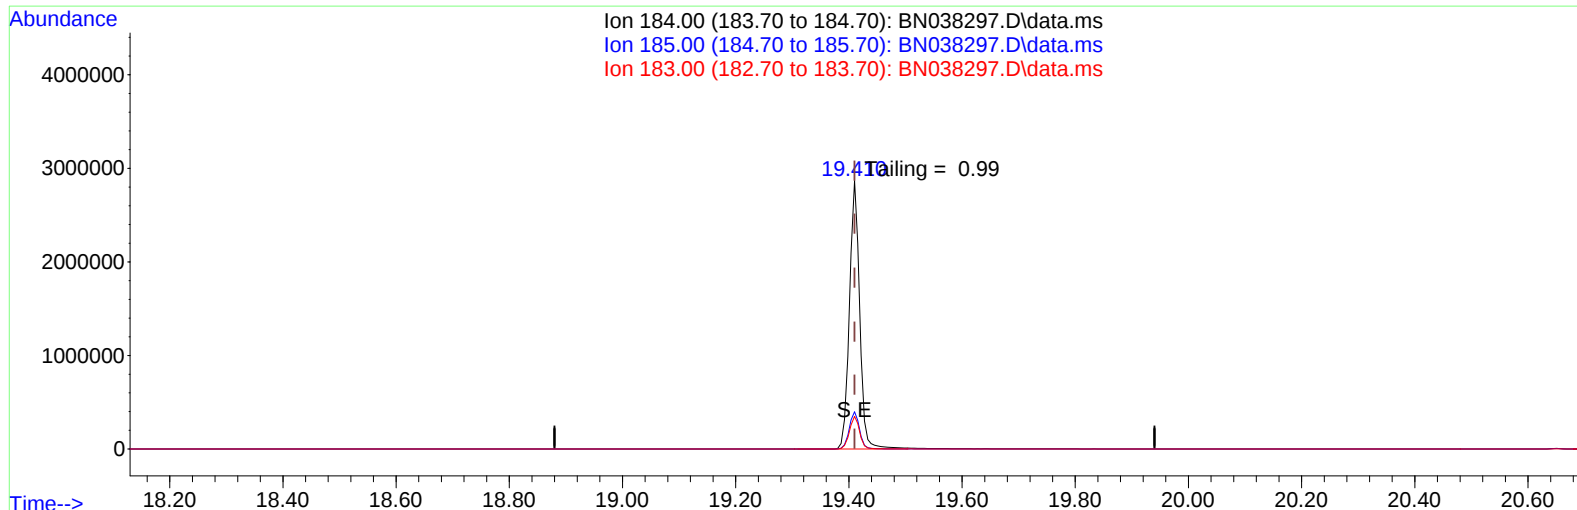

TIC: BN038297.D\data.ms

(77) Benzidine

19.410min (0.000) 0.00 ng

response 3647174

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	12.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2025	BNA_N	<u>BN038297.D</u>
Compound Name	Response	Retention Time
DDT	1762895	20.651
DDD	8462	20.263
DDE	533	18.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8995	1771890	0.51

Instrument :
BNA_N
ClientSampleId :
DFTPP