

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003811.D
 Acq On : 11 Dec 2018 13:04
 Operator : JU/SJ
 Sample : J6137-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 11 14:56:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5064	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20315	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	10647	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1425490	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.71	264	15925	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9839	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.57	252	4723	0.083	ng/ul#	Ovalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003811.D
 Acq On : 11 Dec 2018 13:04
 Operator : JU/SJ
 Sample : J6137-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 11 14:56:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

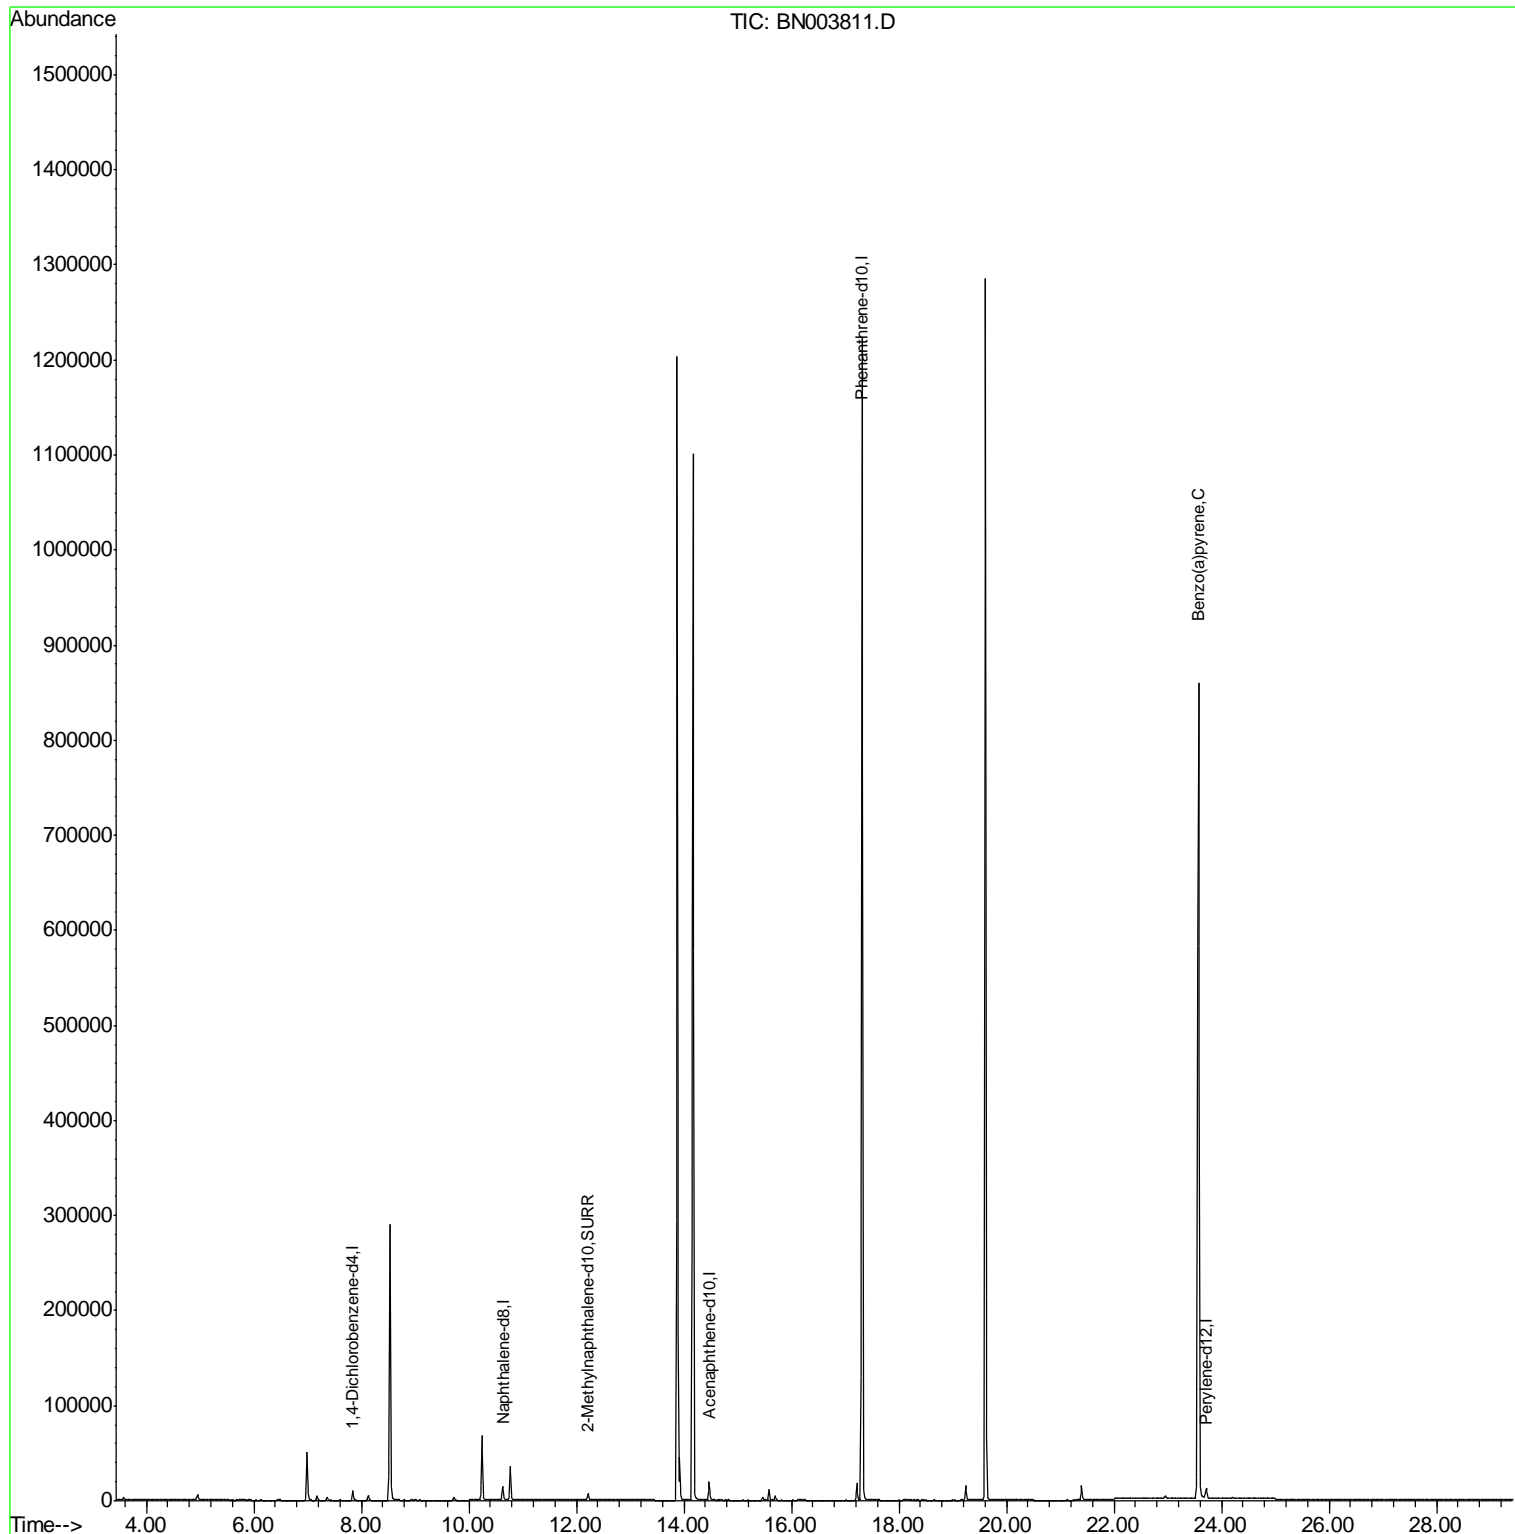

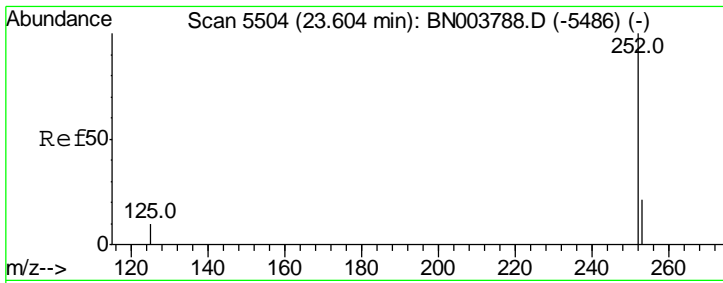

#23
 Benzo(a)pyrene
 Concen: 0.083 ng/ul
 RT: 23.57 min Scan# 5492
 Delta R.T. -0.04 min
 Lab File: BN003811.D
 Acq: 11 Dec 2018 13:04

Instrument :
 BNA_N
 ClientSampled :

Tot Ion	252	253	125
Resp:	4723		
Ion Ratio	100	41.3	34.2
Lower		19.0	10.2
Upper		28.4#	15.4#

