

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003812.D
 Acq On : 11 Dec 2018 13:39
 Operator : JU/SJ
 Sample : J6137-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 11 14:56:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4927	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19389	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9856	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1114224	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.71	264	15594	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	7606	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	2227	0.049	ng/ul#	14
23) Benzo(a)pyrene	23.57	252	3743	0.067	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
Data File : BN003812.D
Acq On : 11 Dec 2018 13:39
Operator : JU/SJ
Sample : J6137-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 11 14:56:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

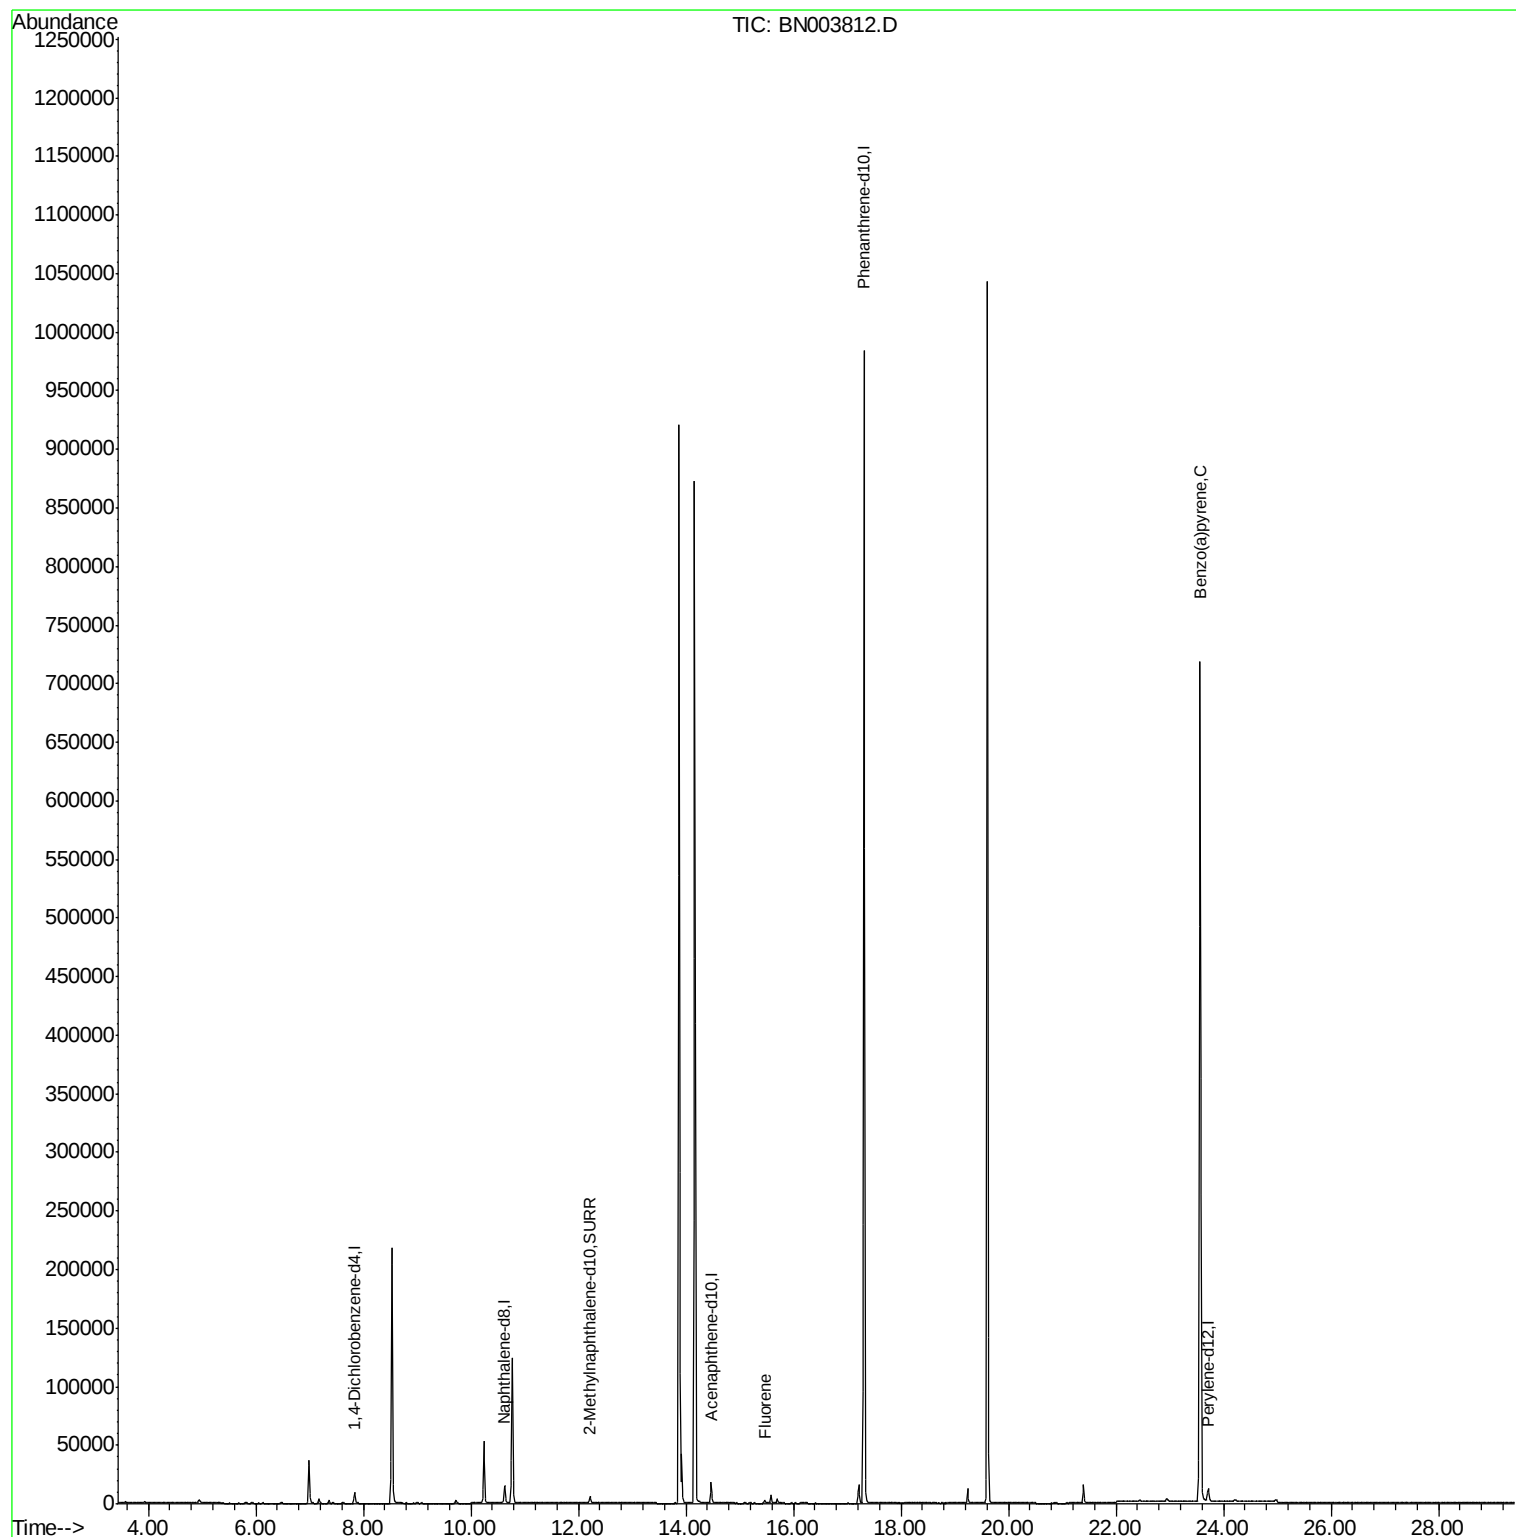

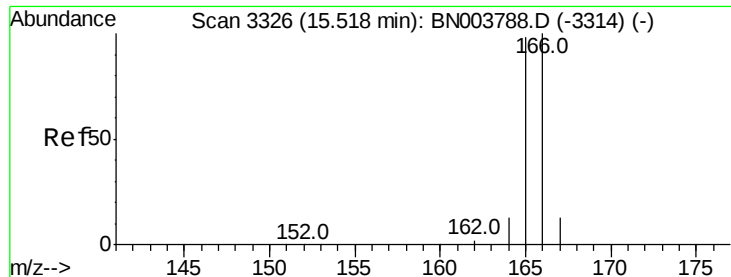

#9

Fluorene

Concen: 0.049 ng/ul

RT: 15.46 min Scan# 3314

Delta R.T. -0.06 min

Lab File: BN003812.D

Acq: 11 Dec 2018 13:39

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 2227

Ion Ratio Lower Upper


166 100

165 7.3 78.3 117.5#



167 33.2 11.3 16.9#

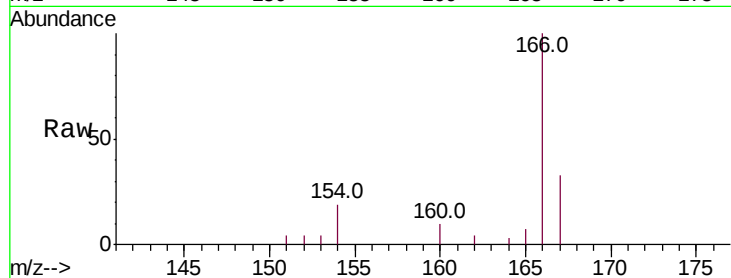

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

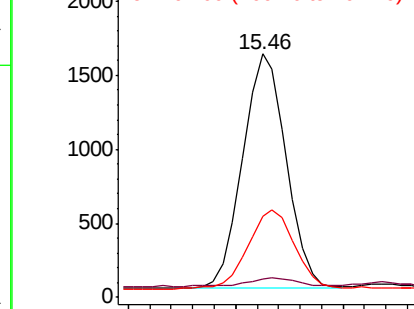

Time-->

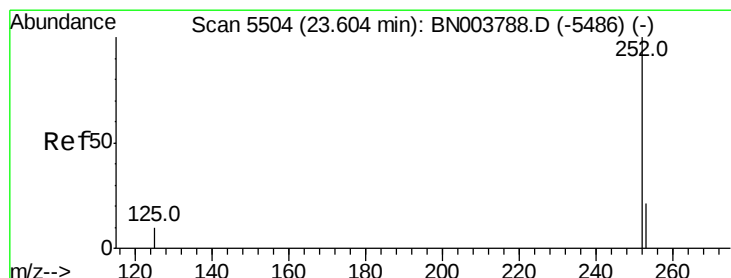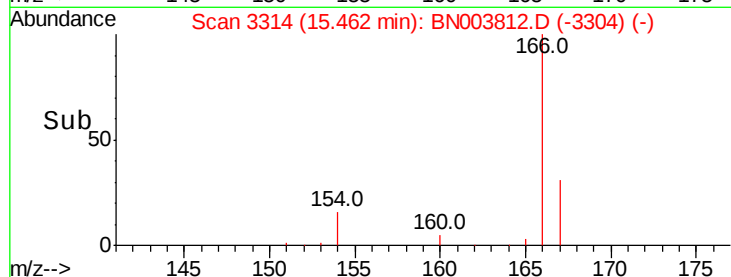

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.57 min Scan# 5491

Delta R.T. -0.04 min

Lab File: BN003812.D

Acq: 11 Dec 2018 13:39


Tgt Ion:252 Resp: 3743

Ion Ratio Lower Upper


252 100

253 43.3 19.0 28.4#

125 36.9 10.2 15.4#

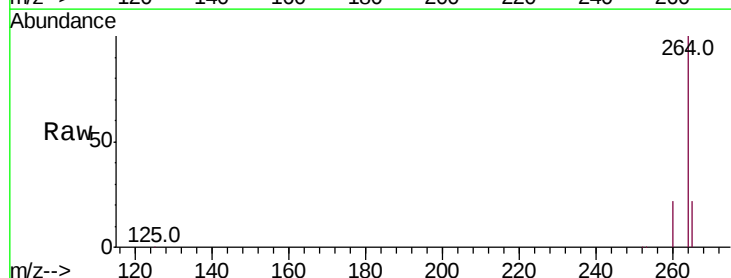

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

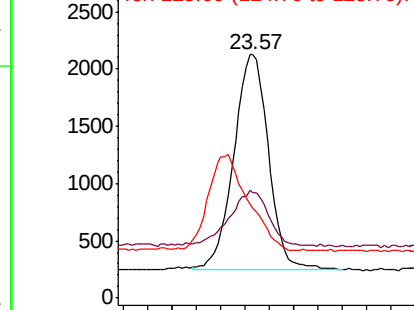

Time-->

