

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003814.D
 Acq On : 11 Dec 2018 14:50
 Operator : JU/SJ
 Sample : J6137-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 11 16:00:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 15:12:40 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5315	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20871	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	10220	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	19674	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	14460	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	15943	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	8890	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	13900	0.24	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.68	128	3376	0.058	ng/ul#	94
8) Acenaphthene	14.53	153	2323	0.058	ng/ul	99
9) Fluorene	15.52	166	2304	0.049	ng/ul	99
12) Phenanthrene	17.25	178	5297	0.082	ng/ul	97
23) Benzo(a)pyrene	23.56	252	1693	0.030	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
Data File : BN003814.D
Acq On : 11 Dec 2018 14:50
Operator : JU/SJ
Sample : J6137-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 11 16:00:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 15:12:40 2018
Response via : Initial Calibration

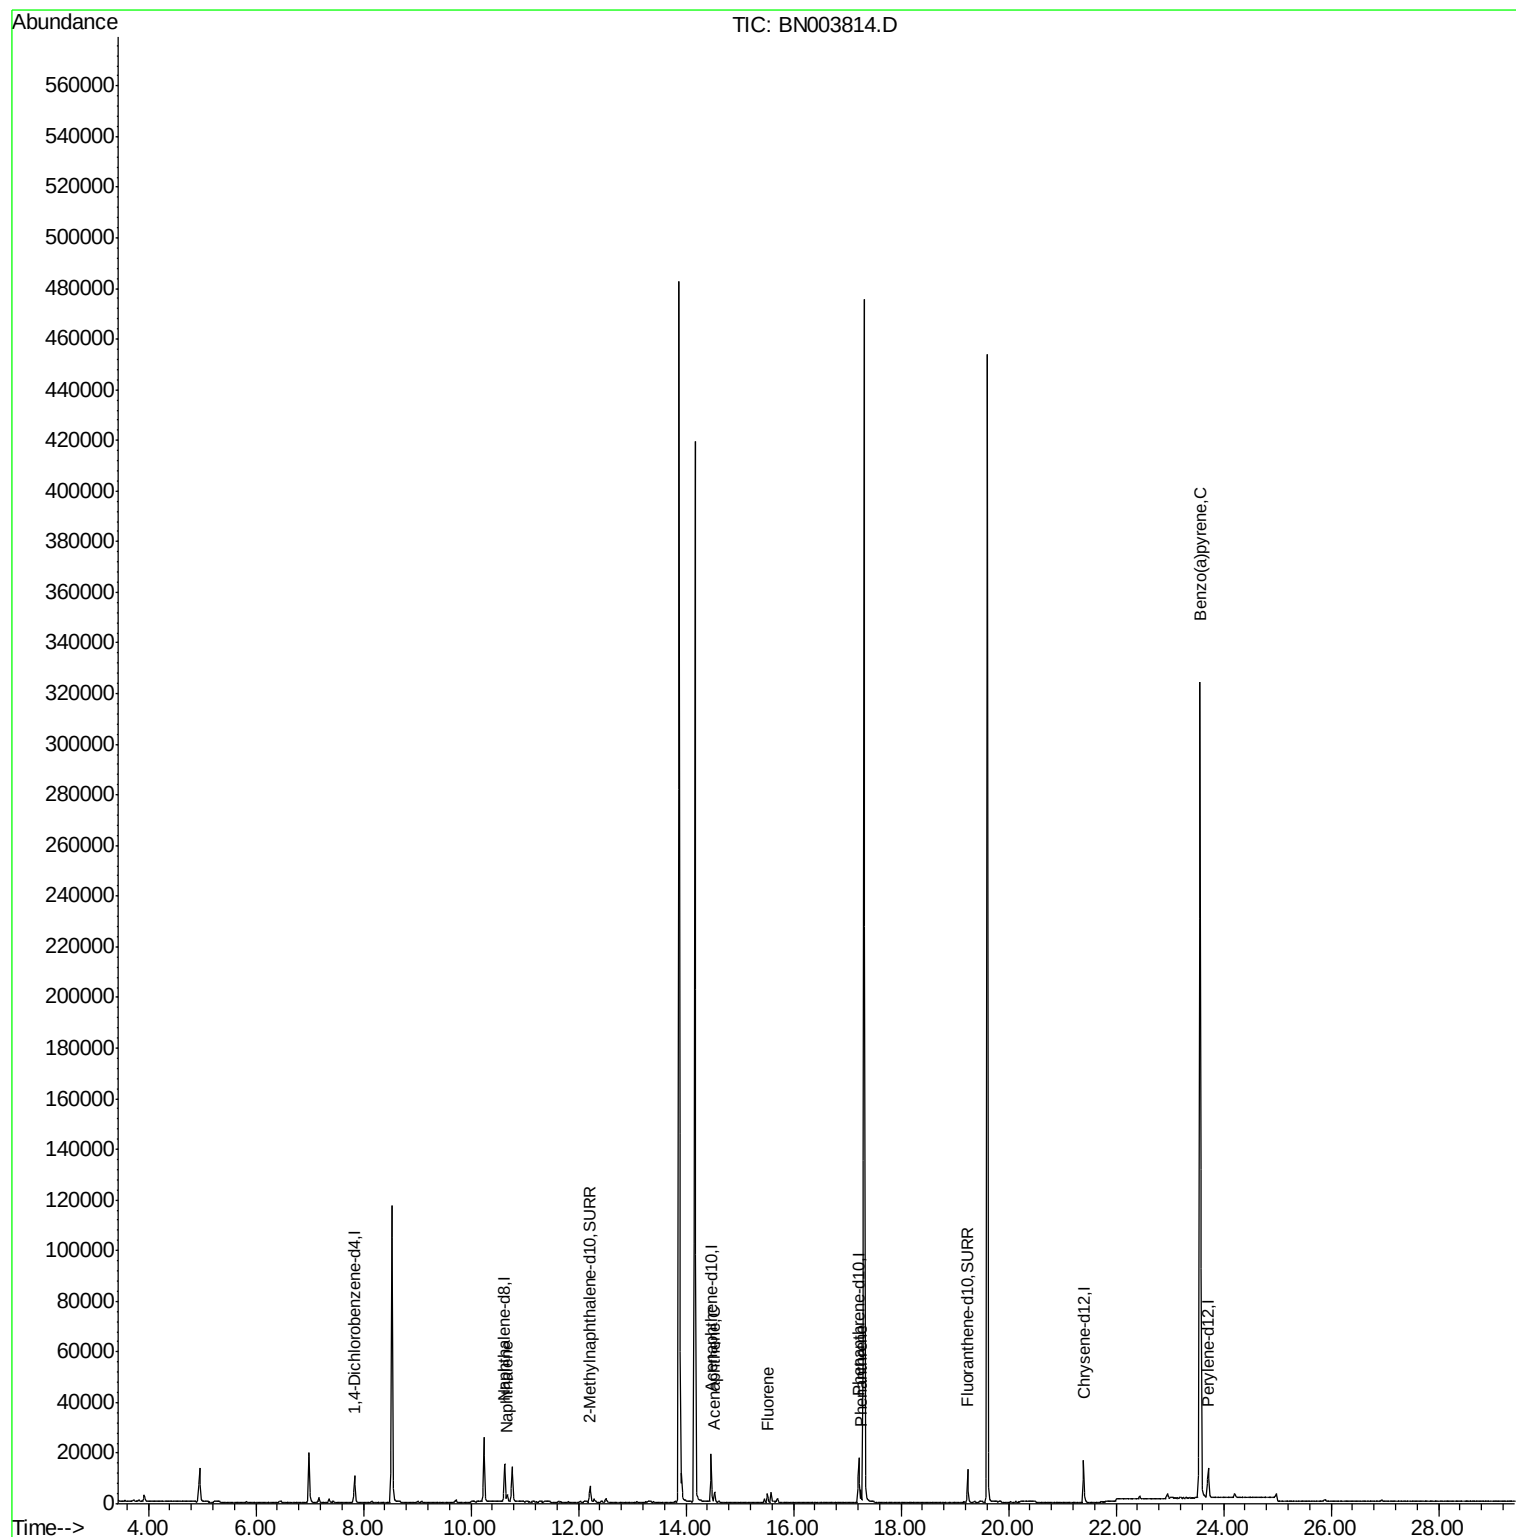

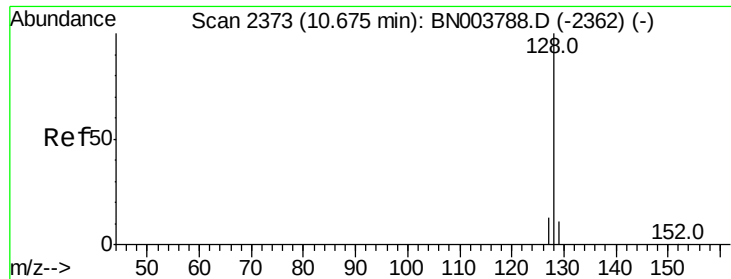

#3

Naphthalene

Concen: 0.058 ng/ul

RT: 10.68 min Scan# 2374

Delta R.T. 0.01 min

Lab File: BN003814.D

Acq: 11 Dec 2018 14:50

Instrument :

BNA_N

ClientSampled :


Tot Ion:128 Resp: 3376

Ion Ratio Lower Upper

128 100

129 14.4 9.0 13.6#




127 15.0 10.5 15.7

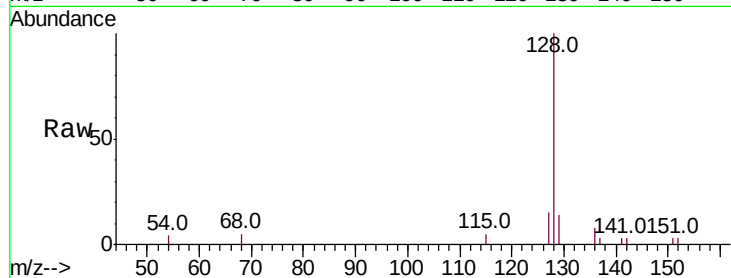

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

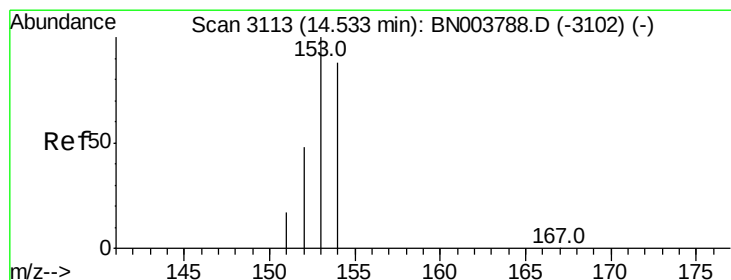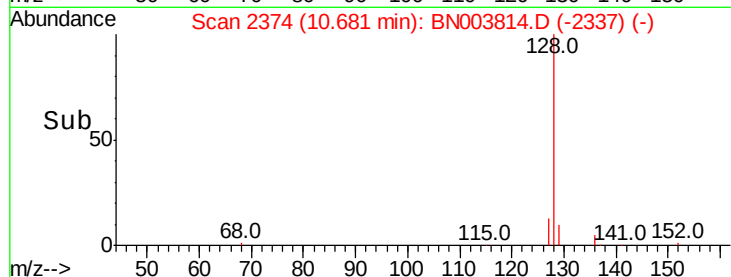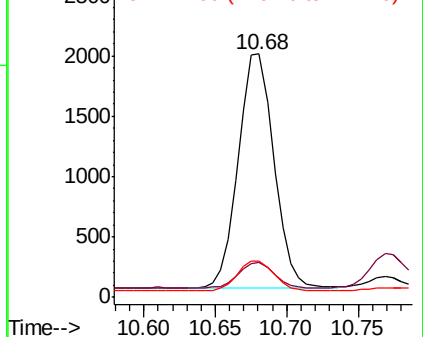

#8

Acenaphthene

Concen: 0.058 ng/ul

RT: 14.53 min Scan# 3113

Delta R.T. -0.00 min

Lab File: BN003814.D

Acq: 11 Dec 2018 14:50


Tgt Ion:153 Resp: 2323

Ion Ratio Lower Upper

153 100

152 50.1 39.3 58.9



154 89.2 70.3 105.5

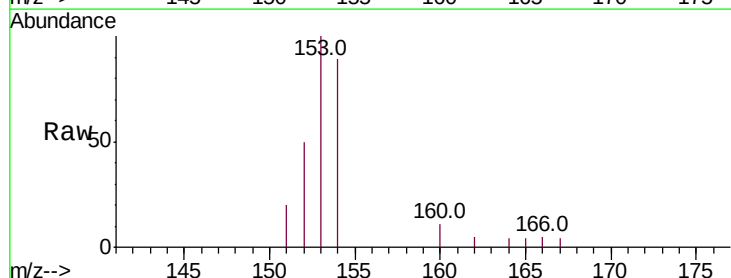


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



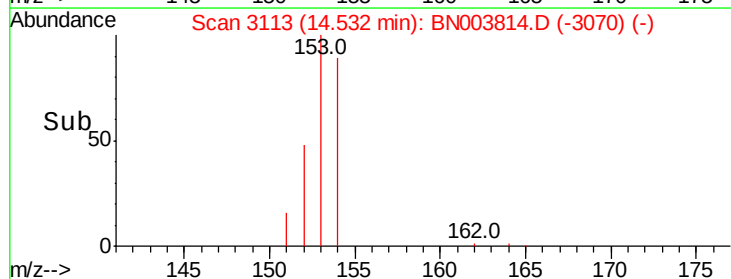
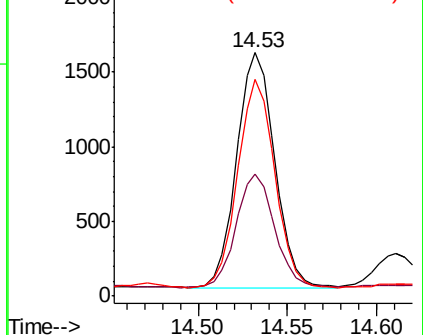


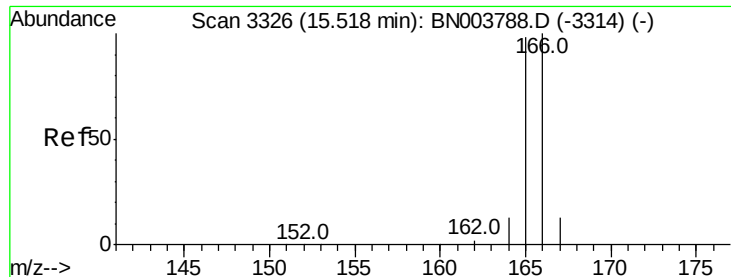

#9
Fluorene
 Concen: 0.049 ng/ul
 RT: 15.52 min Scan# 3326
 Delta R.T. -0.00 min
 Lab File: BN003814.D
 Acq: 11 Dec 2018 14:50




Instrument :
 BNA_N
 ClientSampleId :


Tot Ion:166 Resp: 2304
 Ion Ratio Lower Upper
 166 100
 165 98.0 78.3 117.5
 167 16.7 11.3 16.9

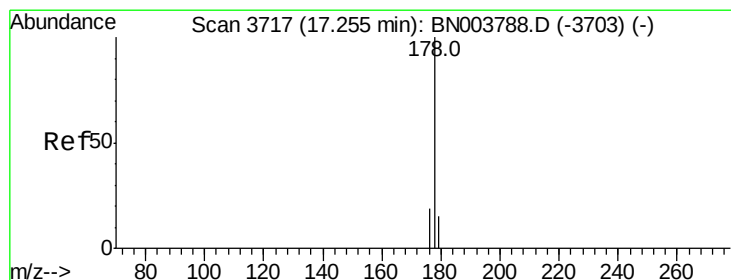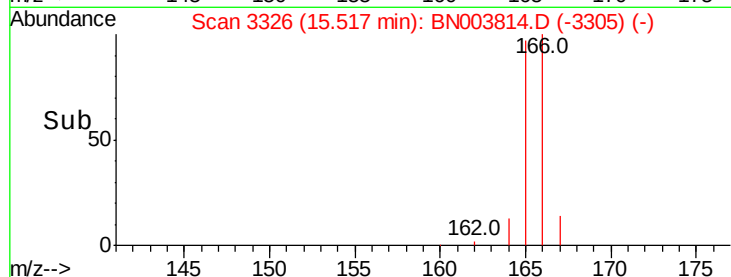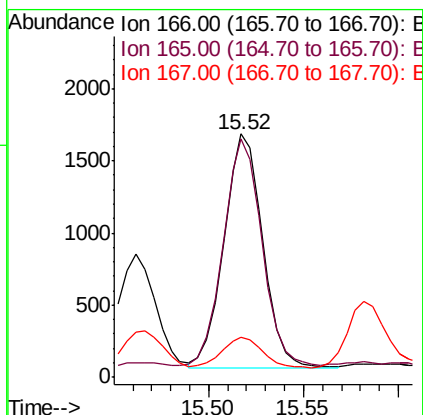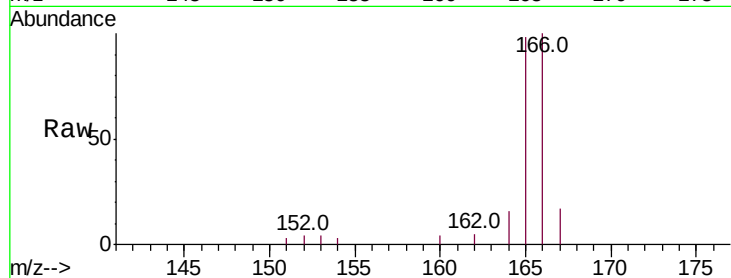

#12
Phenanthrene
 Concen: 0.082 ng/ul
 RT: 17.25 min Scan# 3717
 Delta R.T. -0.00 min
 Lab File: BN003814.D
 Acq: 11 Dec 2018 14:50

Tgt Ion:178 Resp: 5297
 Ion Ratio Lower Upper
 178 100
 179 16.8 12.5 18.7
 176 20.4 15.0 22.4

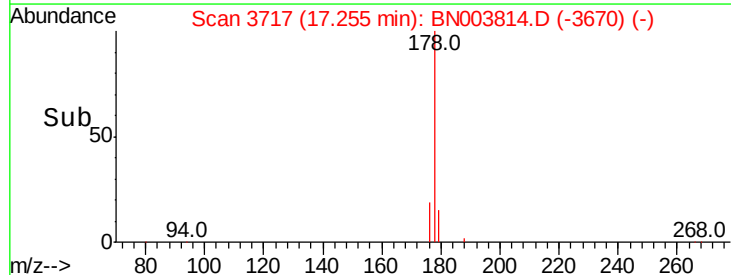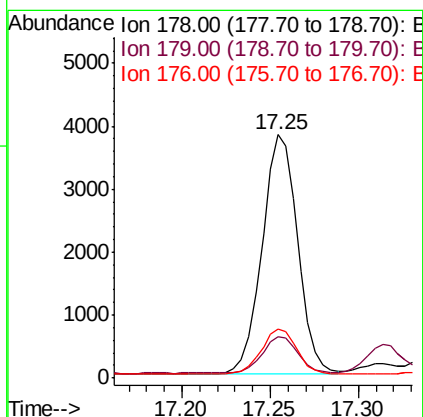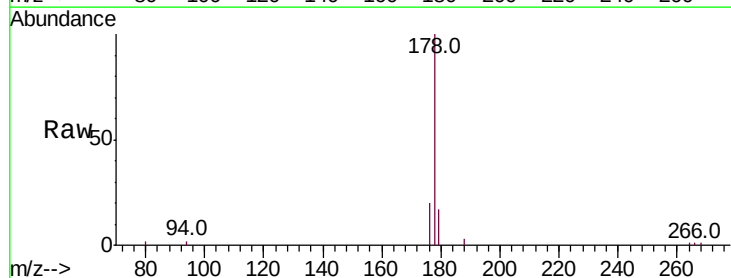

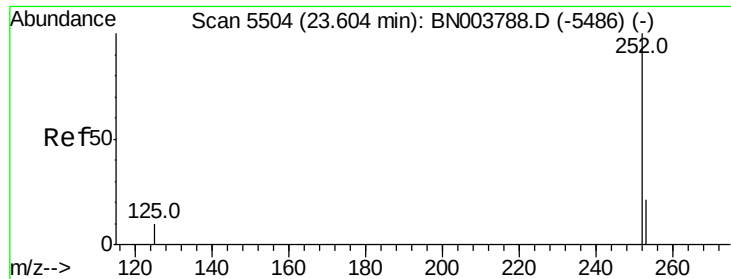

#23

Benzo(a)pyrene

Concen: 0.030 ng/ul

RT: 23.56 min Scan# 5490

Delta R.T. -0.04 min


Lab File: BN003814.D

Acq: 11 Dec 2018 14:50

Instrument :

BNA_N

ClientSampleId :

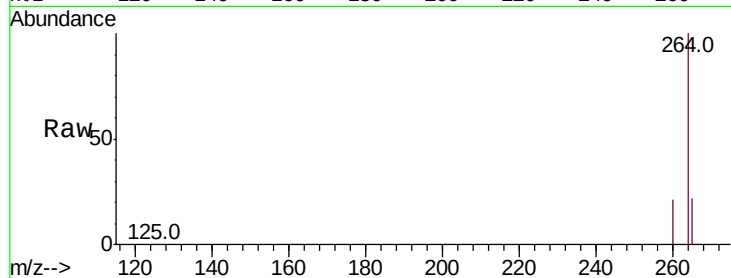


Tot Ion: 252 Resp: 1693

Ion Ratio Lower Upper

252 100

253 61.7 19.0 28.4#

125 73.2 10.2 15.4#

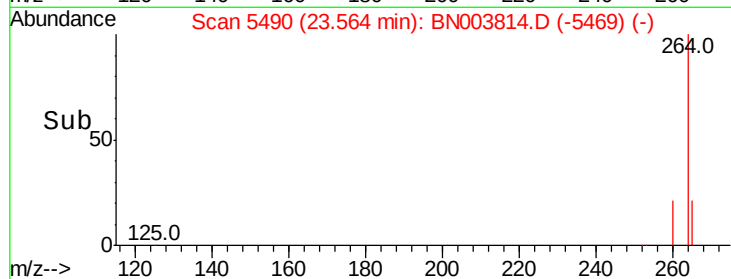

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

