

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Not Reviewed)

Data File : BN003822.D
Acq On : 11 Dec 2018 19:34
Operator : JU/SJ
Sample : J6170-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M11

Quant Time: Dec 12 02:56:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4856	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19096	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9663	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1033591	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	14109	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	7271	0.25	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.57	252	3139	0.062	ng/ul#	Qvalue 51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003822.D
Acq On : 11 Dec 2018 19:34
Operator : JU/SJ
Sample : J6170-16
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M11

Quant Time: Dec 12 02:56:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

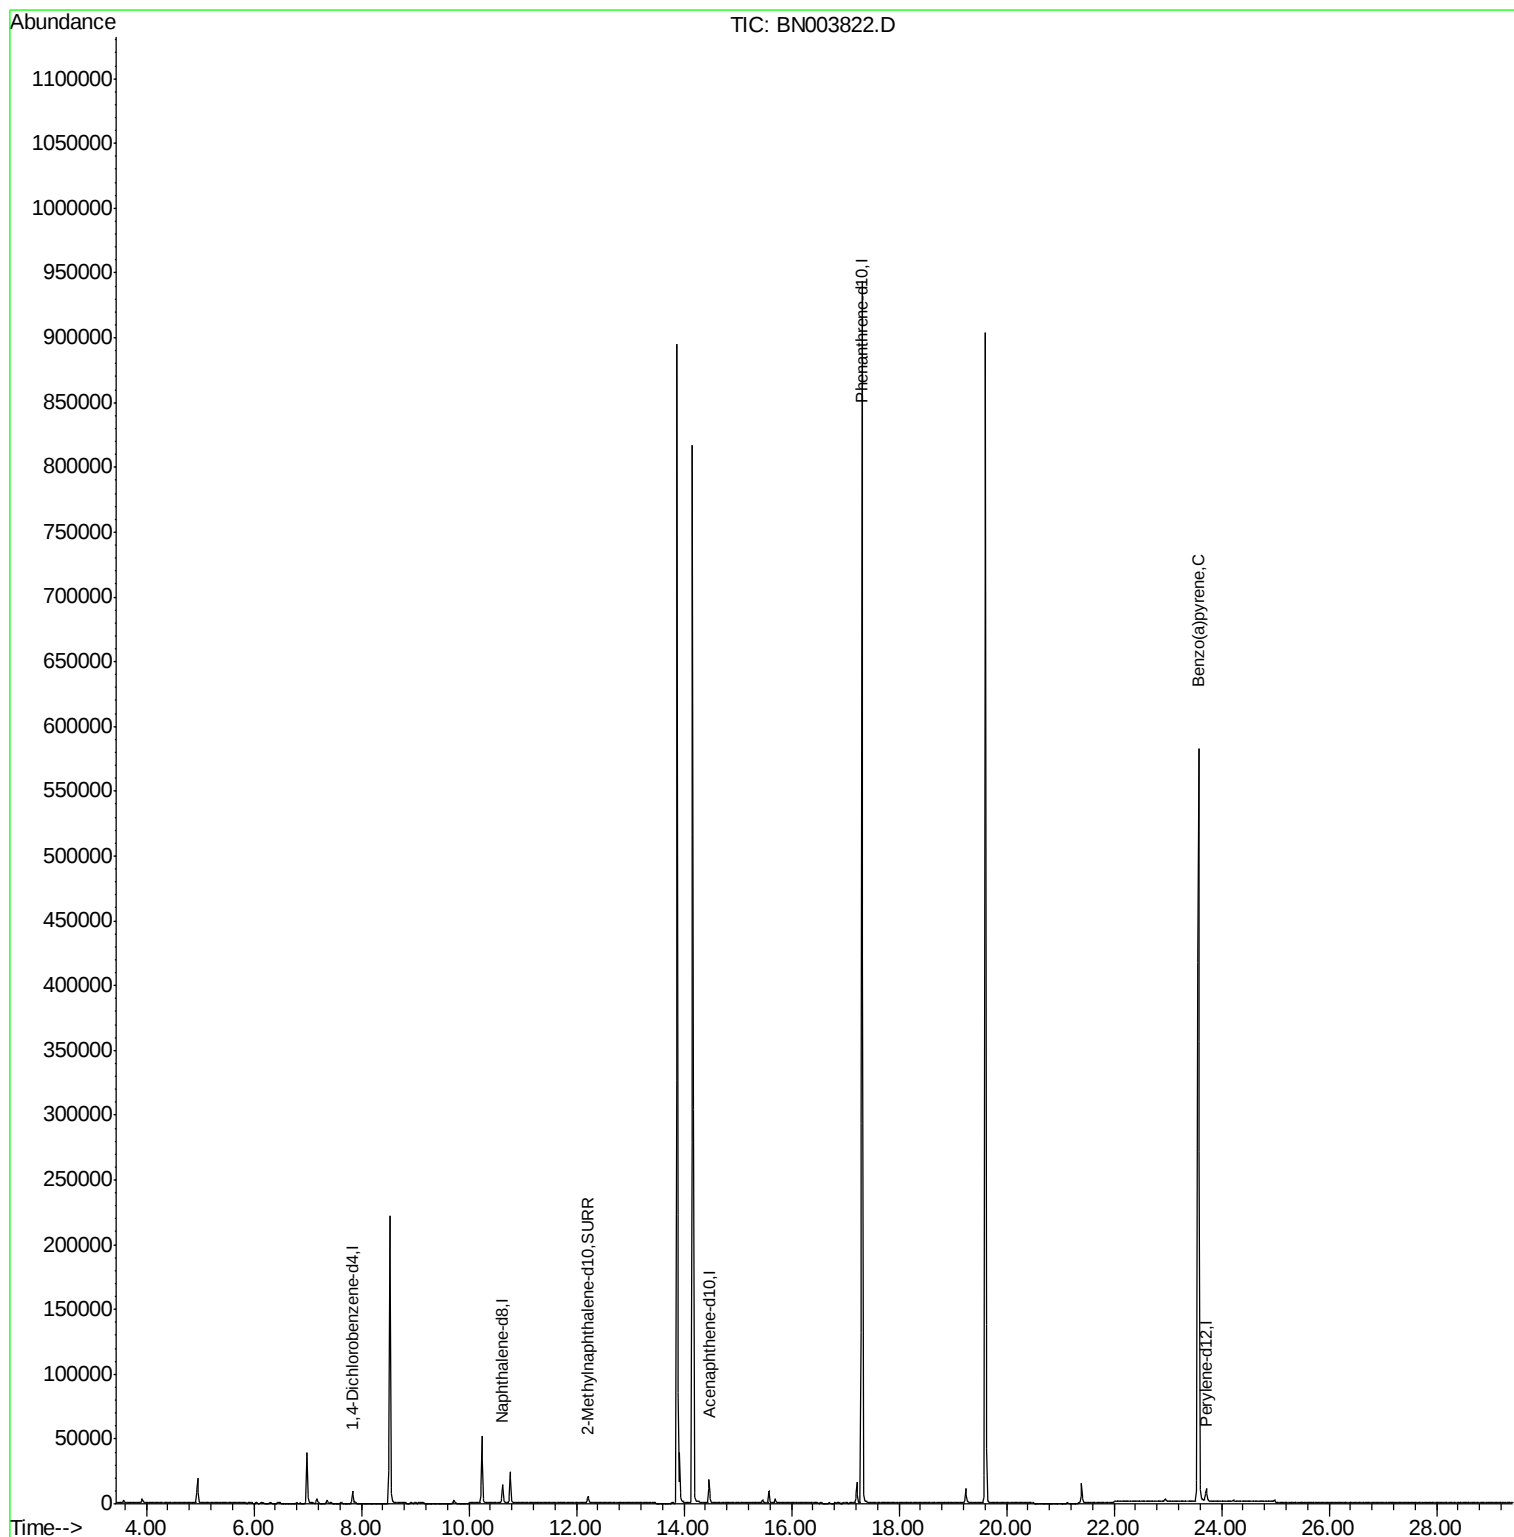

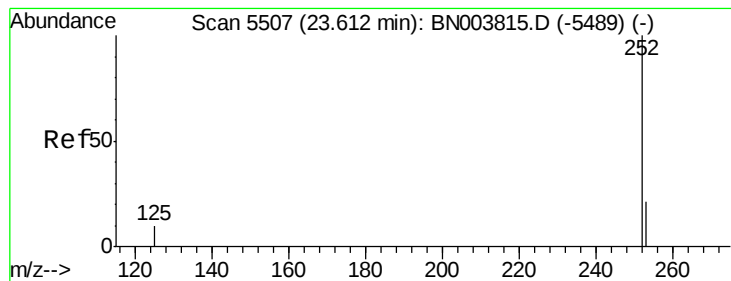

#23

Benzo(a)pyrene

Concen: 0.062 ng/ul

RT: 23.57 min Scan# 5491

Delta R.T. -0.05 min

Lab File: BN003822.D


Acq: 11 Dec 2018 19:34

Instrument :

BNA_N

ClientSampleId :

F9M11

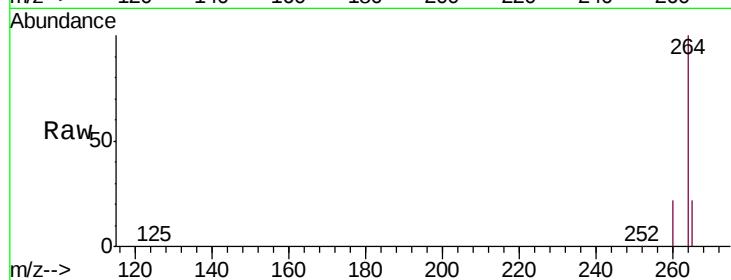


Tgt Ion: 252 Resp: 3139

Ion Ratio Lower Upper

252 100

253 44.2 19.0 28.4#

125 37.7 10.2 15.4#

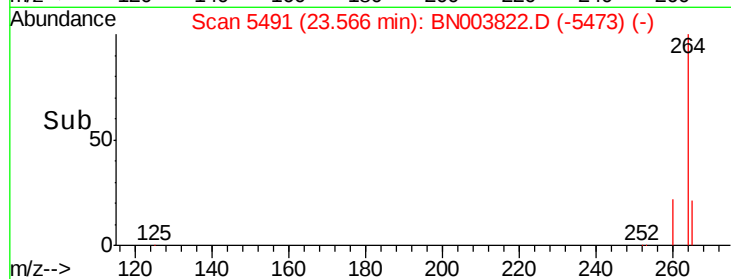

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

