

Data File : BN003829.D
Acq On : 11 Dec 2018 23:39
Operator : JU/SJ
Sample : J6170-19DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14DL

Quant Time: Dec 12 02:57:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4894	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	18592	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	8467	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	15357	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	11749	0.40	ng/ul	0.00
20) Perylene-d12	23.70	264	12910	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	1069	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1517	0.03	ng/ul	0.00
Target Compounds				Qvalue		
12) Phenanthrene	17.25	178	4995	0.099	ng/ul	97
15) Fluoranthene	19.27	202	16868	0.283	ng/ul	96
17) Pyrene	19.63	202	13957	0.331	ng/ul	95
18) Benzo(a)anthracene	21.38	228	6618	0.178	ng/ul	96
19) Chrysene	21.43	228	8369	0.197	ng/ul	97
21) Benzo(b)fluoranthene	23.01	252	16701	0.313	ng/ul	91
22) Benzo(k)fluoranthene	23.01	252	16701	0.321	ng/ul#	91
23) Benzo(a)pyrene	23.60	252	6985	0.151	ng/ul#	88
24) Indeno(1,2,3-cd)pyrene	26.06	276	6441	0.121	ng/ul#	93
25) Dibenzo(a,h)anthracene	26.06	278	1549	0.036	ng/ul#	56
26) Benzo(g,h,i)perylene	26.78	276	5029	0.109	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003829.D
Acq On : 11 Dec 2018 23:39
Operator : JU/SJ
Sample : J6170-19DL 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14DL

Quant Time: Dec 12 02:57:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

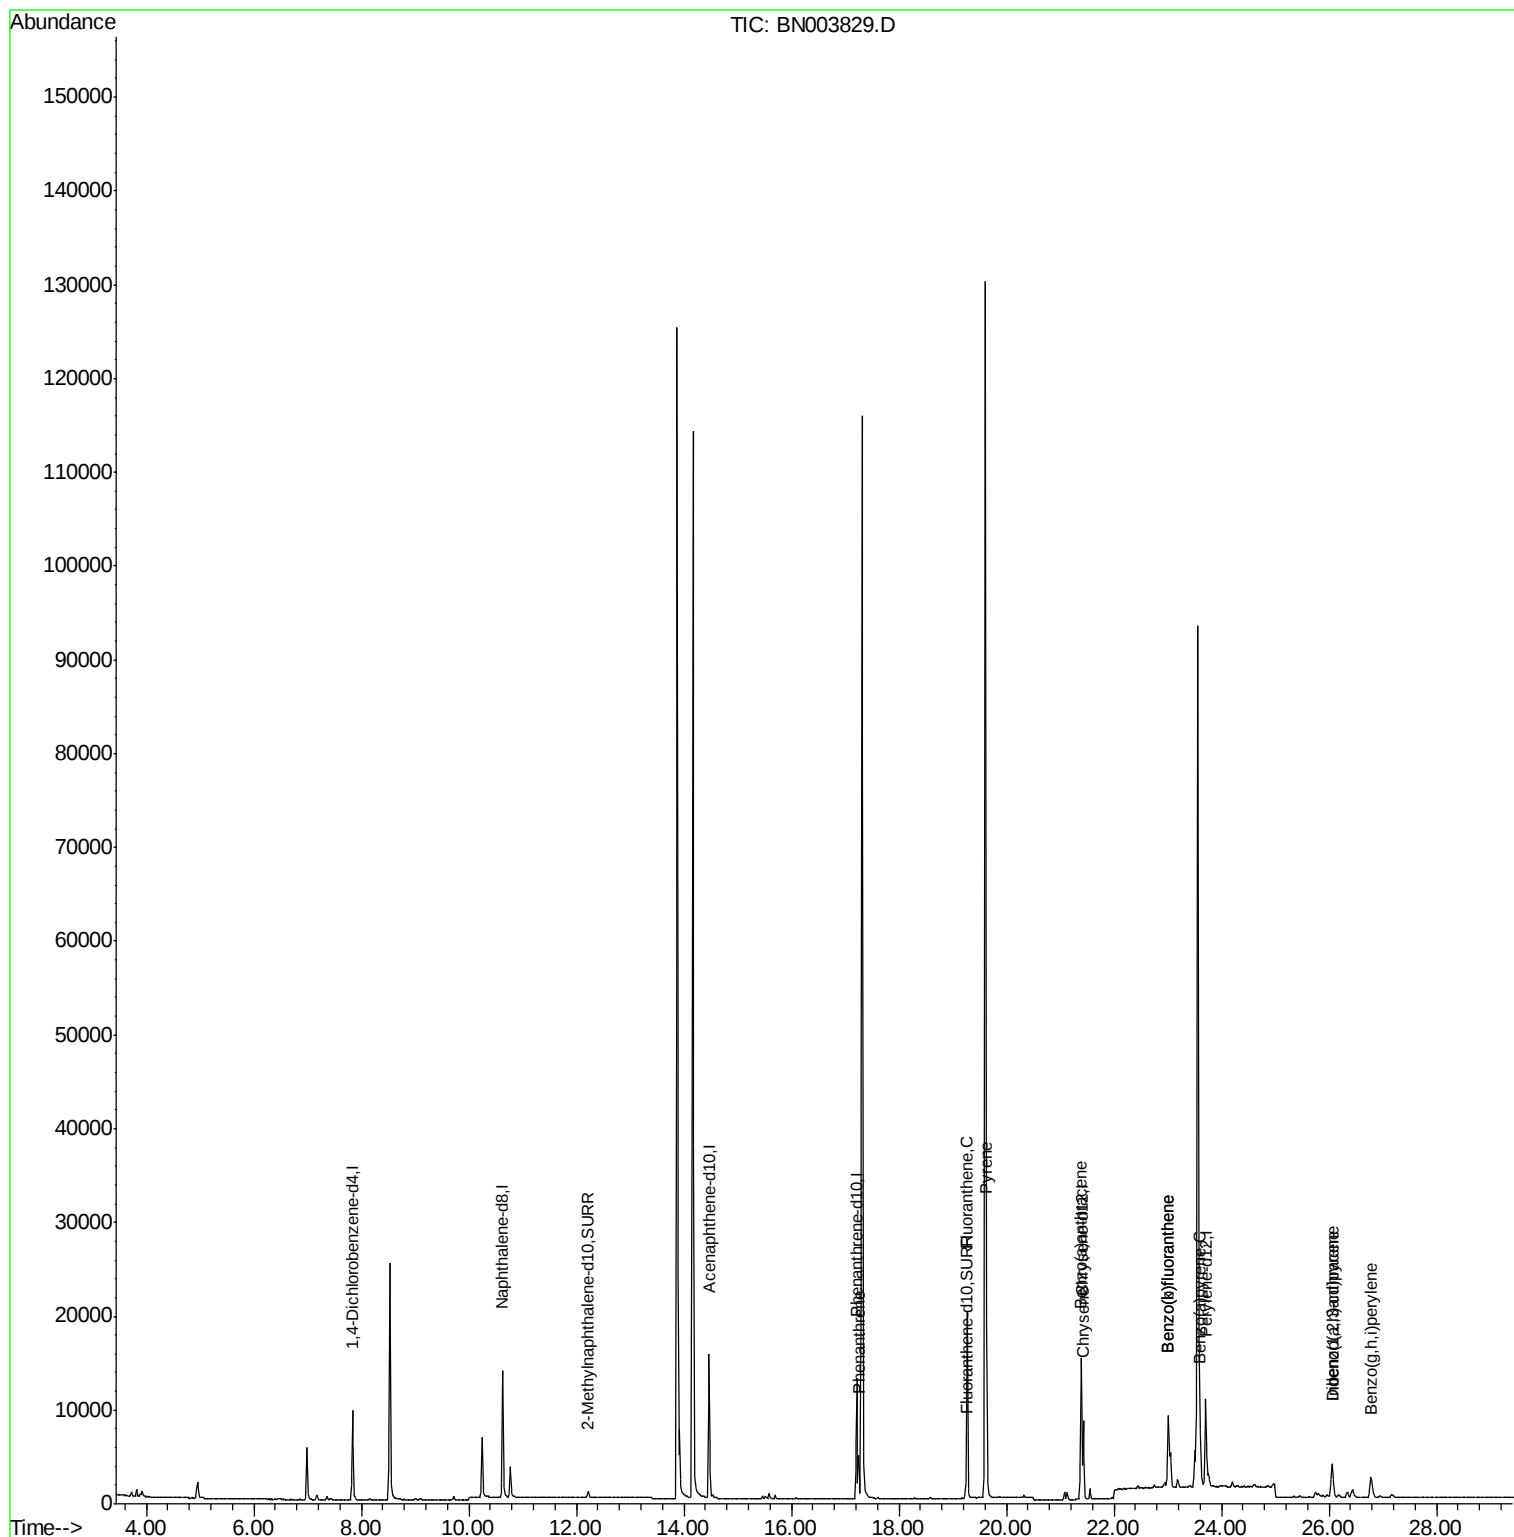

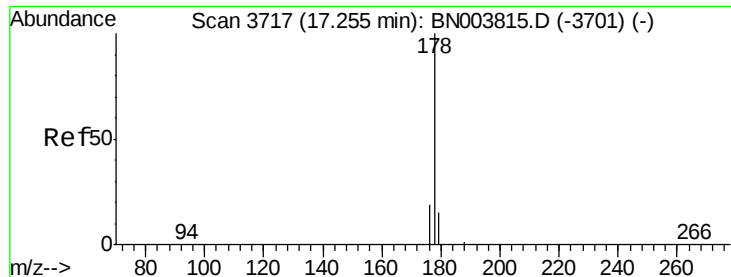

#12

Phenanthrene

Concen: 0.099 ng/ul

RT: 17.25 min Scan# 3717

Delta R.T. -0.00 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39

Instrument :

BNA_N

ClientSampleId :

F9M14DL


Tgt Ion:178 Resp: 4995

Ion Ratio Lower Upper




178 100

179 16.9 12.5 18.7

176 19.7 15.0 22.4

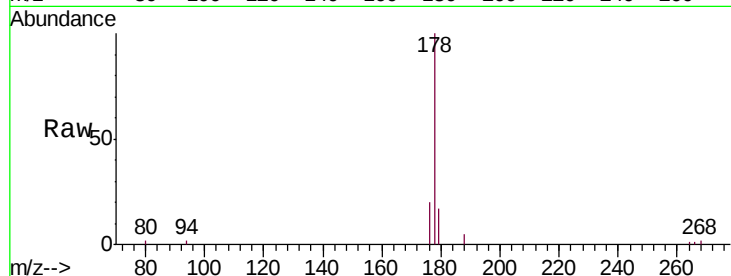

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

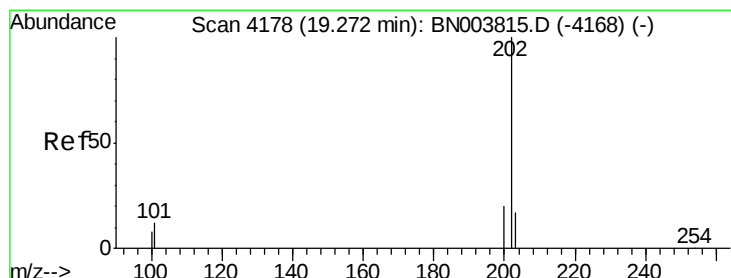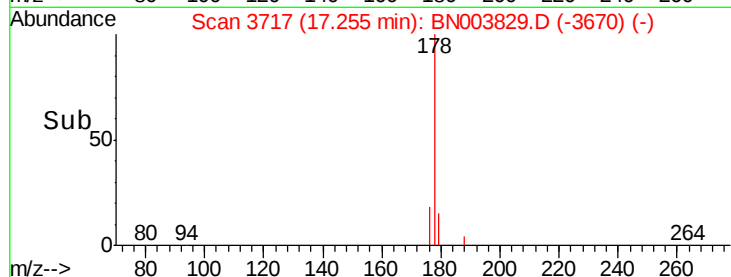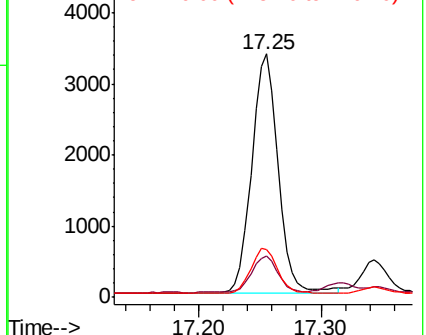

#15

Fluoranthene

Concen: 0.283 ng/ul

RT: 19.27 min Scan# 4177

Delta R.T. -0.00 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39


Tgt Ion:202 Resp: 16868

Ion Ratio Lower Upper



202 100


101 12.2 0.0 30.7

100 9.5 0.0 28.1

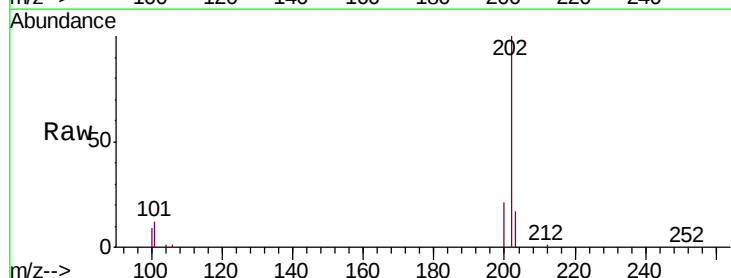

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

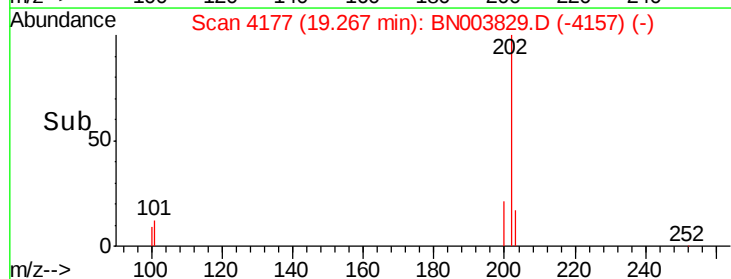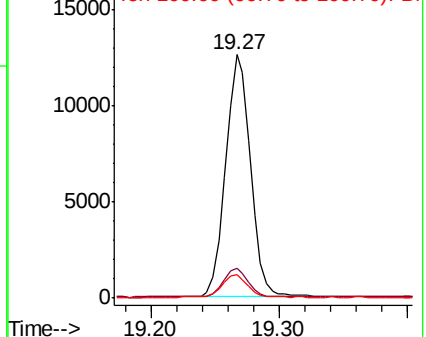

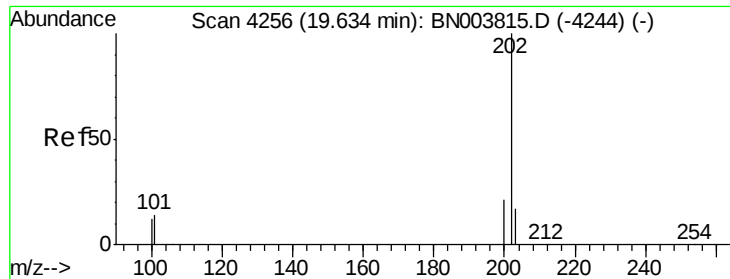

#17

Pyrene

Concen: 0.331 ng/ul

RT: 19.63 min Scan# 4255

Delta R.T. -0.00 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39

Instrument :

BNA_N

ClientSampleId :

F9M14DL


Tgt Ion:202 Resp: 13957

Ion Ratio Lower Upper

202 100

101 15.1 10.3 15.5




100 12.3 8.5 12.7

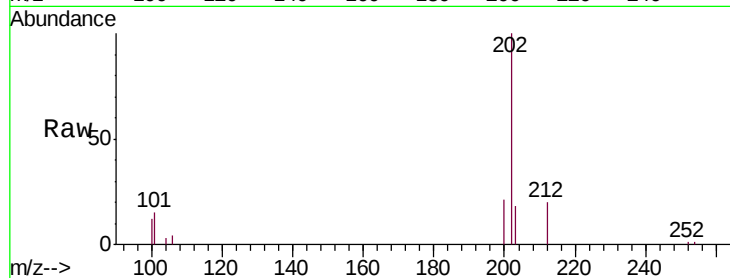

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

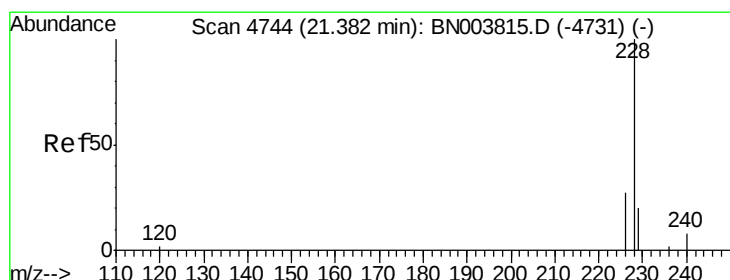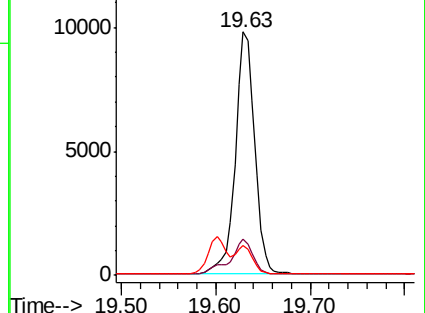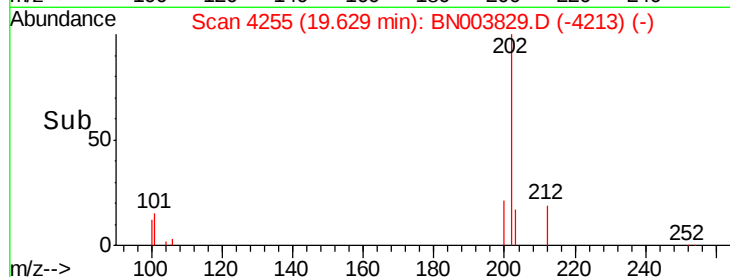

#18

Benzo(a)anthracene

Concen: 0.178 ng/ul

RT: 21.38 min Scan# 4742

Delta R.T. -0.00 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39


Tgt Ion:228 Resp: 6618

Ion Ratio Lower Upper

228 100

229 21.6 15.6 23.4



226 28.7 21.1 31.7

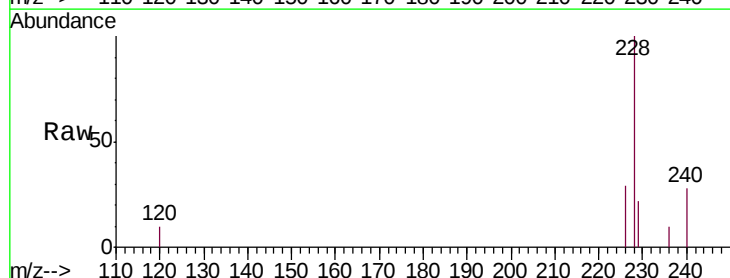


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

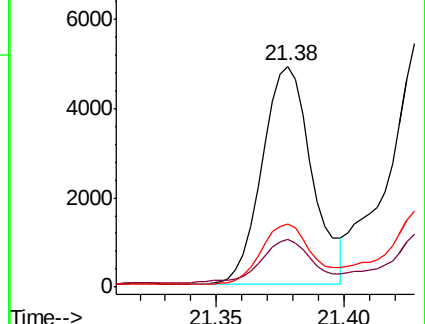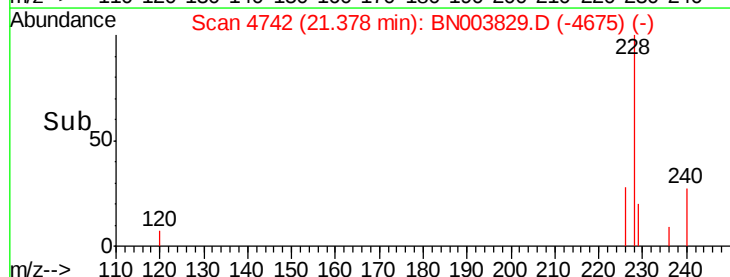

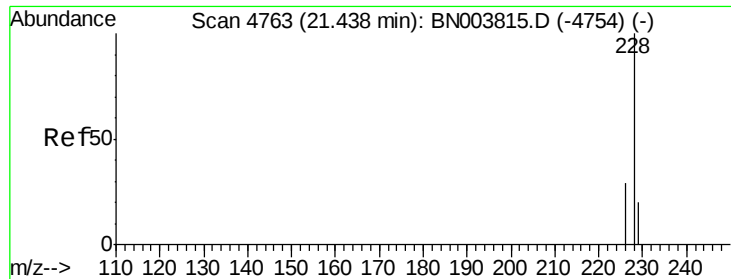

#19

Chrysene

Concen: 0.197 ng/ul

RT: 21.43 min Scan# 4760

Delta R.T. -0.01 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39

Instrument :

BNA_N

ClientSampleId :

F9M14DL


Tgt Ion:228 Resp: 8369

Ion Ratio Lower Upper

228 100

226 31.0 24.0 36.0




229 21.8 15.7 23.5

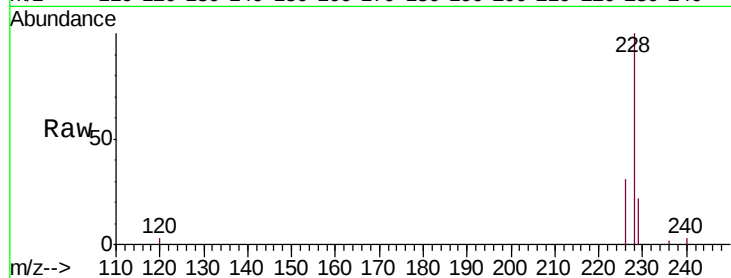

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

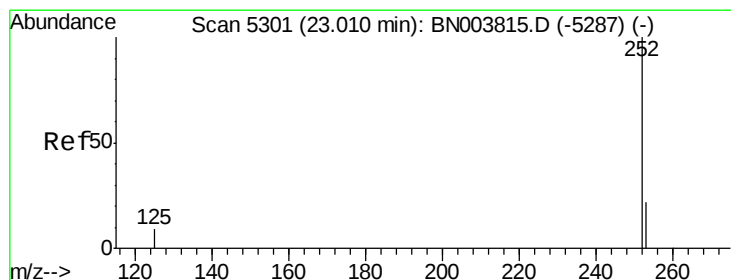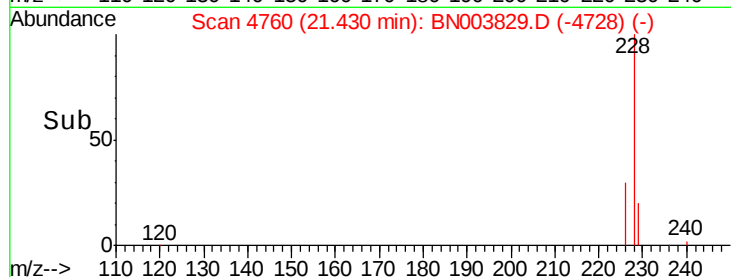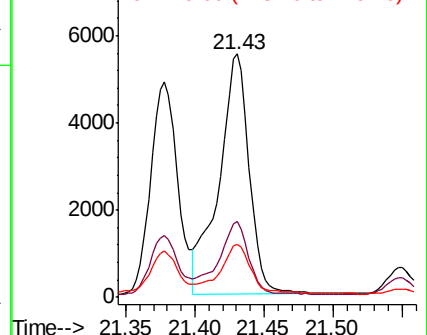

#21

Benzo(b)fluoranthene

Concen: 0.313 ng/ul

RT: 23.01 min Scan# 5299

Delta R.T. -0.00 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39


Tgt Ion:252 Resp: 16701

Ion Ratio Lower Upper

252 100

253 27.2 0.0 46.0



125 15.0 0.0 22.4

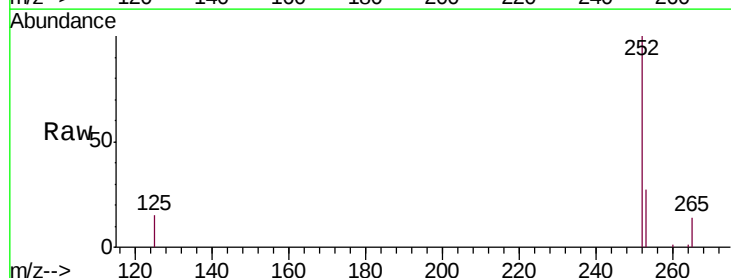


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

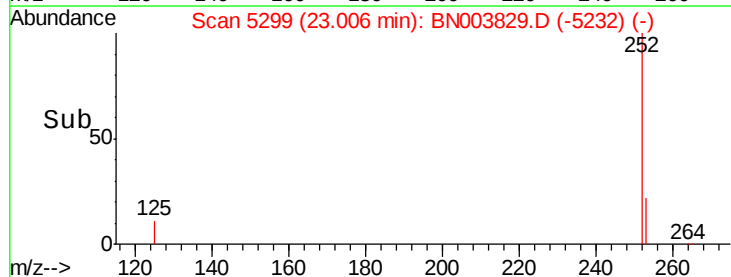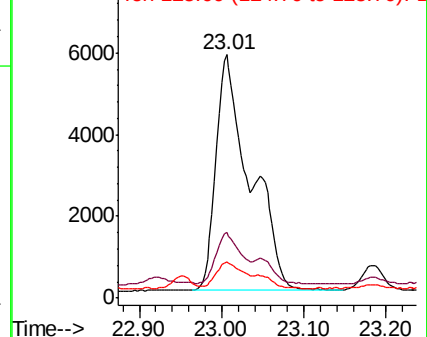

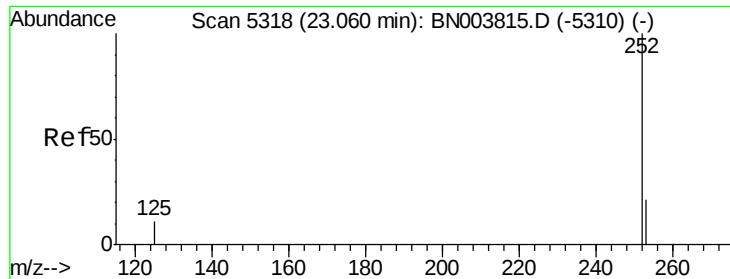

#22

Benzo(k)fluoranthene

Concen: 0.321 ng/u1

RT: 23.01 min Scan# 5299

Delta R.T. -0.05 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39

Instrument :

BNA_N

ClientSampleId :

F9M14DL


Tgt Ion:252 Resp: 16701

Ion Ratio Lower Upper

252 100

253 27.2 18.5 27.7




125 15.0 9.0 13.6#

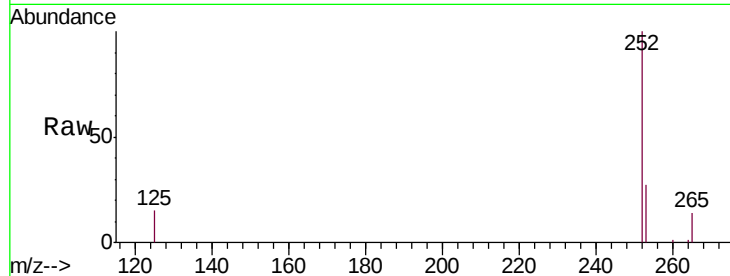

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

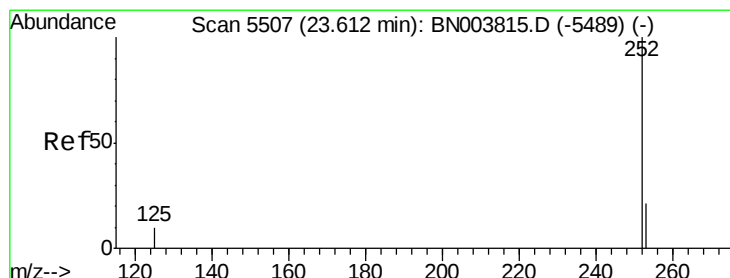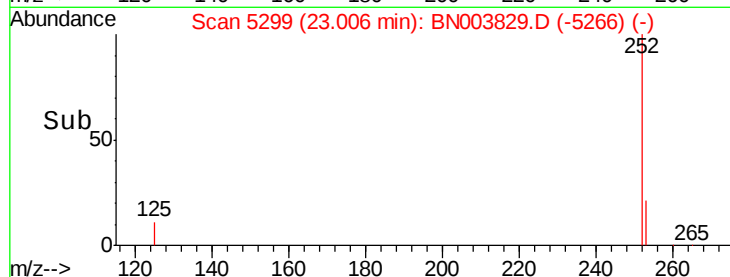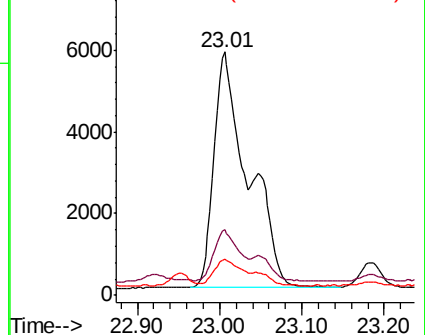

#23

Benzo(a)pyrene

Concen: 0.151 ng/u1

RT: 23.60 min Scan# 5503

Delta R.T. -0.01 min

Lab File: BN003829.D

Acq: 11 Dec 2018 23:39


Tgt Ion:252 Resp: 6985

Ion Ratio Lower Upper

252 100

253 29.8 19.0 28.4#



125 17.3 10.2 15.4#

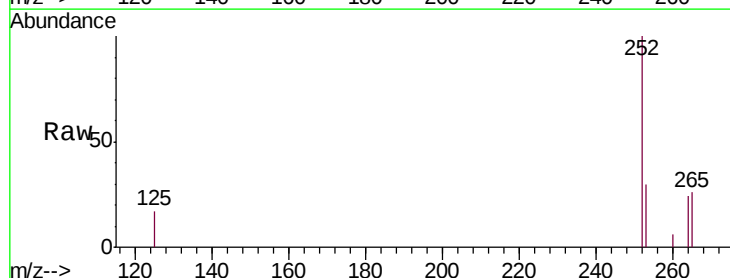


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

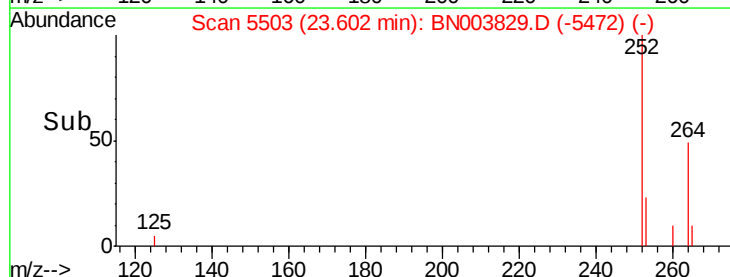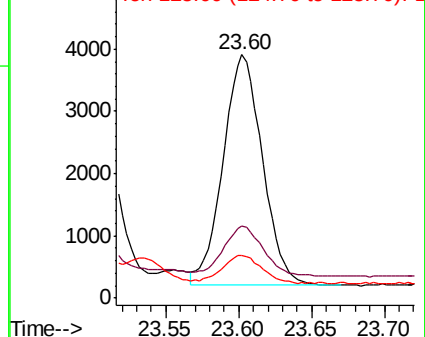

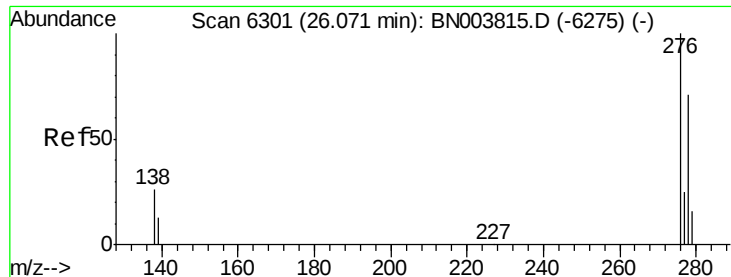


#24




Indeno(1,2,3-cd)pyrene
Concen: 0.121 ng/ul
RT: 26.06 min Scan# 6297
Delta R.T. -0.01 min
Lab File: BN003829.D
Acq: 11 Dec 2018 23:39

Instrument :
BNA_N
ClientSampleId :
F9M14DL

Tgt Ion: 276 Resp: 6441
Ion Ratio Lower Upper
276 100
138 22.0 20.3 30.5
227 0.1 0.2 0.2#

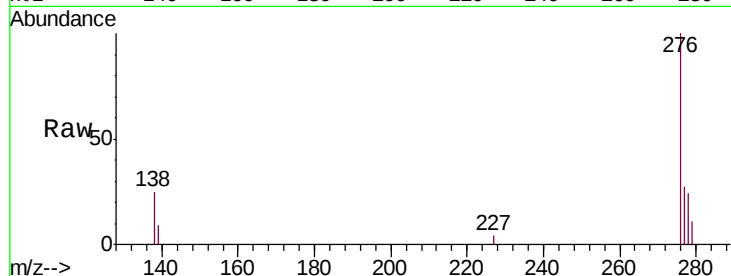


Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 227.00 (226.70 to 227.70): E

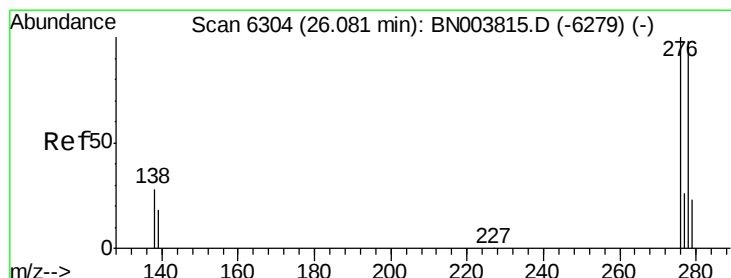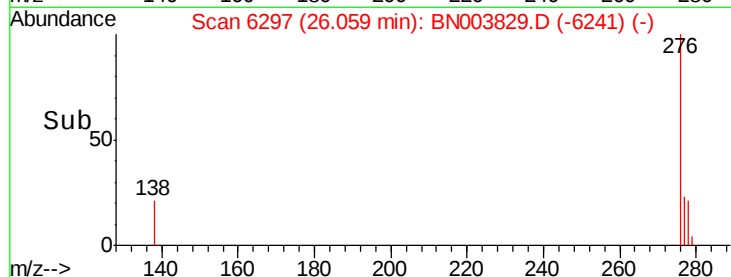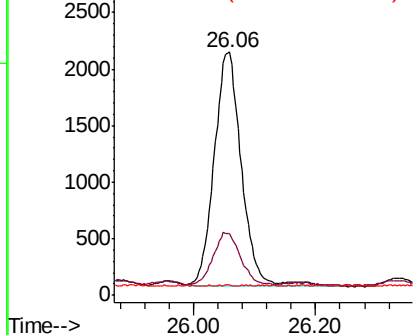



#25


Dibenzo(a,h)anthracene
Concen: 0.036 ng/ul
RT: 26.06 min Scan# 6298
Delta R.T. -0.02 min
Lab File: BN003829.D
Acq: 11 Dec 2018 23:39

Tgt Ion: 278 Resp: 1549
Ion Ratio Lower Upper
278 100
139 34.3 14.2 21.4#
279 48.9 19.8 29.6#

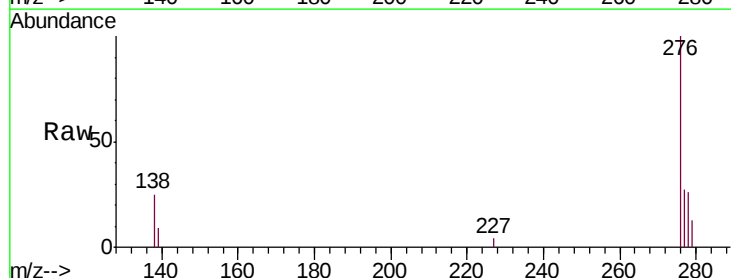

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

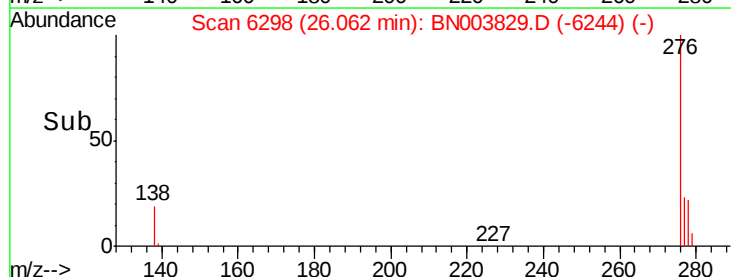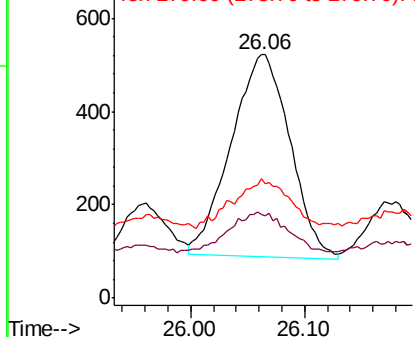

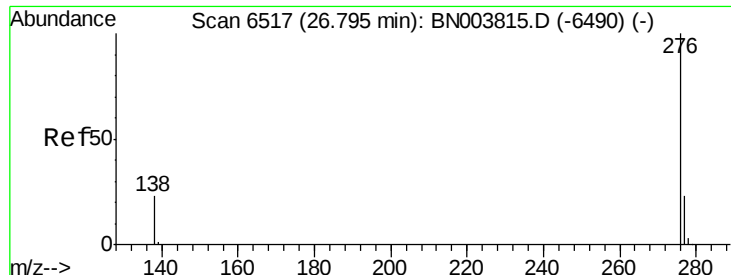

#26

Benzo(g,h,i)perylene

Concen: 0.109 ng/ul

RT: 26.78 min Scan# 6512

Delta R.T. -0.02 min

Lab File: BN003829.D


Acq: 11 Dec 2018 23:39

Instrument :

BNA_N

ClientSampleId :

F9M14DL

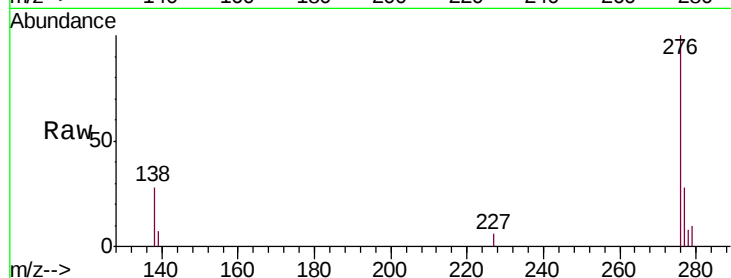


Tgt Ion: 276 Resp: 5029

Ion Ratio Lower Upper

276 100

138 28.2 17.7 26.5#

277 27.9 19.3 28.9

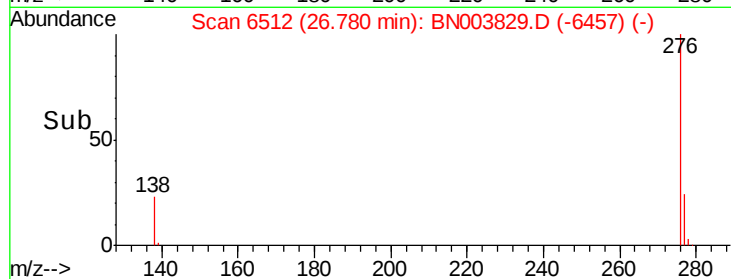

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

