

Data File : BN003831.D
Acq On : 12 Dec 2018 00:52
Operator : JU/SJ
Sample : PB115306BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Time: Dec 12 03:49:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	4661	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	18035	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9279	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1263640	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.71	264	13423	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	8078	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	2506	0.059	ng/ul#	13
23) Benzo(a)pyrene	23.56	252	3955	0.082	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003831.D
Acq On : 12 Dec 2018 00:52
Operator : JU/SJ
Sample : PB115306BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Time: Dec 12 03:49:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

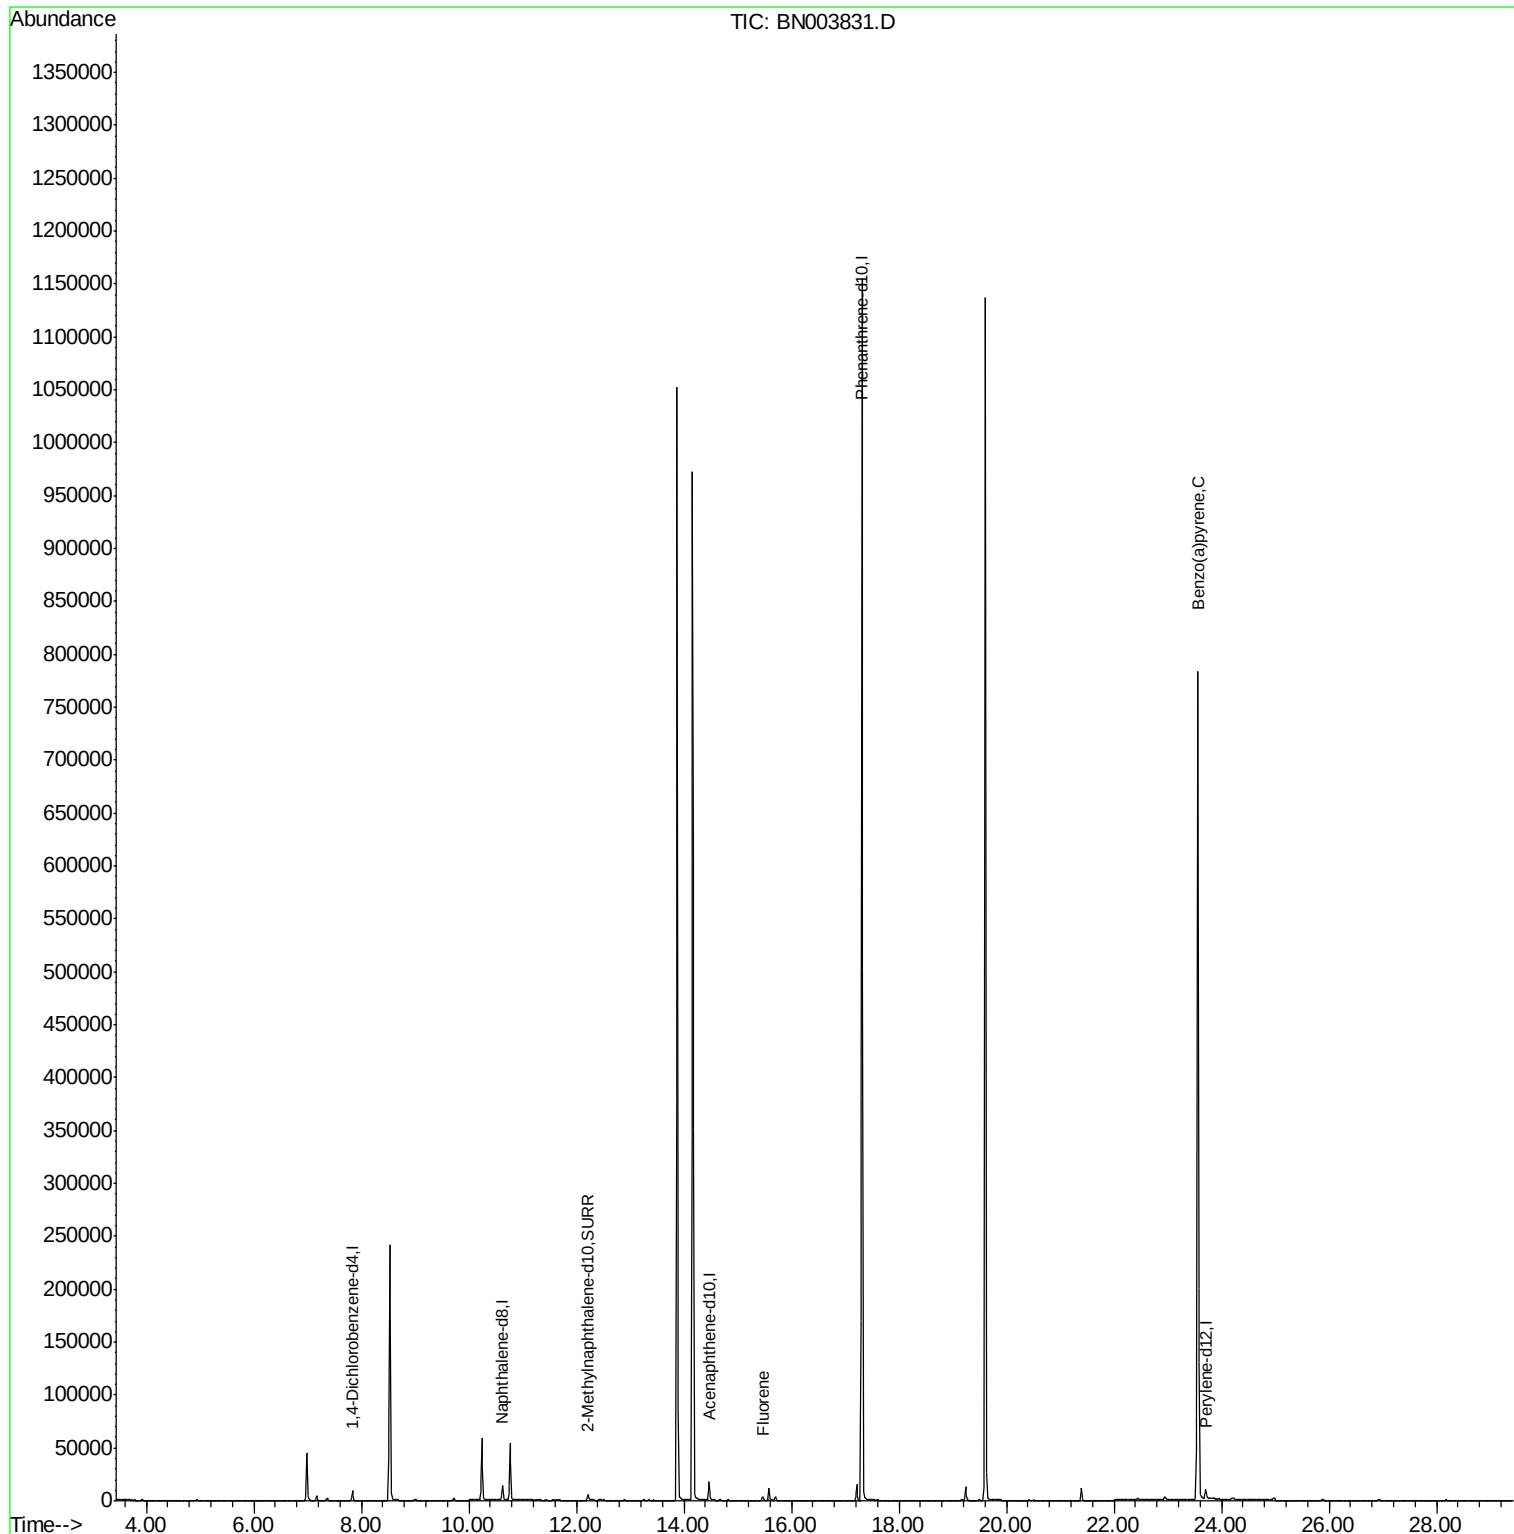

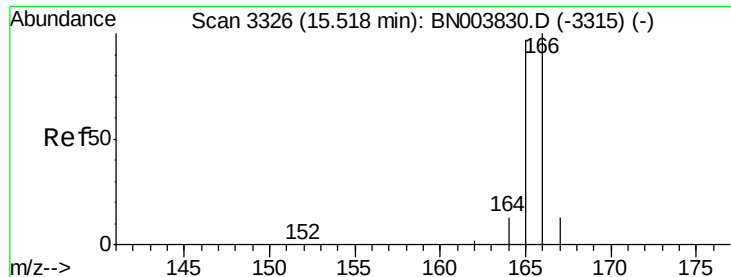

#9

Fluorene

Concen: 0.059 ng/ul

RT: 15.46 min Scan# 3314

Delta R.T. -0.06 min

Lab File: BN003831.D

Acq: 12 Dec 2018 00:52

Instrument :

BNA_N

ClientSampleId :

SBLK06


Tgt Ion:166 Resp: 2506

Ion Ratio Lower Upper

166 100

165 6.5 78.3 117.5#




167 35.3 11.3 16.9#

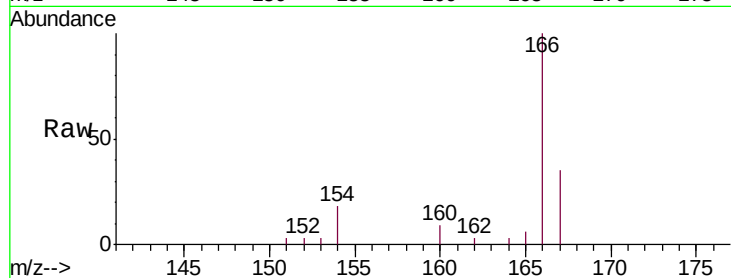

Abundance Ion 166.00 (165.70 to 166.70): E

2500 Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

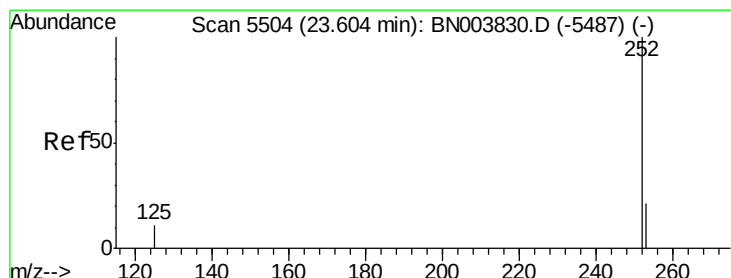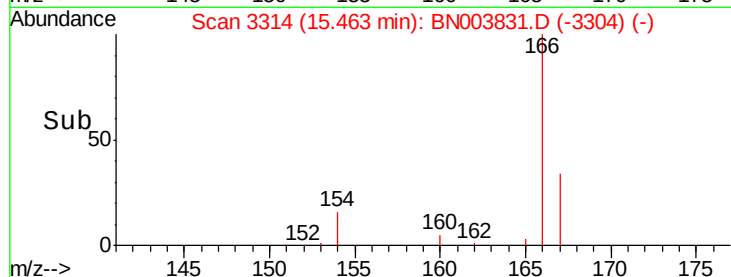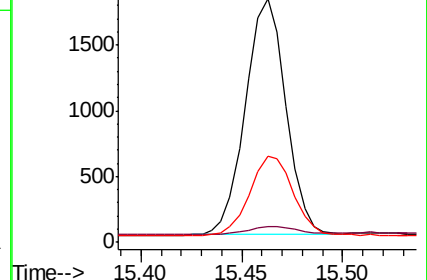

#23

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.56 min Scan# 5489

Delta R.T. -0.04 min

Lab File: BN003831.D

Acq: 12 Dec 2018 00:52


Tgt Ion:252 Resp: 3955

Ion Ratio Lower Upper

252 100

253 38.1 19.0 28.4#

125 28.8 10.2 15.4#

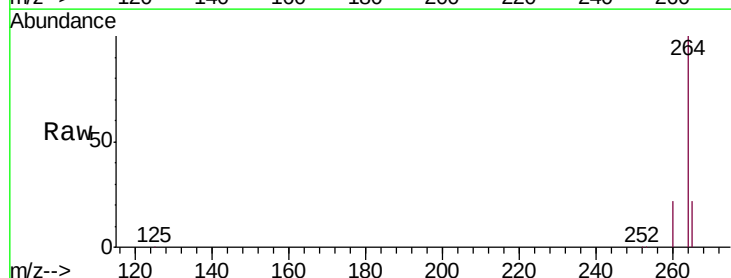

Abundance Ion 252.00 (251.70 to 252.70): E

3000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

