

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Not Reviewed)

Data File : BN003838.D
Acq On : 12 Dec 2018 04:57
Operator : JU/SJ
Sample : J6171-08DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y12DL

Quant Time: Dec 12 07:23:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4781	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	18986	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9778	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	19298	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	12575	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	12586	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	1789	0.06	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	2614	0.05	ng/ul	0.00
Target Compounds						
18) Benzo(a)anthracene	21.41	228	882	0.022	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003838.D
Acq On : 12 Dec 2018 04:57
Operator : JU/SJ
Sample : J6171-08DL 5X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y12DL

Quant Time: Dec 12 07:23:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

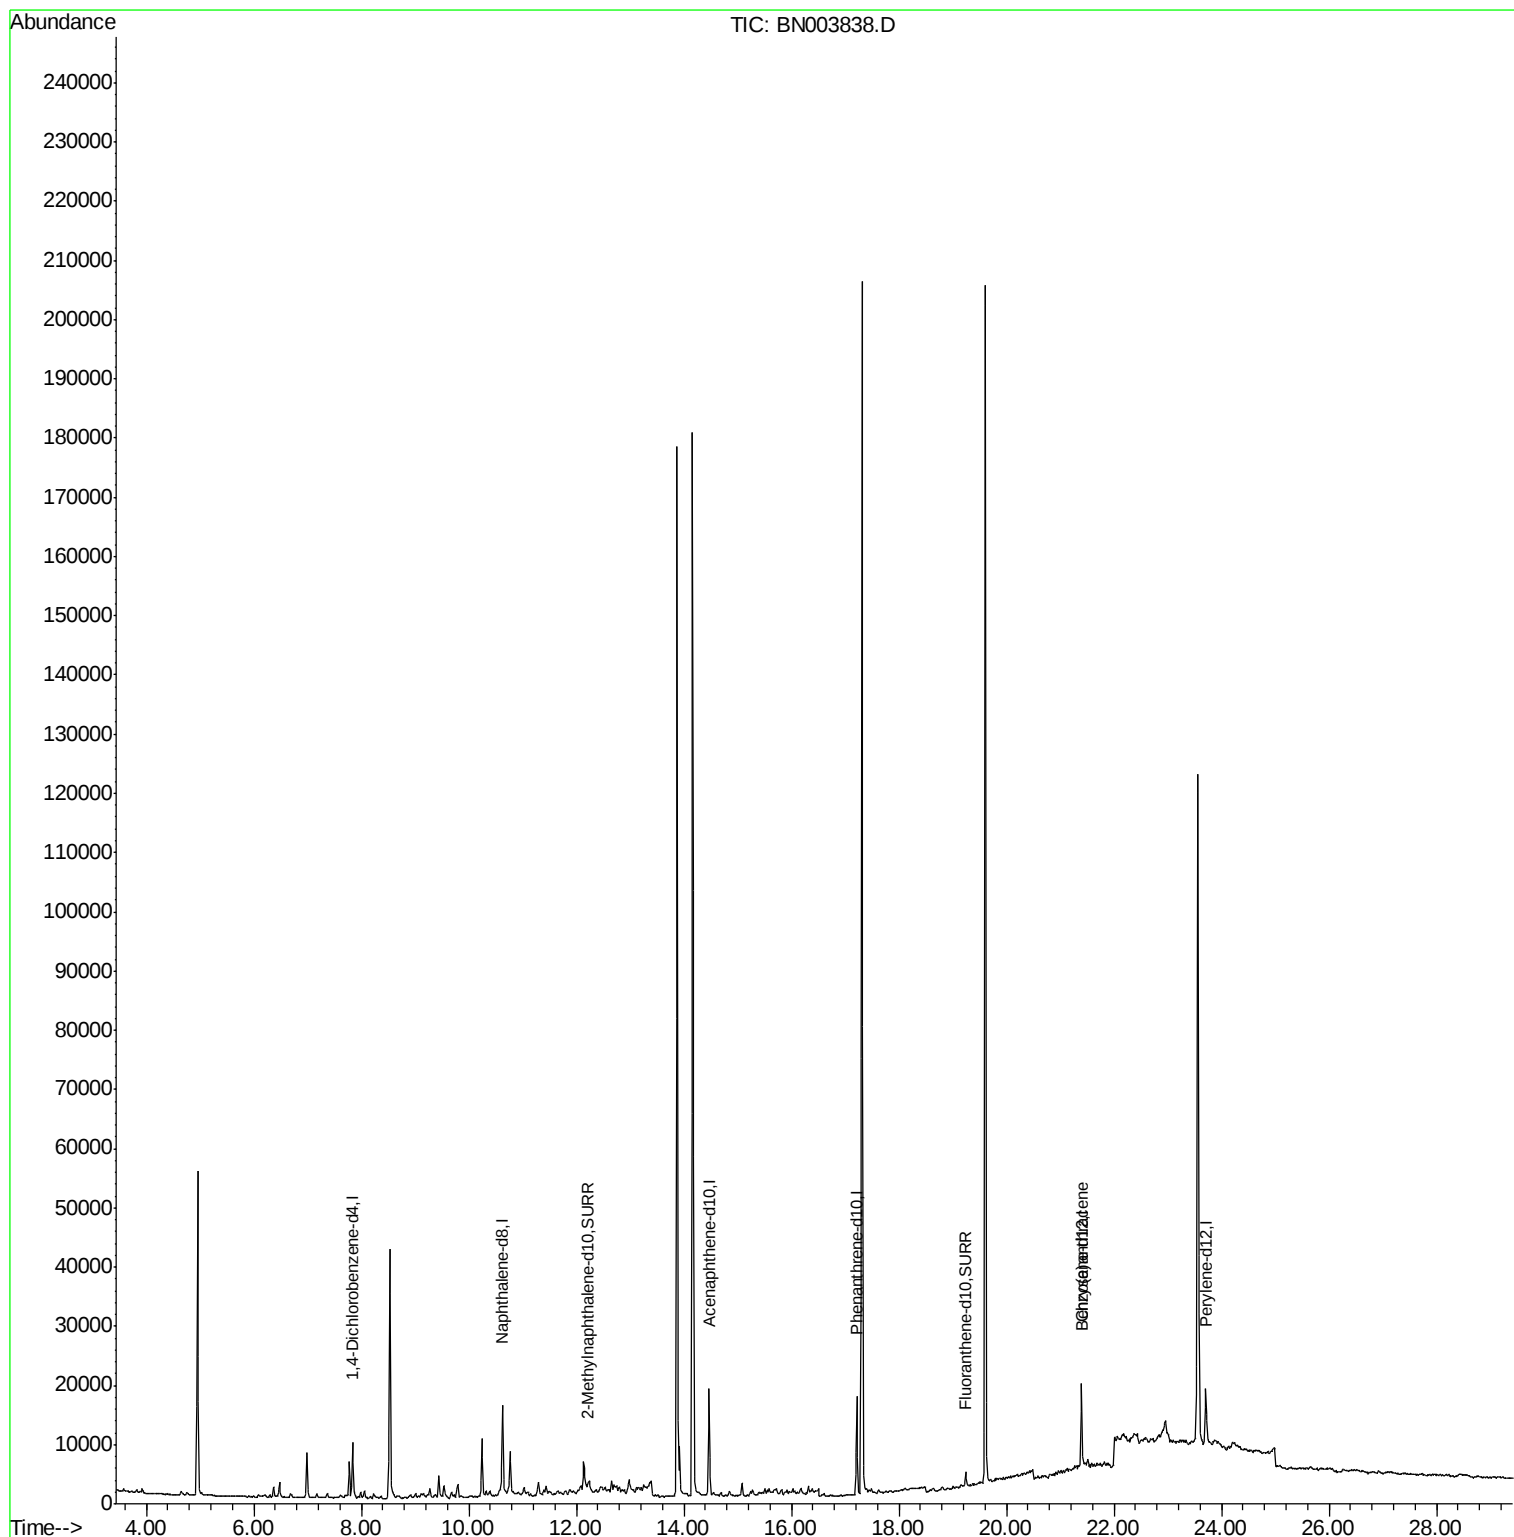

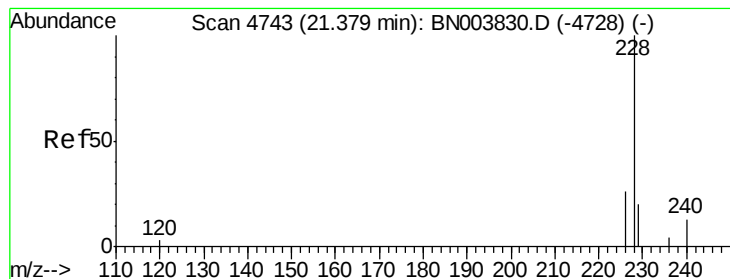

#18

Benzo(a)anthracene

Concen: 0.022 ng/ul

RT: 21.41 min Scan# 4753

Delta R.T. 0.03 min

Lab File: BN003838.D


Acq: 12 Dec 2018 04:57

Instrument :

BNA_N

ClientSampleId :

F9Y12DL

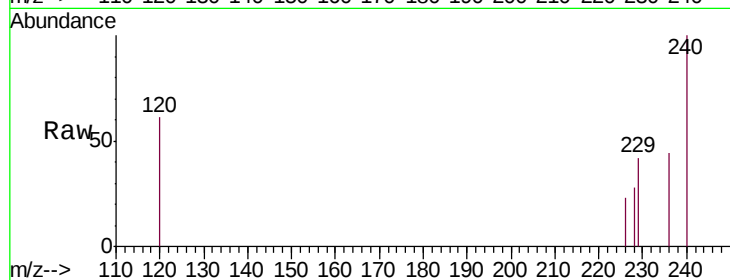


Tgt Ion: 228 Resp: 882

Ion Ratio Lower Upper

228 100

229 150.1 15.6 23.4#

226 83.9 21.1 31.7#

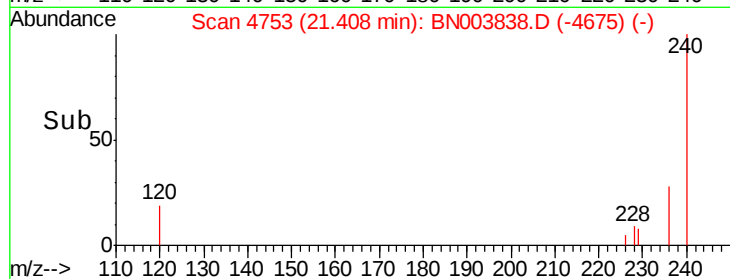

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

