

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003810.D
 Acq On : 11 Dec 2018 12:29
 Operator : JU/SJ
 Sample : J6137-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sampled :
 F9J12

Quant Time: Dec 11 15:16:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:49:51 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4921	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19205	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9526	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	17764m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	13272m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	15408	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	6571	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	10111m	0.19	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003810.D
 Acq On : 11 Dec 2018 12:29
 Operator : JU/SJ
 Sample : J6137-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9J12

Quant Time: Dec 11 15:15:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:49:51 PM

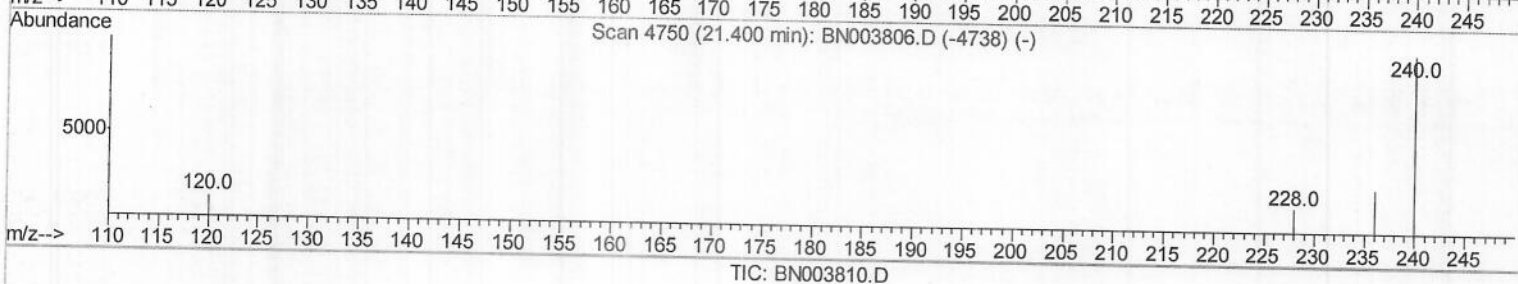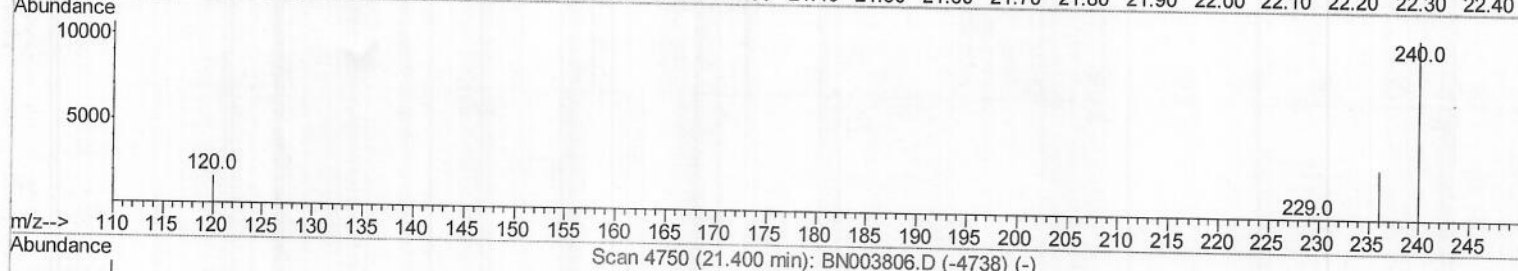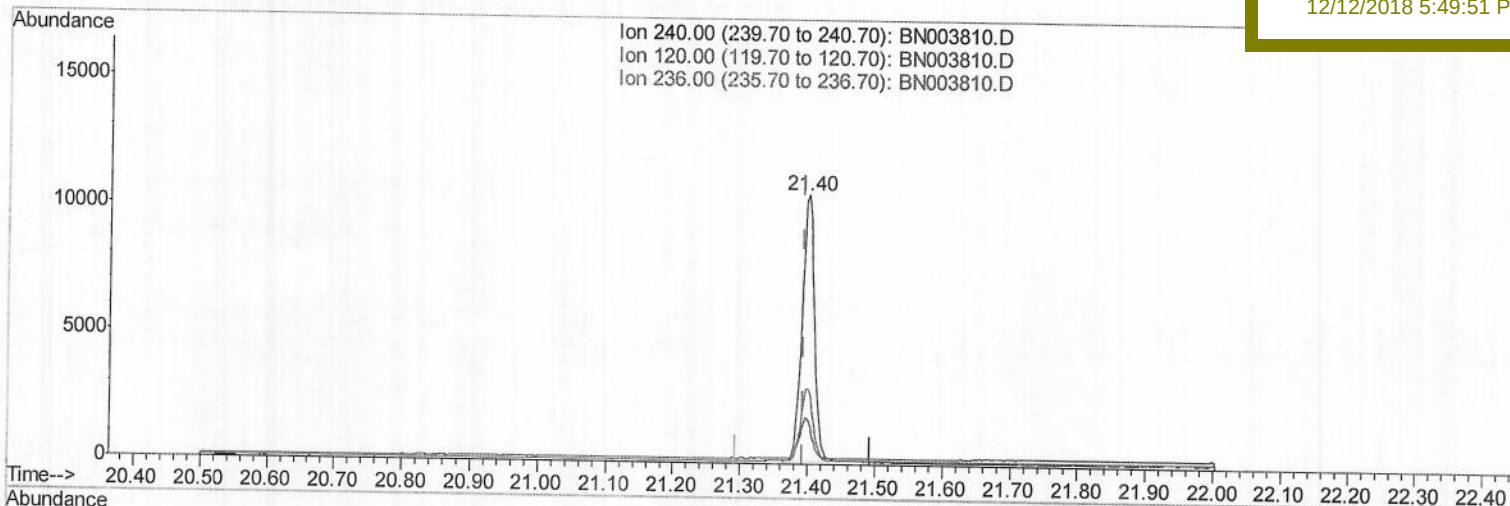

(16) Chrysene-d12 (I)

21.400min (+0.006) 0.40ng/ul m

response 13272

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.30
236.00	27.60	28.41
0.00	0.00	0.00

SJ 12/12/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
Data File : BN003810.D
Acq On : 11 Dec 2018 12:29
Operator : JU/SJ
Sample : J6137-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9J12

Quant Time: Dec 11 15:15:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/12/2018 5:49:51 PM

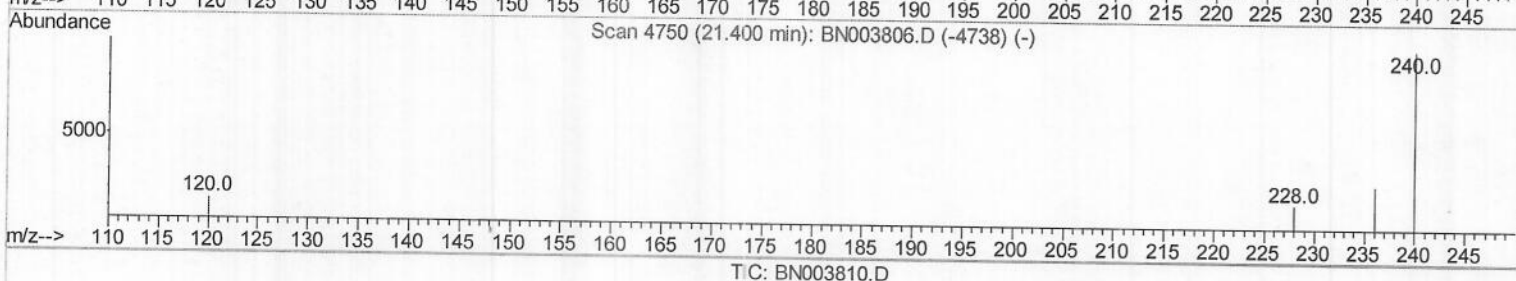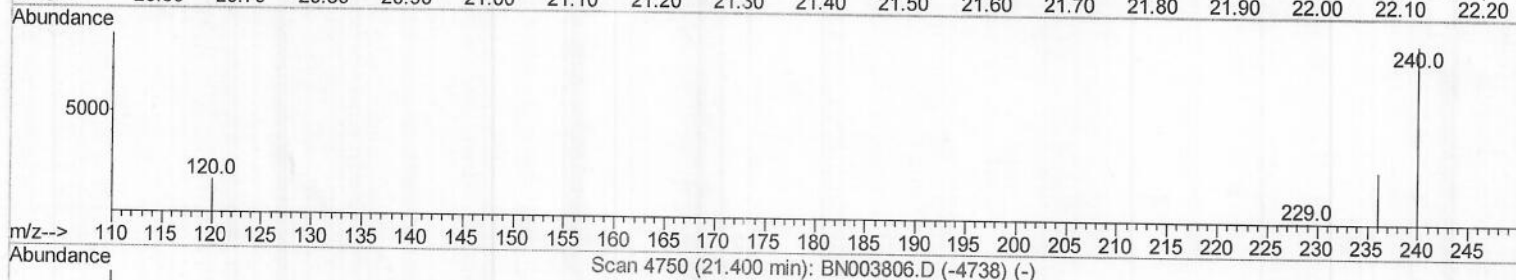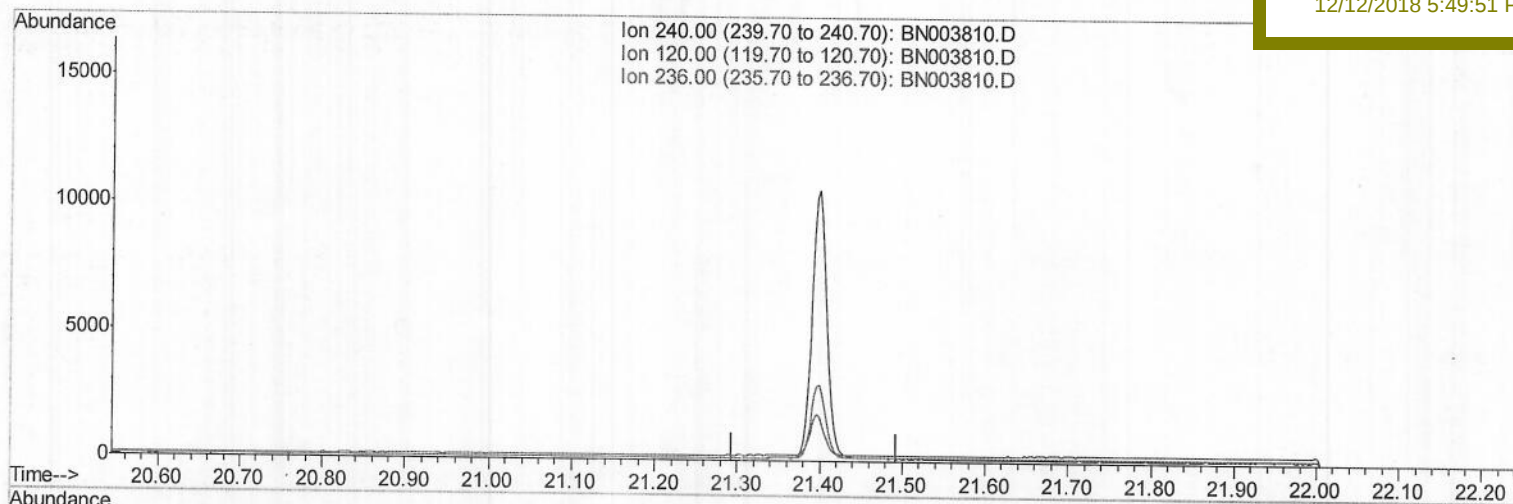

(16) Chrysene-d12 (I)

21.394min (-21.394) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\EN121118\

Data File : BN003810.D

Acq On : 11 Dec 2018 12:29

Operator : JU/SJ

Sample : J6137-10

Misc :

ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 11 15:15:18 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 11 04:22:54 2018

Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

F9J12

Manual Integrations
APPROVED

Sohil

12/12/2018 5:49:51 PM

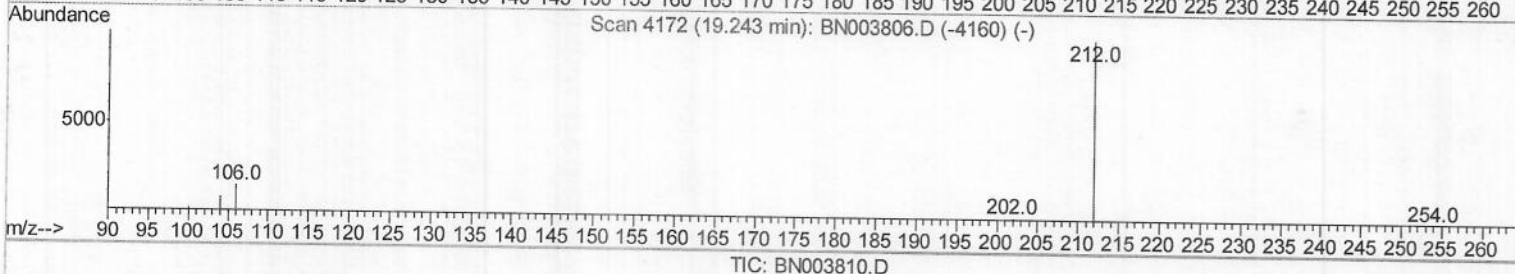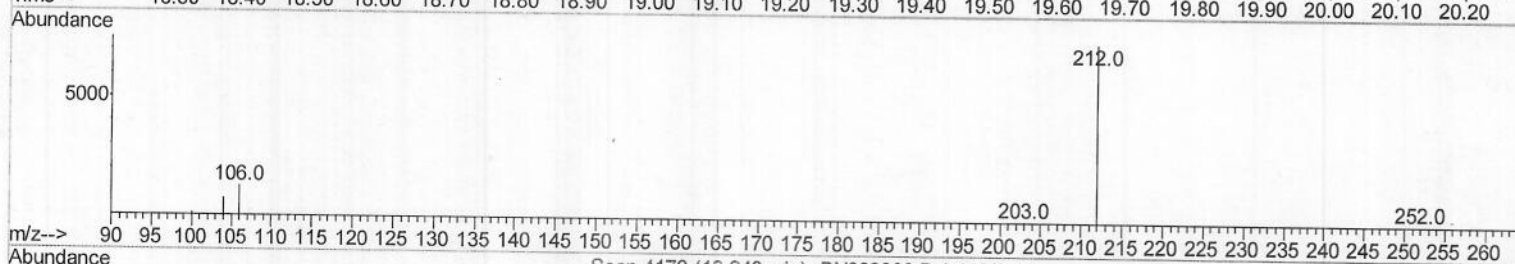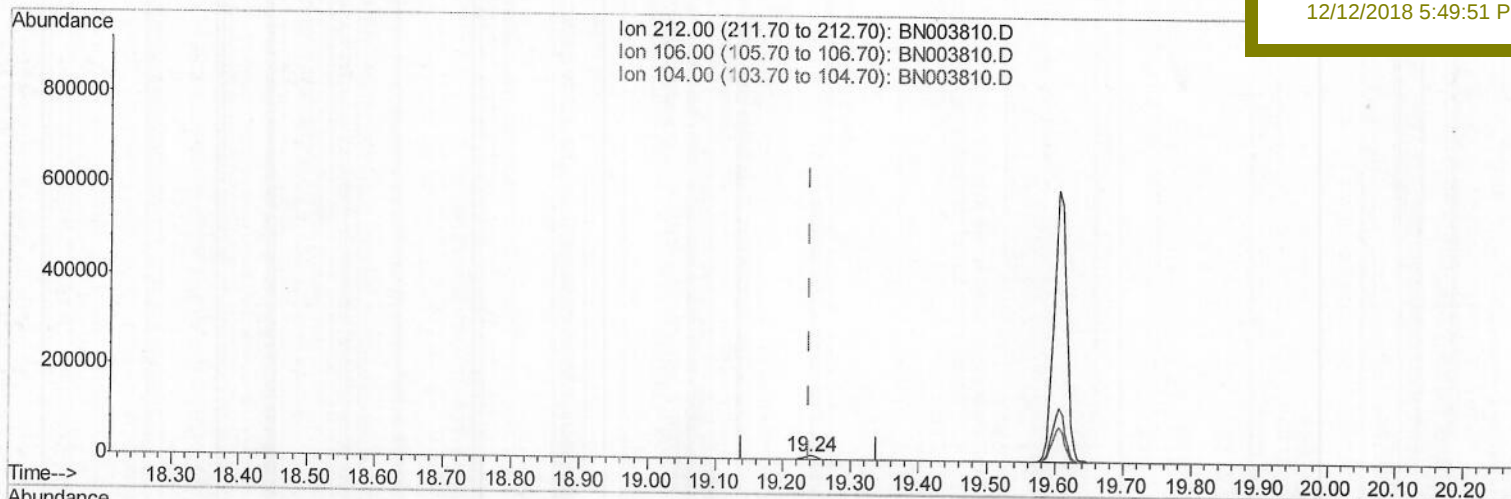

TIC: BN003810.D

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.19ng/ul m

response 10111

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

SJ 12/12/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003810.D
 Acq On : 11 Dec 2018 12:29
 Operator : JU/SJ
 Sample : J6137-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 11 15:15:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 F9J12

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:49:51 PM

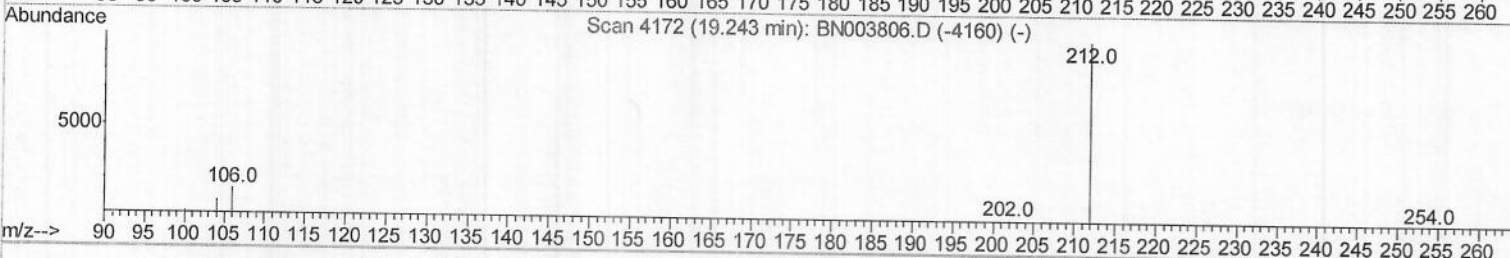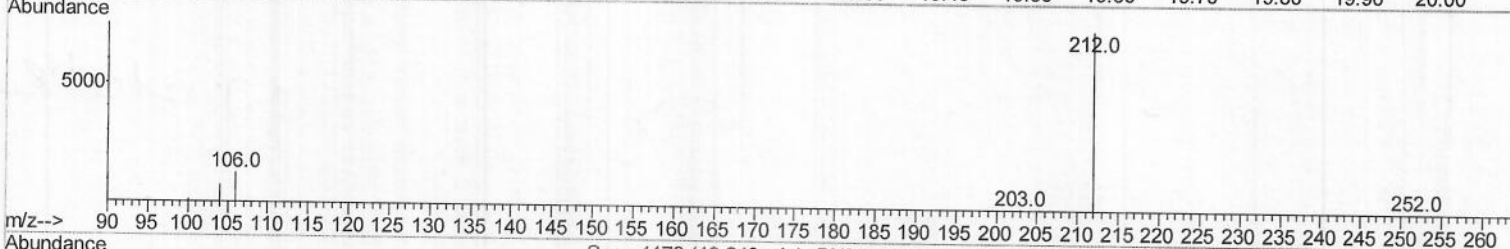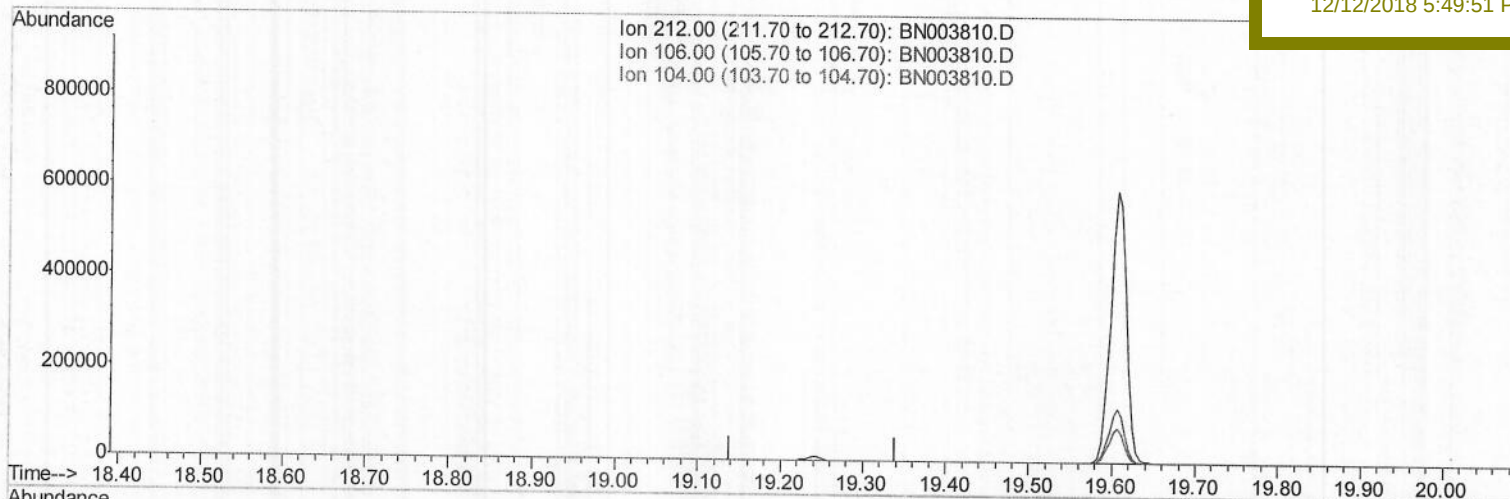

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
Data File : BN003810.D
Acq On : 11 Dec 2018 12:29
Operator : JU/SJ
Sample : J6137-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Dec 11 14:56:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

F9J12

Manual Integrations
APPROVED

Sohil

12/12/2018 5:49:51 PM

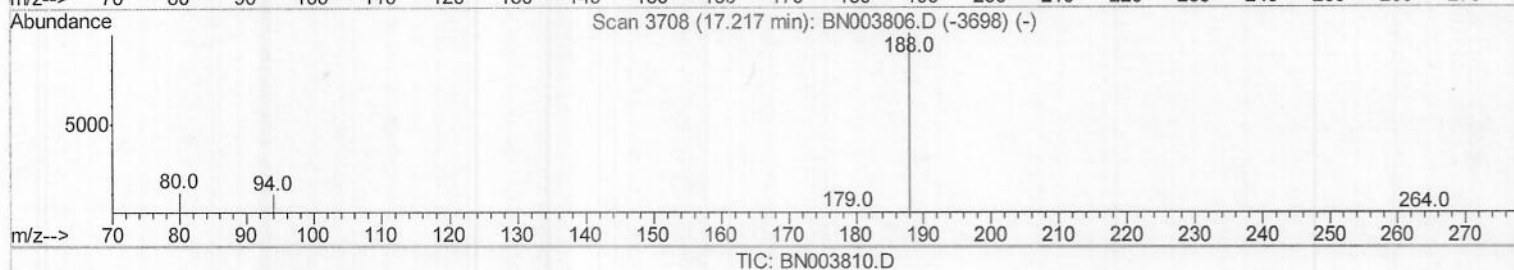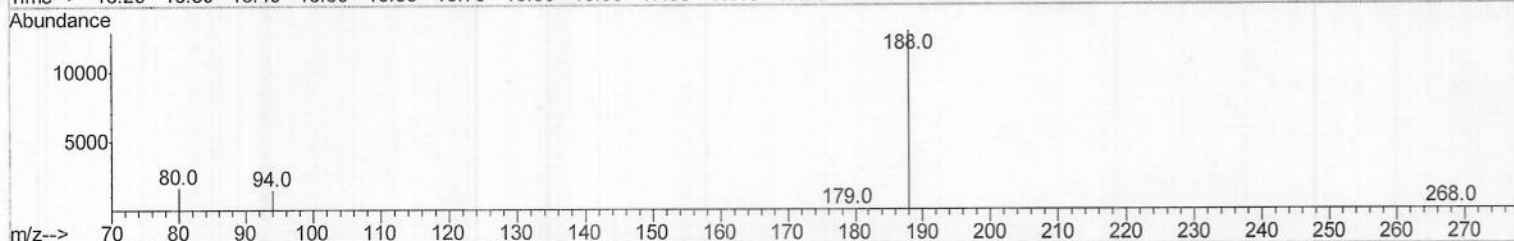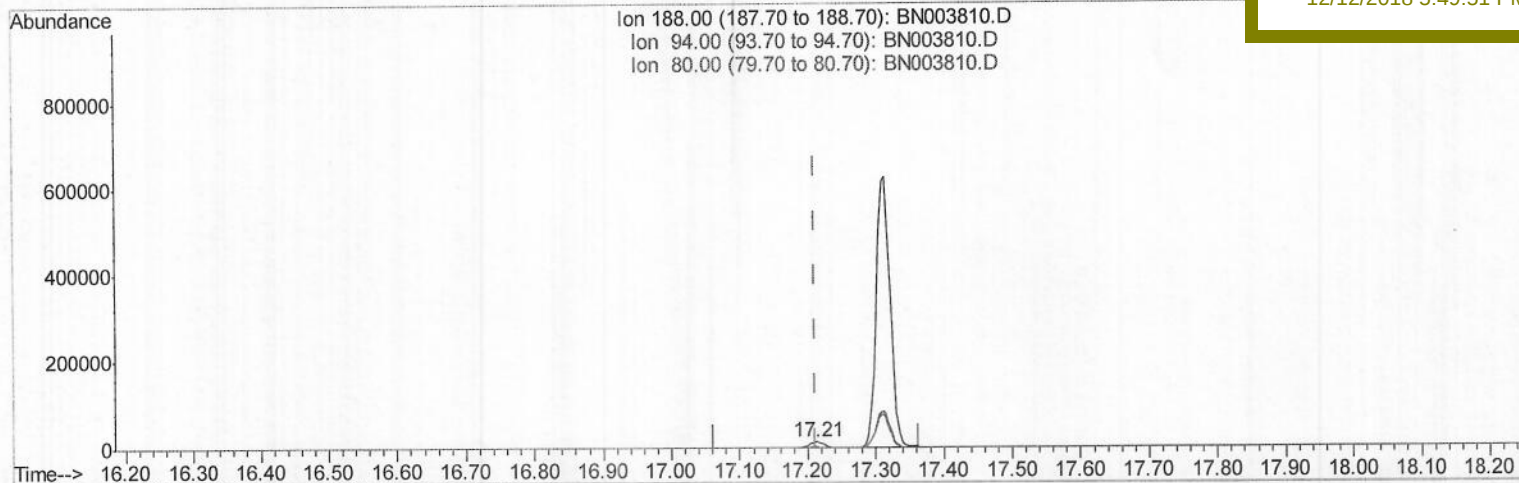

(10) Phenanthrene-d10 (I)

17.213min (0.000) 0.40ng/ul m

response 17764

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.28
80.00	11.60	12.42
0.00	0.00	0.00

SJ 12/12/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003810.D
 Acq On : 11 Dec 2018 12:29
 Operator : JU/SJ
 Sample : J6137-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9J12

Quant Time: Dec 11 14:56:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:49:51 PM

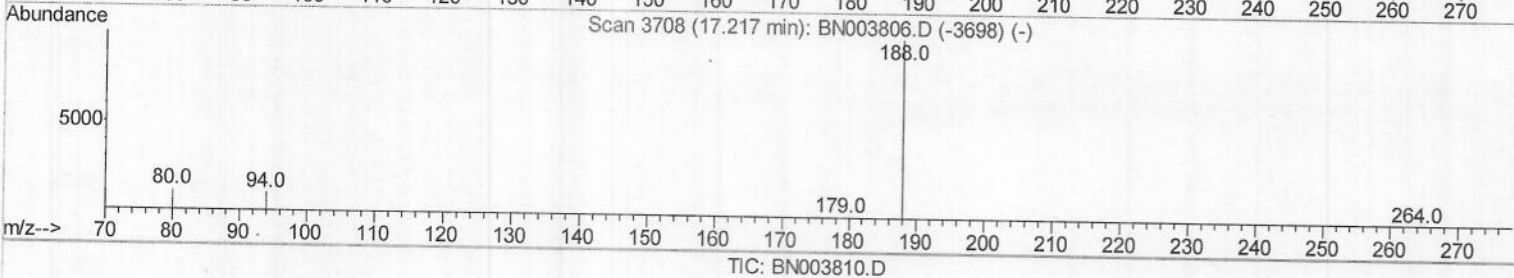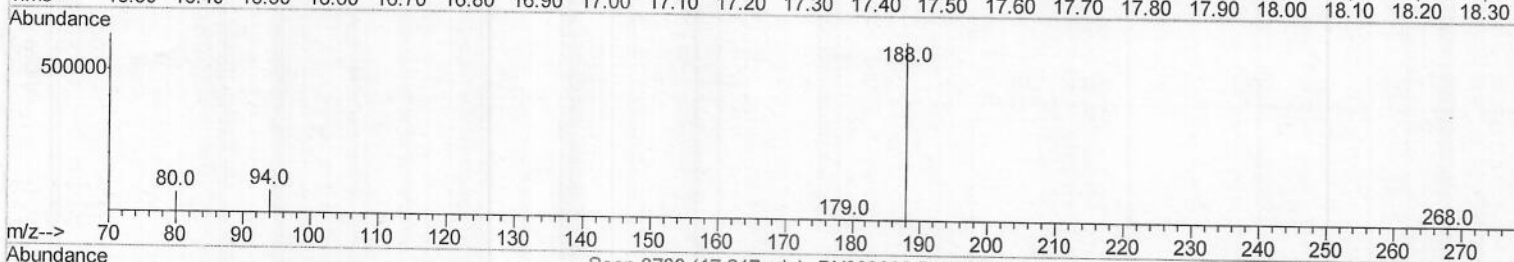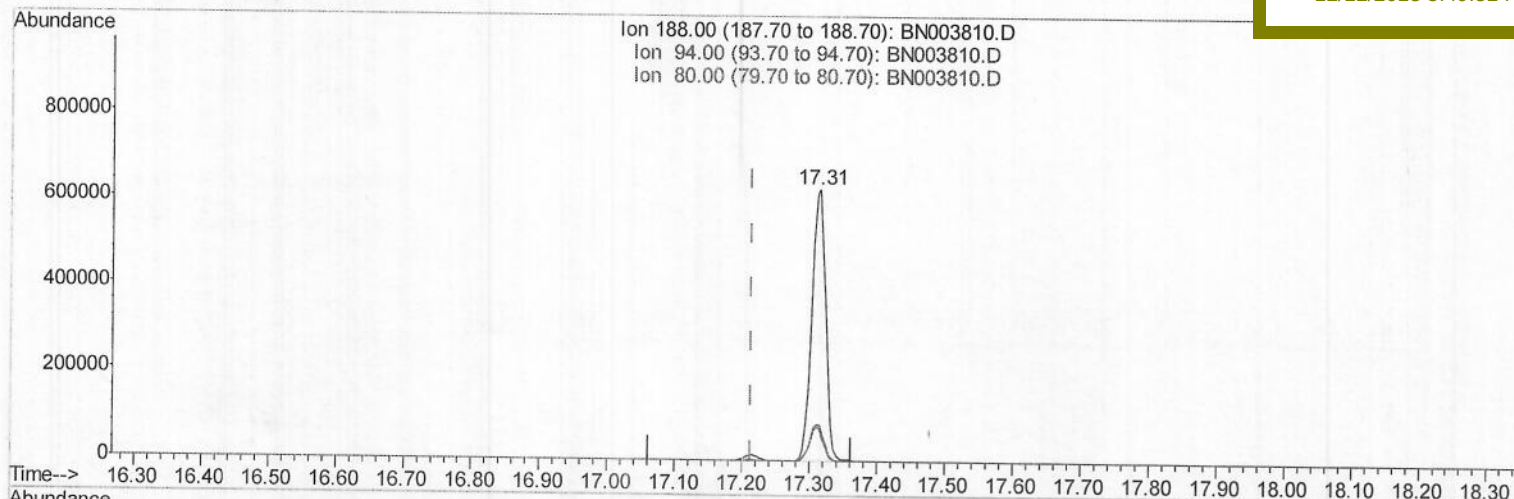

(10) Phenanthrene-d10 (I)
 17.314min (+0.101) 0.40ng/ul
 response 880534

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.57#
80.00	11.60	11.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121118\
 Data File : BN003810.D
 Acq On : 11 Dec 2018 12:29
 Operator : JU/SJ
 Sample : J6137-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9J12

Quant Time: Dec 11 15:16:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 04:22:54 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:49:51 PM

