


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
 Quantitation Report (QT Reviewed)
 Data File : BN003825.D
 Acq On : 11 Dec 2018 21:19
 Operator : JU/SJ
 Sample : J6170-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9M14

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:36:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 02:52:45 2018
 Response via : Initial Calibration

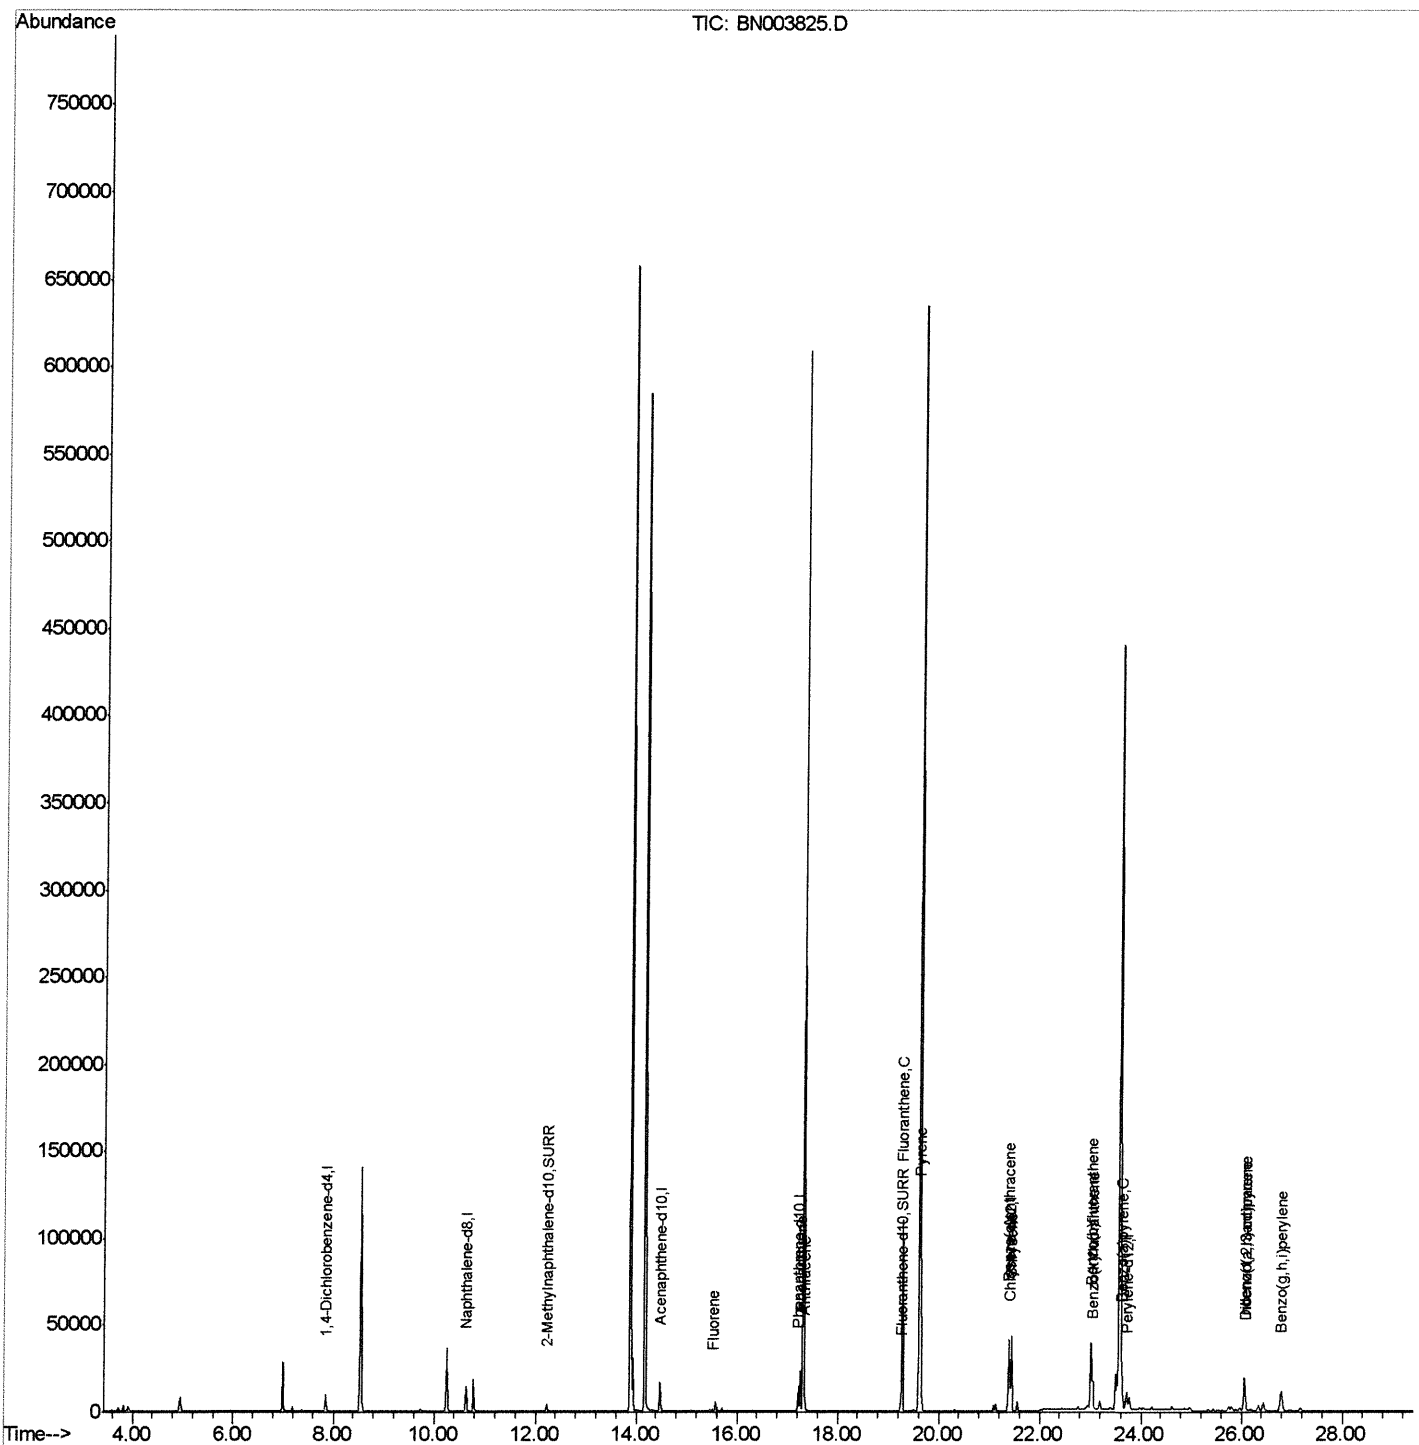

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 02:56:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

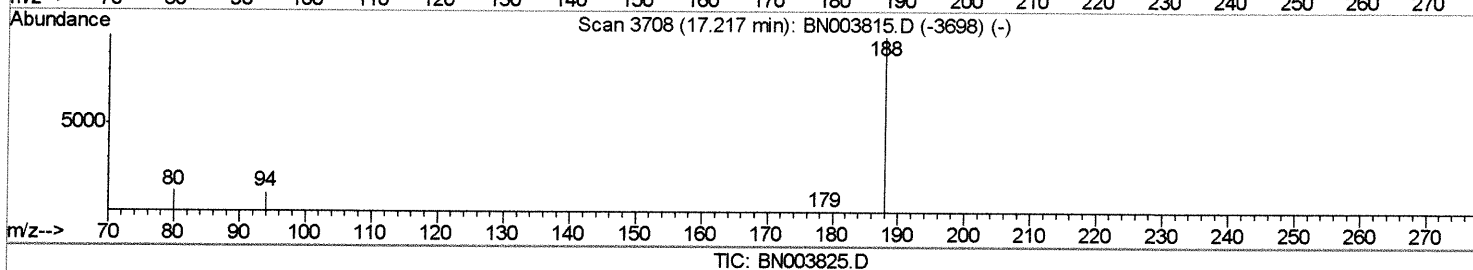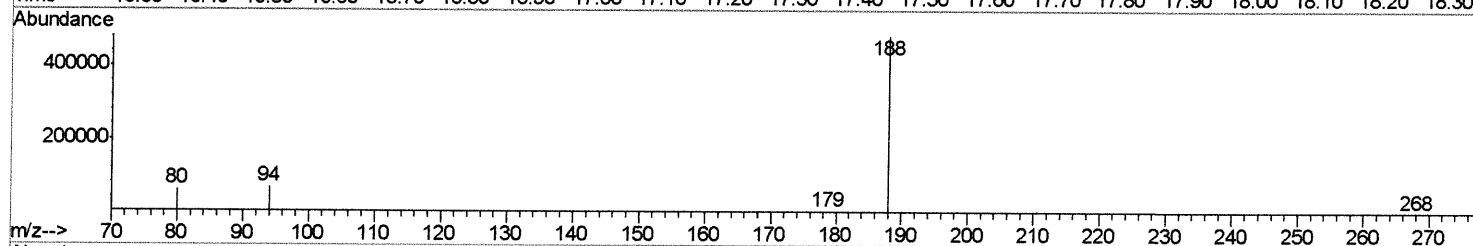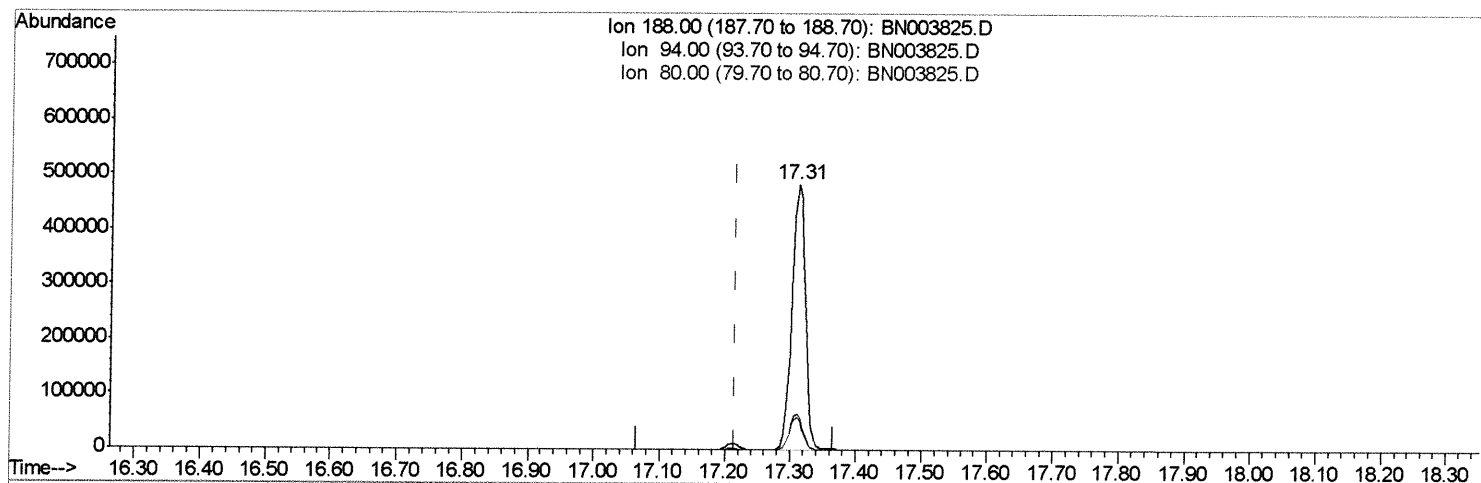

(10) Phenanthrene-d10 (I)

17.310min (+0.093) 0.40ng/ul

response 682633

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.66#
80.00	11.60	12.22
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 02:56:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

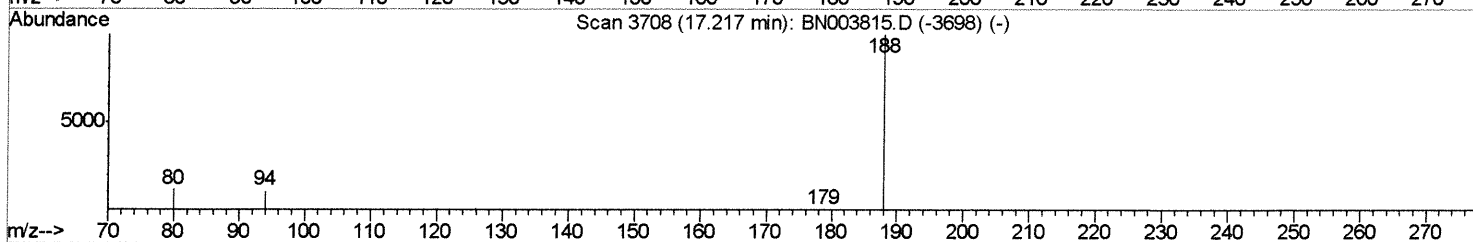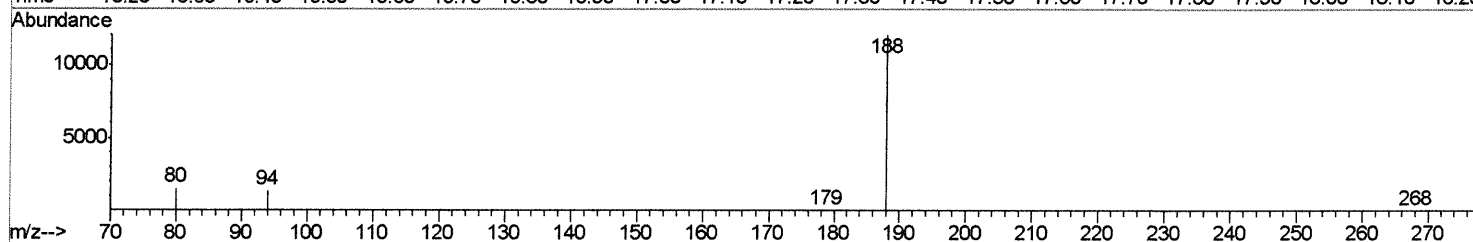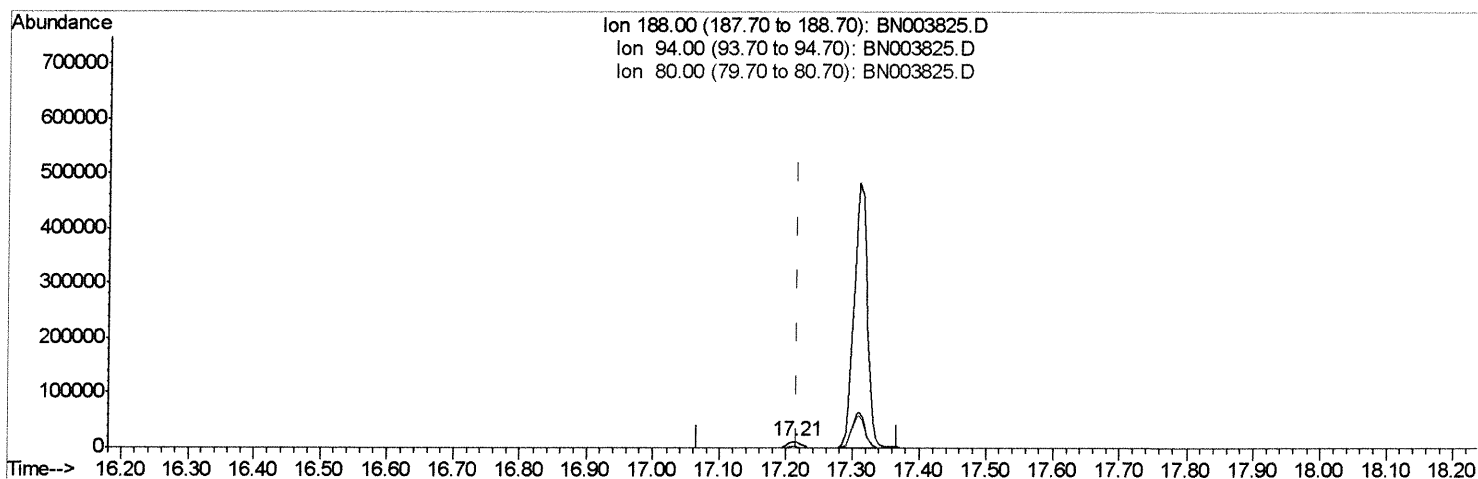

TIC: BN003825.D

(10) Phenanthrene-d10 (I)

17.213min (-0.004) 0.40ng/ul m> SJ 12/13/18

response 16682

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.52
80.00	11.60	12.73
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

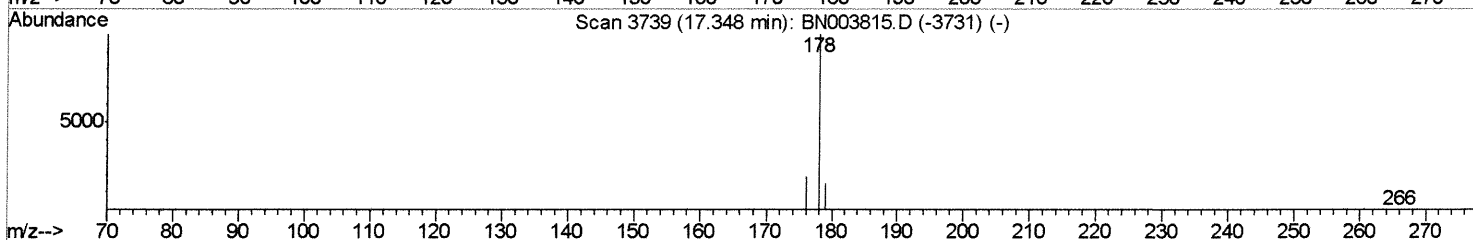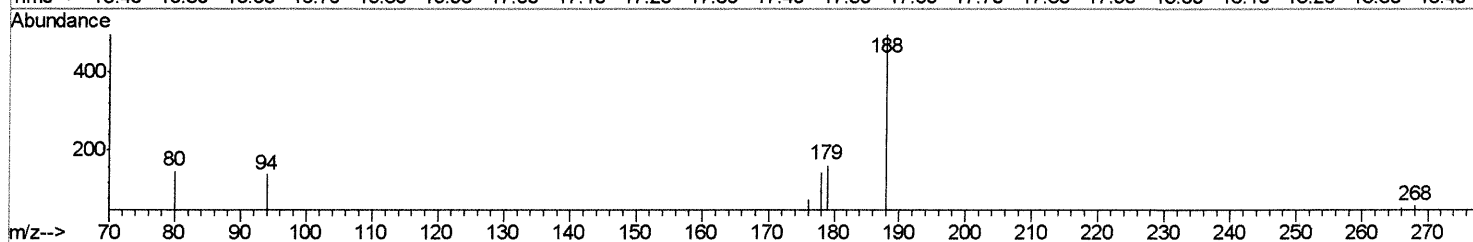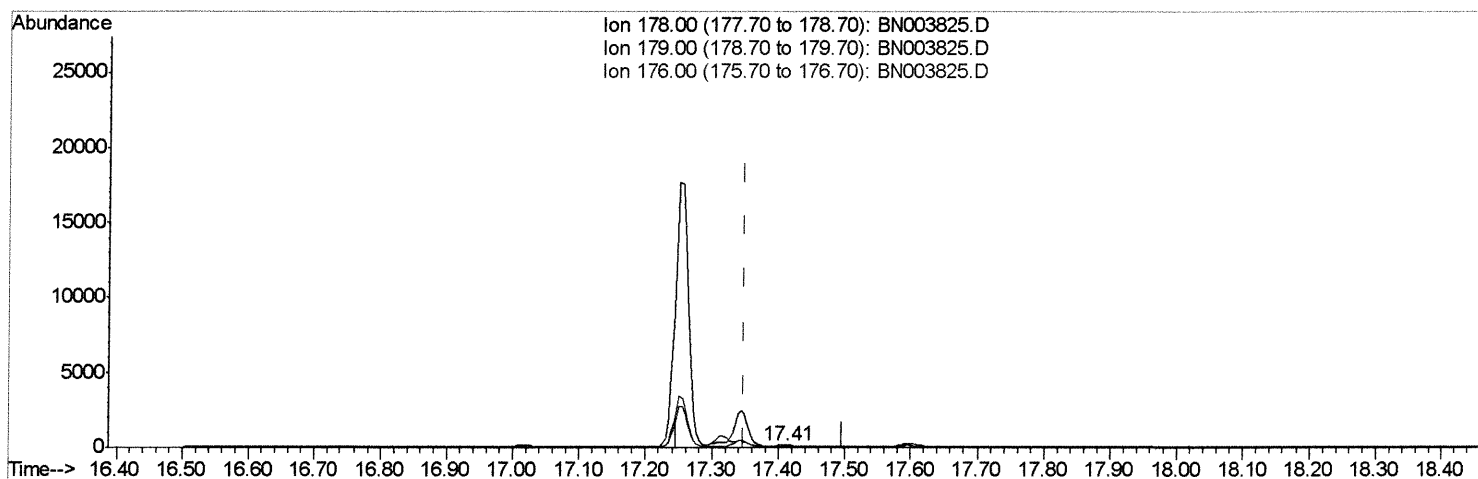

TIC: BN003825.D

(13) Anthracene

17.411min (+0.063) 0.00ng/ul

response 109

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	112.50#
176.00	18.50	52.08#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

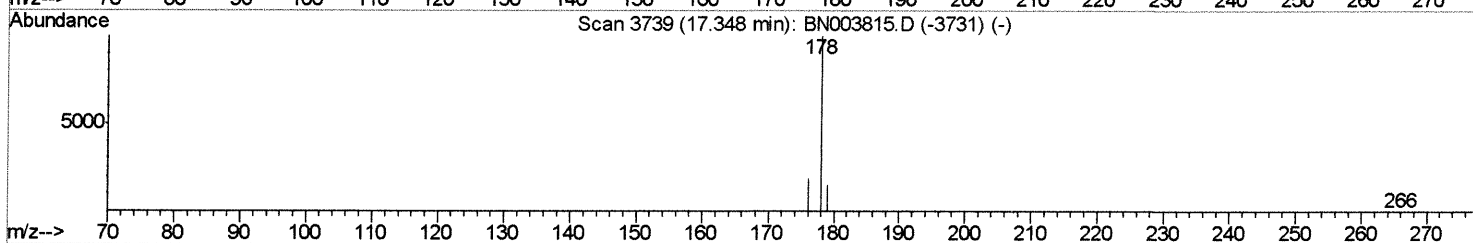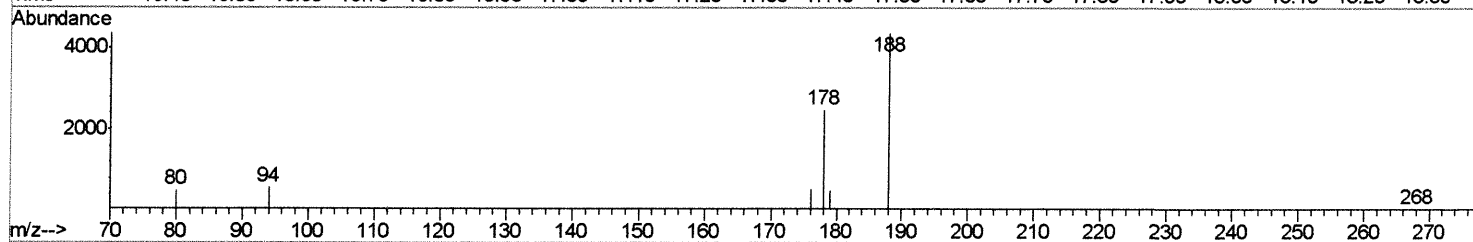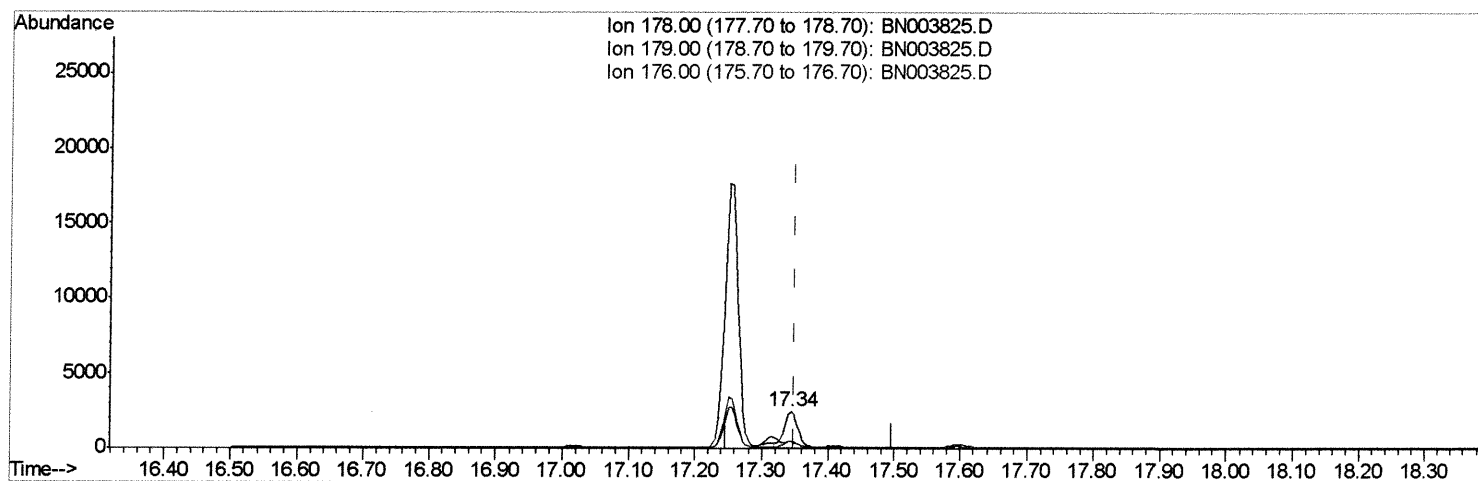

TIC: BN003825.D

(13) Anthracene

17.344min (-0.004) 0.08ng/ul m) SJ 12/13/14

response 3423

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	19.40#
176.00	18.50	20.52
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

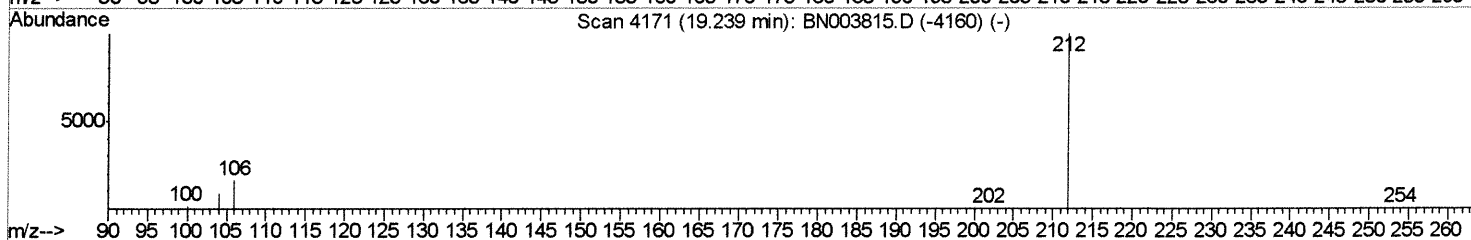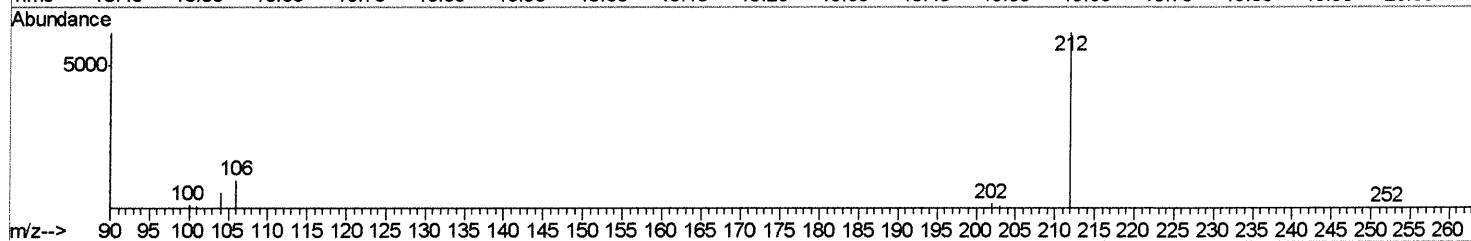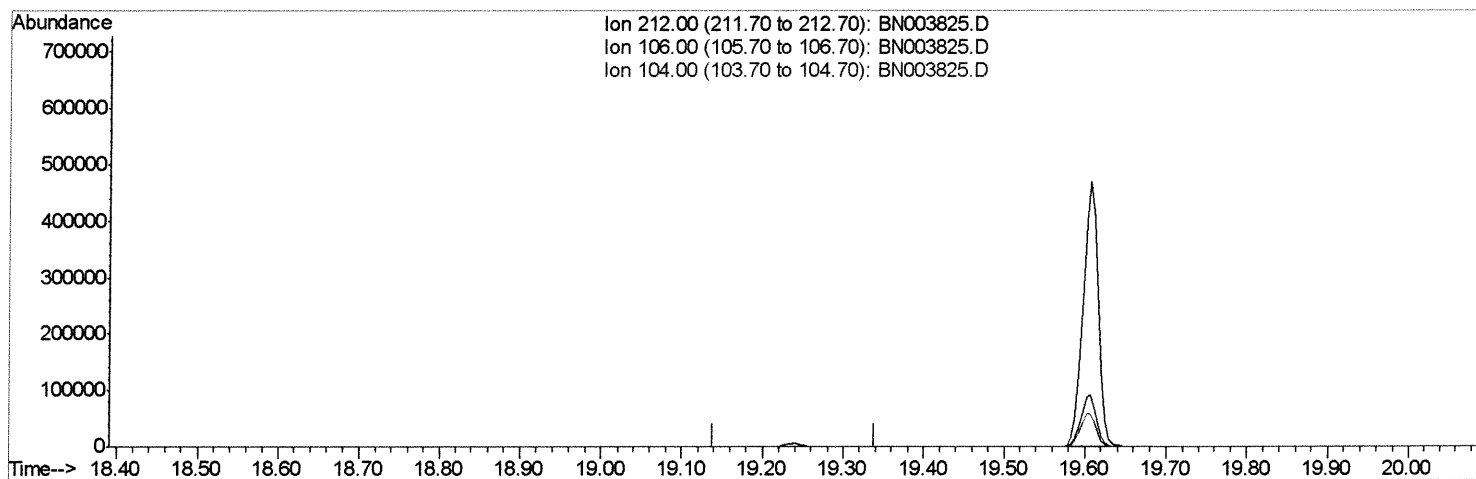

TIC: BN003825.D

(14) Fluoranthene-d10 (SURR)

19.239min (-19.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

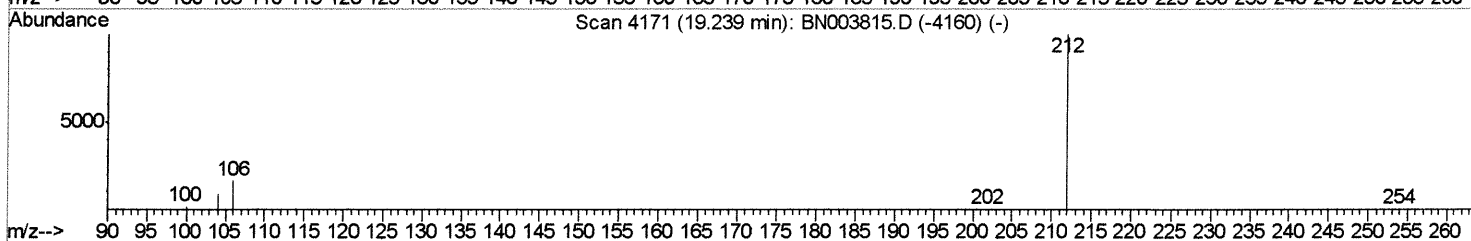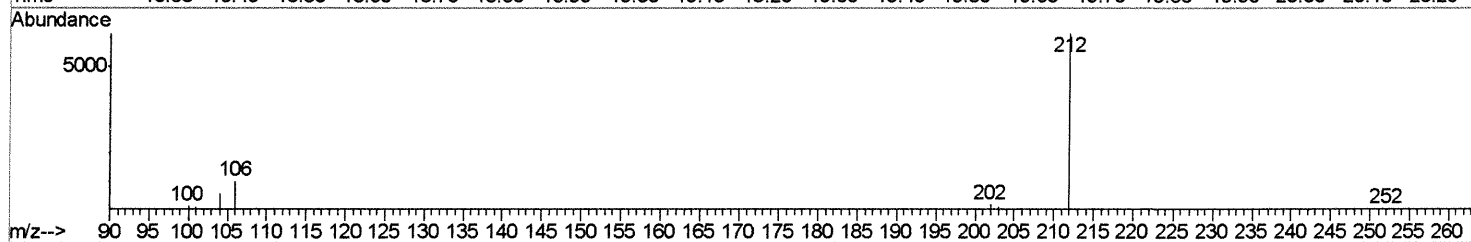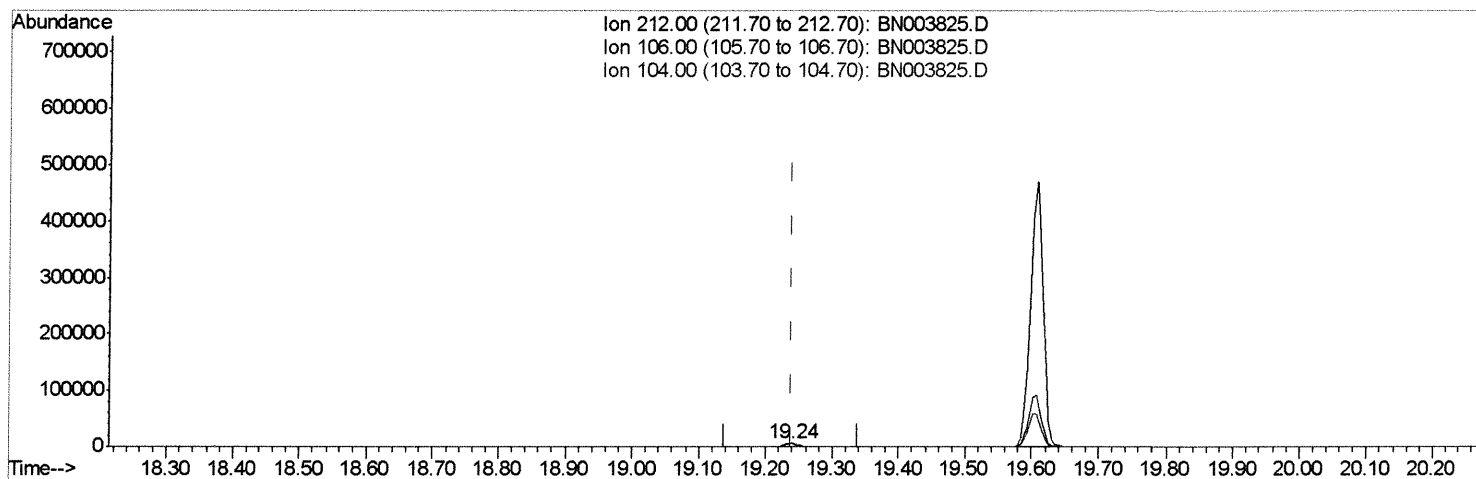

TIC: BN003825.D

(14) Fluoranthene-d10 (SURR)

19.239min (-0.000) 0.16ng/ul m> SJ 12/13/18

response 8034

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

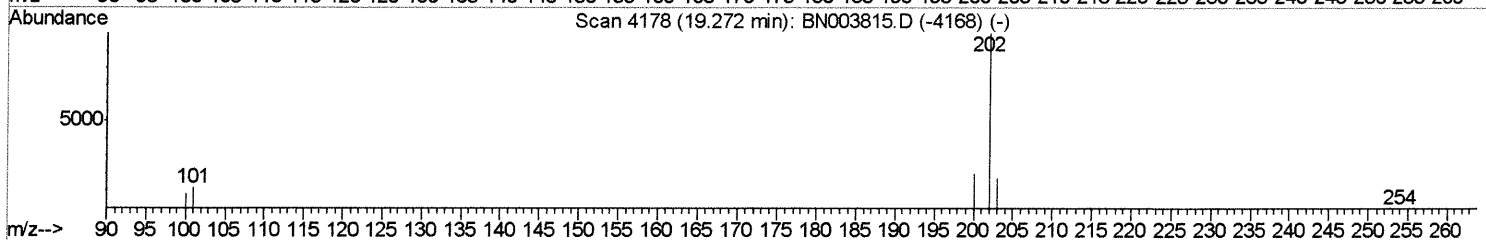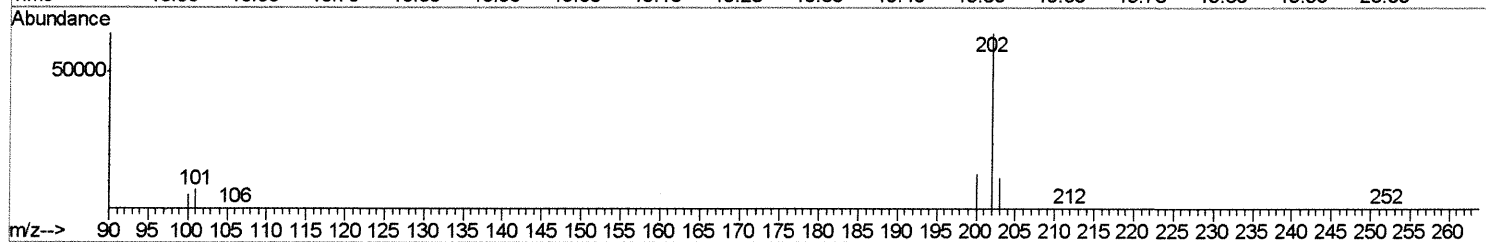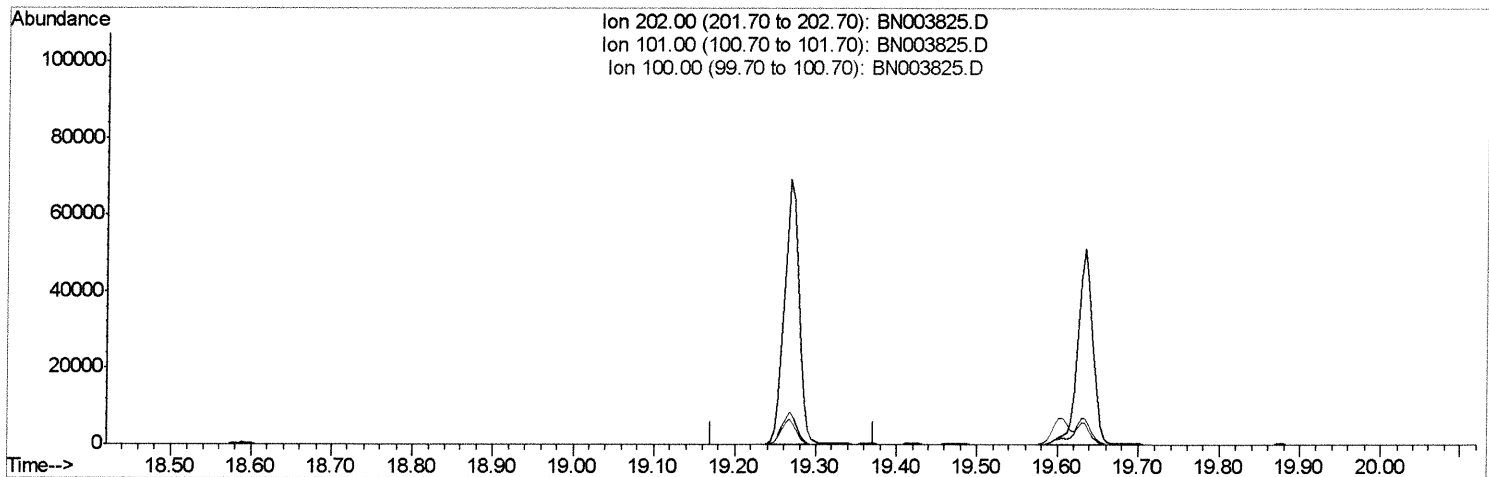

TIC: BN003825.D

(15) Fluoranthene (C)

19.272min (-19.272) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.70	0.00
100.00	8.10	0.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

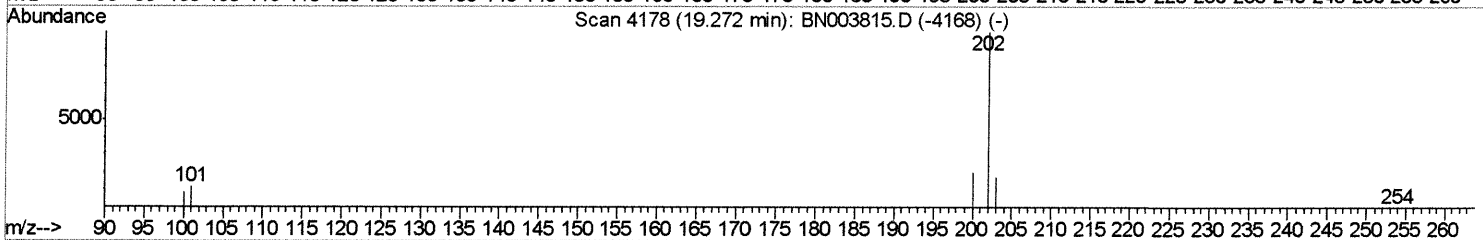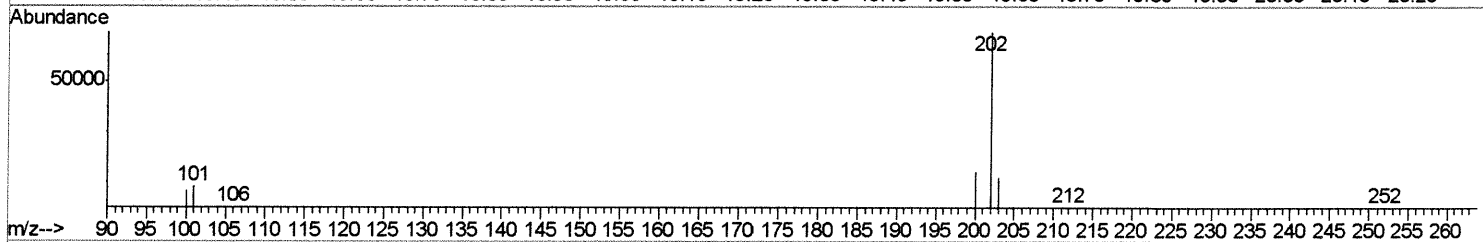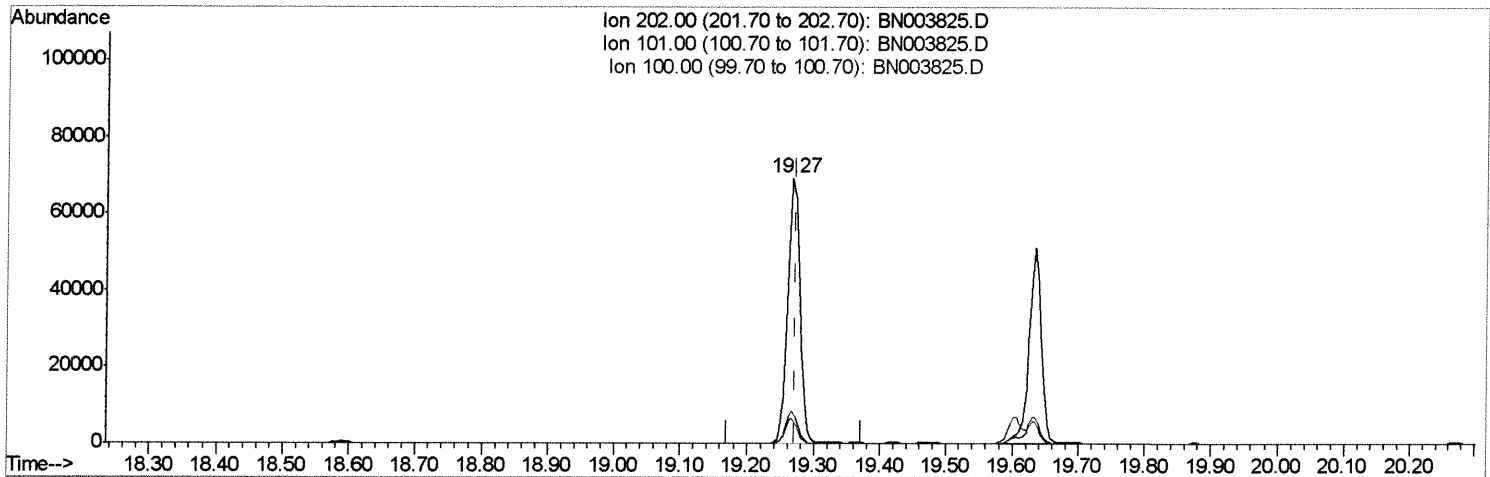

TIC: BN003825.D

(15) Fluoranthene (C)

19.267min (-0.005) 1.35ng/ul m> SJ 12/13/18

response 87607

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	12.36
100.00	8.10	9.54
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
 Quantitation Report (Qedit)
 Data File : BN003825.D
 Acq On : 11 Dec 2018 21:19
 Operator : JU/SJ
 Sample : J6170-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9M14

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 02:52:45 2018
 Response via : Initial Calibration

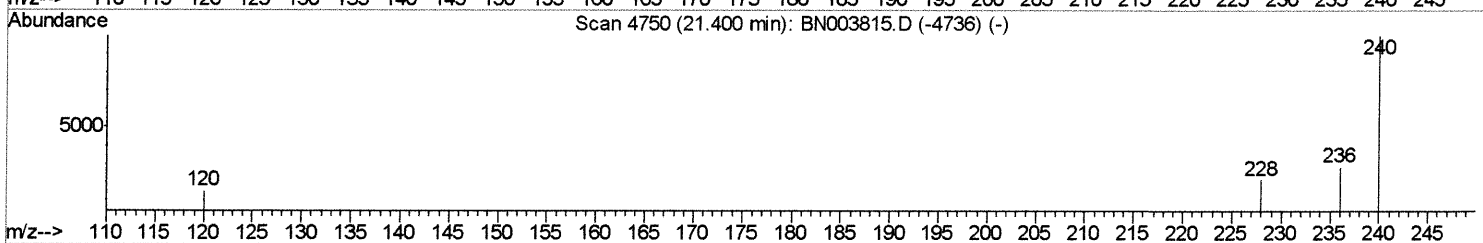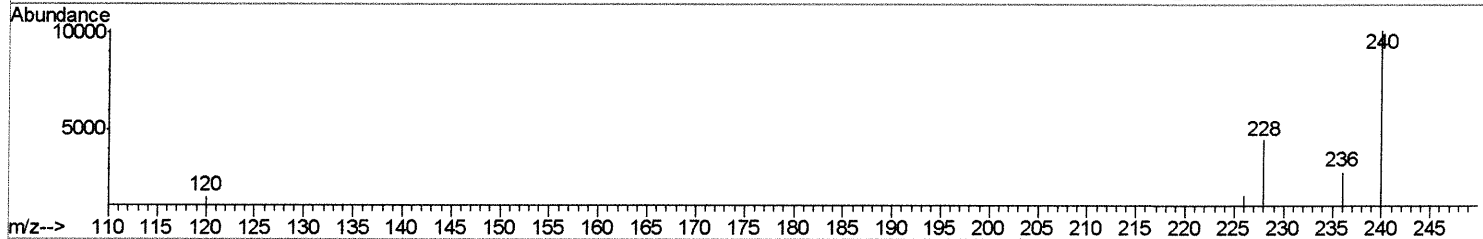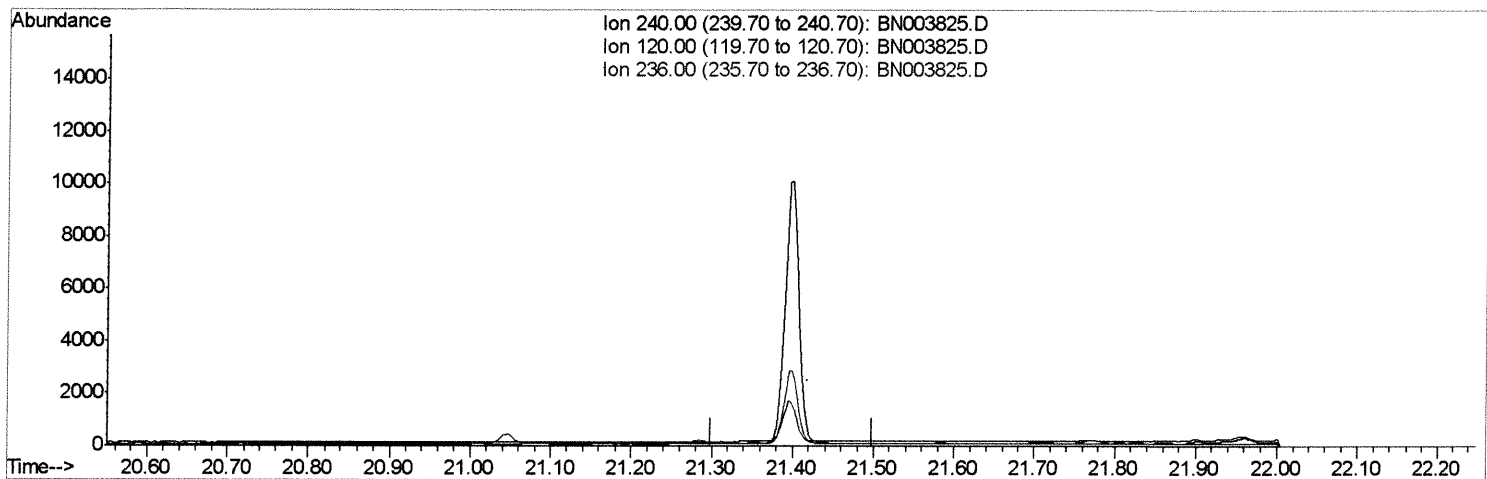

(16) Chrysene-d12 (I)
 21.400min (-21.400) 0.00ng/ul
 response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:33:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

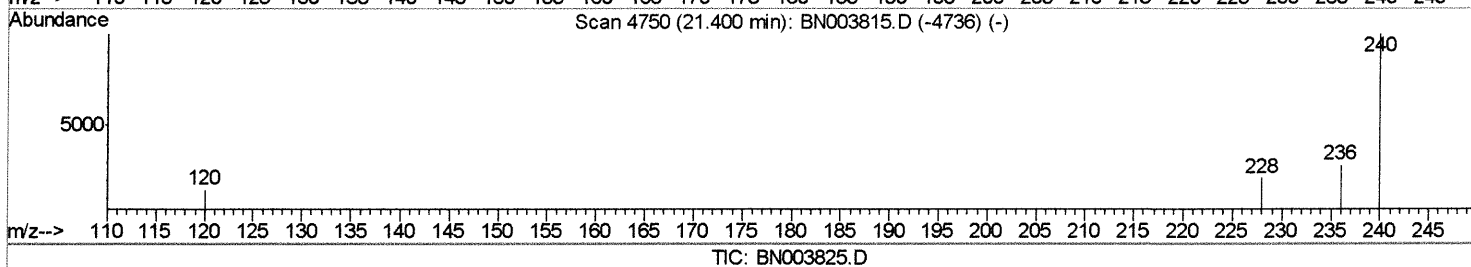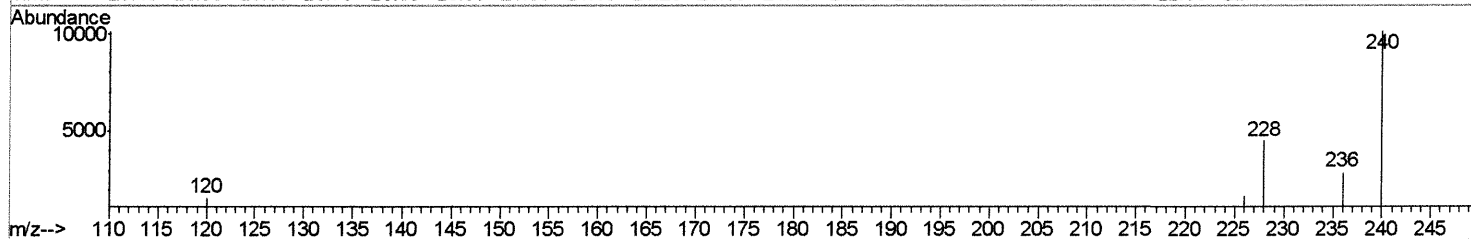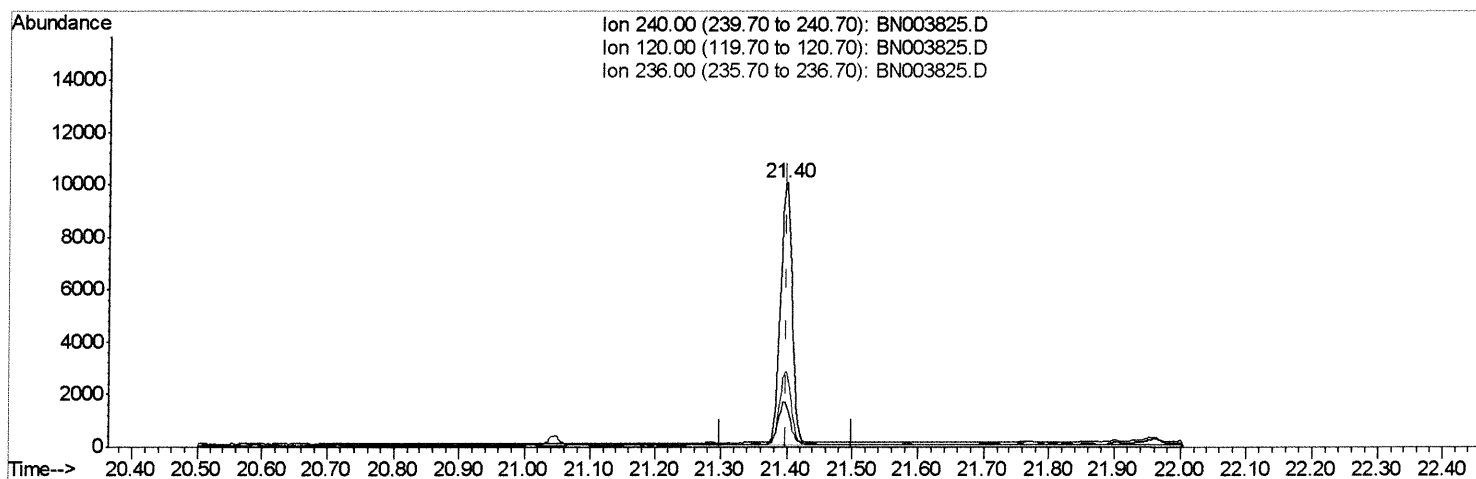

(16) Chrysene-d12 (I)

21.400min (-0.000) 0.40ng/ul m> SJ 12/13/18

response 12464

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.56
236.00	27.60	28.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:34:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

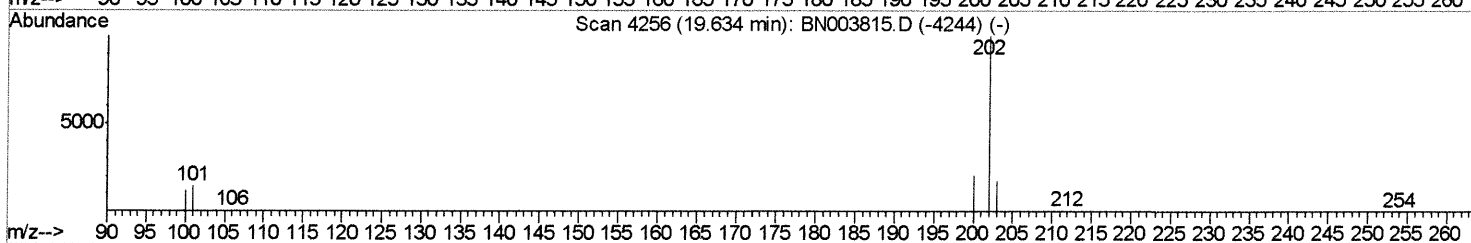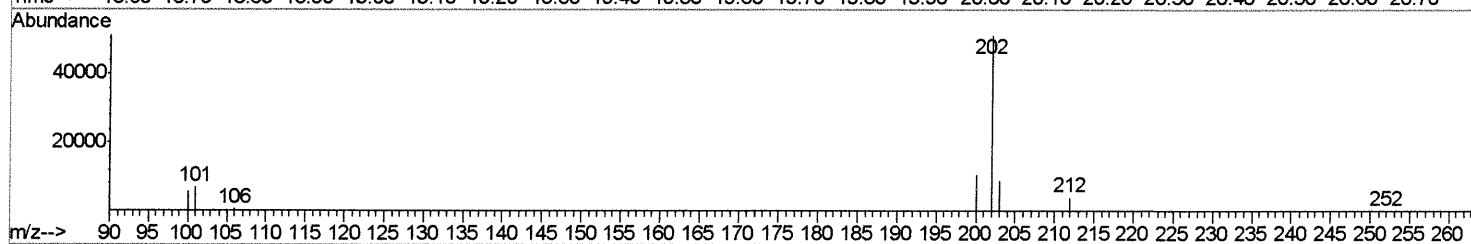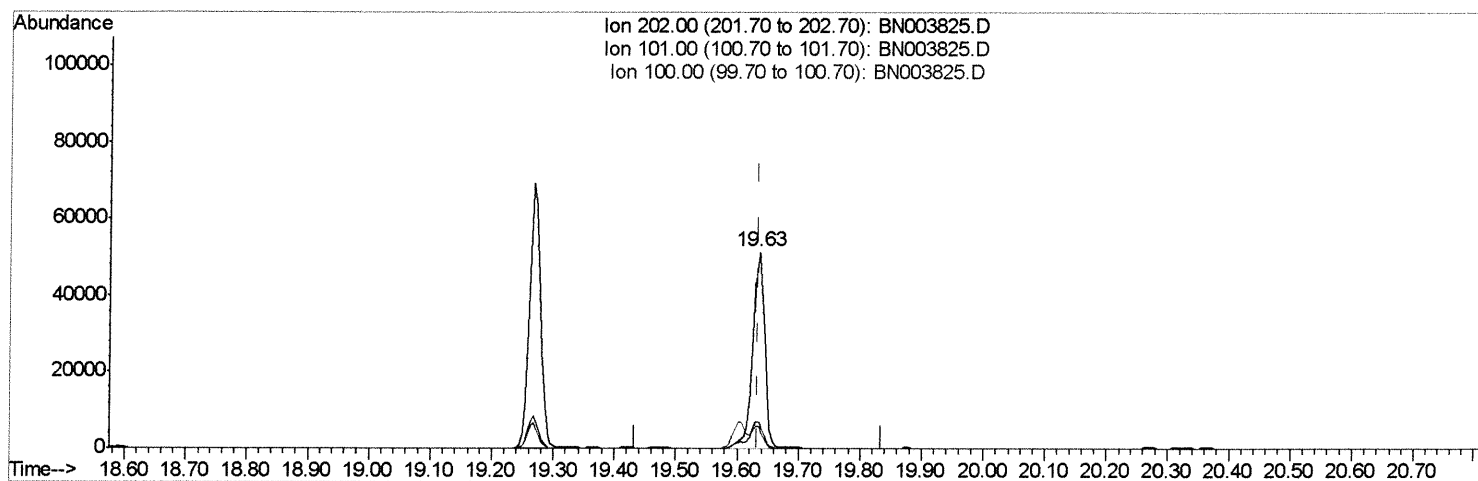

TIC: BN003825.D

(17) Pyrene

19.634min (-0.000) 1.51ng/ul

response 67482

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	13.67
100.00	10.60	10.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:34:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

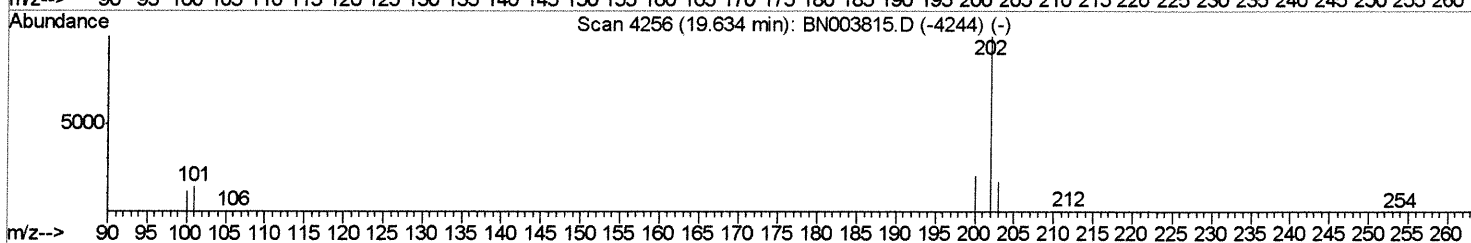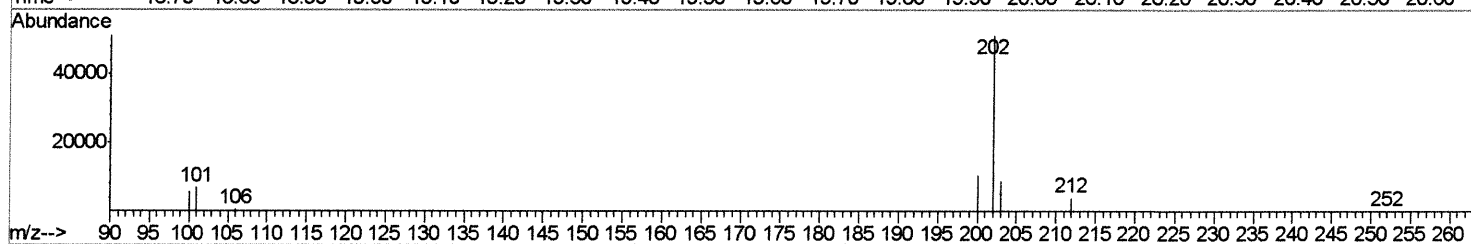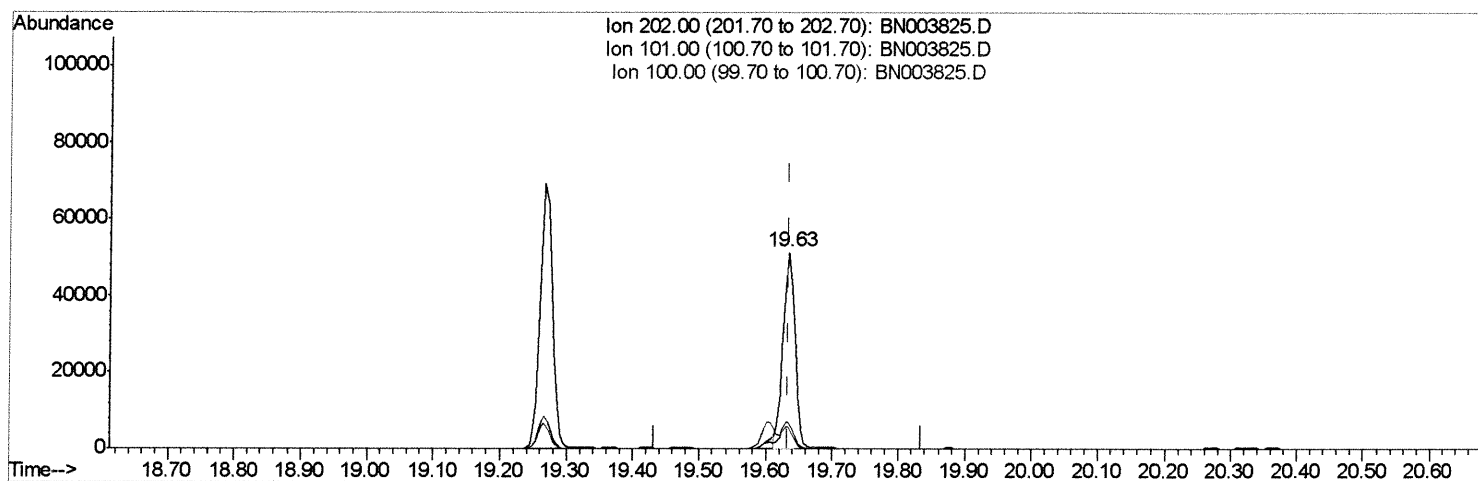

TIC: BN003825.D

(17) Pyrene

19.634min (-0.000) 1.44ng/ul m) SD 12/13/18

response 64274

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	13.67
100.00	10.60	10.99
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:34:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

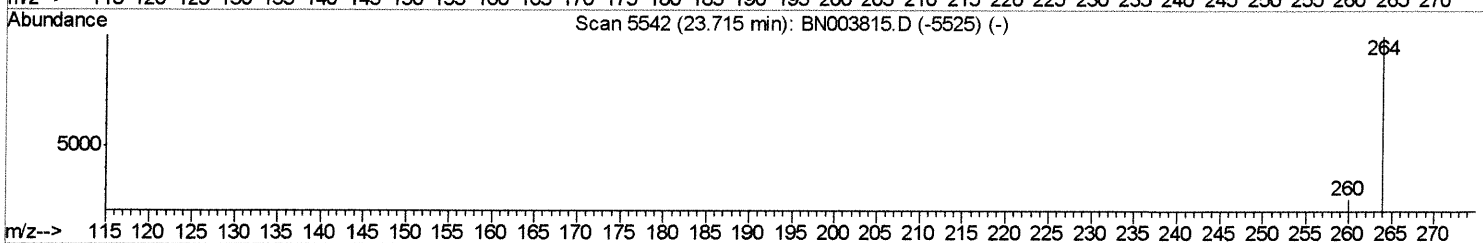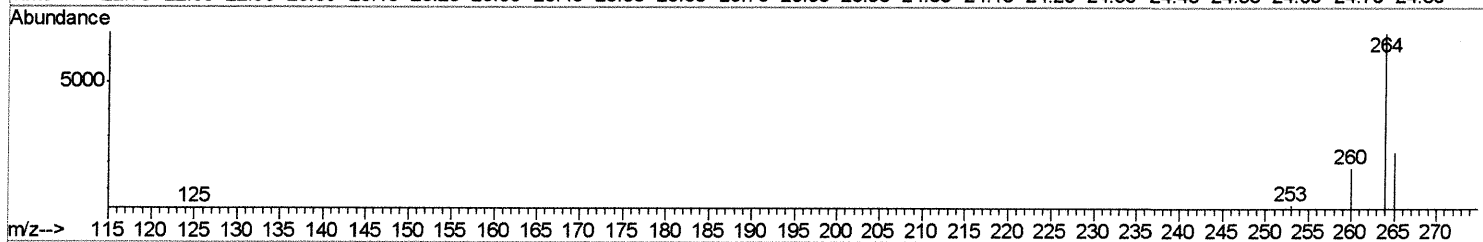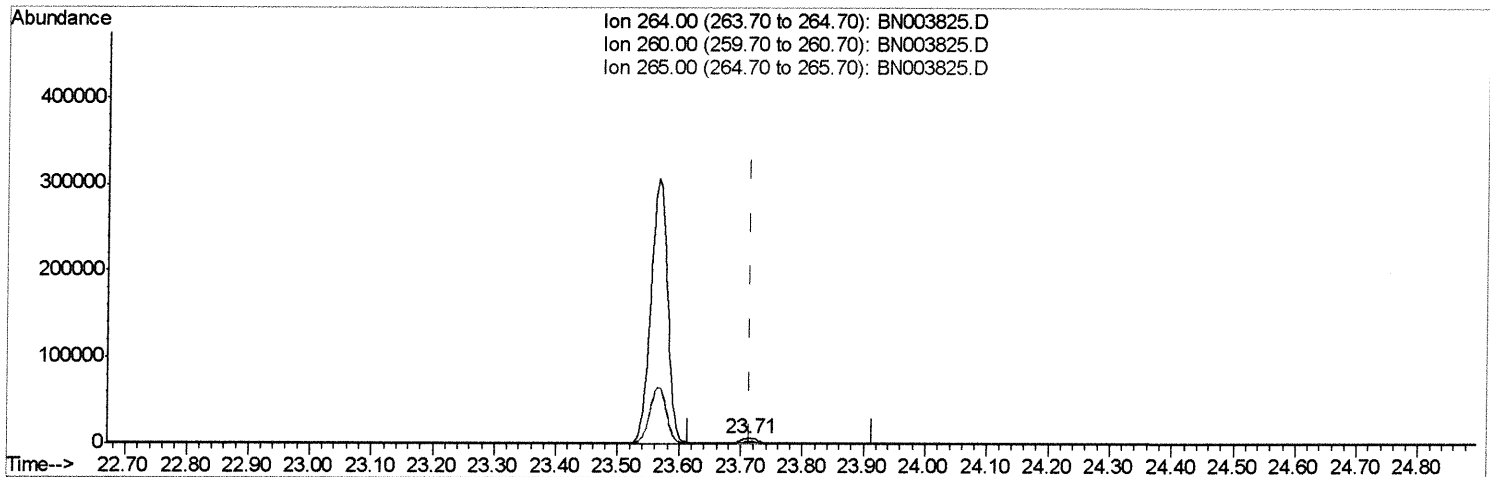

TIC: BN003825.D

(20) Perylene-d12 (I)

23.712min (-0.003) 0.40ng/ul

response 14448

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.33
265.00	33.50	34.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:34:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

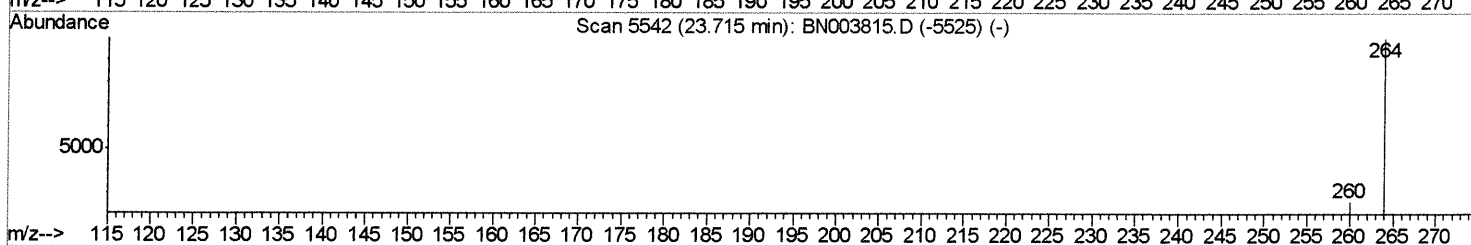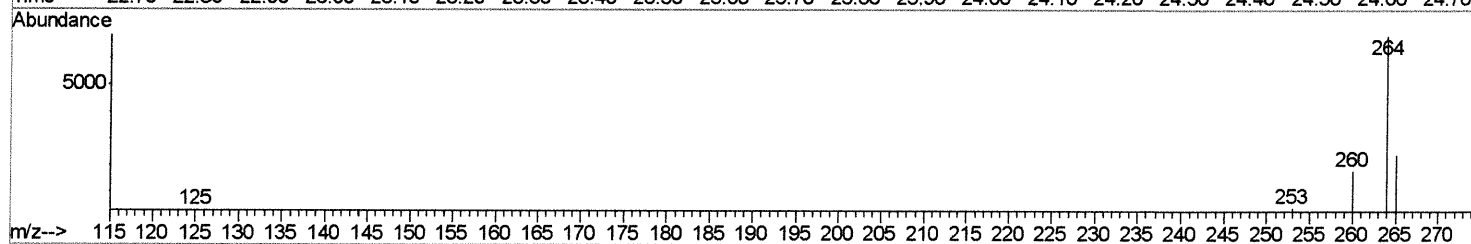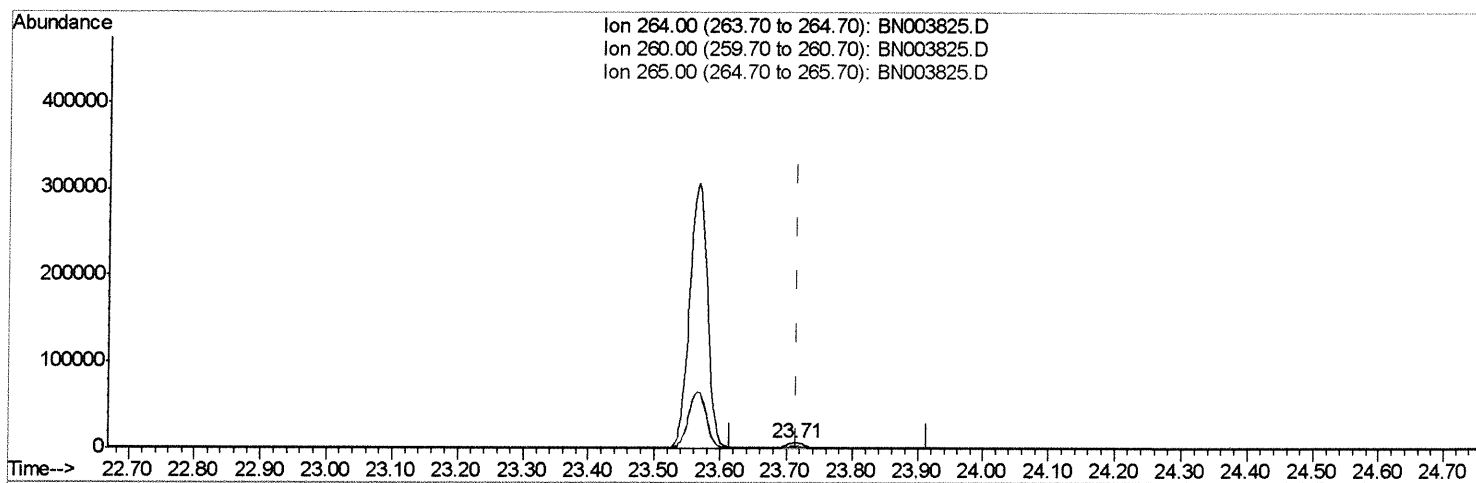

TIC: BN003825.D

(20) Perylene-d12 (I)

23.712min (-0.003) 0.40ng/ul m> SJ 12/13/18

response 12430

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.33
265.00	33.50	34.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

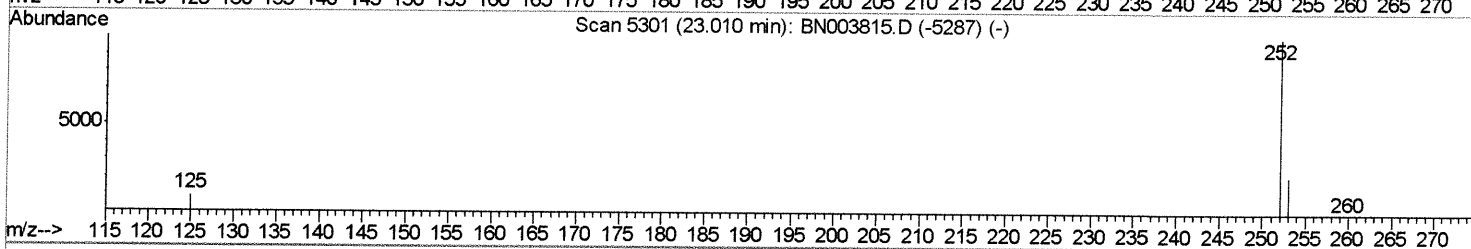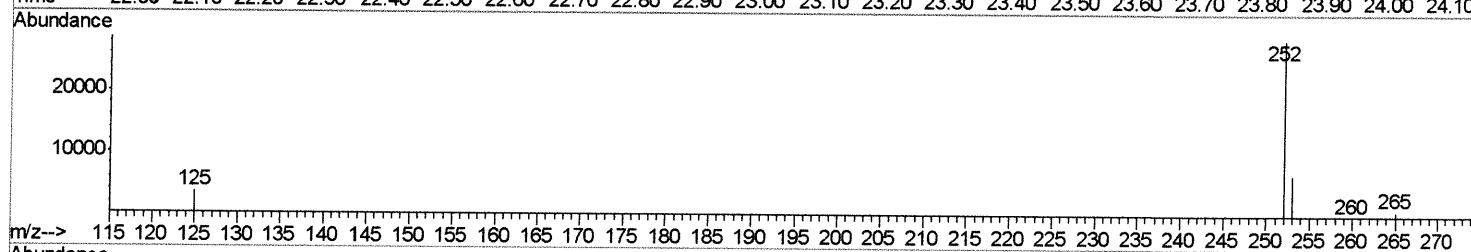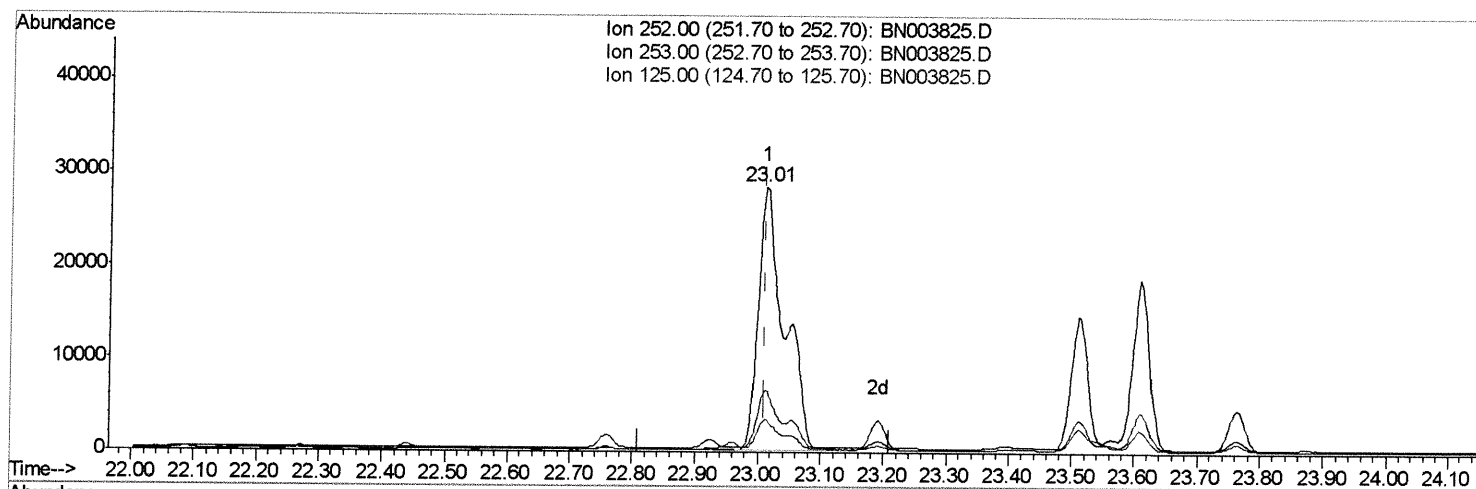

TIC: BN003825.D

(21) Benzo(b)fluoranthene

23.010min (-0.000) 1.58ng/ul

response 81449

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	23.38
125.00	11.20	12.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

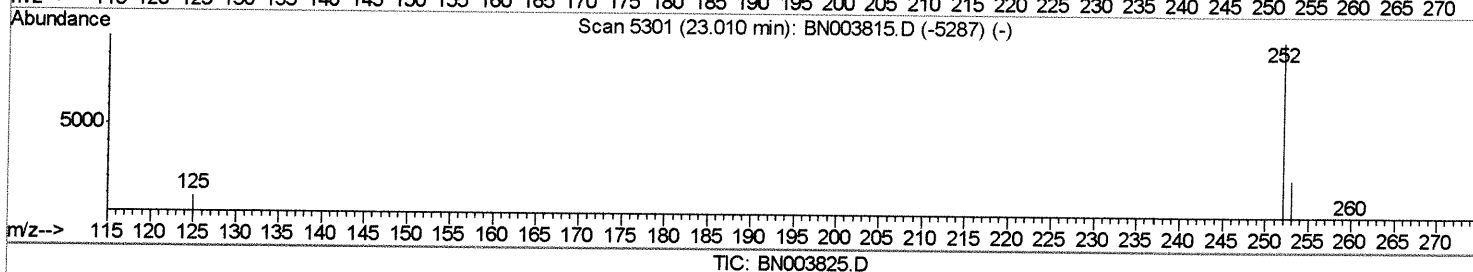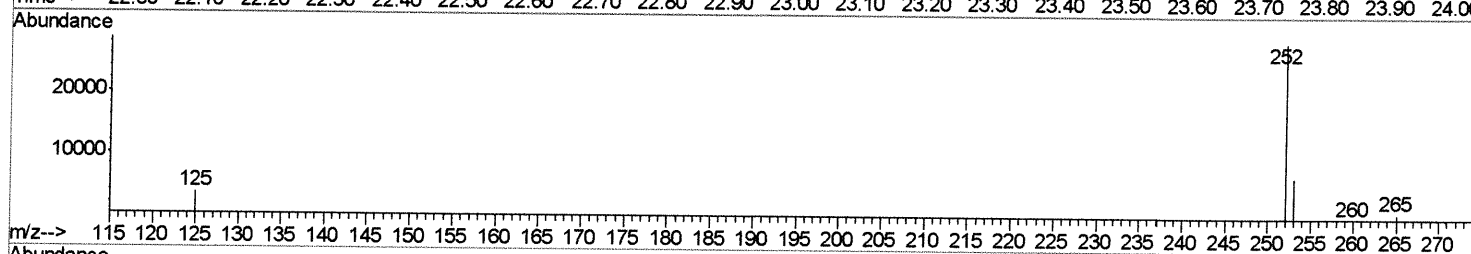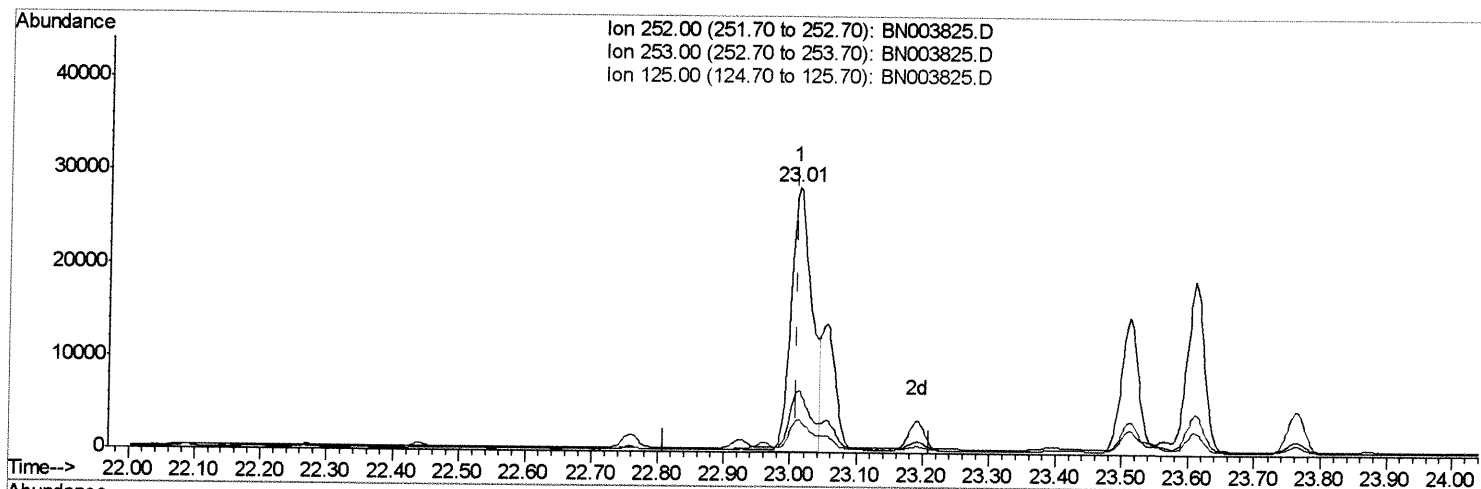

(21) Benzo(b)fluoranthene

23.010min (-0.000) 1.19ng/ul m > SJ 12/13/14

response 61315

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	23.38
125.00	11.20	12.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

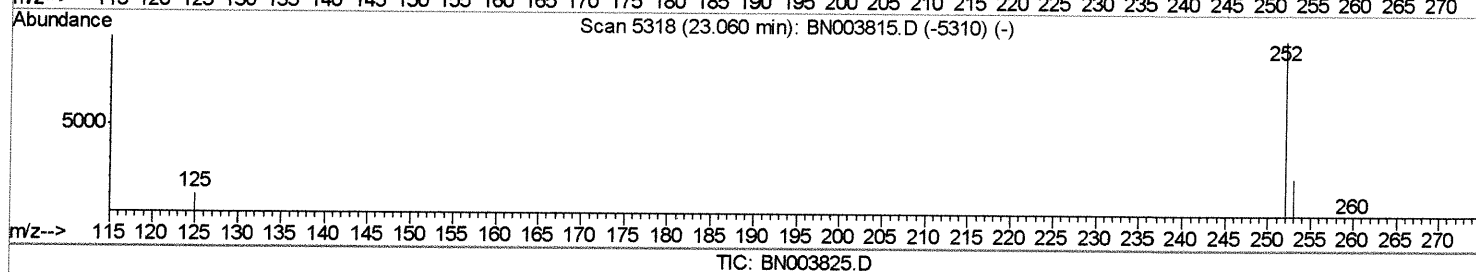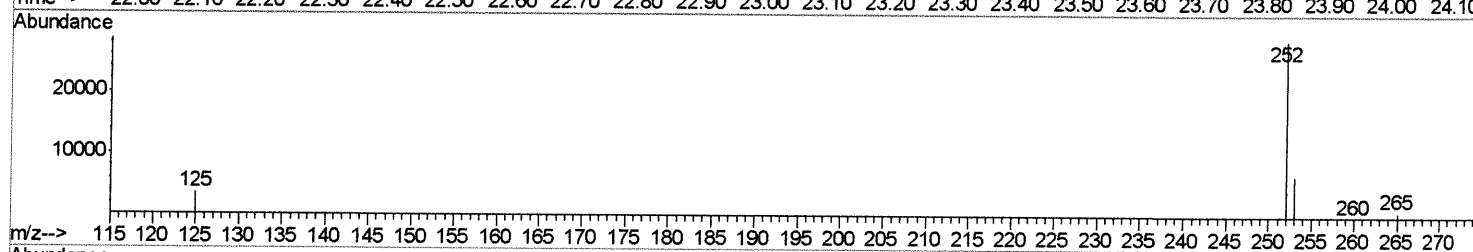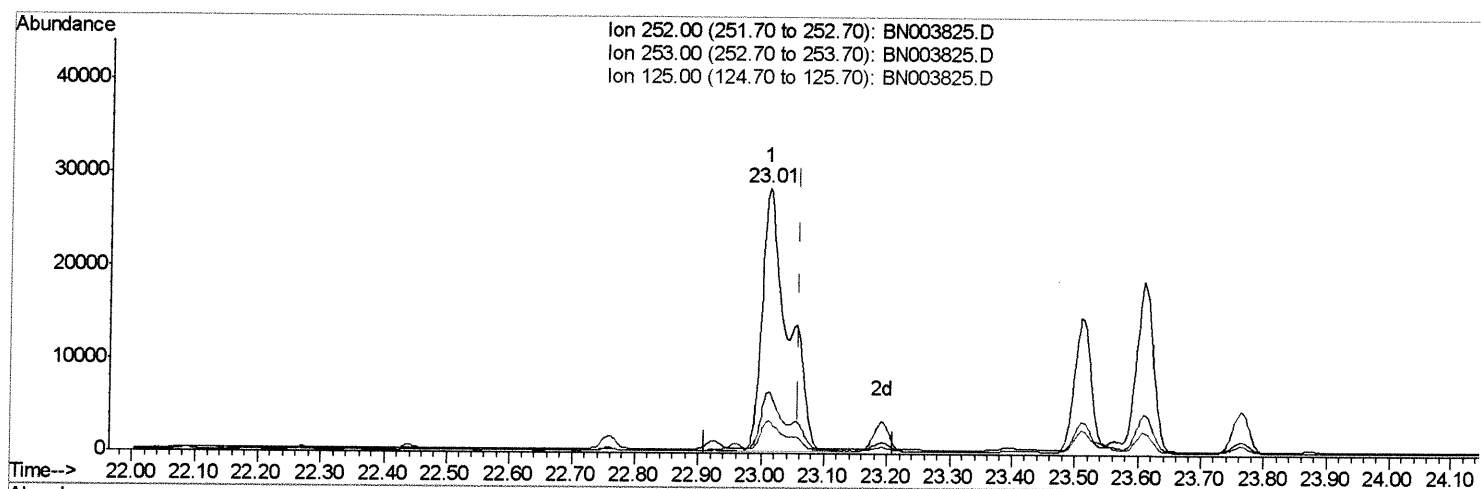

(22) Benzo(k)fluoranthene

23.010min (-0.050) 1.63ng/ul

response 81443

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	23.38
125.00	11.30	12.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:35:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

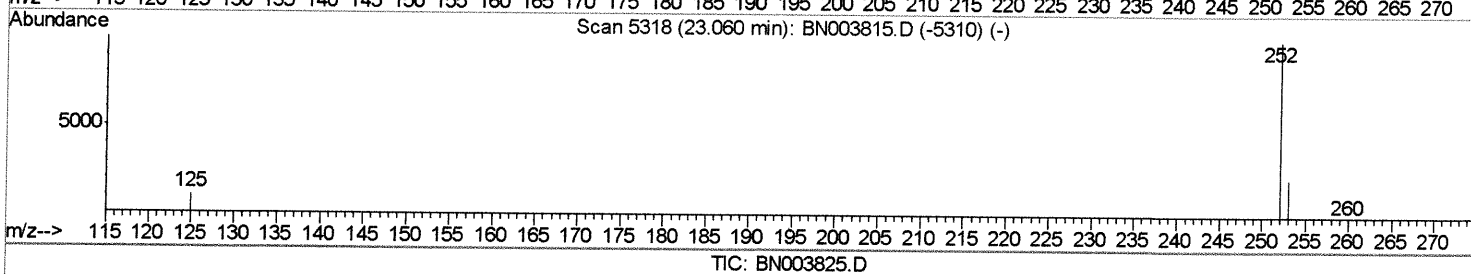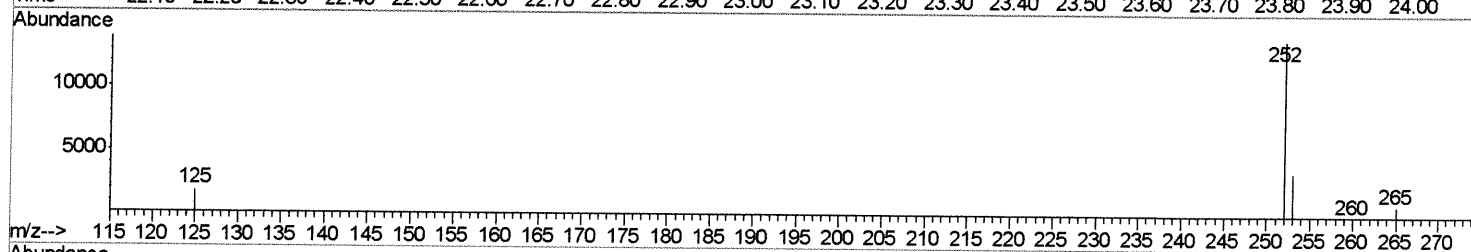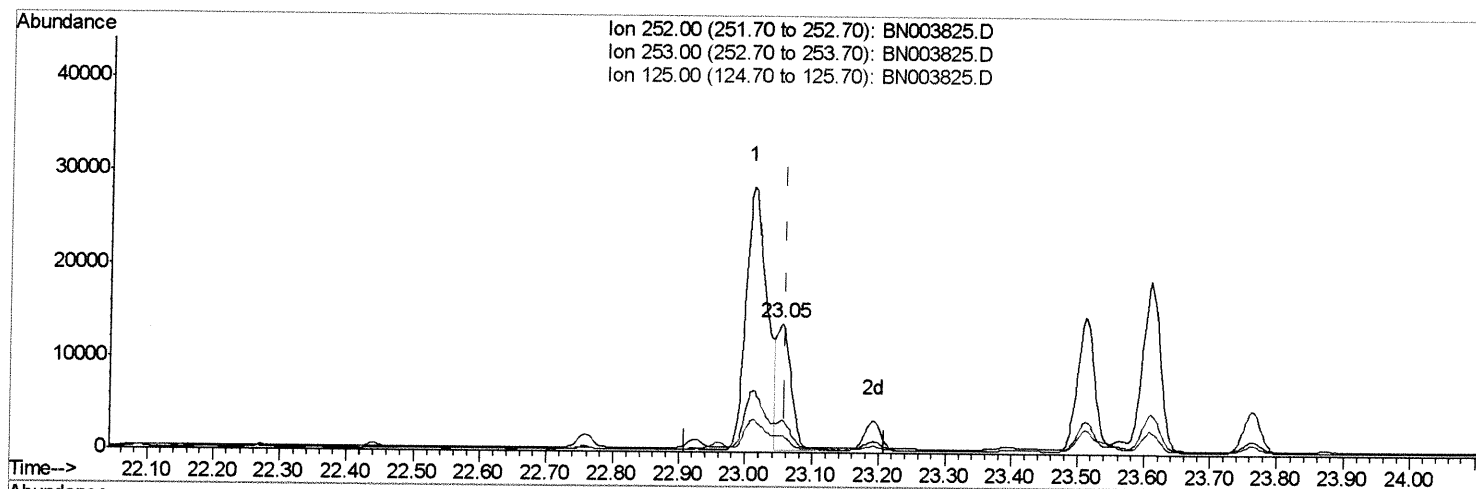

(22) Benzo(k)fluoranthene

23.054min (-0.006) 0.41ng/ul m> SJ 12/13/18

response 20602

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	25.16
125.00	11.30	13.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (QT Reviewed)

Data File : BN003825.D
Acq On : 11 Dec 2018 21:19
Operator : JU/SJ
Sample : J6170-19
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9M14

Manual Integrations
APPROVED

Sohil
12/12/2018 5:50:29 PM

Quant Time: Dec 12 03:36:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 02:52:45 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4935	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	18933	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	8911	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	16682m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	12464m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	12430m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	5331	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	8034m	0.16	ng/ul	0.00
Target Compounds						
9) Fluorene	15.52	166	1058	0.026	ng/ul#	96
12) Phenanthrene	17.25	178	24586	0.449	ng/ul	99
13) Anthracene	17.34	178	3423m	0.076	ng/ul	
15) Fluoranthene	19.27	202	87607m	1.355	ng/ul	
17) Pyrene	19.63	202	64274m	1.438	ng/ul	
18) Benzo(a)anthracene	21.38	228	34404	0.874	ng/ul	97
19) Chrysene	21.43	228	41263	0.916	ng/ul	99
21) Benzo(b)fluoranthene	23.01	252	61315m	1.192	ng/ul	
22) Benzo(k)fluoranthene	23.05	252	20602m	0.411	ng/ul	
23) Benzo(a)pyrene	23.61	252	33947	0.762	ng/ul	99
24) Indeno(1,2,3-cd)pyrene	26.06	276	30865	0.604	ng/ul	95
25) Dibenzo(a,h)anthracene	26.07	278	7653	0.186	ng/ul#	88
26) Benzo(g,h,i)perylene	26.78	276	24541	0.553	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 12/13/18

SJ 12/13/18