


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (QT Reviewed)
Data File : BN003840.D
Acq On : 12 Dec 2018 06:07
Operator : JU/SJ
Sample : J6171-04DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y08DL

Manual Integrations
APPROVED

Sohil
12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:48:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

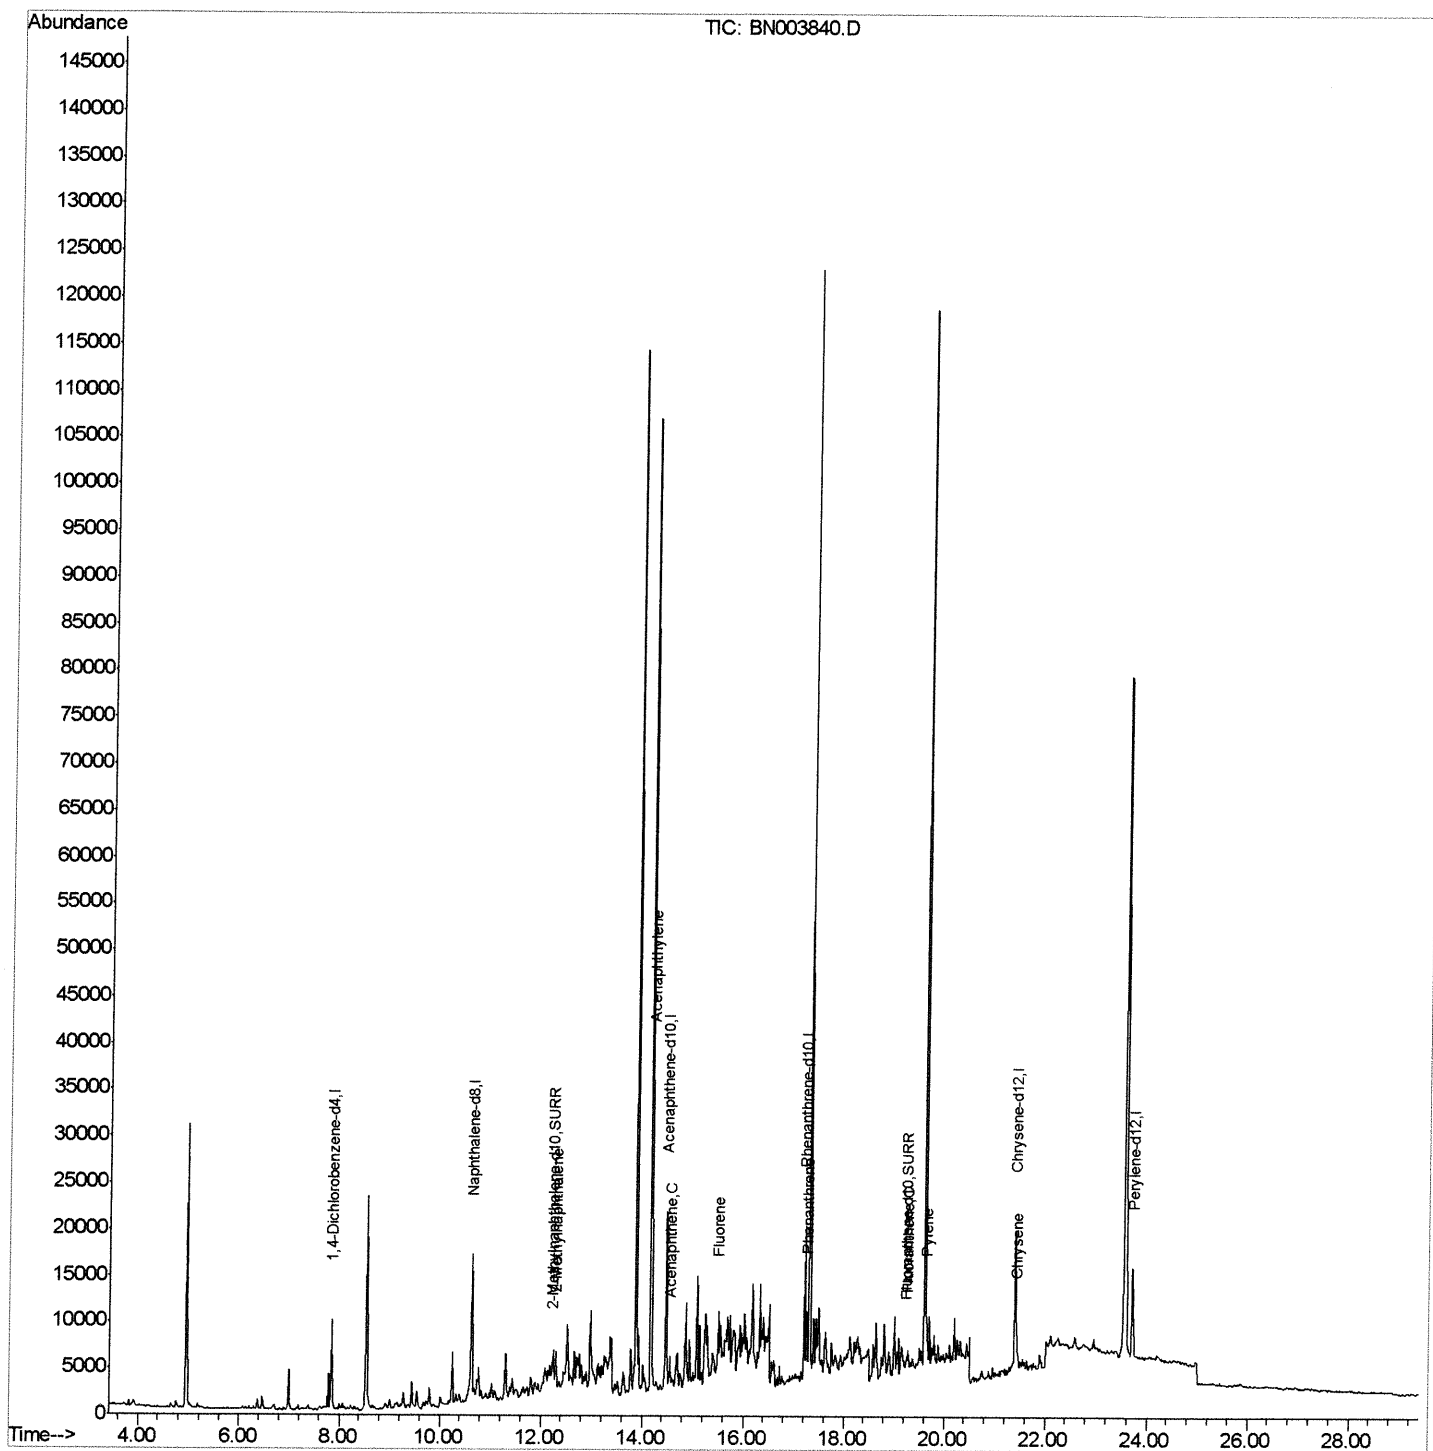

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003840.D
Acq On : 12 Dec 2018 06:07
Operator : JU/SJ
Sample : J6171-04DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y08DL

Manual Integrations
APPROVED

Sohil
12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:23:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

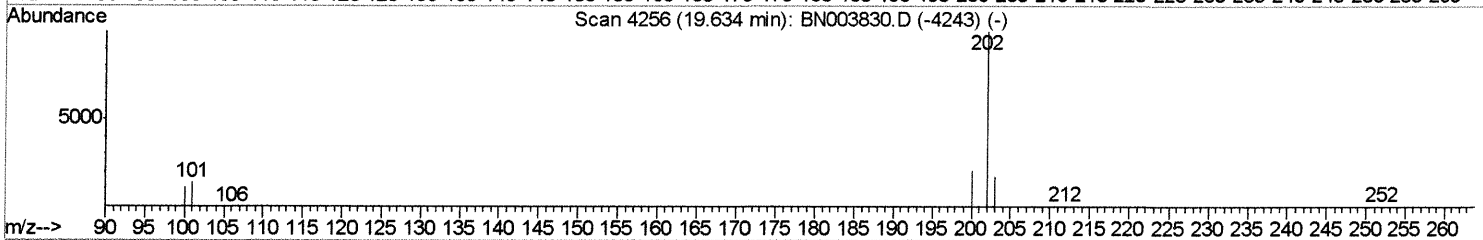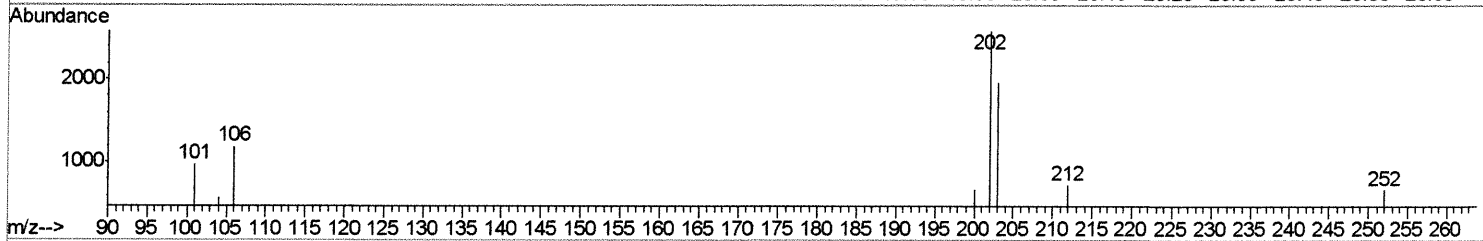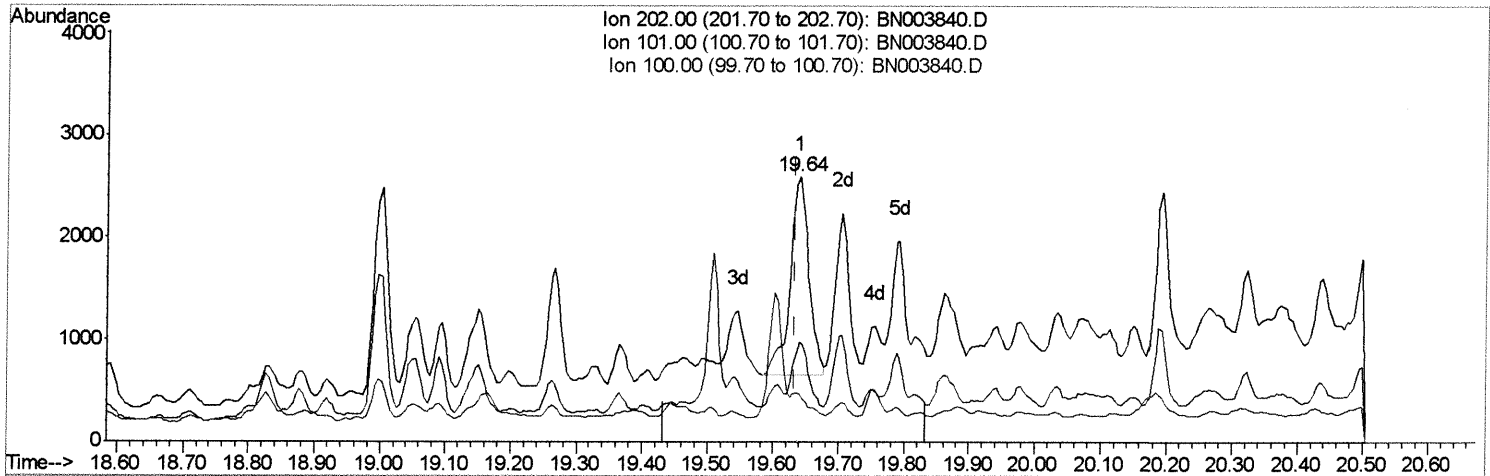

TIC: BN003840.D

(17) Pyrene

19.639min (+0.005) 0.08ng/ul

response 3777

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	37.55#
100.00	10.60	18.17#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003840.D
Acq On : 12 Dec 2018 06:07
Operator : JU/SJ
Sample : J6171-04DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y08DL

Manual Integrations
APPROVED

Sohil
12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:23:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

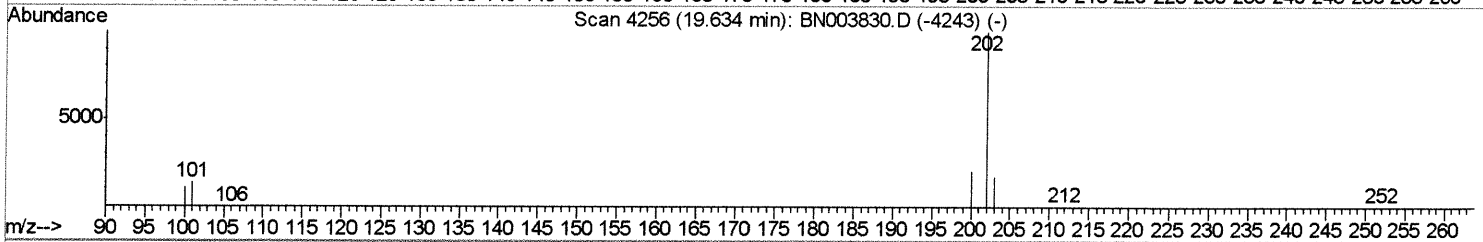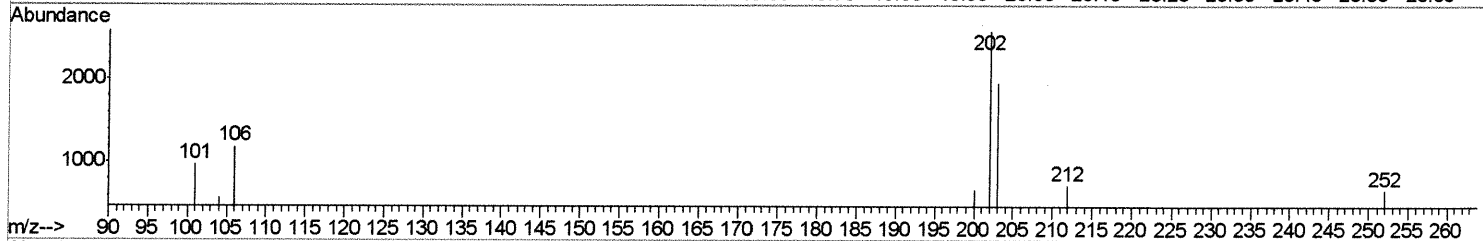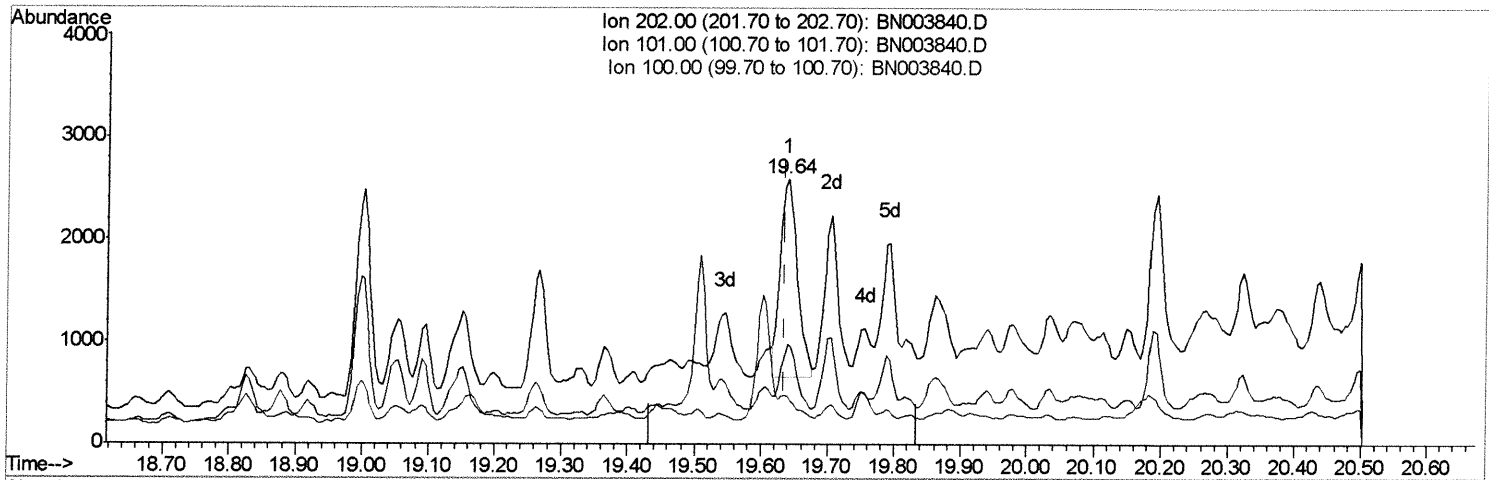

TIC: BN003840.D

(17) Pyrene

19.639min (+0.005) 0.08ng/ul m) SJ 12/13/14

response 3429

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	37.55#
100.00	10.60	18.17#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003840.D
Acq On : 12 Dec 2018 06:07
Operator : JU/SJ
Sample : J6171-04DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y08DL

Manual Integrations
APPROVED

Sohil
12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:23:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

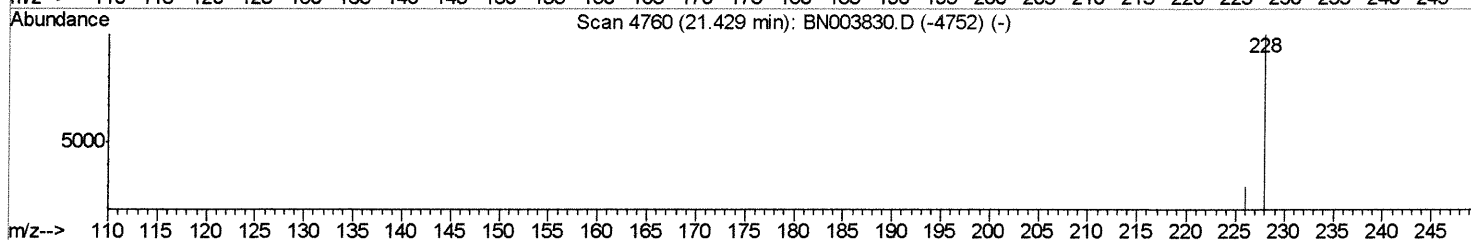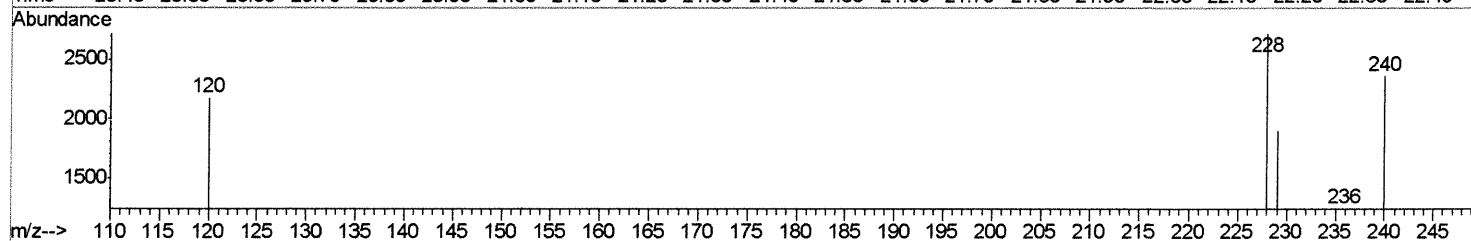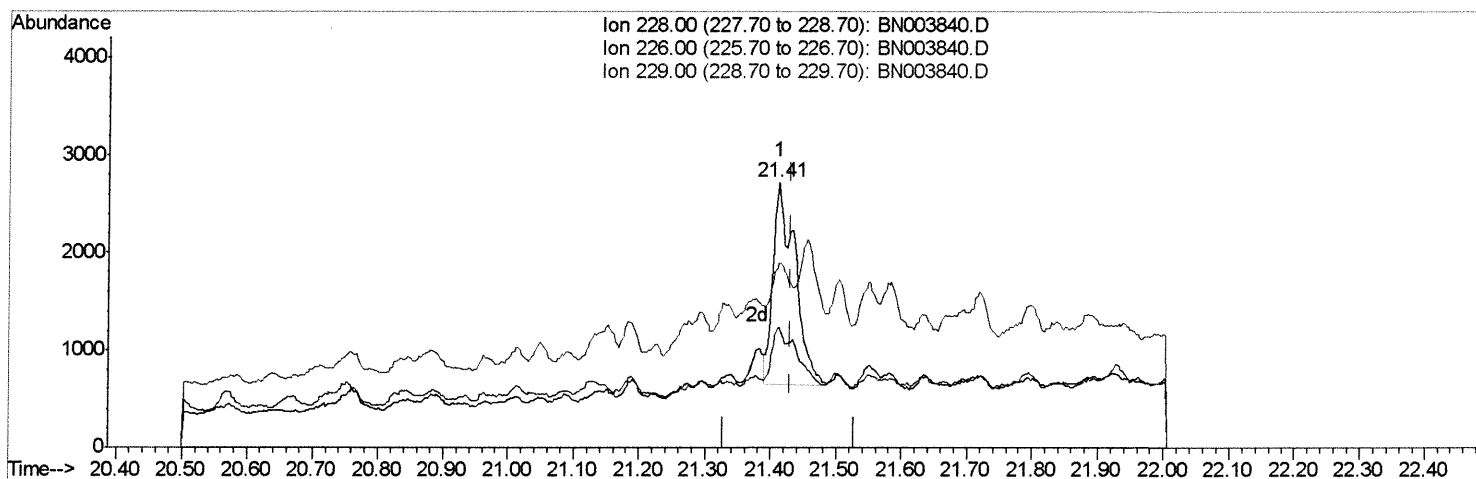

TIC: BN003840.D

(19) Chrysene

21.411min (-0.018) 0.11ng/ul

response 4854

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	45.24#
229.00	19.60	69.47#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
Quantitation Report (Qedit)




Data File : BN003840.D
Acq On : 12 Dec 2018 06:07
Operator : JU/SJ
Sample : J6171-04DL 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y08DL

Manual Integrations
APPROVED

Sohil
12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:23:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 03:46:49 2018
Response via : Initial Calibration

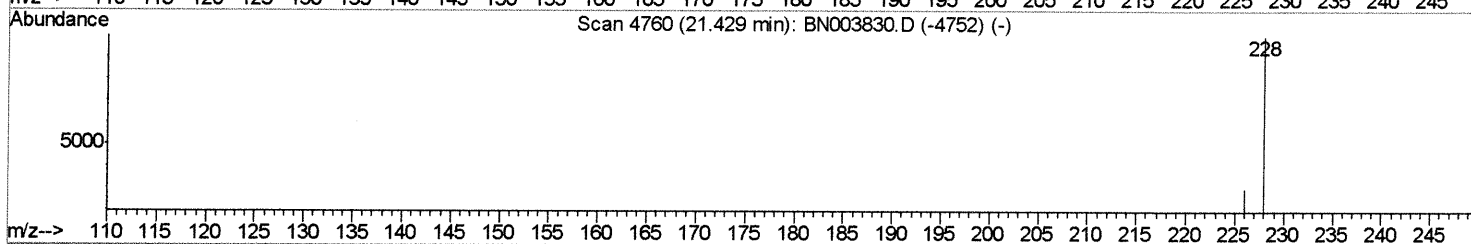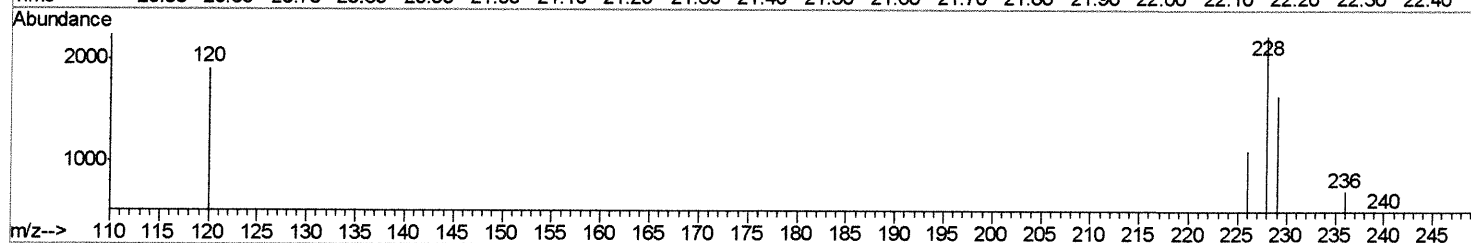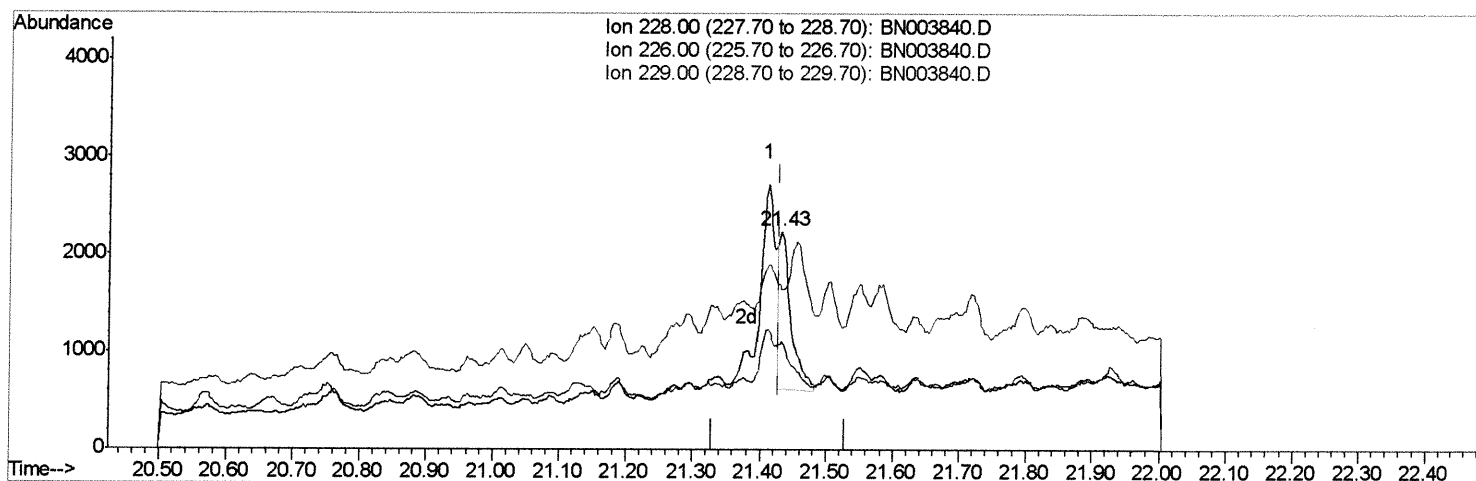

TIC: BN003840.D

(19) Chrysene

21.432min (+0.003) 0.04ng/ul m> SJ 12/13/18

response 1927

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	49.84#
229.00	19.60	73.67#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121118\
 Quantitation Report (QT Reviewed)
 Data File : BN003840.D
 Acq On : 12 Dec 2018 06:07
 Operator : JU/SJ
 Sample : J6171-04DL 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y08DL

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:51:06 PM

Quant Time: Dec 12 07:48:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 03:46:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	4886	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19547	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	9893	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	18833	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	12583	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	13295	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	1397	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1585	0.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) 2-Methylnaphthalene	12.29	142	2675	0.070	ng/ul	100
7) Acenaphthylene	14.19	152	1129	0.025	ng/ul#	1
8) Acenaphthene	14.55	153	1697	0.043	ng/ul#	51
9) Fluorene	15.52	166	3397	0.075	ng/ul#	79
12) Phenanthrene	17.25	178	7451	0.121	ng/ul#	76
15) Fluoranthene	19.27	202	1676	0.023	ng/ul#	51
17) Pyrene	19.64	202	3429m	0.076	ng/ul	
19) Chrysene	21.43	228	1927m	0.042	ng/ul	

SD 12/13/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed