

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\  
 Data File : BN008917.D  
 Acq On : 11 Dec 2019 15:11  
 Operator : JU  
 Sample : K6088-04  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :

Quant Time: Dec 12 00:21:52 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 11 10:35:08 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.56  | 152  | 2043     | 0.40 | ng/ul | 0.00     |
| 2) Naphthalene-d8         | 10.32 | 136  | 9259     | 0.40 | ng/ul | 0.00     |
| 6) Acenaphthene-d10       | 14.19 | 164  | 6076     | 0.40 | ng/ul | 0.00     |
| 10) Phenanthrene-d10      | 0.00  | 188  | 0        | 0.00 | ng/ul | -16.93   |
| 16) Chrysene-d12          | 21.13 | 240  | 12365    | 0.40 | ng/ul | 0.00     |
| 20) Perylene-d12          | 23.28 | 264  | 13881    | 0.40 | ng/ul | 0.00     |

|                             |       |     |      |      |       |      |
|-----------------------------|-------|-----|------|------|-------|------|
| System Monitoring Compounds |       |     |      |      |       |      |
| 4) 2-Methylnaphthalene-d10  | 11.91 | 152 | 3262 | 0.21 | ng/ul | 0.00 |
| 14) Fluoranthene-d10        | 18.96 | 212 | 9321 | 0.00 | ng/ul | 0.00 |


|                            |       |     |       |        |        |    |
|----------------------------|-------|-----|-------|--------|--------|----|
| Target Compounds           |       |     |       | Ovalue |        |    |
| 3) Naphthalene             | 10.36 | 128 | 5242  | 0.188  | ng/ul  | 97 |
| 5) 2-Methylnaphthalene     | 11.98 | 142 | 4724  | 0.242  | ng/ul  | 99 |
| 7) Acenaphthylene          | 13.90 | 152 | 2247  | 0.067  | ng/ul# | 90 |
| 9) Fluorene                | 15.24 | 166 | 703   | 0.024  | ng/ul# | 84 |
| 17) Pyrene                 | 19.36 | 202 | 25006 | 0.504  | ng/ul  | 99 |
| 18) Benzo(a)anthracene     | 21.12 | 228 | 14860 | 0.299  | ng/ul  | 96 |
| 19) Chrysene               | 21.17 | 228 | 17955 | 0.368  | ng/ul  | 96 |
| 21) Benzo(b)fluoranthene   | 22.65 | 252 | 30835 | 0.539  | ng/ul  | 94 |
| 22) Benzo(k)fluoranthene   | 22.65 | 252 | 30835 | 0.543  | ng/ul  | 96 |
| 23) Benzo(a)pyrene         | 23.19 | 252 | 13015 | 0.242  | ng/ul  | 93 |
| 24) Indeno(1,2,3-cd)pyrene | 25.39 | 276 | 9465  | 0.151  | ng/ul# | 94 |
| 25) Dibenzo(a,h)anthracene | 25.40 | 278 | 2911  | 0.057  | ng/ul# | 64 |
| 26) Benzo(g,h,i)perylene   | 26.02 | 276 | 8607  | 0.164  | ng/ul  | 97 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\  
Data File : BN008917.D  
Acq On : 11 Dec 2019 15:11  
Operator : JU  
Sample : K6088-04  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :

Quant Time: Dec 12 00:21:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 11 10:35:08 2019  
Response via : Initial Calibration

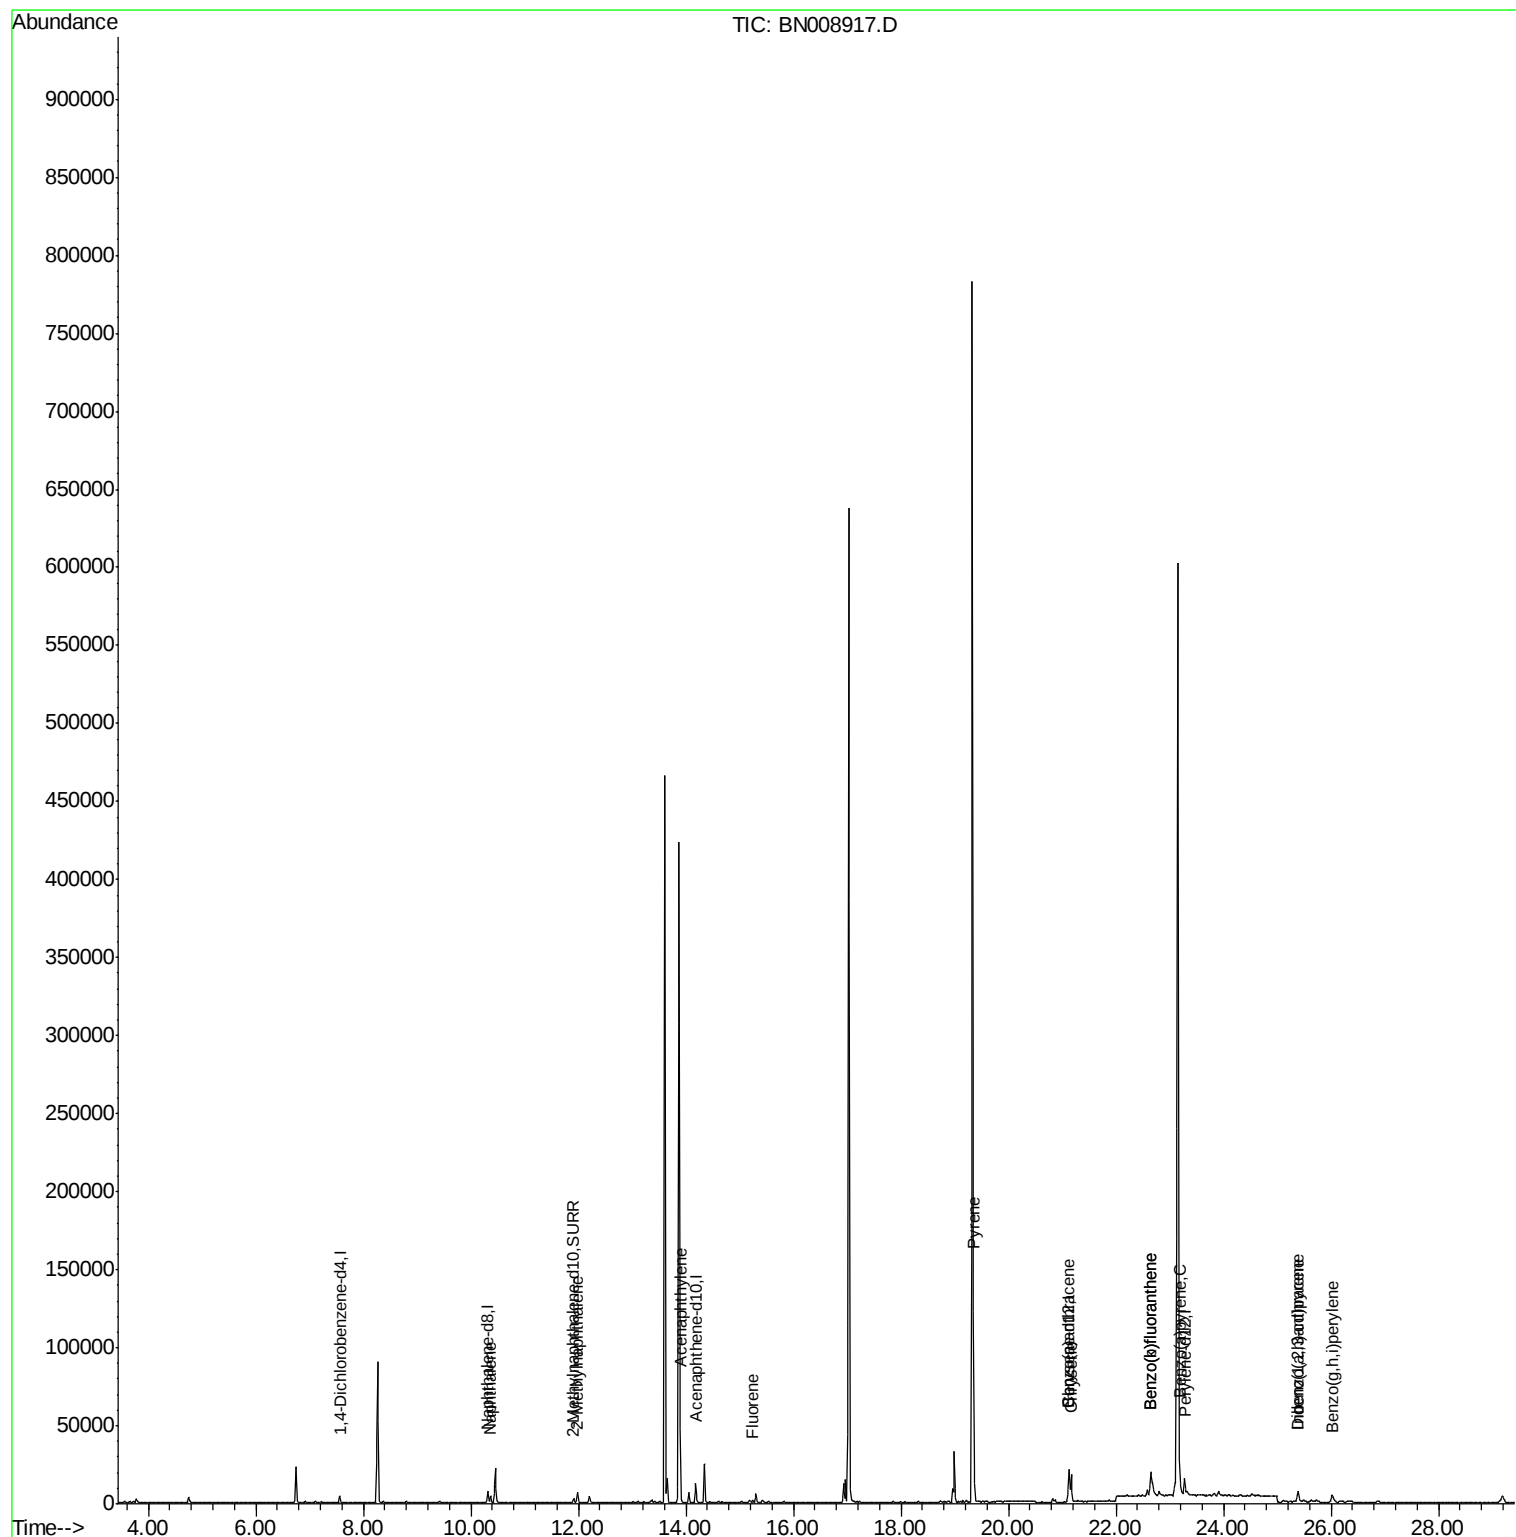



#3

Naphthalene

Concen: 0.188 ng/ul

RT: 10.36 min Scan# 2316

Delta R.T. -0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11

Instrument :

BNA\_N

ClientSampleId :


Tot Ion:128 Resp: 5242

Ion Ratio Lower Upper

128 100

129 12.7 9.1 13.7




127 14.5 10.7 16.1



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

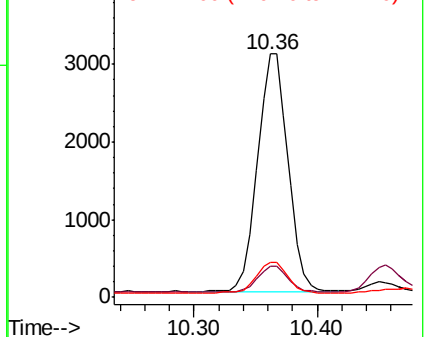

#5

2-Methylnaphthalene

Concen: 0.242 ng/ul

RT: 11.98 min Scan# 2611

Delta R.T. -0.00 min

Lab File: BN008917.D


Acq: 11 Dec 2019 15:11

Tgt Ion:142 Resp: 4724

Ion Ratio Lower Upper



142 100


141 88.1 70.1 105.1



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

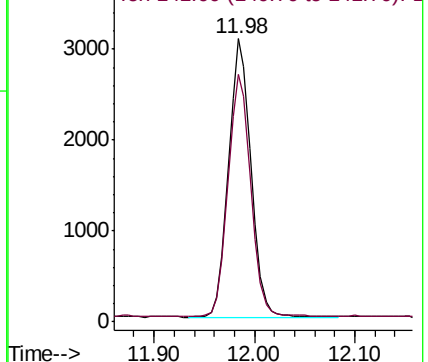



#7

Acenaphthylene

Concen: 0.067 ng/ul

RT: 13.90 min Scan# 2977

Delta R.T. 0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11

Instrument :

BNA\_N

ClientSampled :


Tot Ion:152 Resp: 2247

Ion Ratio Lower Upper




152 100

151 23.4 15.8 23.6

153 18.3 10.6 15.8#



Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 151.00 (150.70 to 151.70): E  
Ion 153.00 (152.70 to 153.70): E

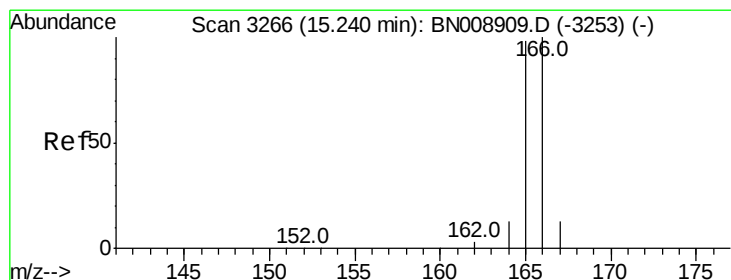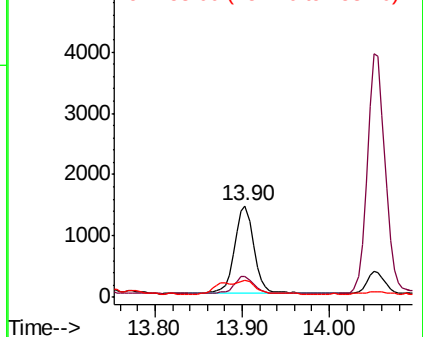

#9

Fluorene

Concen: 0.024 ng/ul

RT: 15.24 min Scan# 3266

Delta R.T. 0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11


Tgt Ion:166 Resp: 703

Ion Ratio Lower Upper



166 100


165 105.7 77.7 116.5

167 40.0 11.1 16.7#



Abundance Ion 166.00 (165.70 to 166.70): E  
Ion 165.00 (164.70 to 165.70): E  
Ion 167.00 (166.70 to 167.70): E




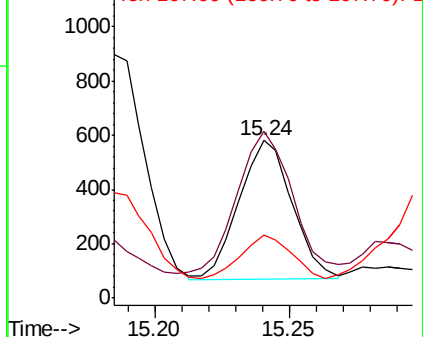


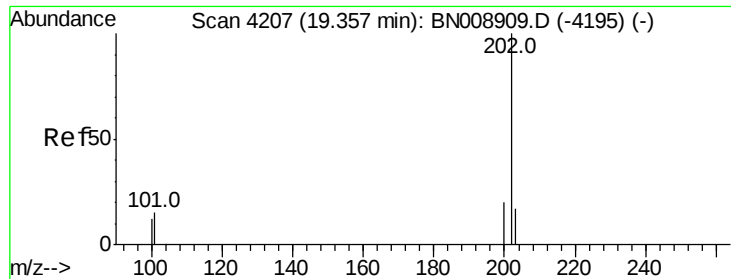

#17  
Pvrene  
Concen: 0.504 ng/ul  
RT: 19.36 min Scan# 4207  
Delta R.T. 0.00 min  
Lab File: BN008917.D  
Acq: 11 Dec 2019 15:11




Instrument :  
BNA\_N  
ClientSampleId :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 15.5  | 12.2  | 18.4  |
| 100     | 12.9  | 9.5   | 14.3  |

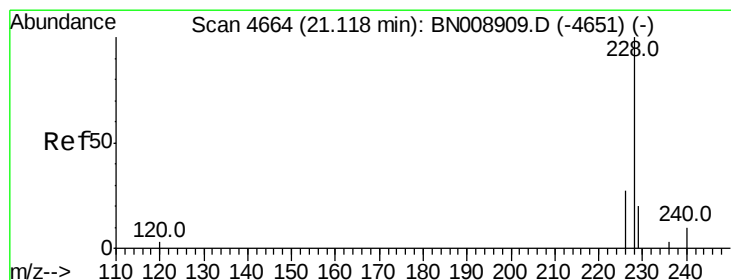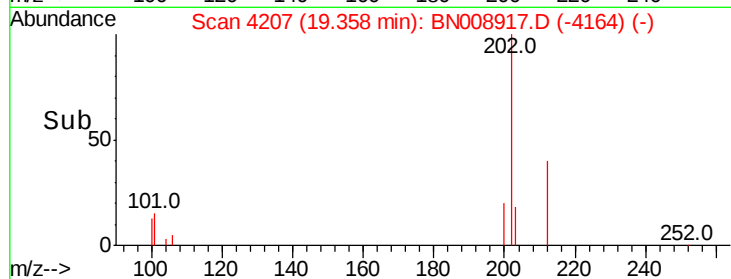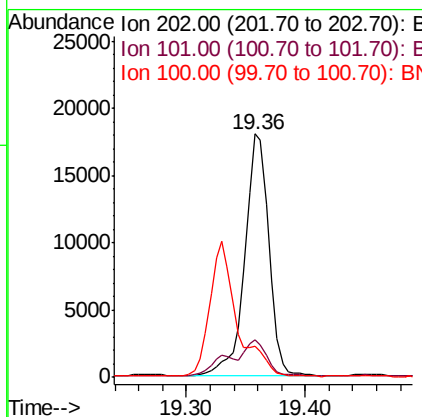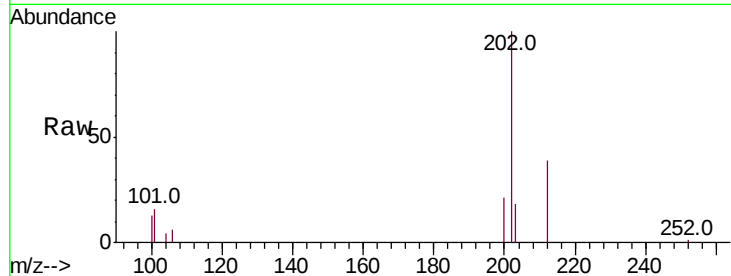

#18  
Benzo(a)anthracene  
Concen: 0.299 ng/ul  
RT: 21.12 min Scan# 4663  
Delta R.T. -0.00 min  
Lab File: BN008917.D  
Acq: 11 Dec 2019 15:11

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 228     | 100   |       |       |
| 229     | 21.6  | 15.7  | 23.5  |
| 226     | 29.1  | 21.5  | 32.3  |

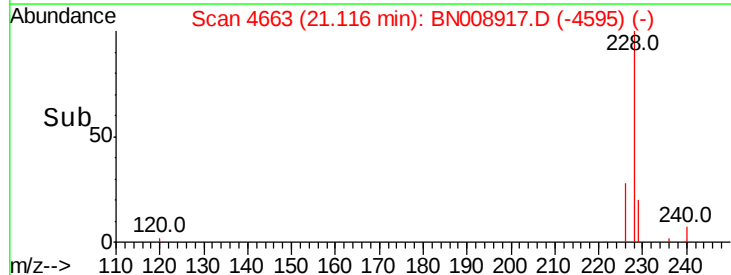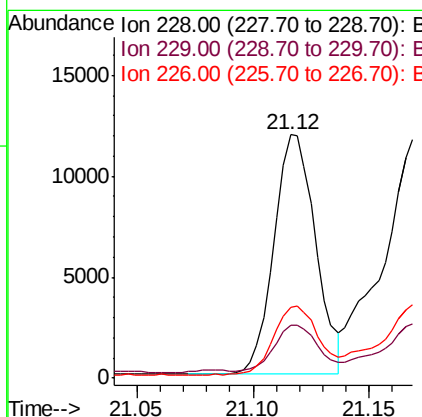

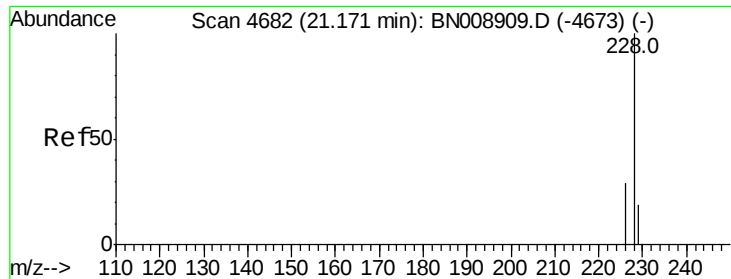

#19

Chrysene

Concen: 0.368 ng/ul

RT: 21.17 min Scan# 4681

Delta R.T. -0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11

Instrument :

BNA\_N

ClientSampleId :


Tot Ion:228 Resp: 17955

Ion Ratio Lower Upper

228 100

226 30.7 23.8 35.6




229 23.0 15.6 23.4

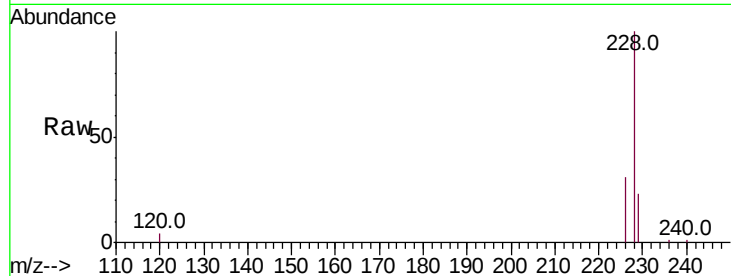

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

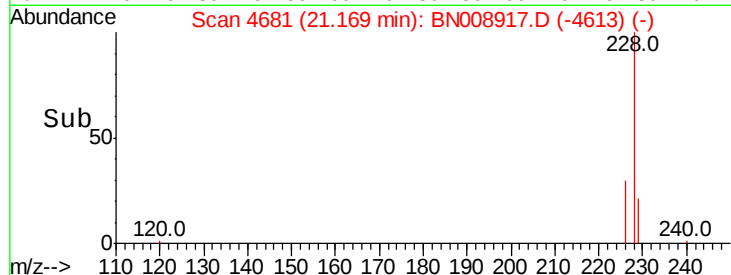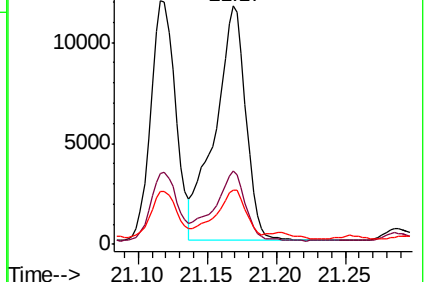

#21

Benzo(b)fluoranthene

Concen: 0.539 ng/ul

RT: 22.65 min Scan# 5187

Delta R.T. 0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11


Tgt Ion:252 Resp: 30835

Ion Ratio Lower Upper

252 100

253 26.2 0.0 48.6



125 19.5 0.0 31.6




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

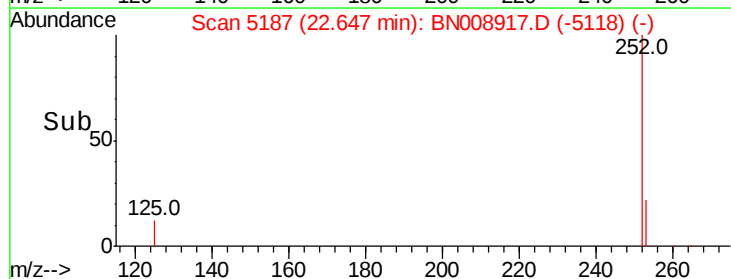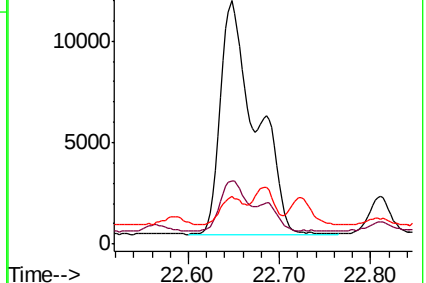

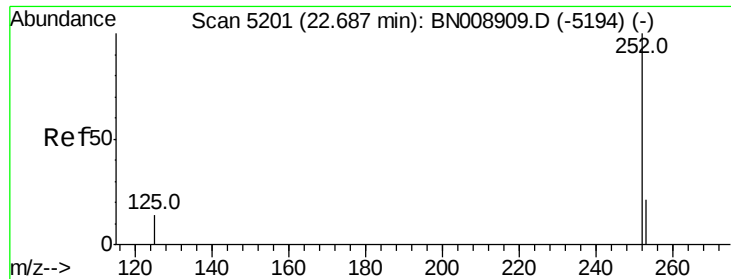

#22

Benzo(k)fluoranthene

Concen: 0.543 ng/ul

RT: 22.65 min Scan# 5187

Delta R.T. -0.04 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11

Instrument :

BNA\_N

ClientSampleId :


Tot Ion:252 Resp: 30835

Ion Ratio Lower Upper

252 100

253 26.2 19.6 29.4




125 19.5 13.8 20.6

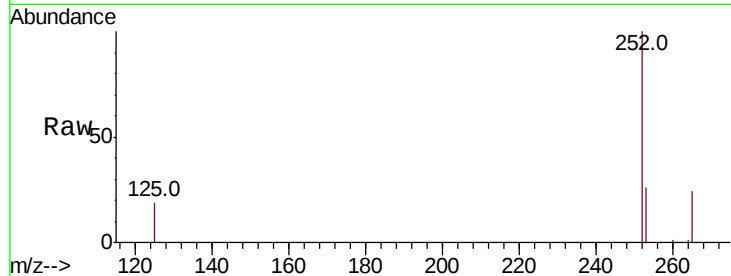

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

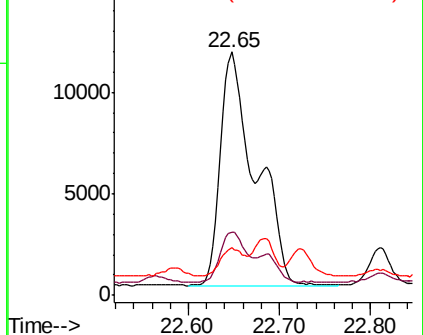

#23

Benzo(a)pyrene

Concen: 0.242 ng/ul

RT: 23.19 min Scan# 5372

Delta R.T. 0.00 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11


Tgt Ion:252 Resp: 13015

Ion Ratio Lower Upper

252 100

253 28.2 19.9 29.9



125 21.9 14.6 22.0




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

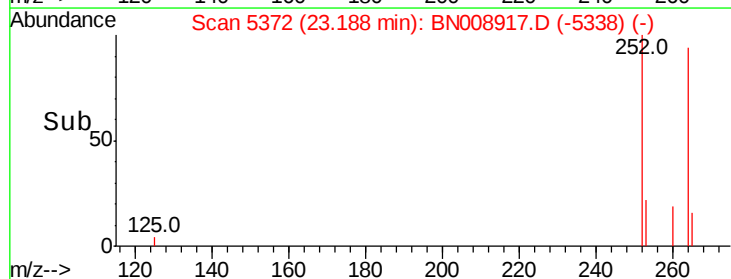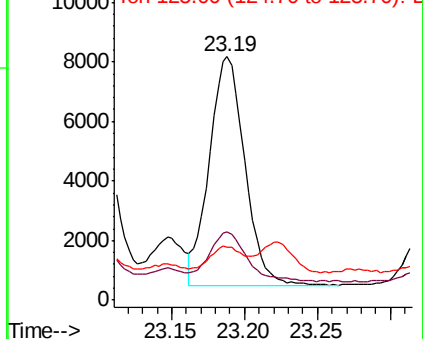

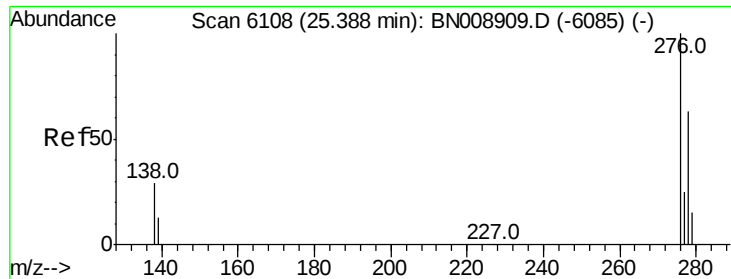


#24




Indeno(1,2,3-cd)pyrene  
Concen: 0.151 ng/ul  
RT: 25.39 min Scan# 6107  
Delta R.T. -0.00 min  
Lab File: BN008917.D  
Acq: 11 Dec 2019 15:11

Instrument :  
BNA\_N  
ClientSampleId :

Tot Ion:276 Resp: 9465  
Ion Ratio Lower Upper  
276 100  
138 26.3 23.8 35.6  
227 0.1 0.2 0.2#




Abundance Ion 276.00 (275.70 to 276.70): E  
Ion 138.00 (137.70 to 138.70): E  
Ion 227.00 (226.70 to 227.70): E

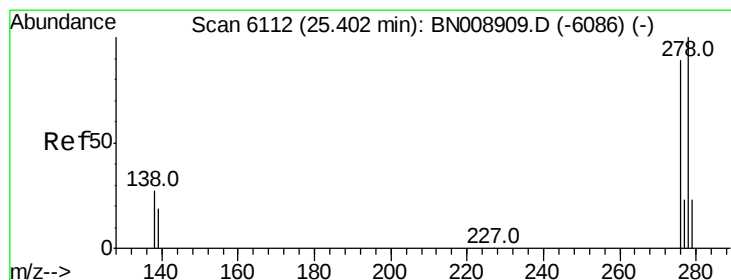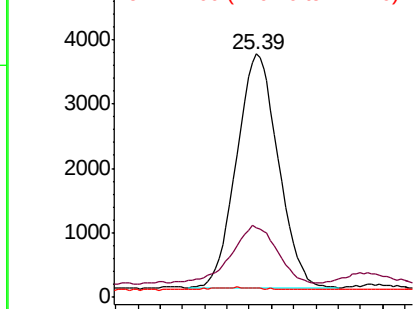



#25


Dibenzo(a,h)anthracene  
Concen: 0.057 ng/ul  
RT: 25.40 min Scan# 6110  
Delta R.T. -0.01 min  
Lab File: BN008917.D  
Acq: 11 Dec 2019 15:11

Tgt Ion:278 Resp: 2911  
Ion Ratio Lower Upper  
278 100  
139 38.3 17.4 26.0#  
279 44.3 20.5 30.7#



Abundance Ion 278.00 (277.70 to 278.70): E  
Ion 139.00 (138.70 to 139.70): E  
Ion 279.00 (278.70 to 279.70): E

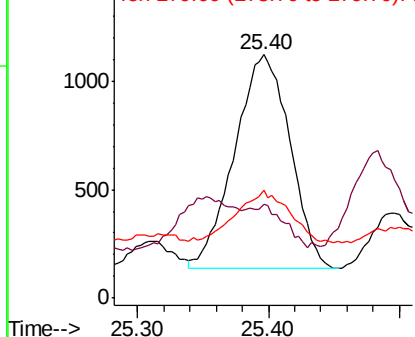



#26

Benzo(a,h,i)perylene

Concen: 0.164 ng/ul

RT: 26.02 min Scan# 6297

Delta R.T. -0.01 min

Lab File: BN008917.D

Acq: 11 Dec 2019 15:11

Instrument :

BNA\_N

ClientSampleId :


Tot Ion:276 Resp: 8607

Ion Ratio Lower Upper

276 100

138 29.4 21.9 32.9

277 26.0 19.9 29.9

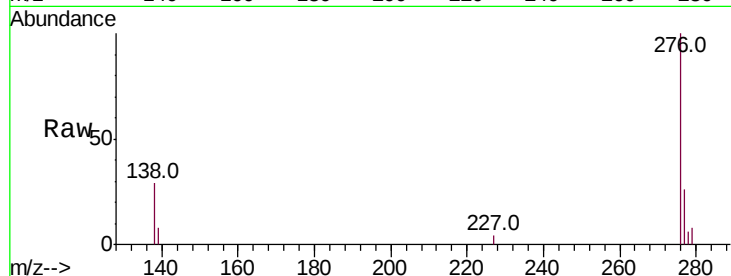

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

