

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008923.D
 Acq On : 11 Dec 2019 18:46
 Operator : JU
 Sample : K6088-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 12 00:22:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 10:35:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2425	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	10613	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6993	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.93
16) Chrysene-d12	21.13	240	14393	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	15771	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	4704	0.27	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	12901	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.33	202	1849	0.032	ng/ul#	1
23) Benzo(a)pyrene	23.15	252	3686	0.060	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008923.D
Acq On : 11 Dec 2019 18:46
Operator : JU
Sample : K6088-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 12 00:22:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 10:35:08 2019
Response via : Initial Calibration




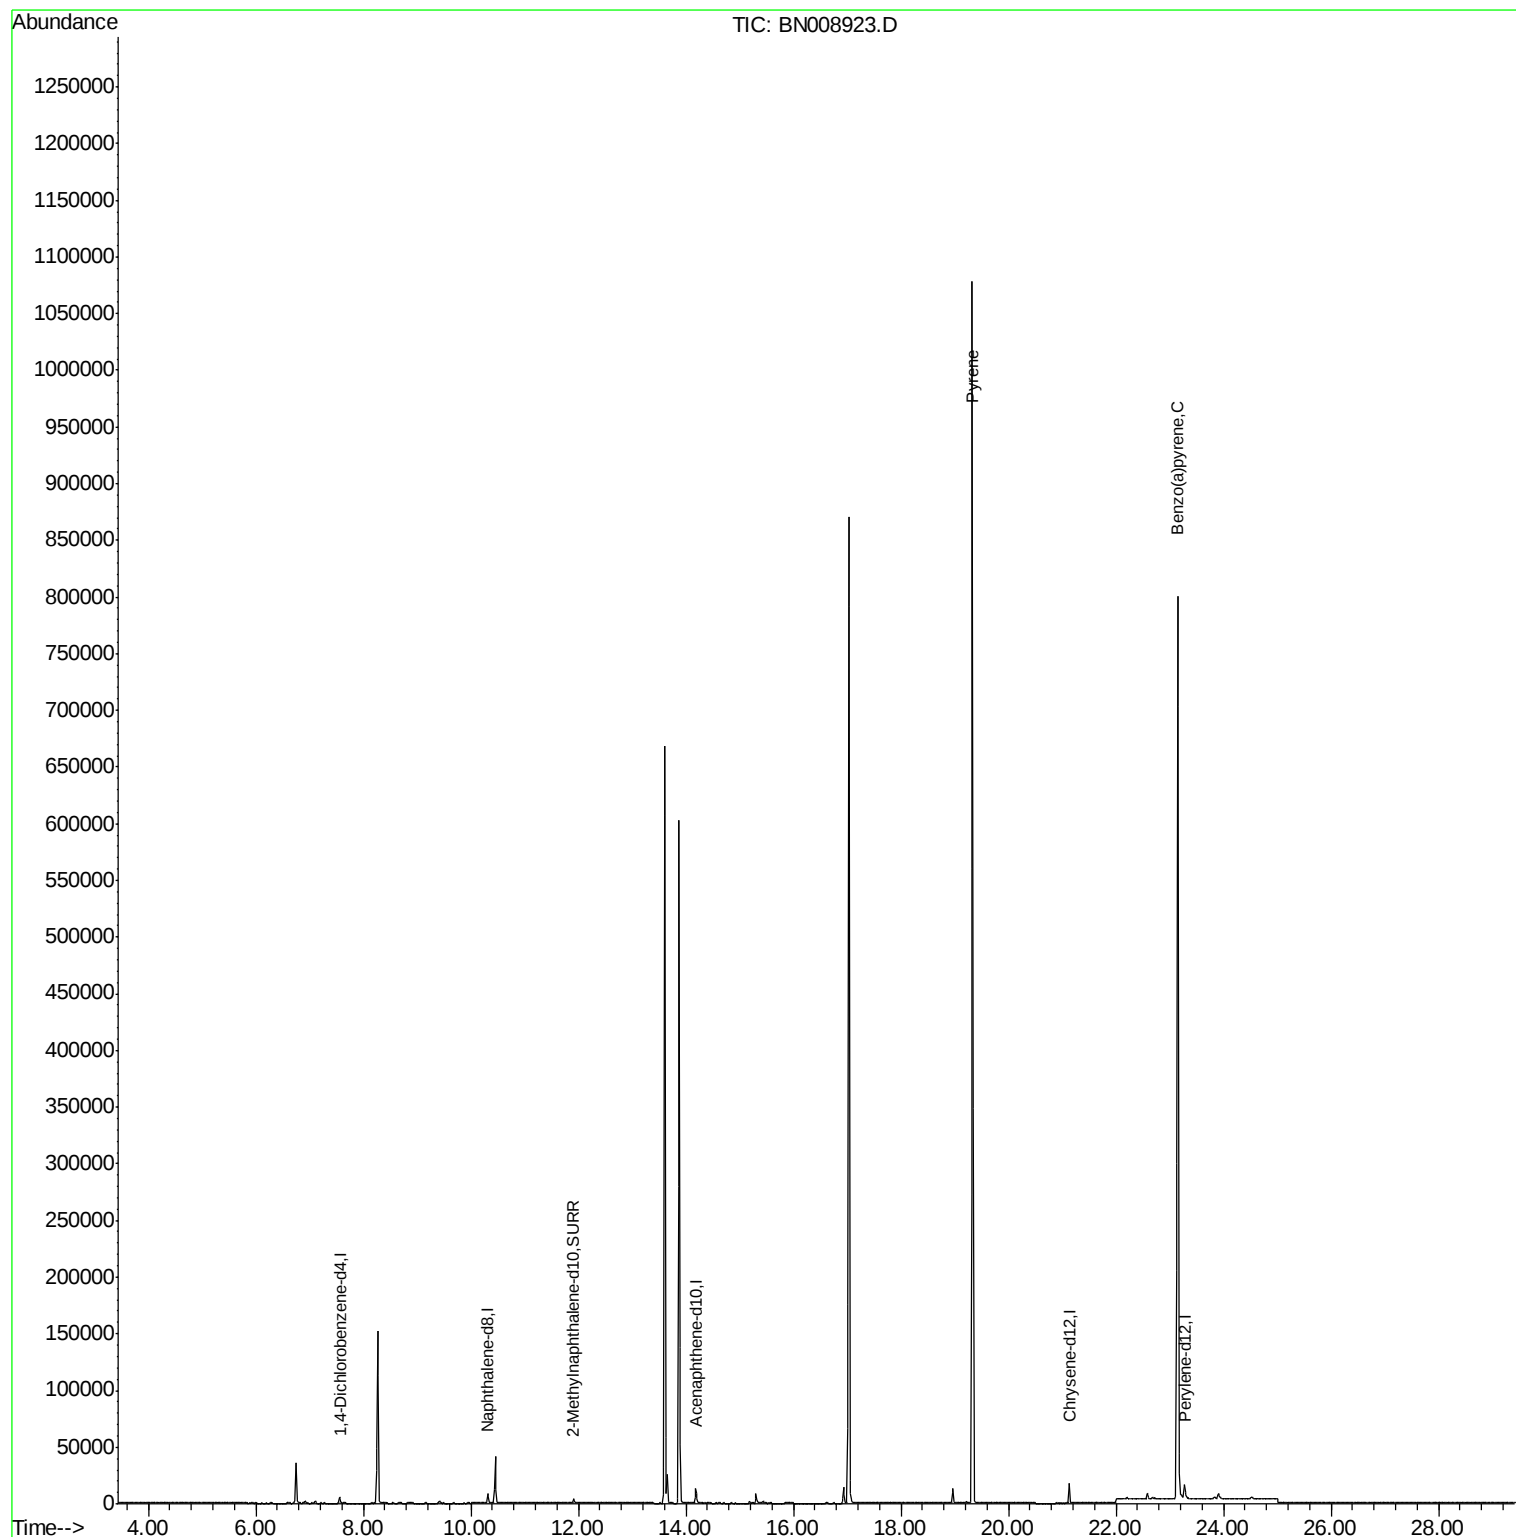


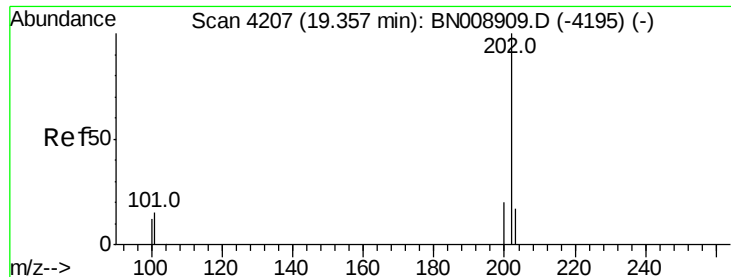

#17
Pvrene
Concen: 0.032 ng/ul
RT: 19.33 min Scan# 4201
Delta R.T. -0.03 min
Lab File: BN008923.D
Acq: 11 Dec 2019 18:46

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 1849
Ion Ratio Lower Upper
202 100
101 167.9 12.2 18.4#
100 1133.9 9.5 14.3#

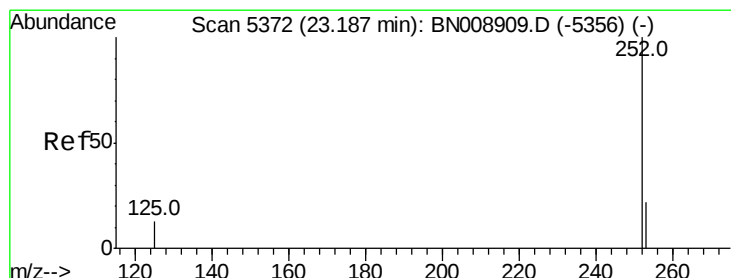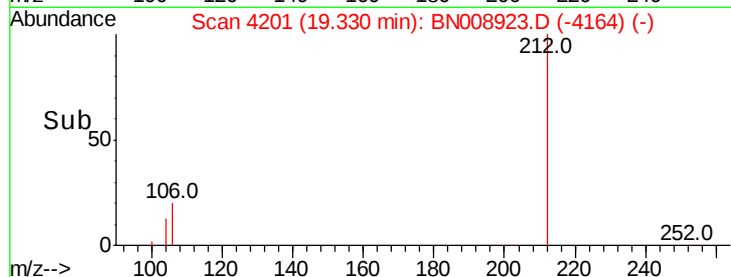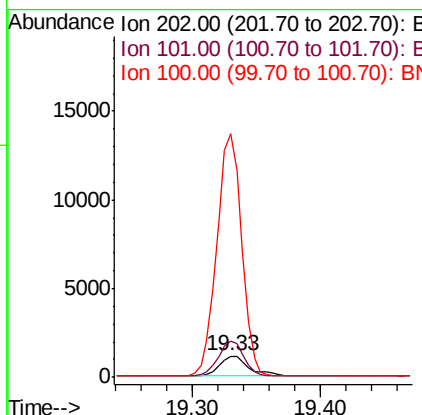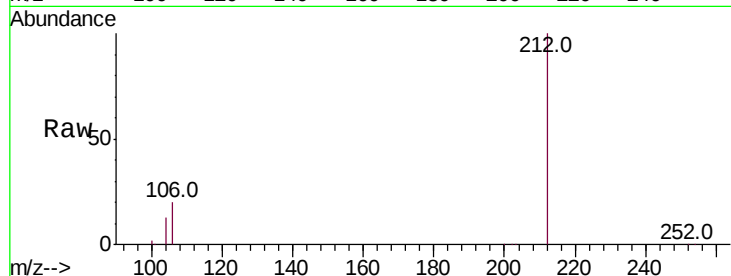

#23
Benzo(a)pyrene
Concen: 0.060 ng/ul
RT: 23.15 min Scan# 5358
Delta R.T. -0.04 min
Lab File: BN008923.D
Acq: 11 Dec 2019 18:46

Tgt Ion:252 Resp: 3686
Ion Ratio Lower Upper
252 100
253 43.0 19.9 29.9#
125 46.0 14.6 22.0#

