

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008935.D
 Acq On : 12 Dec 2019 01:54
 Operator : JU
 Sample : K6088-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 12 02:45:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 01:20:09 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2403	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	10502	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6763	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.93
16) Chrysene-d12	21.13	240	14233	0.40	ng/ul	0.00
20) Perylene-d12	23.27	264	14948	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	4085	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	11043	0.00	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	13.90	152	1121	0.030	ng/ul#	75
23) Benzo(a)pyrene	23.14	252	3599	0.062	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008935.D
Acq On : 12 Dec 2019 01:54
Operator : JU
Sample : K6088-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 12 02:45:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 01:20:09 2019
Response via : Initial Calibration

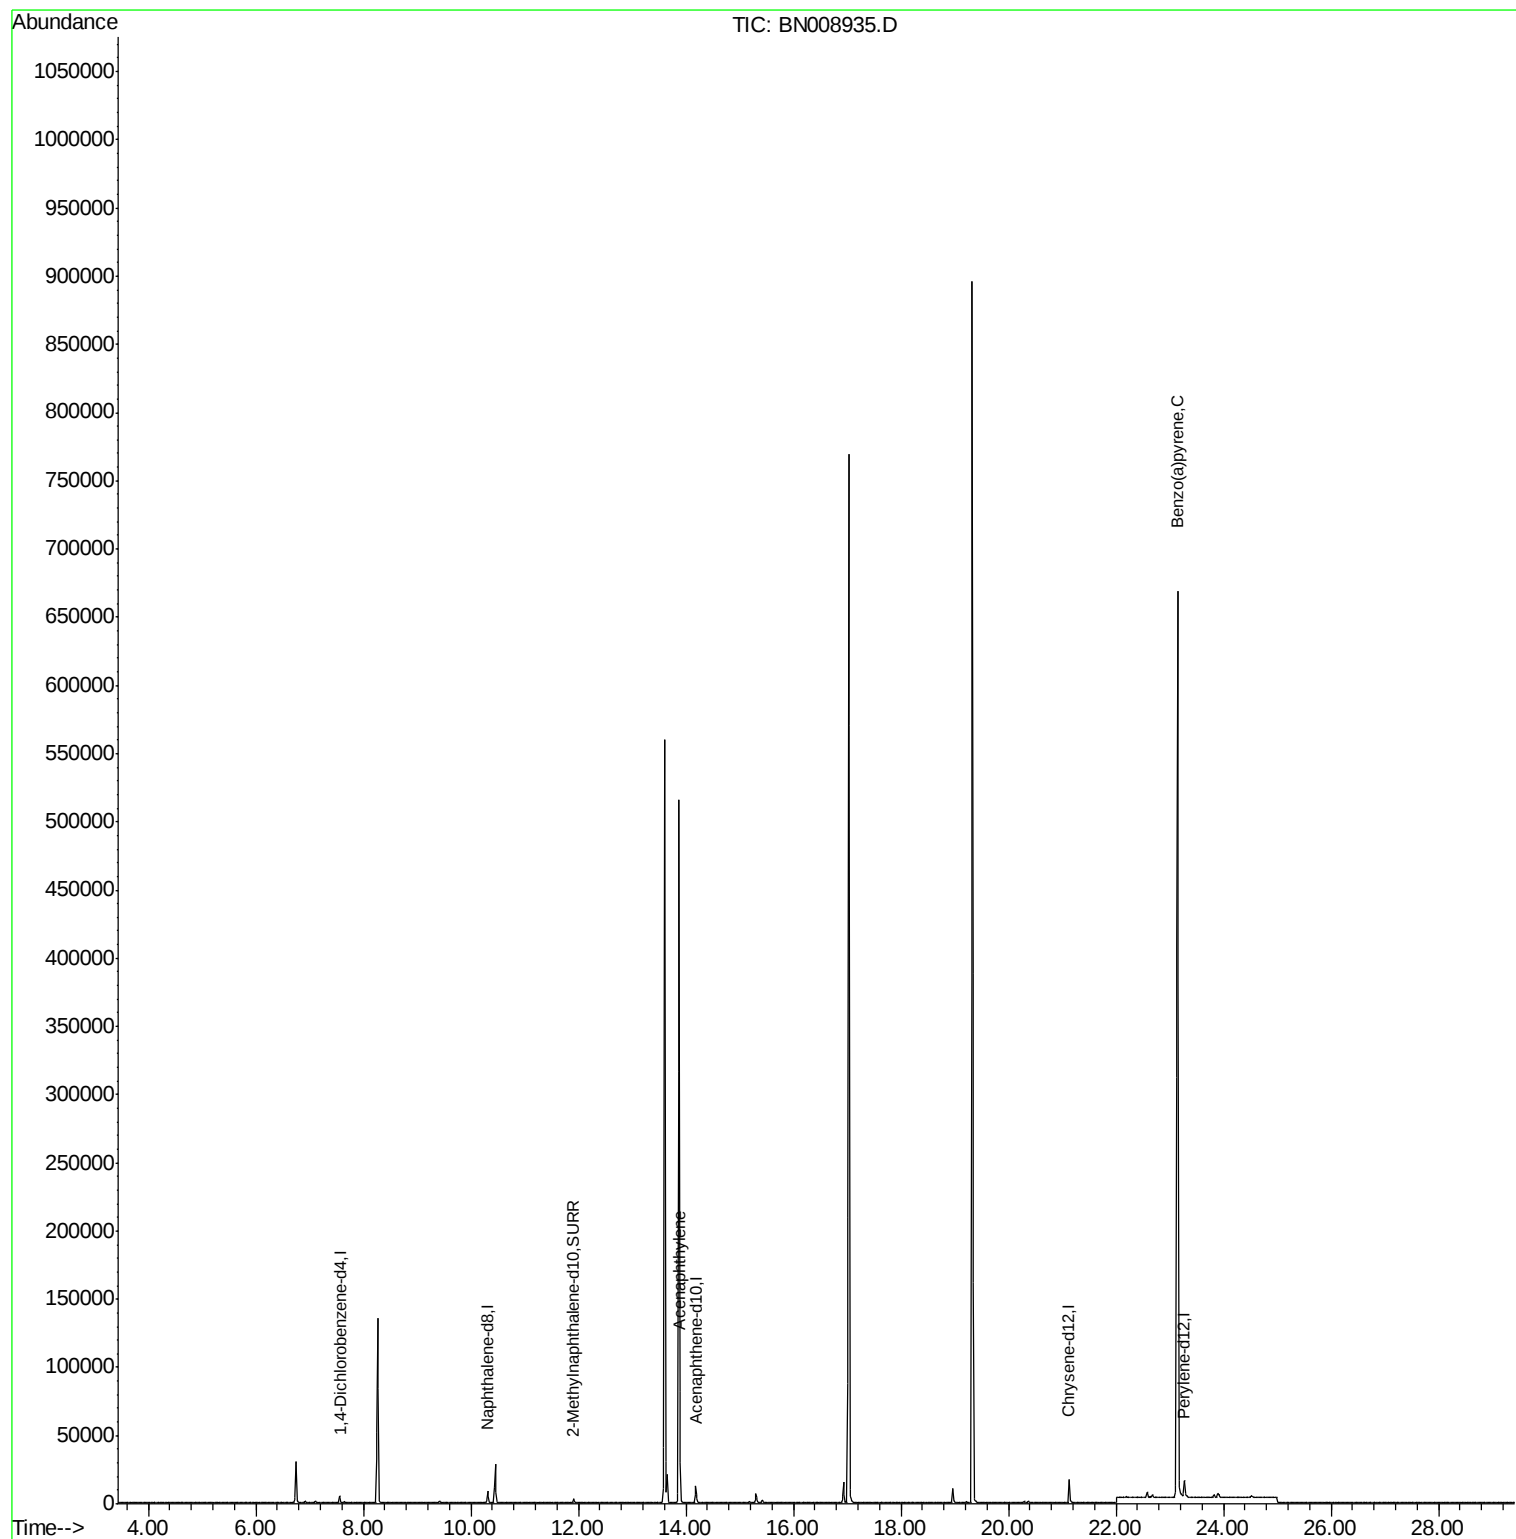

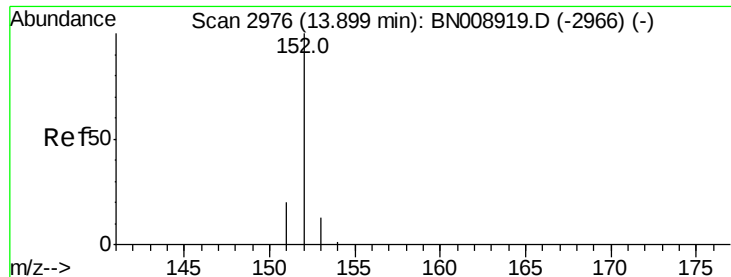

#7

Acenaphthylene

Concen: 0.030 ng/ul

RT: 13.90 min Scan# 2976

Delta R.T. -0.00 min

Lab File: BN008935.D

Acq: 12 Dec 2019 01:54

Instrument :

BNA_N

ClientSampleId :





Tot Ion:152 Resp: 1121

Ion Ratio Lower Upper

152 100

151 30.8 15.8 23.6#

153 24.1 10.6 15.8#

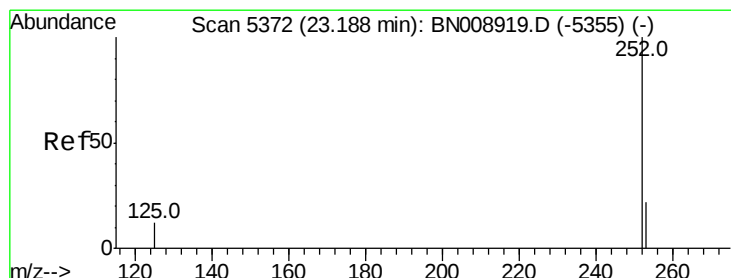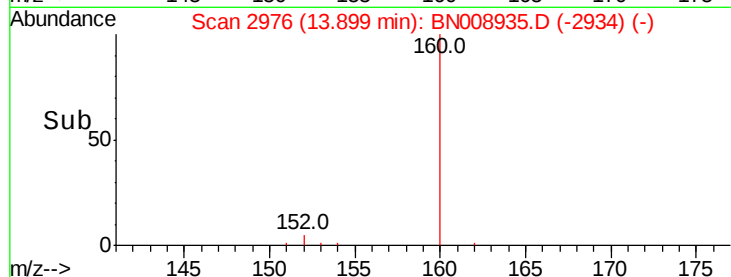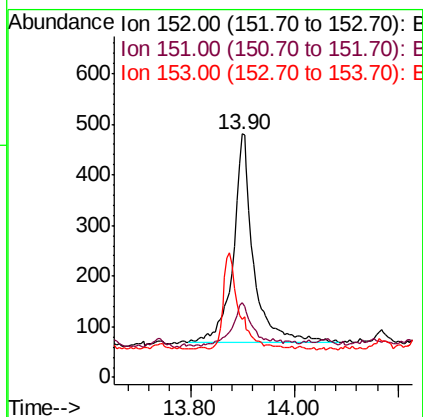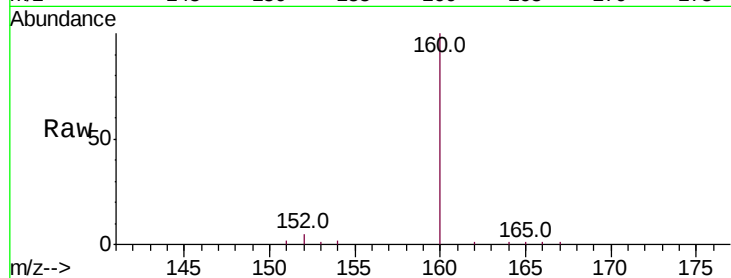

#23

Benzo(a)pyrene

Concen: 0.062 ng/ul

RT: 23.14 min Scan# 5355

Delta R.T. -0.05 min

Lab File: BN008935.D

Acq: 12 Dec 2019 01:54

Tgt Ion:252 Resp: 3599

Ion Ratio Lower Upper

252 100

253 45.4 19.9 29.9#

125 50.1 14.6 22.0#

