

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008913.D
Acq On : 11 Dec 2019 12:48
Operator : JU
Sample : PB125196BL


Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 11 14:31:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:10 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK96

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:57 AM

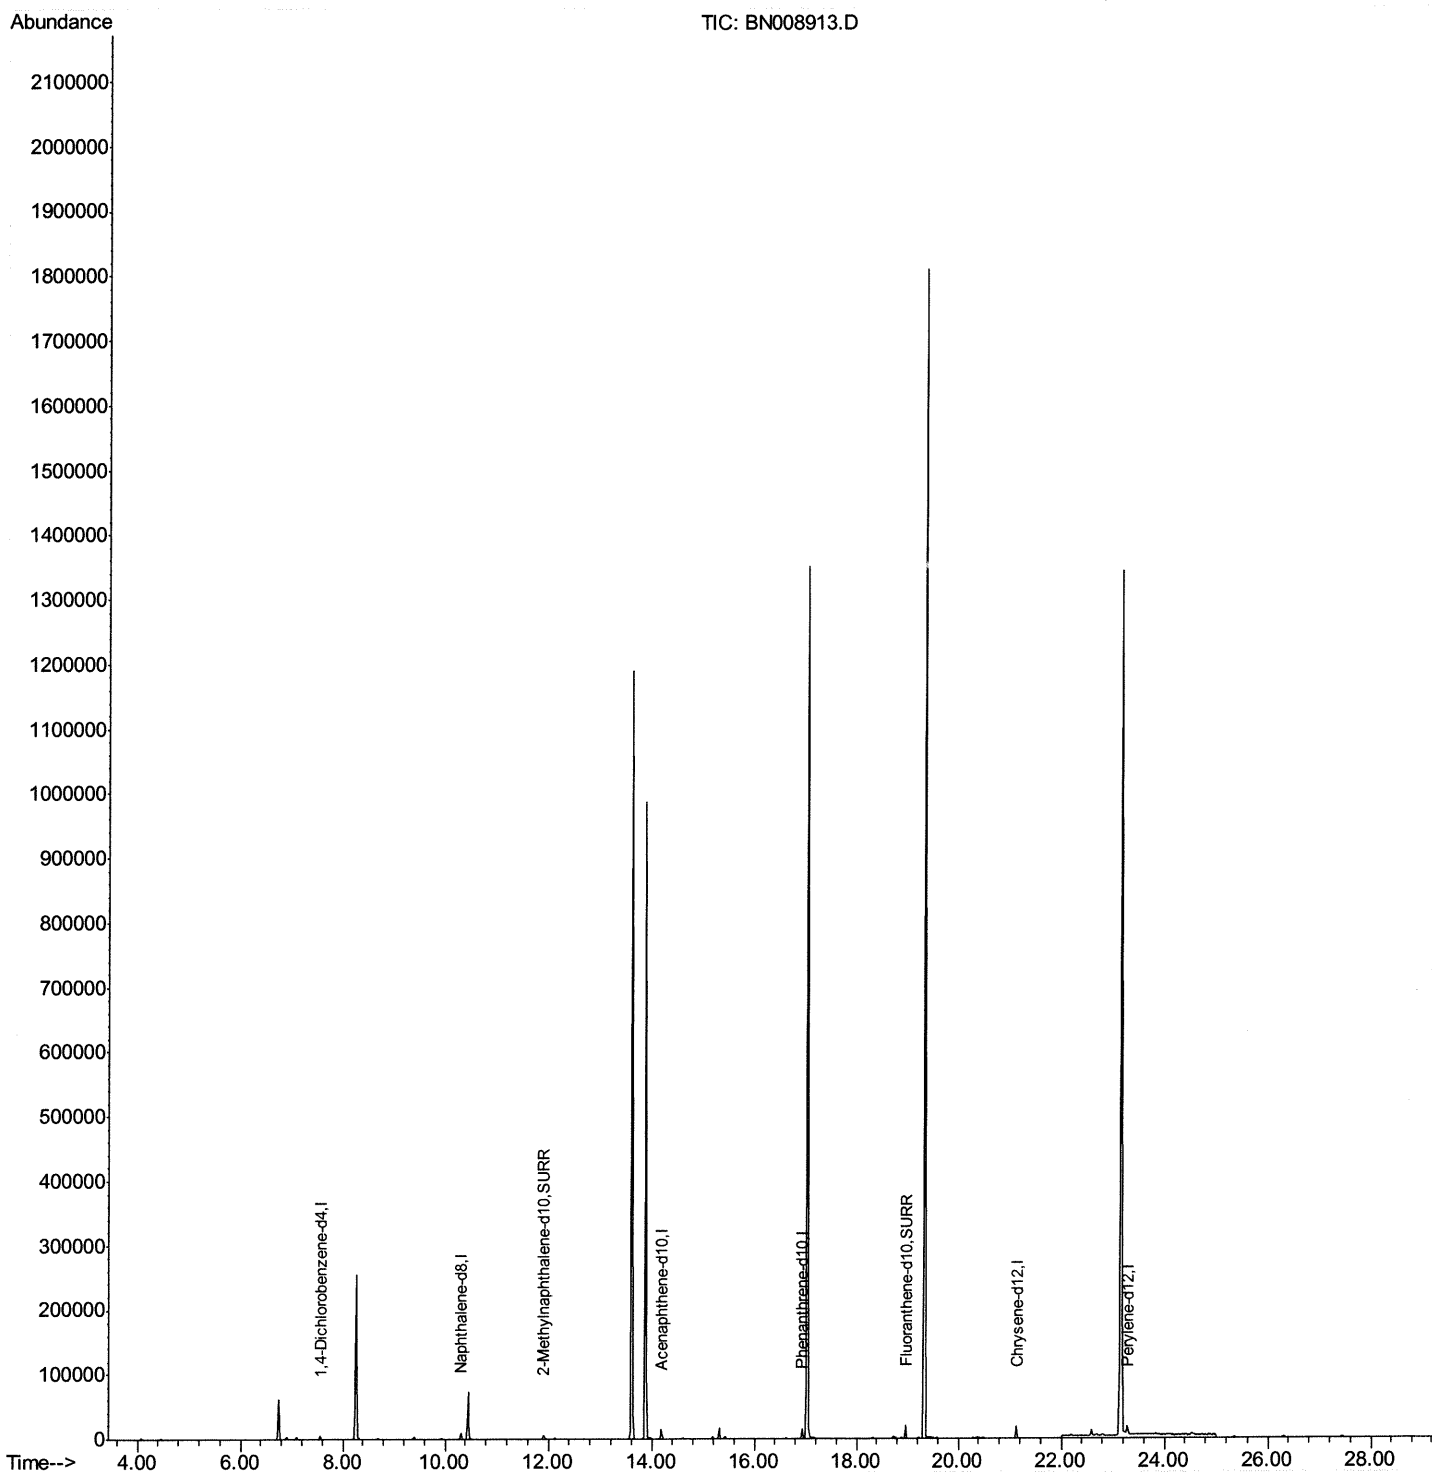

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008913.D
Acq On : 11 Dec 2019 12:48
Operator : JU
Sample : PB125196BL




Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 11 14:28:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 10:35:08 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK96

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:57 AM

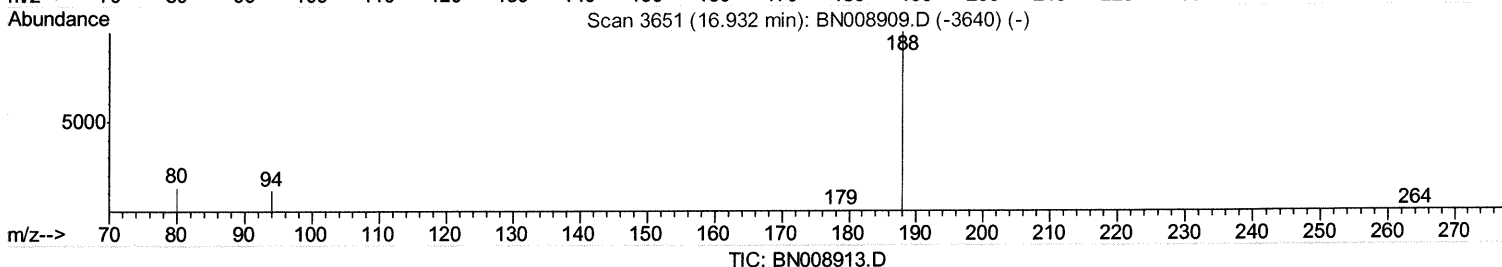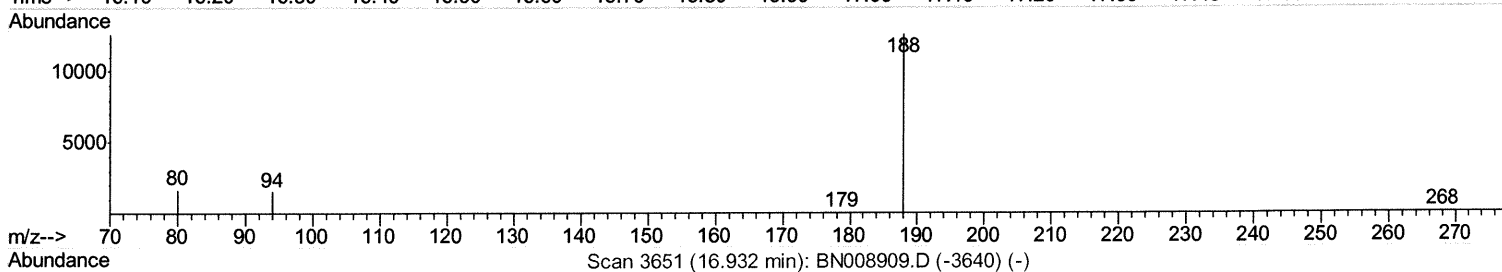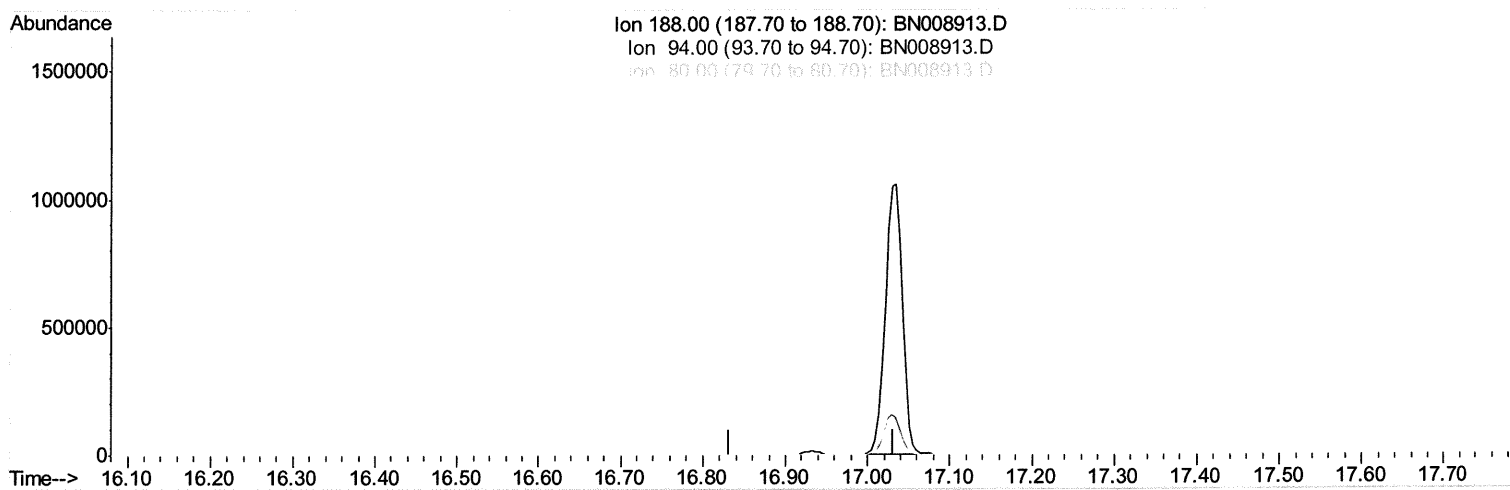

(10) Phenanthrene-d10 (I)

16.932min (-16.932) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008913.D
Acq On : 11 Dec 2019 12:48
Operator : JU
Sample : PB125196BL




Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 11 14:28:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 10:35:08 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK96

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:57 AM

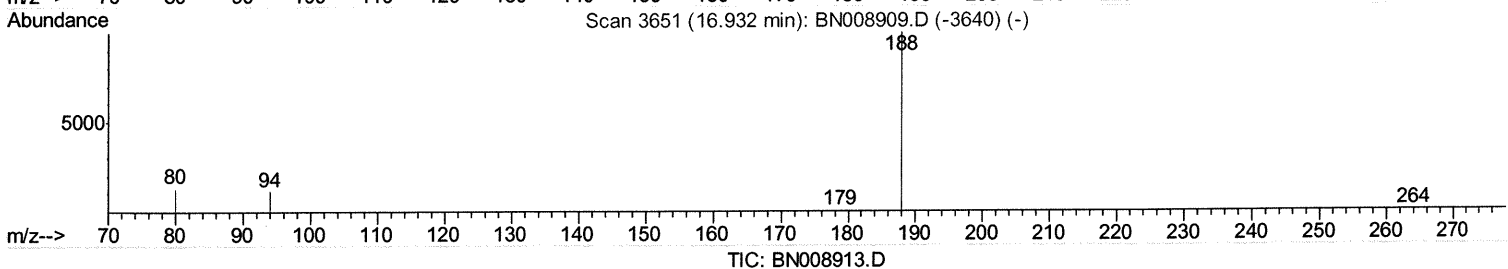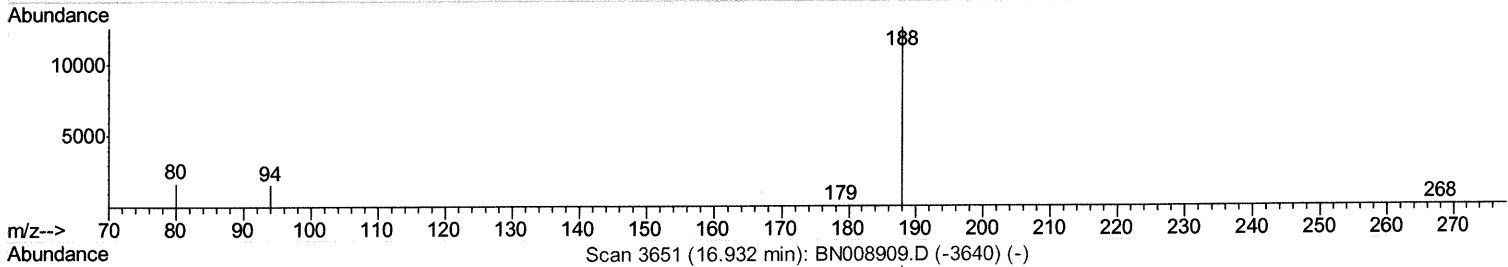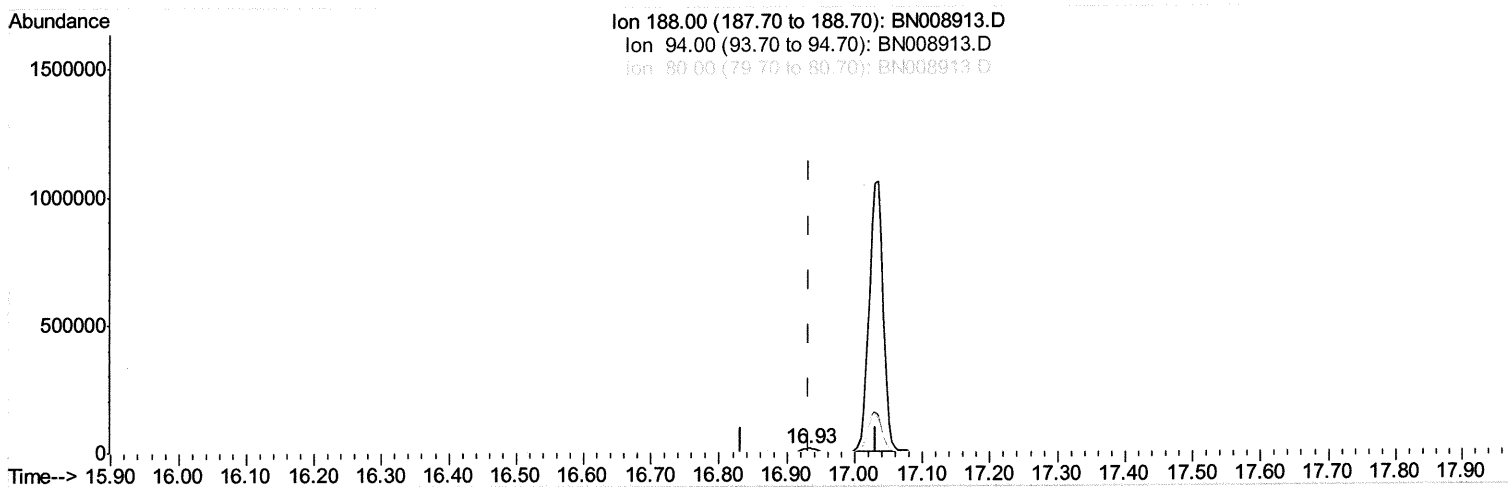

(10) Phenanthrene-d10 (I)

16.933min (+0.001) 0.40ng/ul m JU 12/12/19

response 17090

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.34
80.00	14.40	13.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008913.D
Acq On : 11 Dec 2019 12:48
Operator : JU
Sample : PB125196BL

Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 11 14:31:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:10 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SBLK96

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:57 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2624	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	11811	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	7633	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	17090m	> 0.40	ng/ul	> 0.00
16) Chrysene-d12	21.14	240	15865	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	16443	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.91	152	7740	0.40	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	21344	0.41	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2012/12/19