


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008914.D
Acq On : 11 Dec 2019 13:24
Operator : JU
Sample : K6088-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM7

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:51:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:54 2019
Response via : Initial Calibration

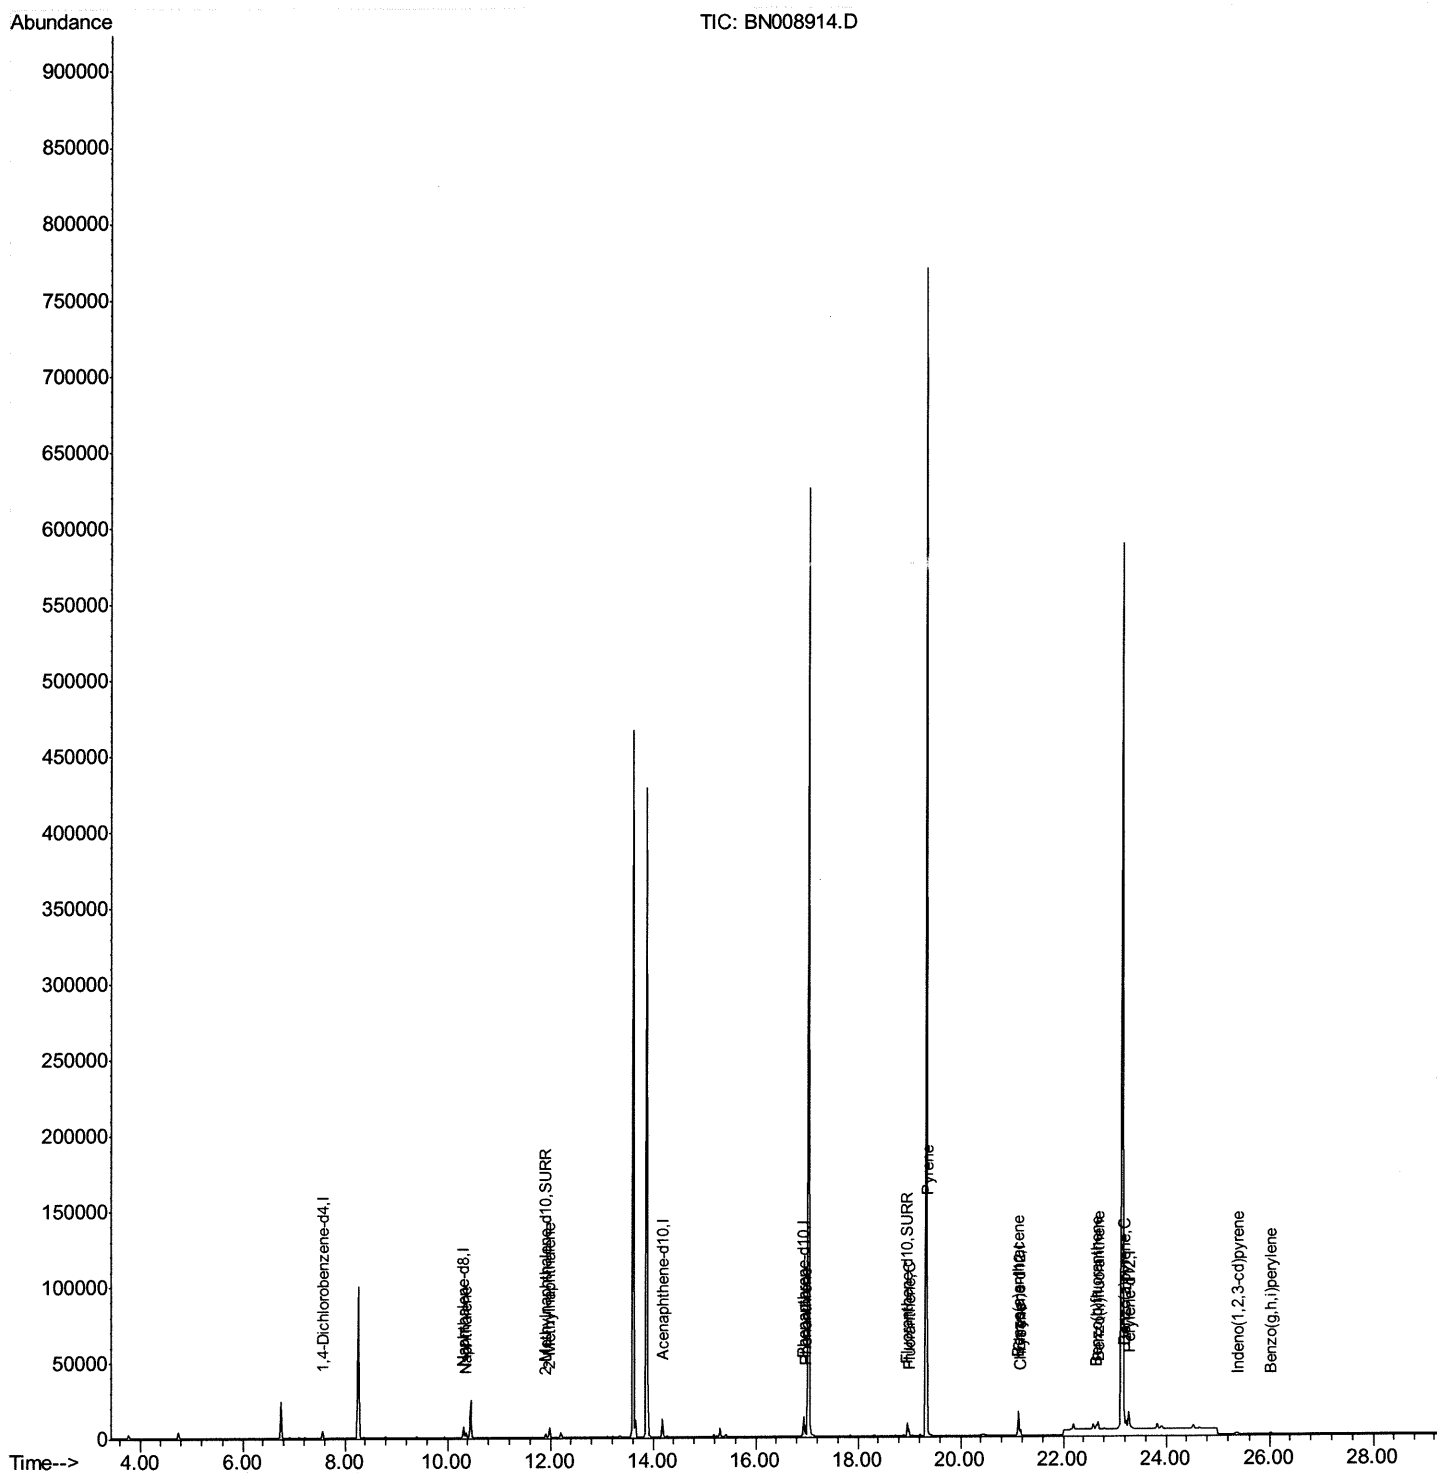

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008914.D
 Acq On : 11 Dec 2019 13:24
 Operator : JU
 Sample : K6088-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM7

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:32:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

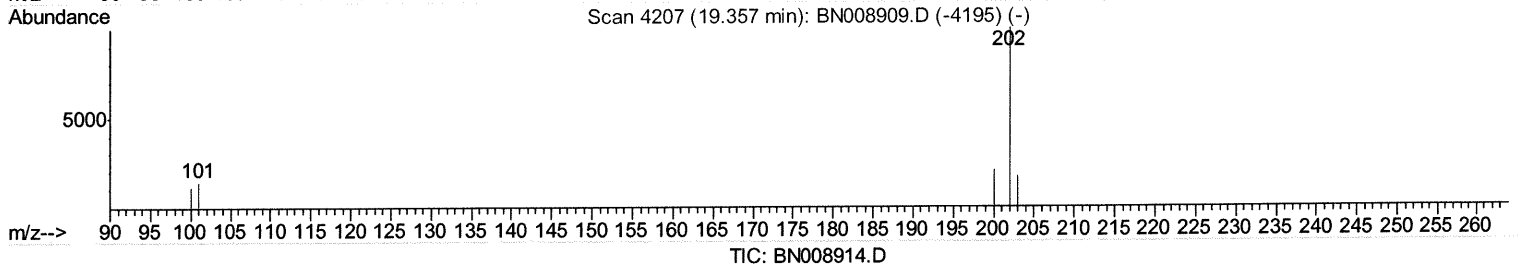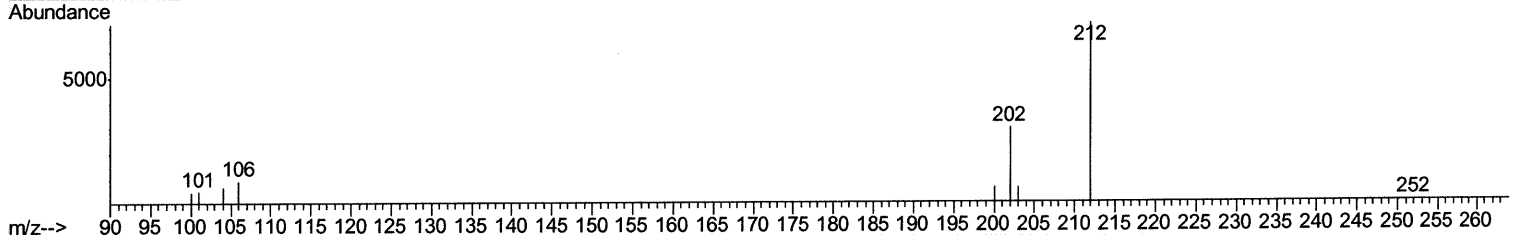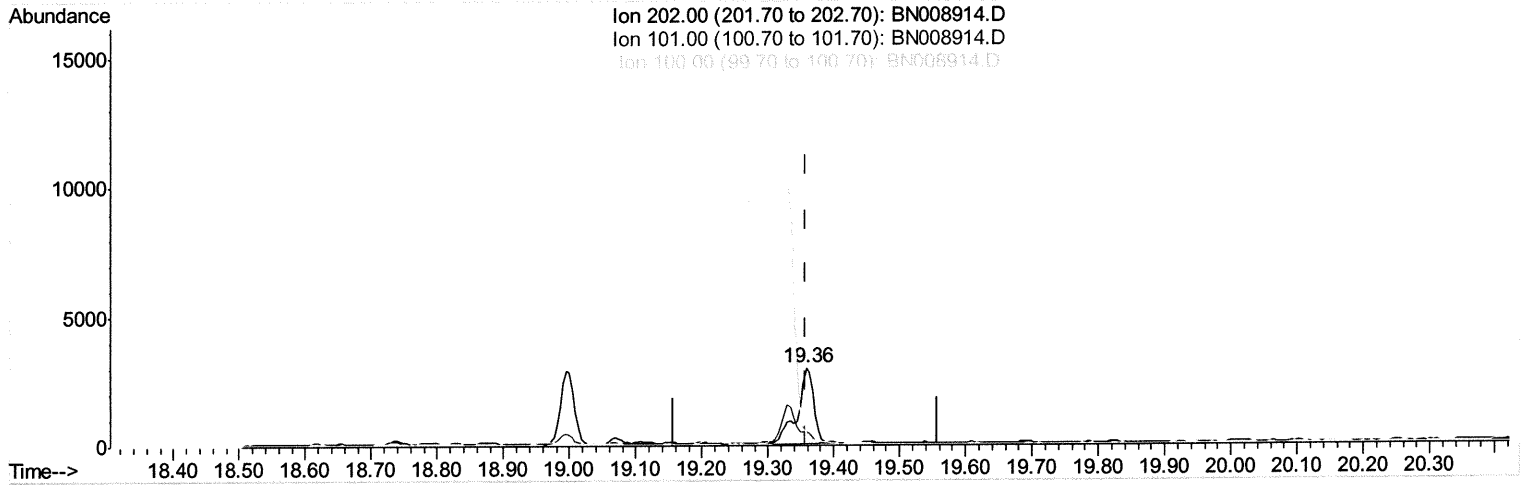

TIC: BN008914.D

(17) Pyrene

19.358min (+0.001) 0.10ng/ul

response 5043

Ion	Exp%	Act%
202.00	100	100
101.00	15.30	18.14
100.00	11.90	16.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008914.D
 Acq On : 11 Dec 2019 13:24
 Operator : JU
 Sample : K6088-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM7

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:32:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

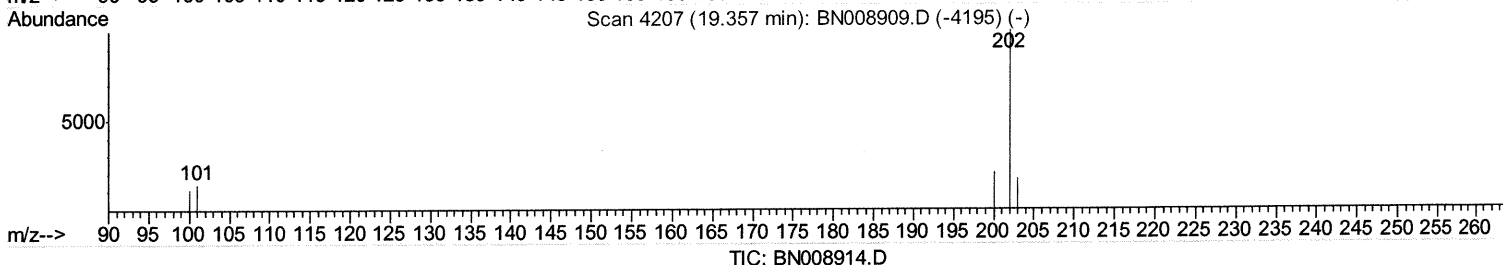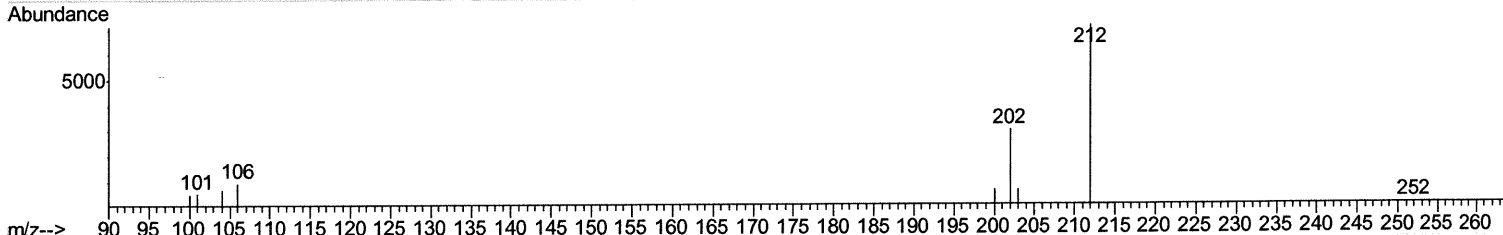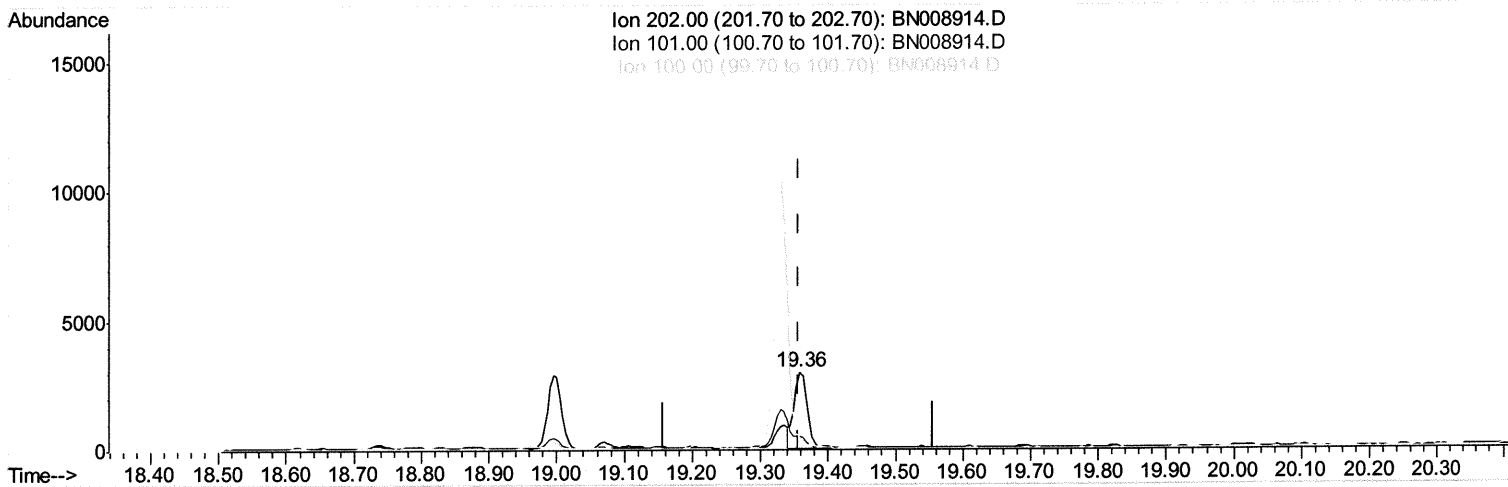

TIC: BN008914.D

(17) Pyrene

19.358min (+0.001) 0.08ng/ul m JU 12/12/19

response 4114

Ion	Exp%	Act%
202.00	100	100
101.00	15.30	18.14
100.00	11.90	16.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008914.D
Acq On : 11 Dec 2019 13:24
Operator : JU
Sample : K6088-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM7

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:32:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:54 2019
Response via : Initial Calibration

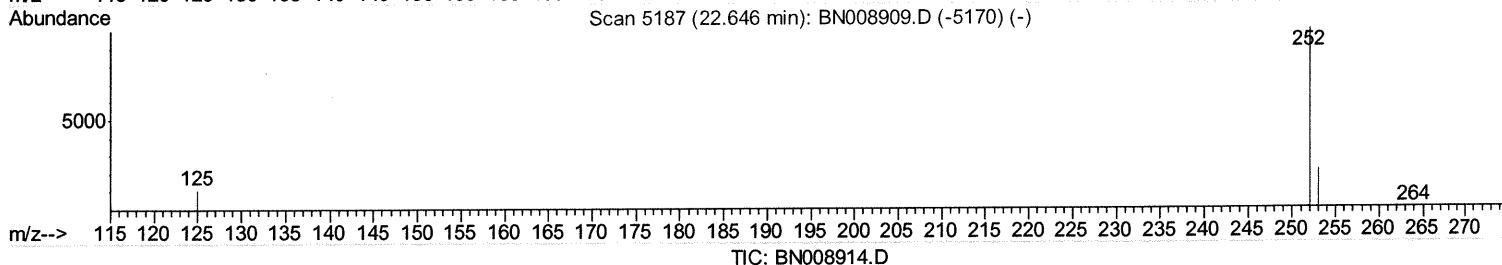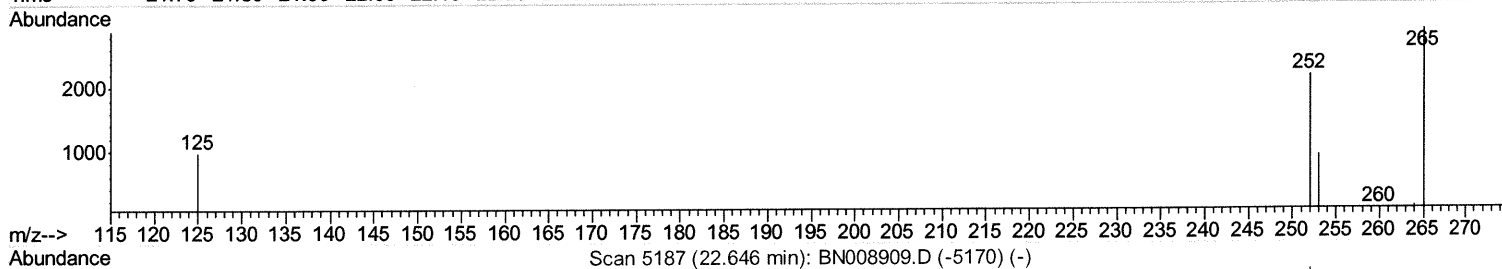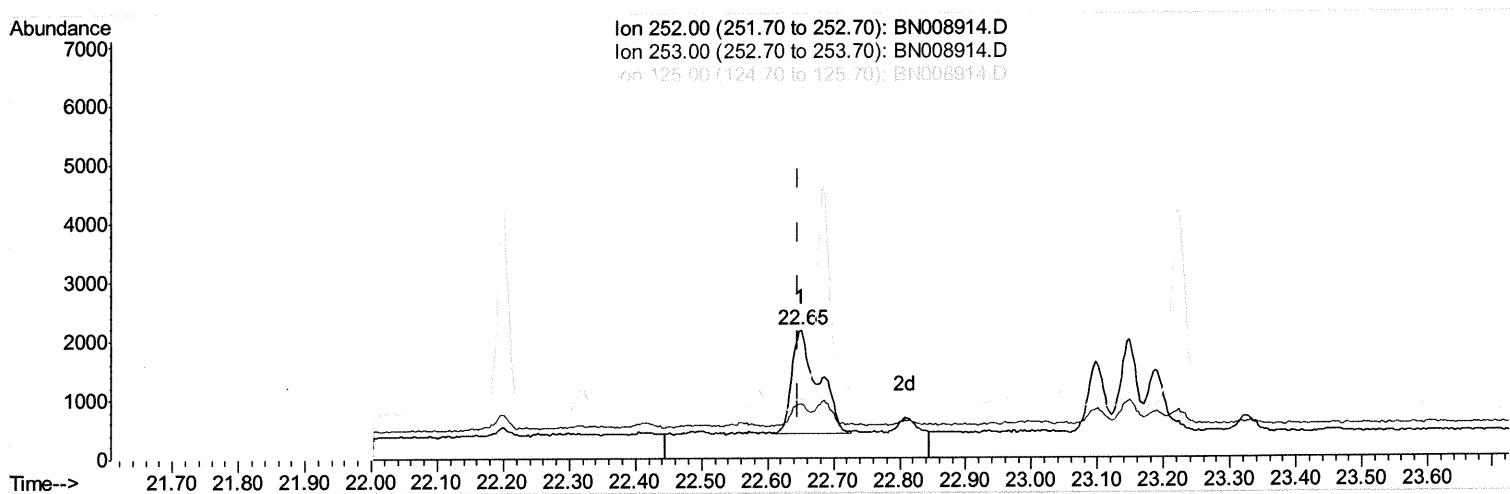

(21) Benzo(b)fluoranthene

22.650min (+0.004) 0.09ng/ul

response 4842

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	42.26
125.00	15.80	45.07#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008914.D
 Acq On : 11 Dec 2019 13:24
 Operator : JU
 Sample : K6088-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM7

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:32:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

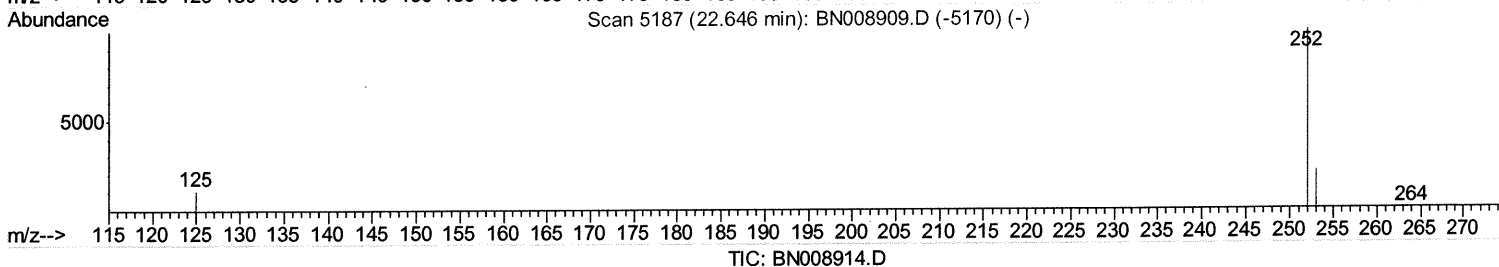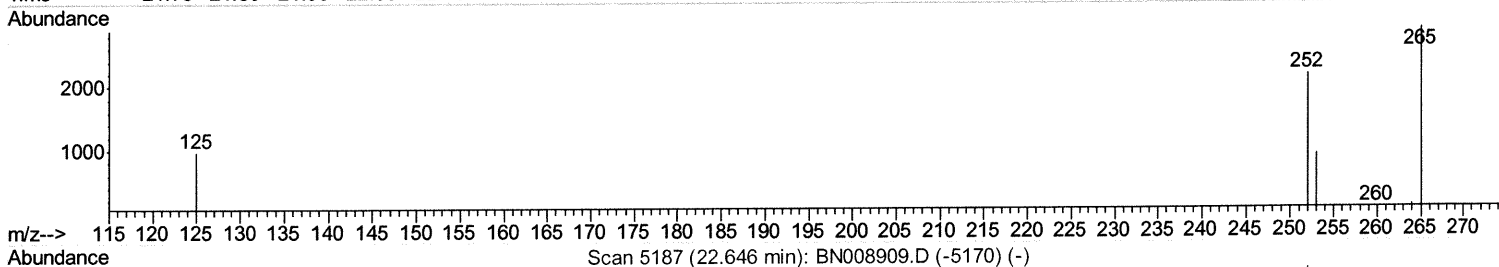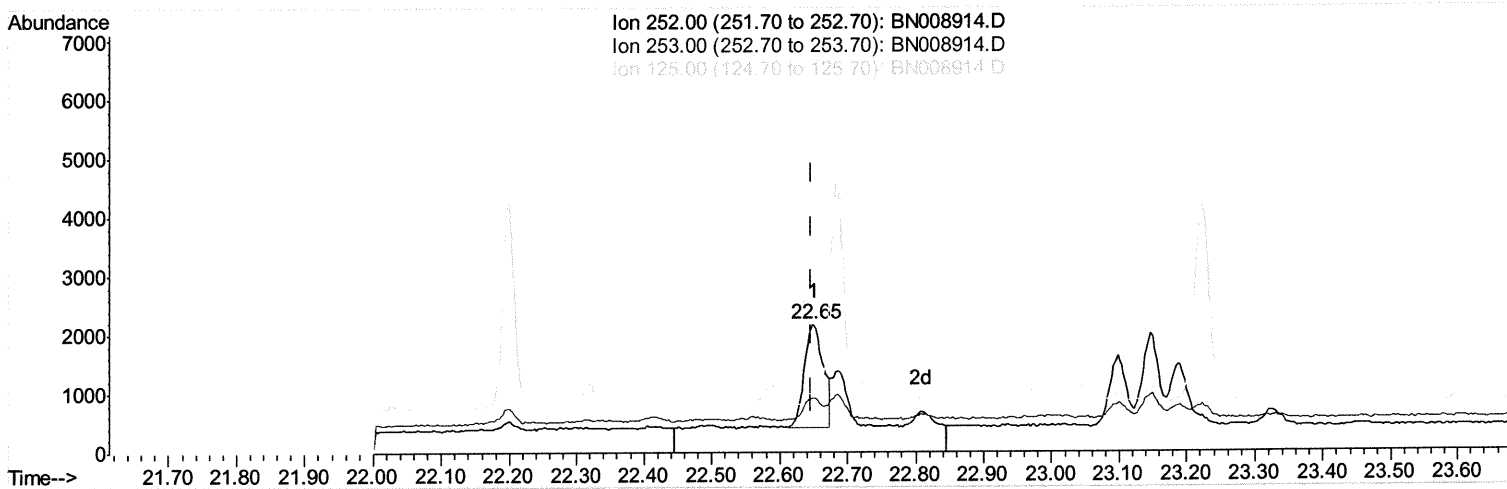

(21) Benzo(b)fluoranthene


22.650min (+0.004) 0.06ng/ul m 5412/12/19

response 3460


Ion	Exp%	Act%
252.00	100	100
253.00	24.30	42.26
125.00	15.80	45.07#
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\  
Data File  : BN008914.D  
Acq On     : 11 Dec 2019   13:24  
Operator   : JU  
Sample     : K6088-01  
Misc      :  
ALS Vial   : 7      Sample Multiplier: 1
```

mohammad
12/12/2019 11:26:52 AM

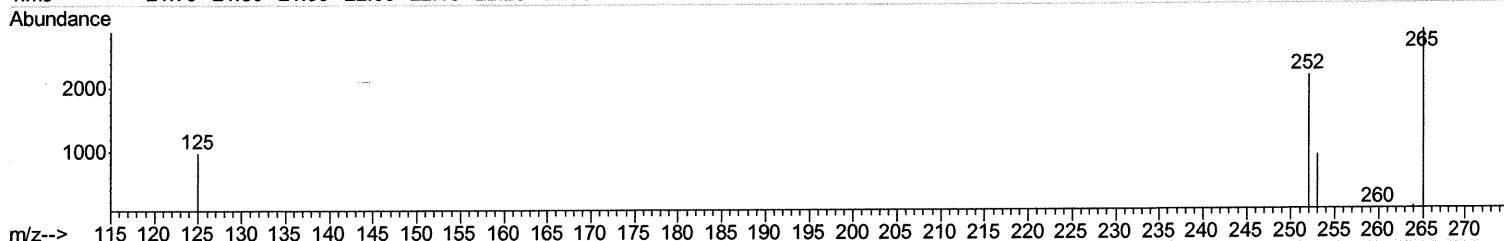

Scan 5201 (22.687 min): BN008909.D (-5194) (-)

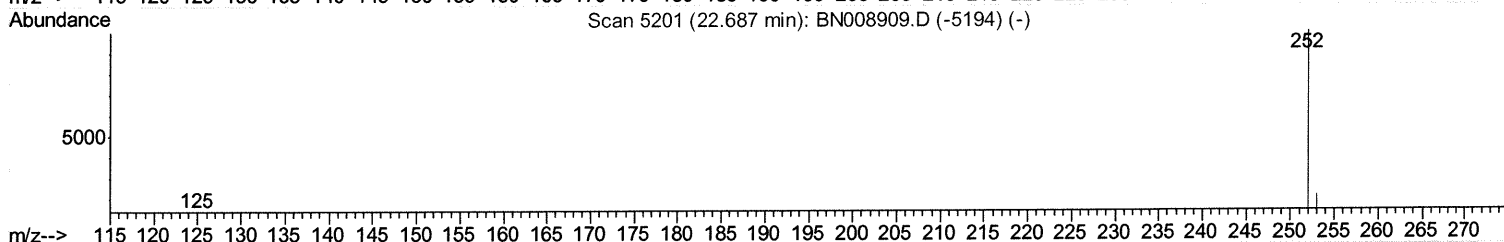

TIC: BN008914.D

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	42.26#
125.00	17.20	45.07#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008914.D
 Acq On : 11 Dec 2019 13:24
 Operator : JU
 Sample : K6088-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM7

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:32:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

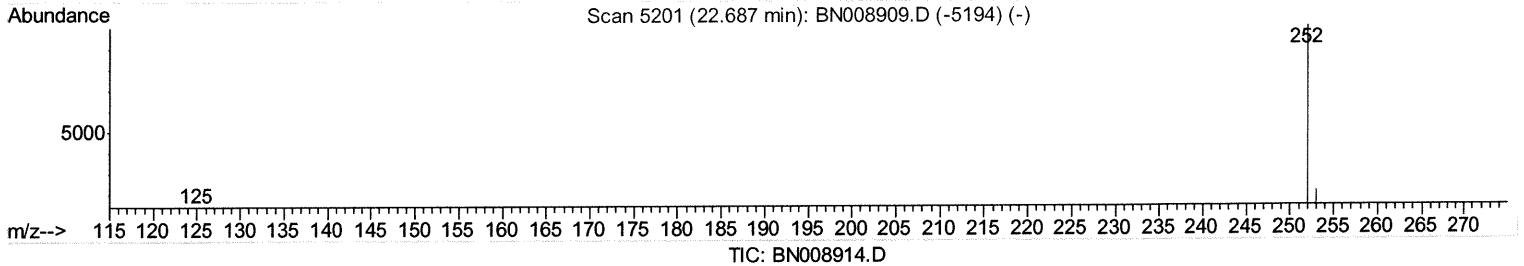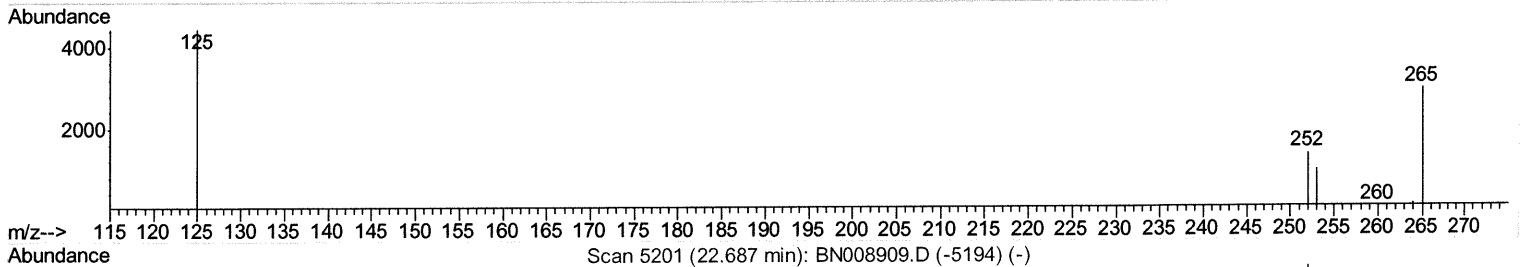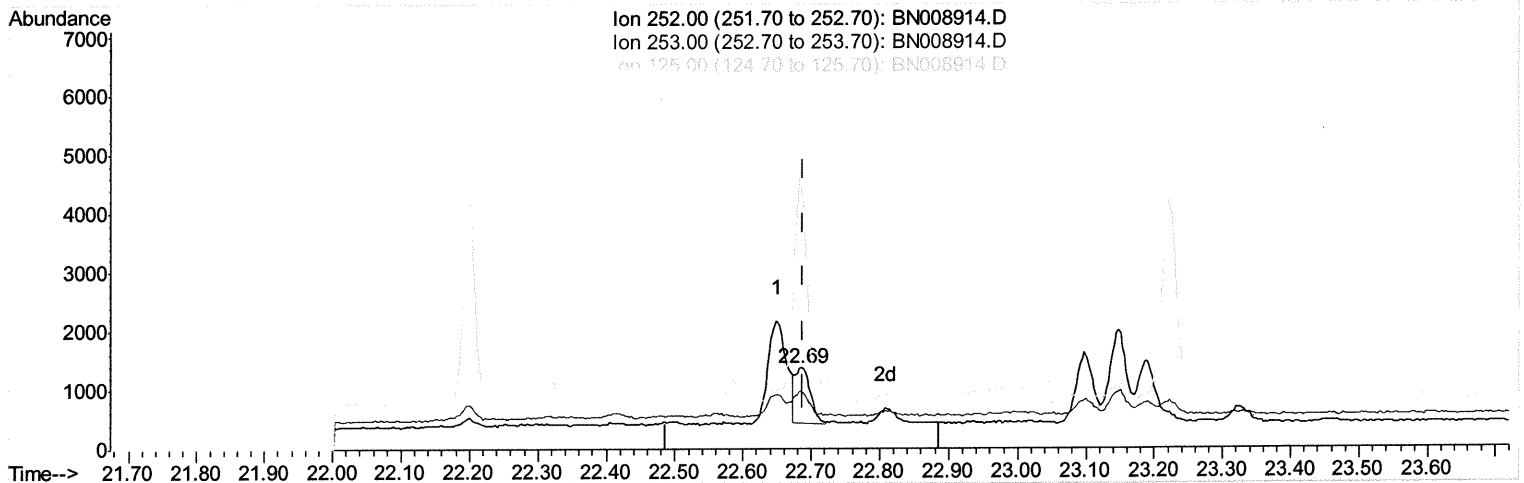

(22) Benzo(k)fluoranthene

22.685min (-0.002) 0.03ng/ul m JU 12/12/19

response 1429

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	71.74#
125.00	17.20	325.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008914.D
 Acq On : 11 Dec 2019 13:24
 Operator : JU
 Sample : K6088-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM7

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:52 AM

Quant Time: Dec 11 14:51:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2290	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	9642	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6302	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	14431	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	12643	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	13386	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.91	152	3282	0.21	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	9042	0.21	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.36	128	4472	0.154	ng/ul	97
5) 2-Methylnaphthalene	11.98	142	4638	0.229	ng/ul	100
12) Phenanthrene	16.97	178	8494	0.175	ng/ul	100
15) Fluoranthene	19.00	202	4098	0.069	ng/ul	92
17) Pyrene	19.36	202	4114m >	0.081	ng/ul	> 94 12/12/19
18) Benzo(a)anthracene	21.12	228	2280	0.045	ng/ul#	89
19) Chrysene	21.17	228	4139	0.083	ng/ul#	90
21) Benzo(b)fluoranthene	22.65	252	3460m }	0.063	ng/ul	} 94 12/12/19
22) Benzo(k)fluoranthene	22.69	252	1429m }	0.026	ng/ul	} 94 12/12/19
23) Benzo(a)pyrene	23.19	252	1841	0.036	ng/ul#	29
24) Indeno(1,2,3-cd)pyrene	25.39	276	1304	0.022	ng/ul#	45
26) Benzo(g,h,i)perylene	26.03	276	1309	0.026	ng/ul#	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed