


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008915.D
Acq On : 11 Dec 2019 13:59
Operator : JU
Sample : K6088-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM8

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:54:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:54 2019
Response via : Initial Calibration

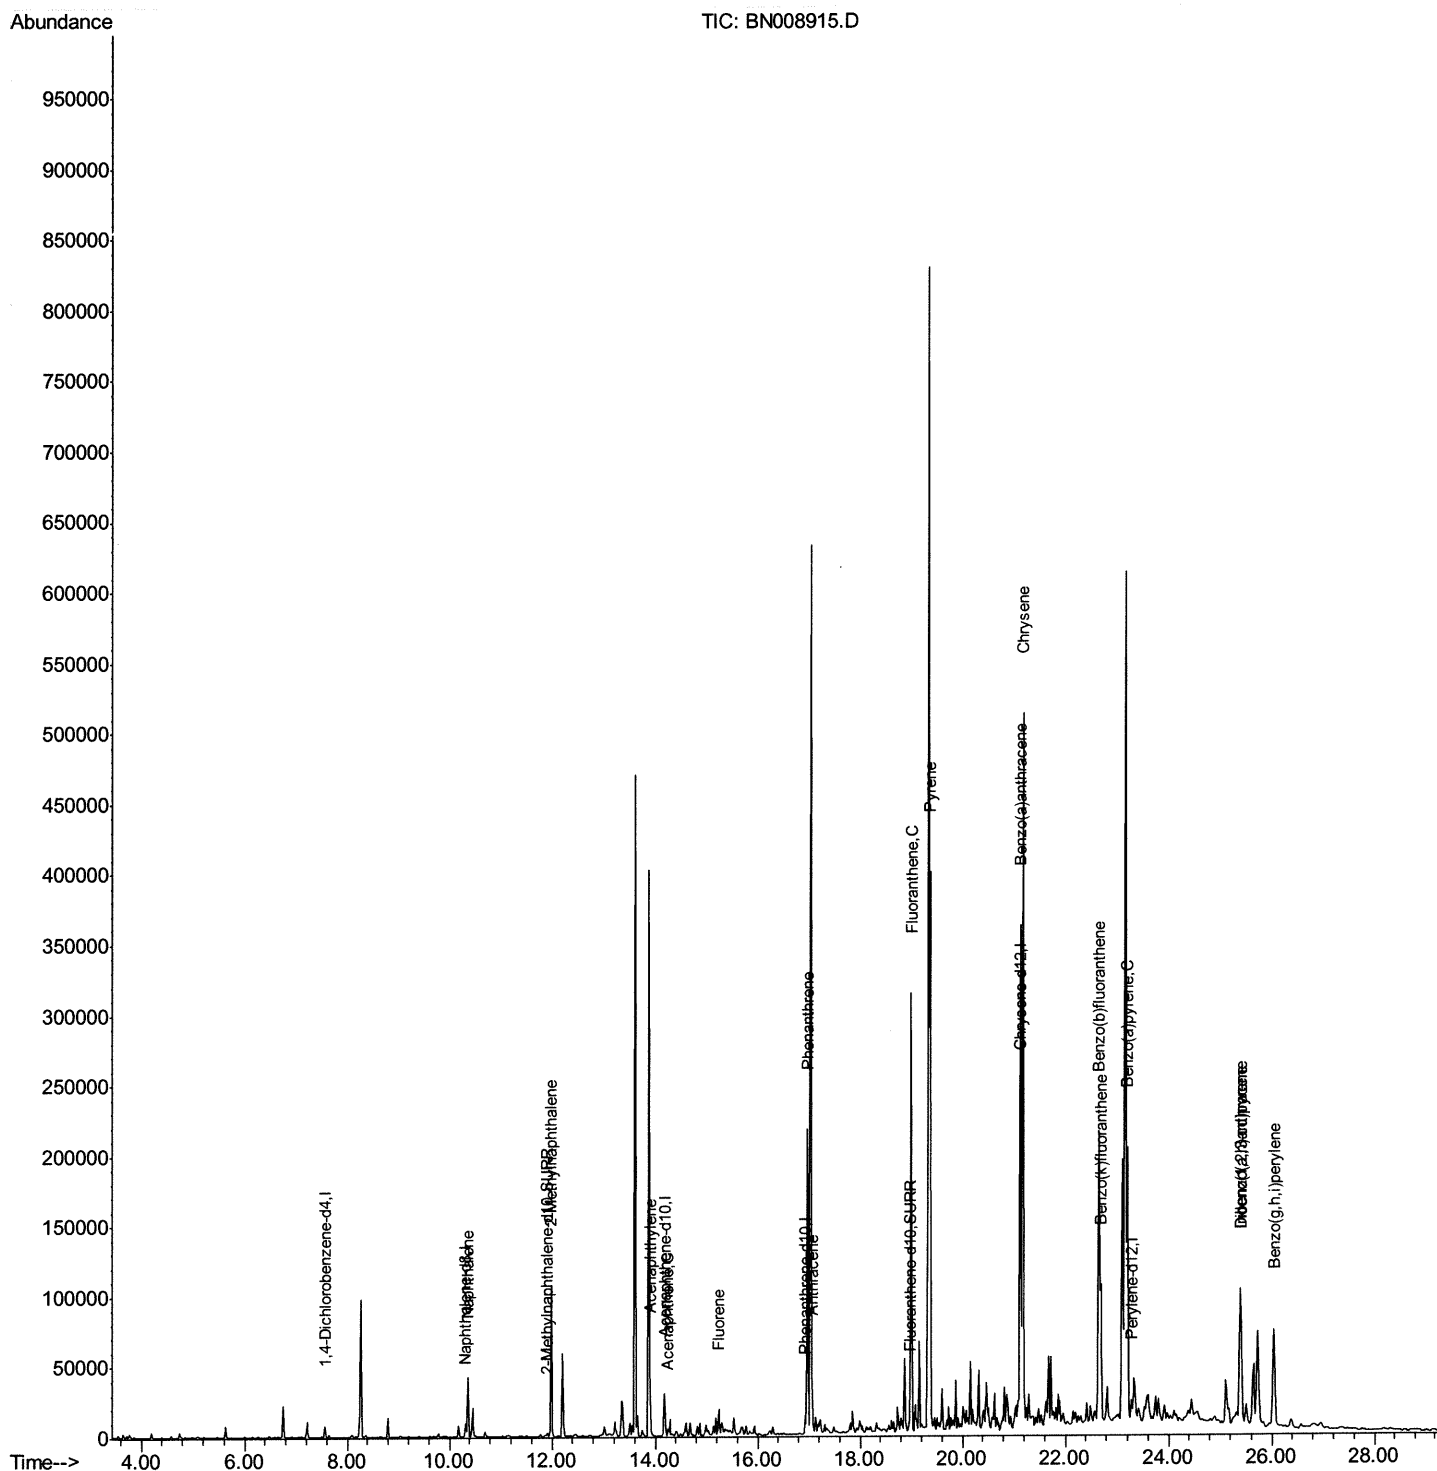

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008915.D
Acq On : 11 Dec 2019 13:59
Operator : JU
Sample : K6088-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM8

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:52:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:54 2019
Response via : Initial Calibration

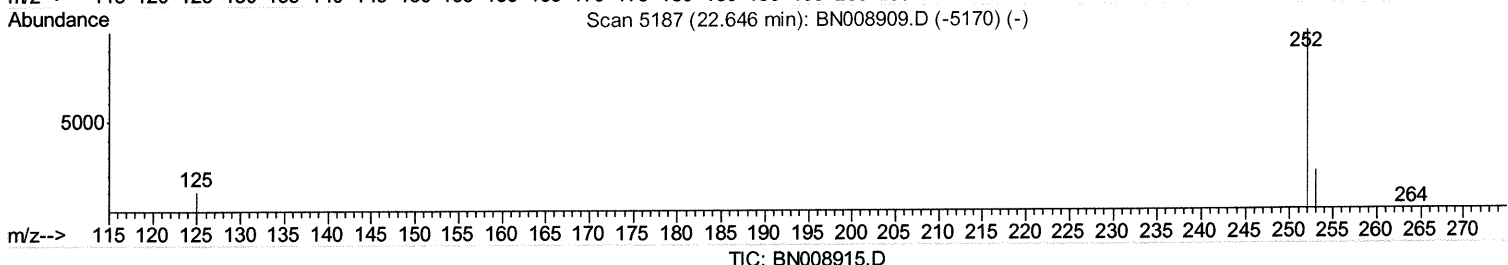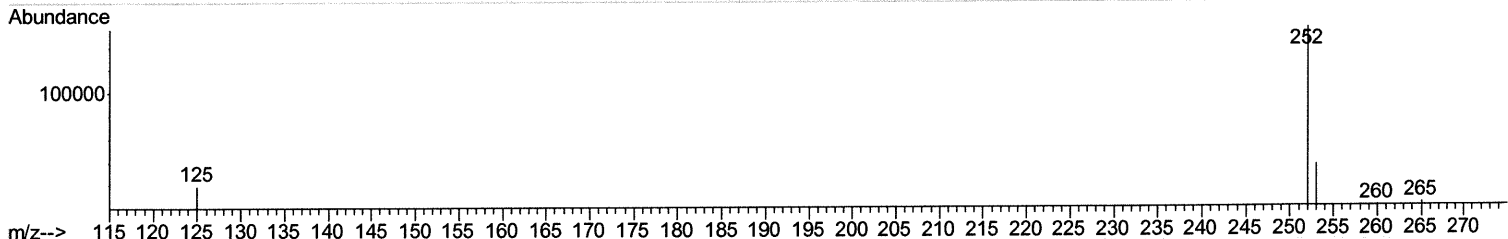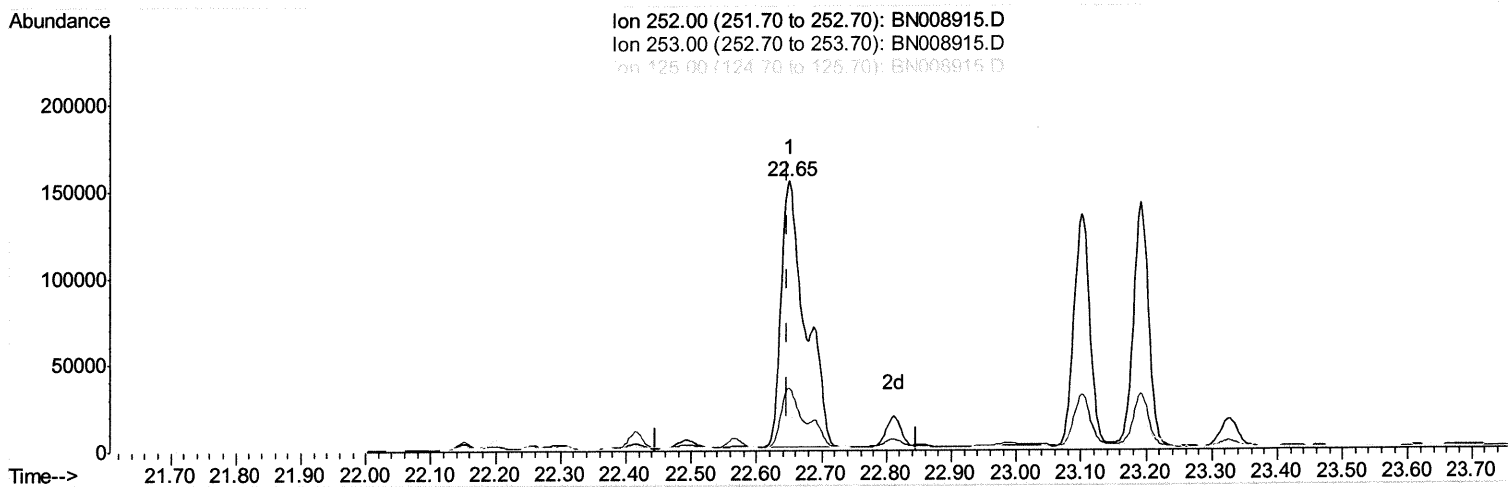

(21) Benzo(b)fluoranthene

22.650min (+0.004) 6.33ng/ul

response 400396

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.13
125.00	15.80	12.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008915.D
 Acq On : 11 Dec 2019 13:59
 Operator : JU
 Sample : K6088-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM8

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:52:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

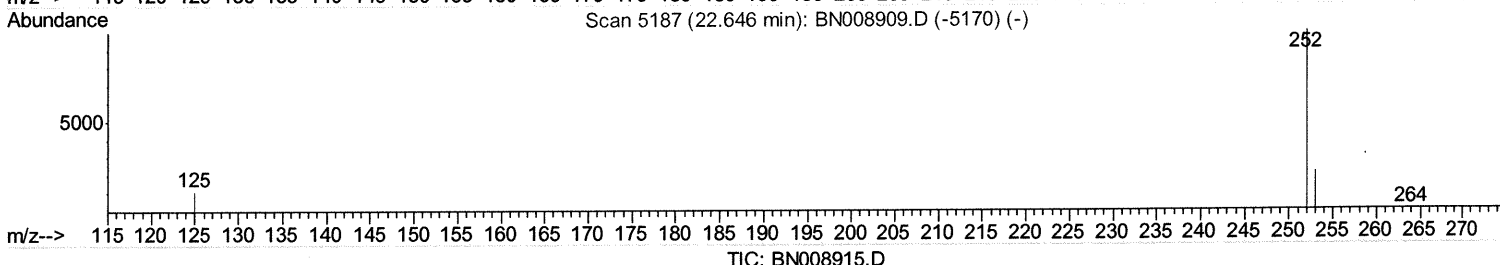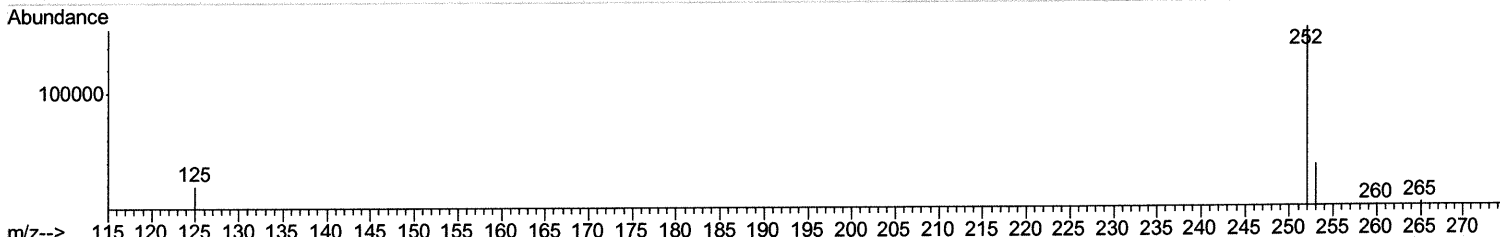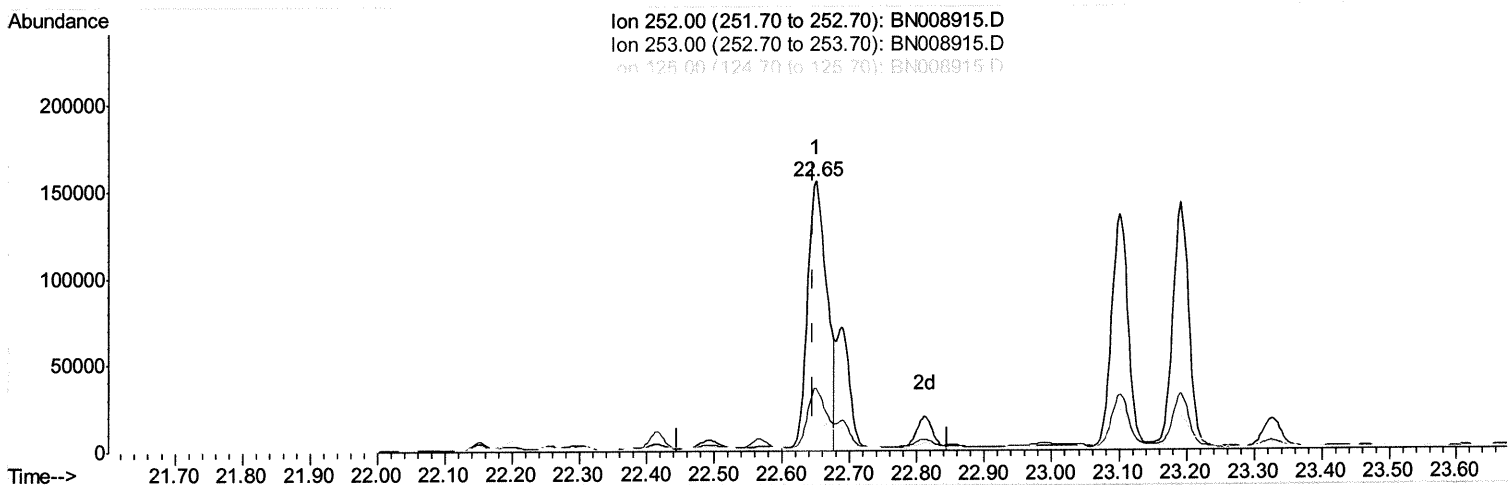

(21) Benzo(b)fluoranthene

22.650min (+0.004) 4.95ng/ul m JU 12/12/19

response 313622

Ion	Exp%	Act%
252.00	100	100
253.00	24.30	23.13
125.00	15.80	12.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008915.D
Acq On : 11 Dec 2019 13:59
Operator : JU
Sample : K6088-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BM8

Manual Integrations
APPROVED

mohammad
12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:52:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 14:04:54 2019
Response via : Initial Calibration

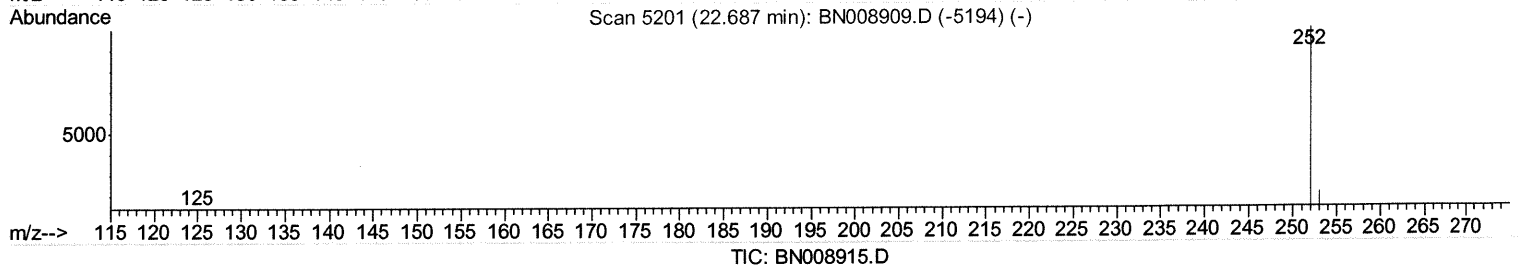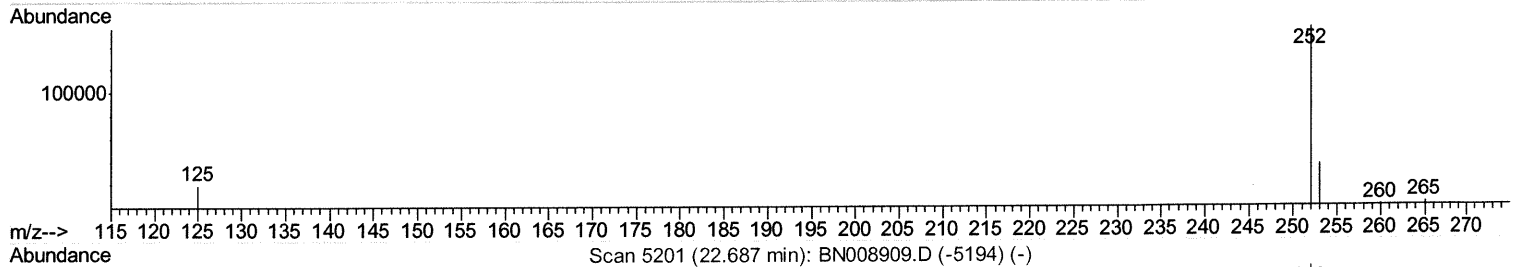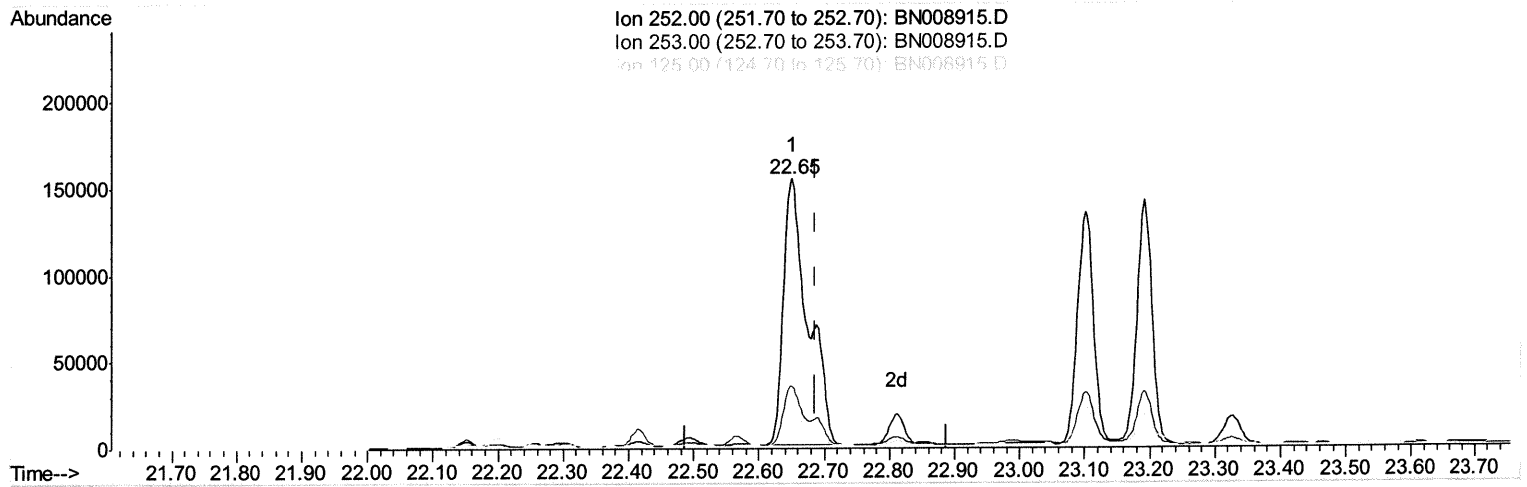

(22) Benzo(k)fluoranthene

22.650min (-0.037) 6.38ng/ul

response 400396

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	23.13
125.00	17.20	12.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008915.D
 Acq On : 11 Dec 2019 13:59
 Operator : JU
 Sample : K6088-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BM8

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:52:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

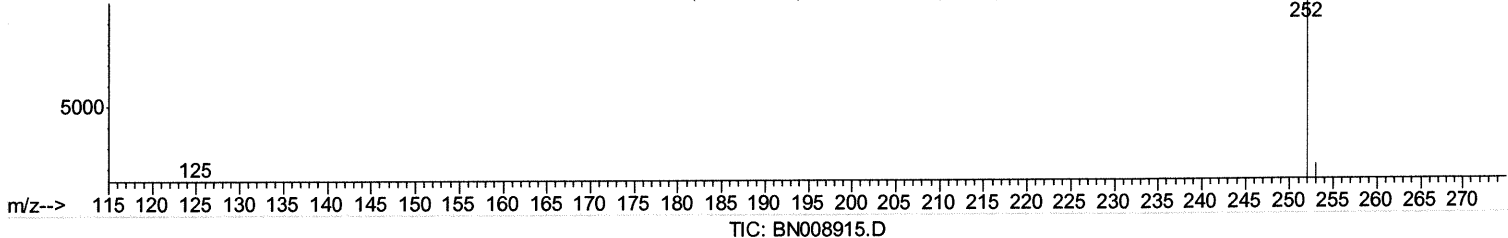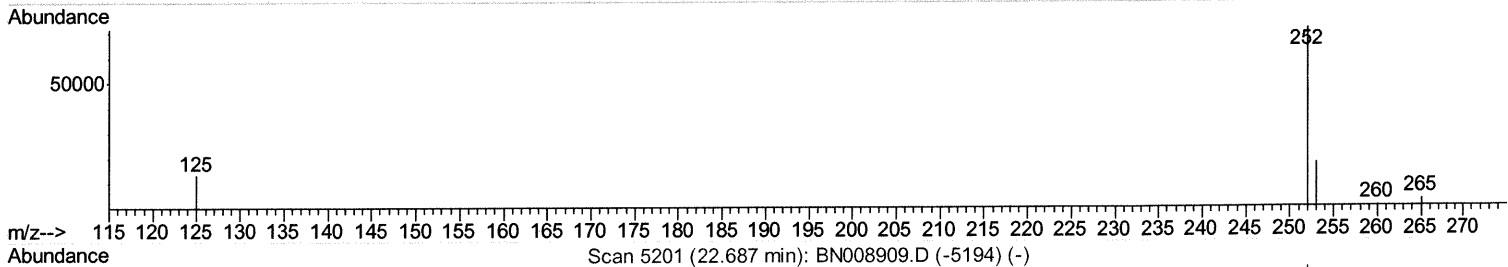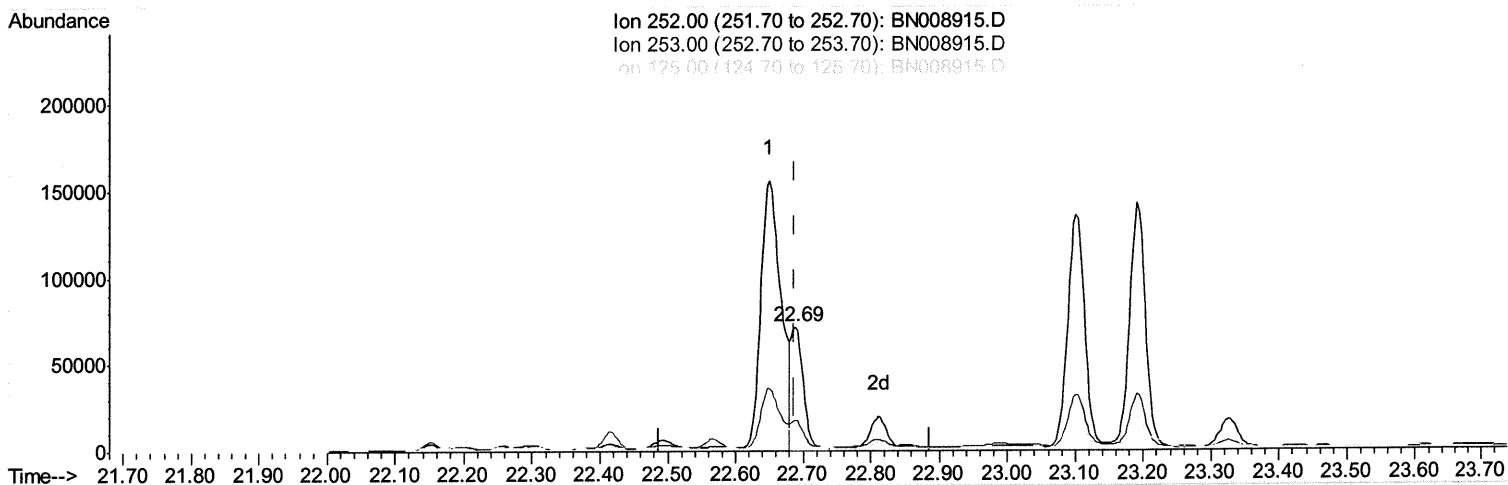

(22) Benzo(k)fluoranthene

22.688min (+0.001) 1.46ng/ul m *Ju 12/12/19*

response 91577

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	24.75
125.00	17.20	18.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008915.D
 Acq On : 11 Dec 2019 13:59
 Operator : JU
 Sample : K6088-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COBM8

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:26:59 AM

Quant Time: Dec 11 14:54:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 14:04:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2363	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	10454	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	7580	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	15787	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	13447	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	15350	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.91	152	3144	0.18	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	10368	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.36	128	55801	1.771	ng/ul	99
5) 2-Methylnaphthalene	11.98	142	77365	3.515	ng/ul	100
7) Acenaphthylene	13.90	152	10621	0.253	ng/ul#	92
8) Acenaphthene	14.25	153	2871	0.092	ng/ul	96
9) Fluorene	15.24	166	8615	0.236	ng/ul#	87
12) Phenanthrene	16.97	178	227370	4.271	ng/ul	100
13) Anthracene	17.06	178	39661	0.788	ng/ul	98
15) Fluoranthene	19.00	202	265063	4.052	ng/ul	99
17) Pyrene	19.36	202	317879	5.892	ng/ul	99
18) Benzo(a)anthracene	21.12	228	288039	5.326	ng/ul	97
19) Chrysene	21.17	228	439340	8.272	ng/ul	97
21) Benzo(b)fluoranthene	22.65	252	313622m	4.955	ng/ul	3
22) Benzo(k)fluoranthene	22.69	252	91577m	1.459	ng/ul	3
23) Benzo(a)pyrene	23.19	252	231278	3.893	ng/ul#	93
24) Indeno(1,2,3-cd)pyrene	25.39	276	106118	1.527	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.40	278	77303	1.378	ng/ul#	87
26) Benzo(g,h,i)perylene	26.03	276	126699	2.180	ng/ul	98

54/2/12/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed