


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008923.D
Acq On : 11 Dec 2019 18:46
Operator : JU
Sample : K6088-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BN5

Manual Integrations
APPROVED

mohammad
12/12/2019 11:28:02 AM

Quant Time: Dec 12 01:30:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 11 10:35:08 2019
Response via : Initial Calibration

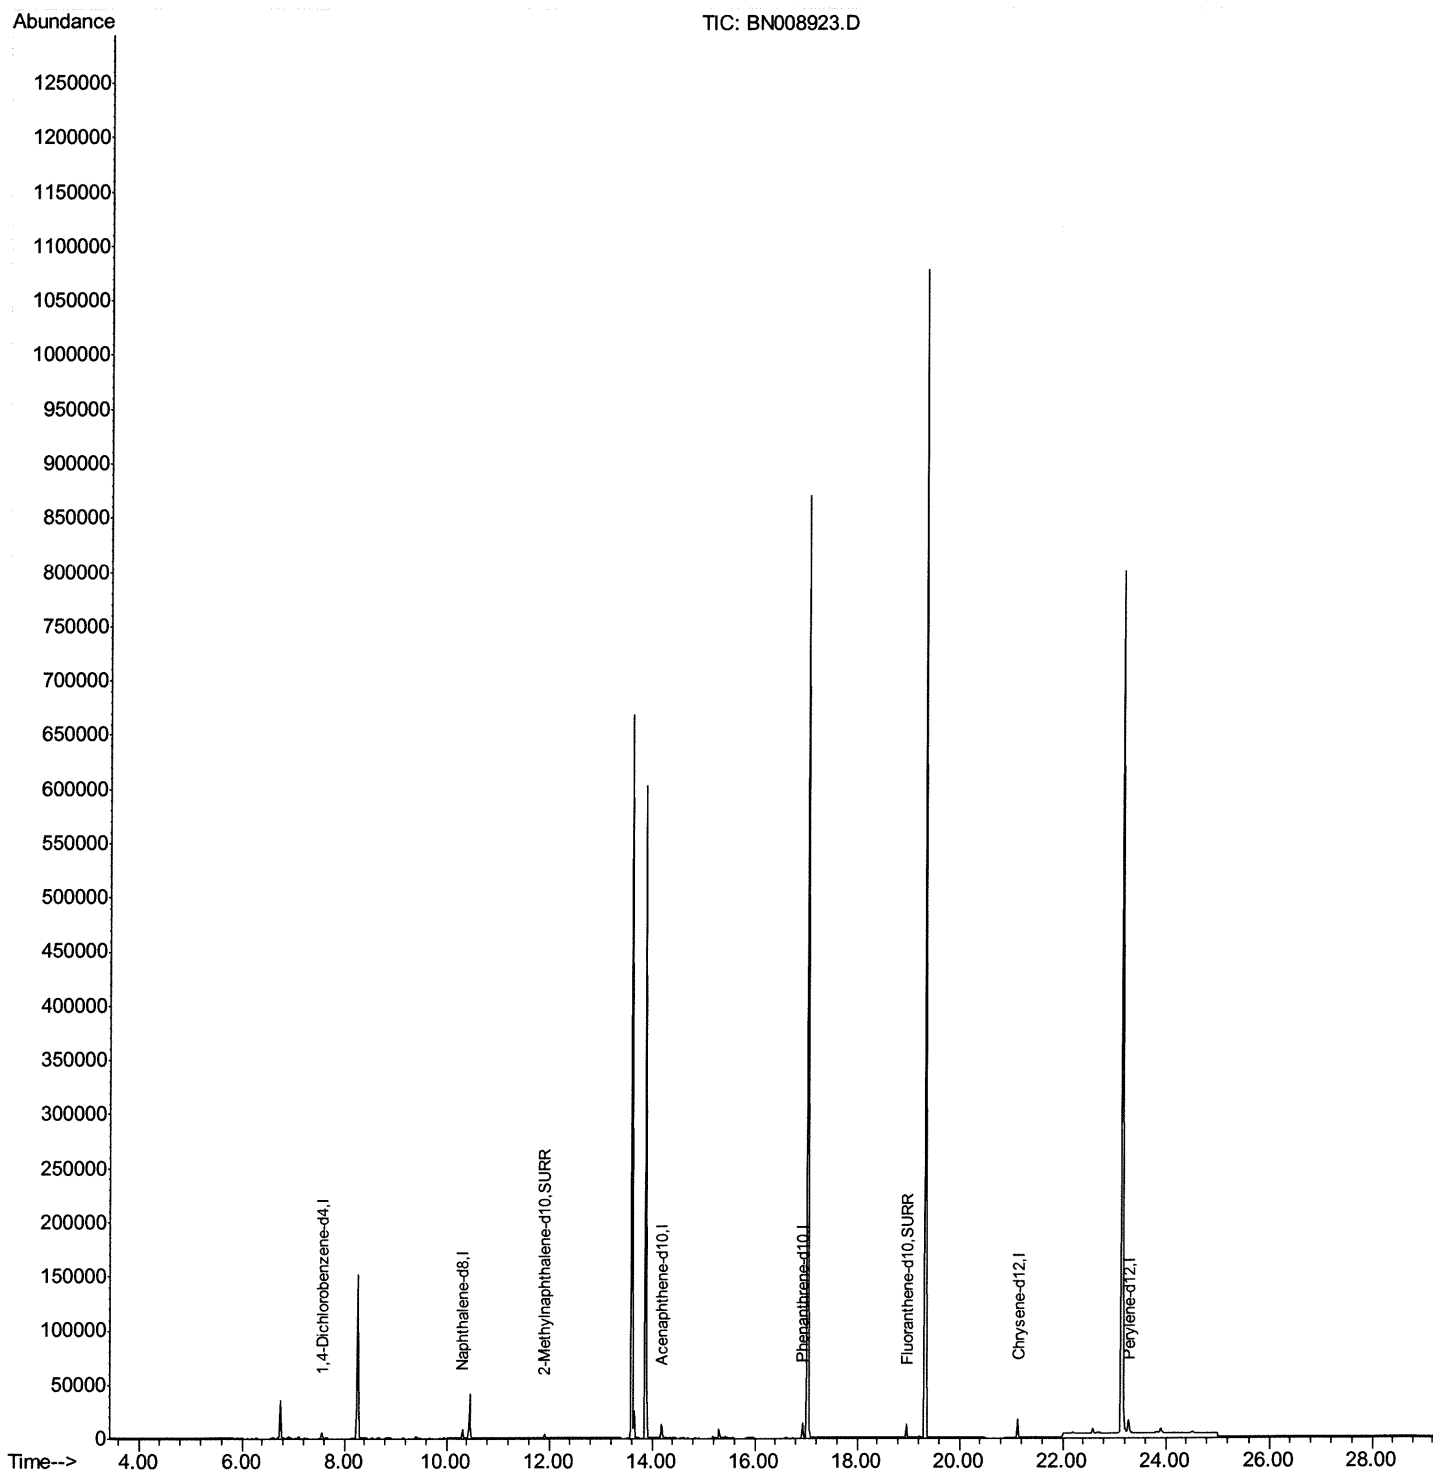

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008923.D
 Acq On : 11 Dec 2019 18:46
 Operator : JU
 Sample : K6088-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BN5

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:28:02 AM

Quant Time: Dec 12 00:22:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 10:35:08 2019
 Response via : Initial Calibration

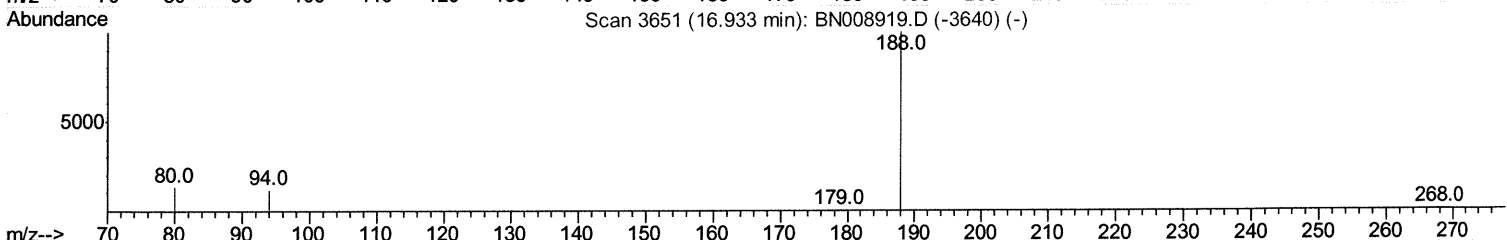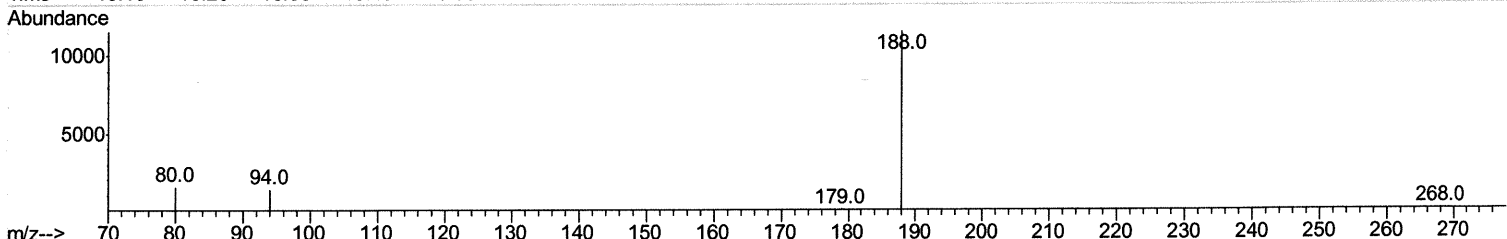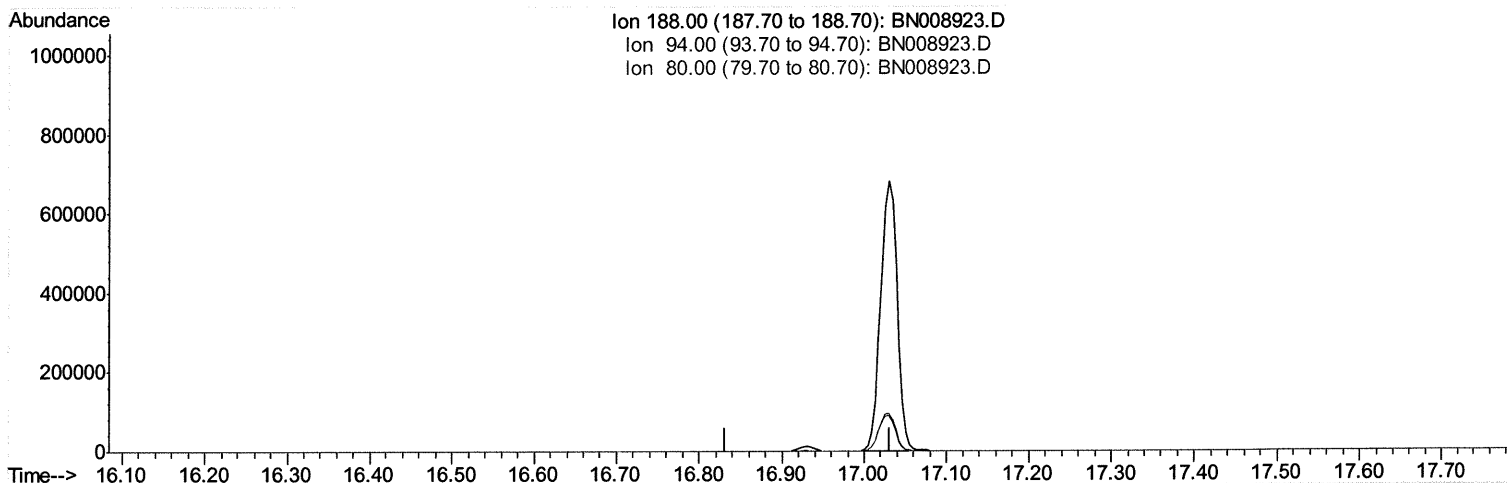

(10) Phenanthrene-d10 (I)

16.932min (-16.932) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008923.D
 Acq On : 11 Dec 2019 18:46
 Operator : JU
 Sample : K6088-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BN5

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:28:02 AM

Quant Time: Dec 12 00:22:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 10:35:08 2019
 Response via : Initial Calibration

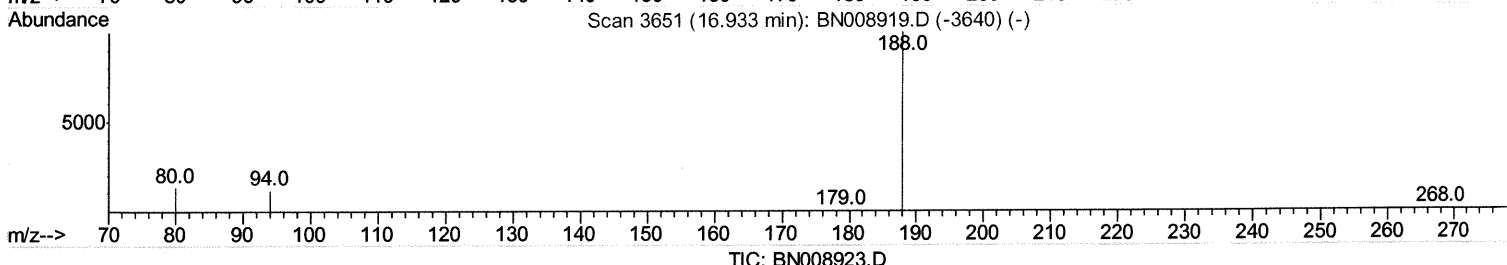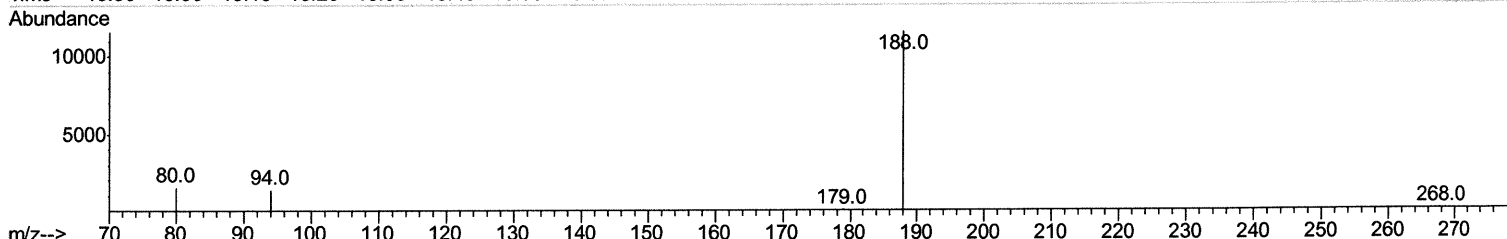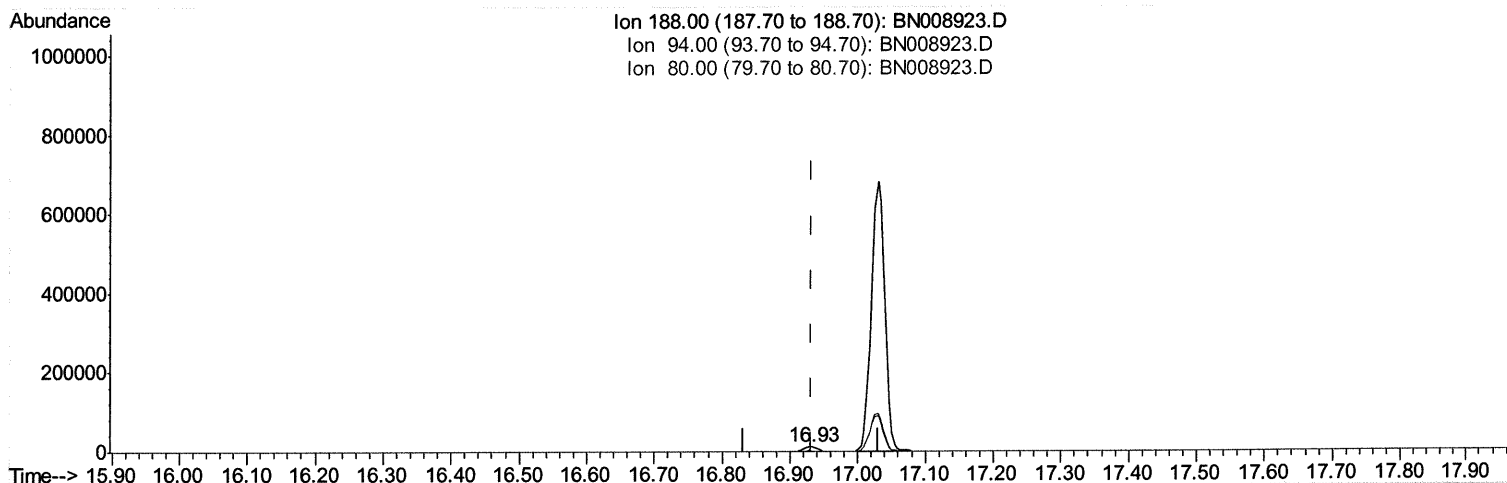

(10) Phenanthrene-d10 (I)

16.932min (+0.001) 0.40ng/ul m 5412/12/19

response 16171

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.24
80.00	14.40	13.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008923.D
 Acq On : 11 Dec 2019 18:46
 Operator : JU
 Sample : K6088-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BN5

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:28:02 AM

Quant Time: Dec 12 01:30:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 11 10:35:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2425	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	10613	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6993	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	16171m	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	14393	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	15771	0.40	ng/ul	0.00

54 12/12/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.91	152	4704	0.27	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	12901	0.26	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed