


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008935.D
Acq On : 12 Dec 2019 01:54
Operator : JU
Sample : K6088-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BQ8

Manual Integrations
APPROVED

mohammad
12/12/2019 11:32:58 AM

Quant Time: Dec 12 02:56:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 01:20:09 2019
Response via : Initial Calibration

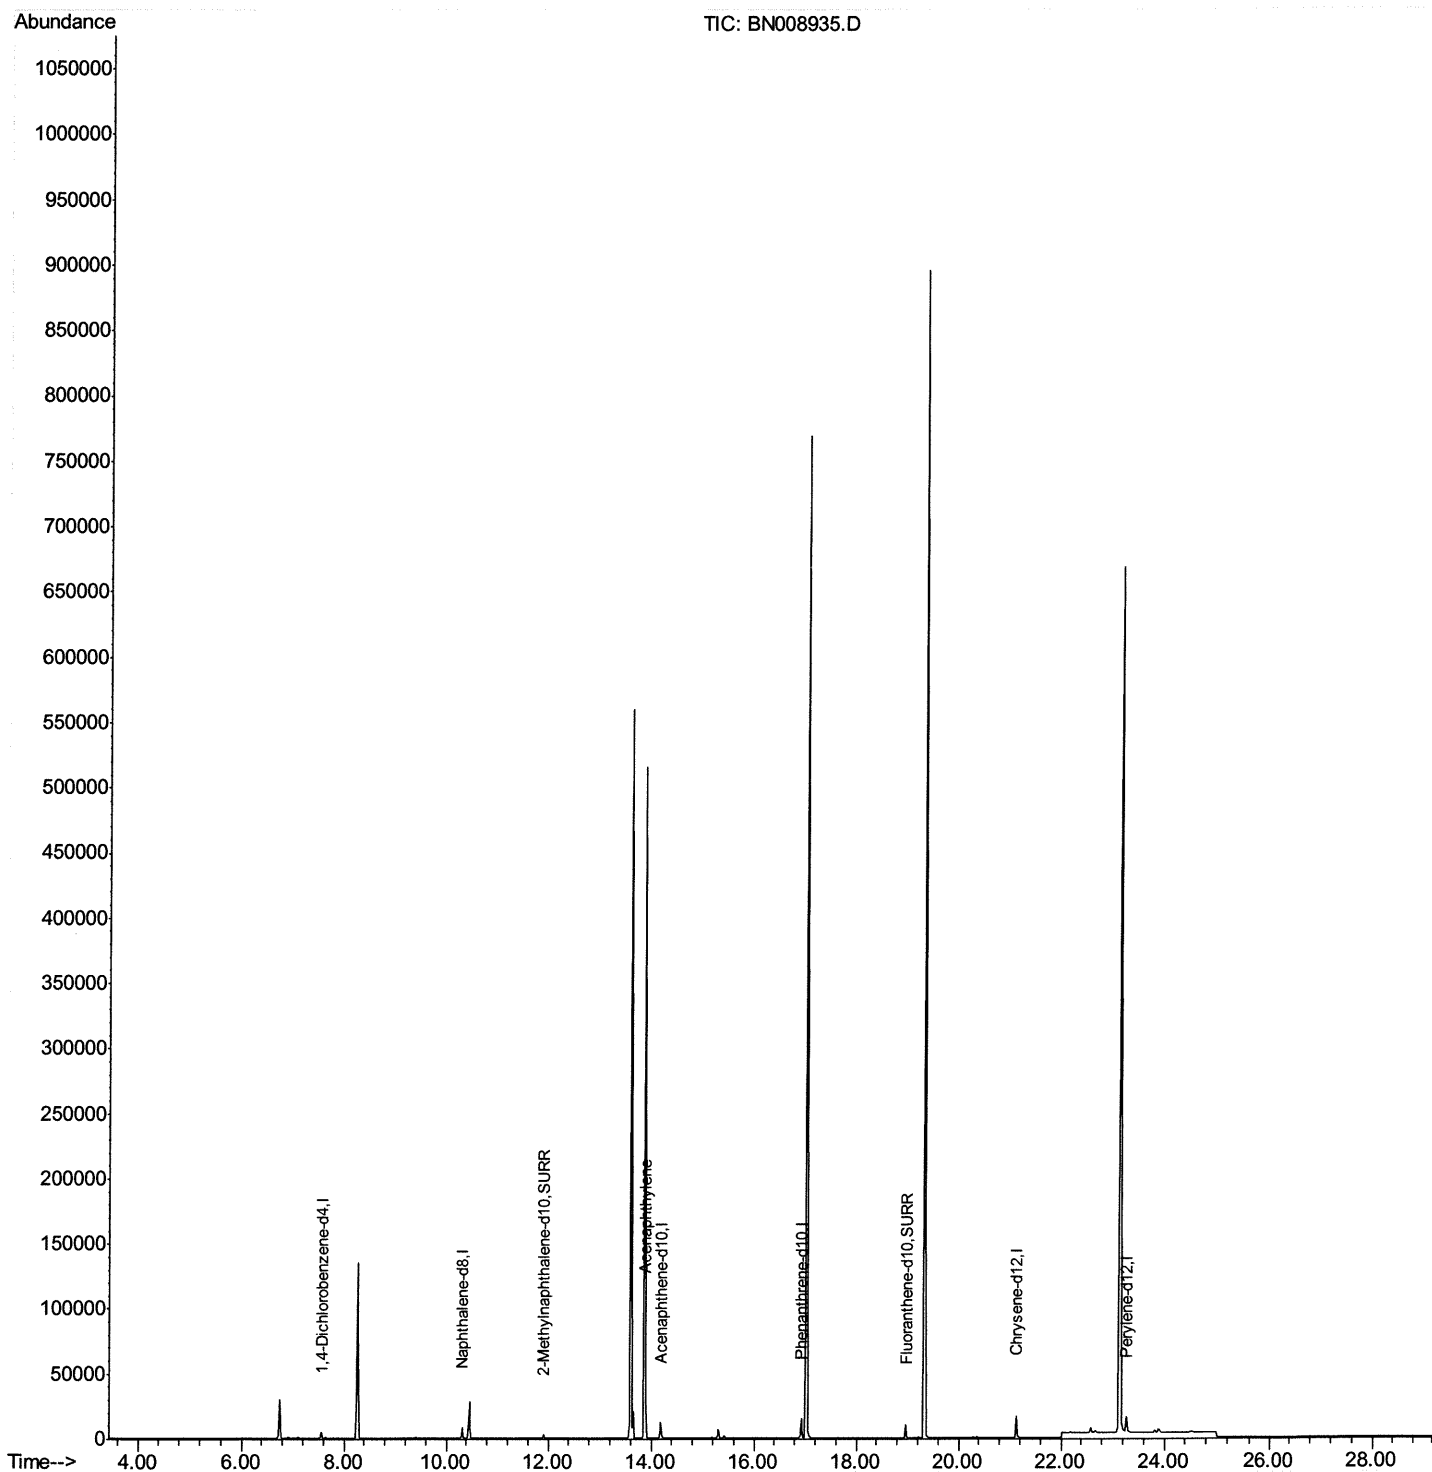

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008935.D
 Acq On : 12 Dec 2019 01:54
 Operator : JU
 Sample : K6088-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BQ8

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:32:58 AM

Quant Time: Dec 12 02:45:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 01:20:09 2019
 Response via : Initial Calibration

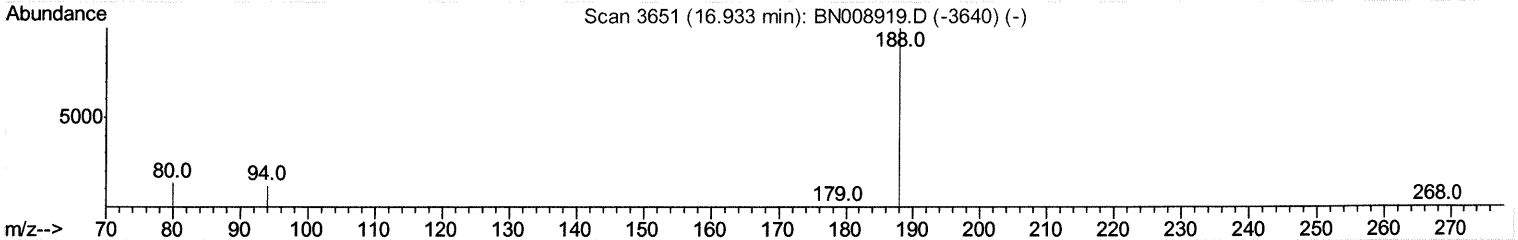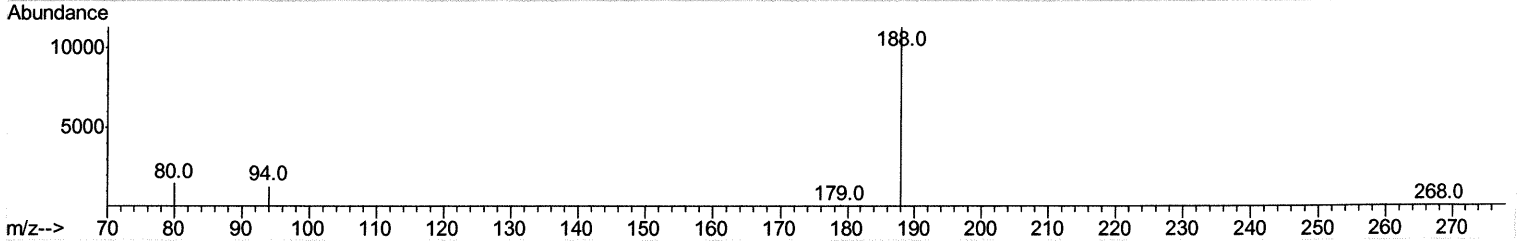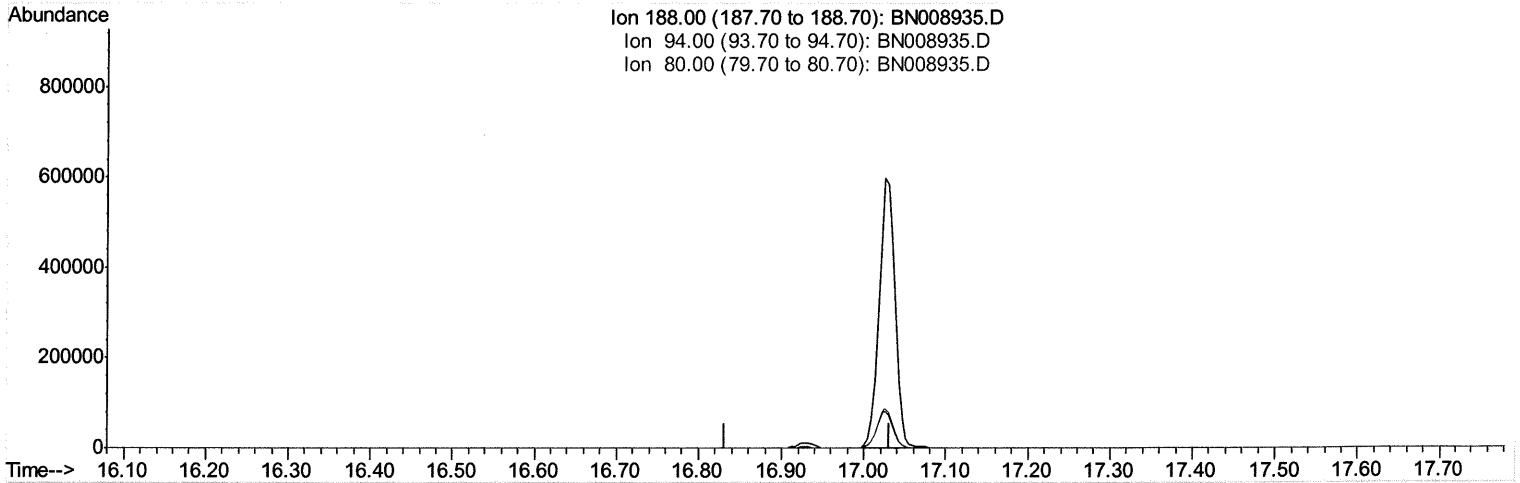

TIC: BN008935.D

(10) Phenanthrene-d10 (I)

16.932min (-16.932) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008935.D
Acq On : 12 Dec 2019 01:54
Operator : JU
Sample : K6088-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BQ8

Manual Integrations
APPROVED

mohammad
12/12/2019 11:32:58 AM

Quant Time: Dec 12 02:45:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 01:20:09 2019
Response via : Initial Calibration

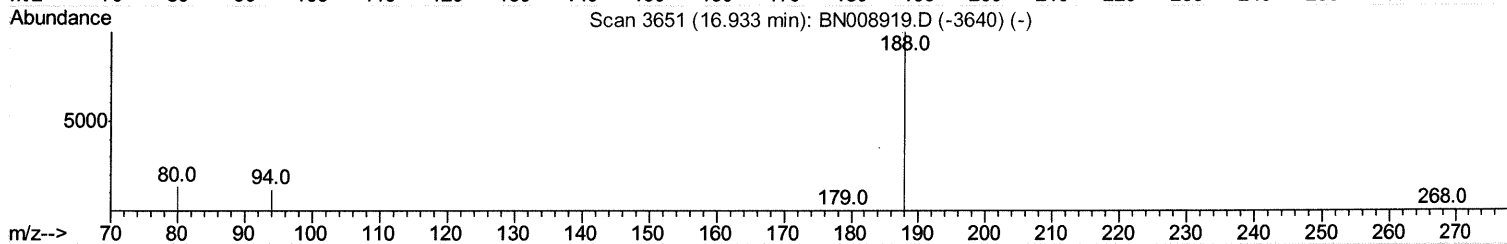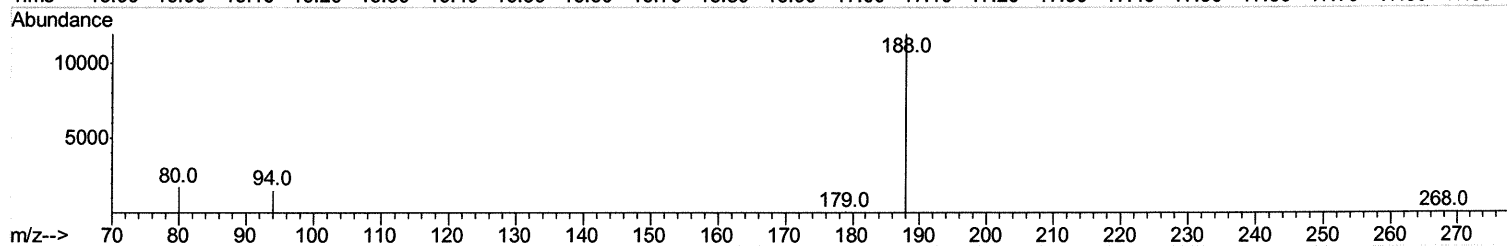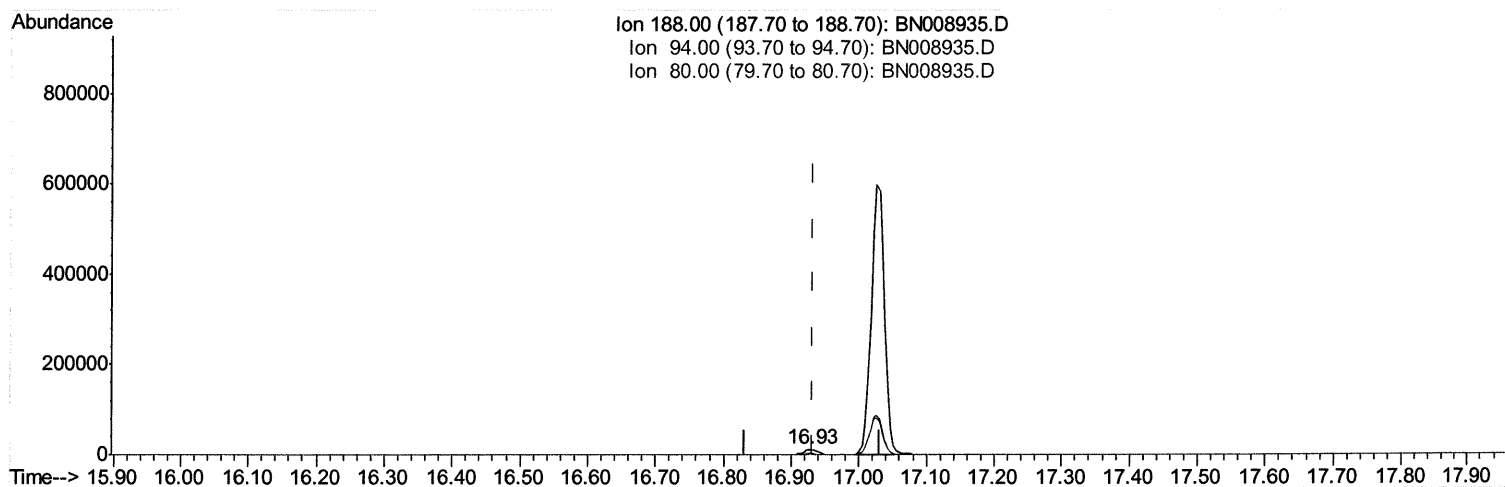

TIC: BN008935.D

(10) Phenanthrene-d10 (I)

16.928min (-0.004) 0.40ng/ul m JU 12/12/19

response 15792

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.98
80.00	14.40	14.53
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008935.D
 Acq On : 12 Dec 2019 01:54
 Operator : JU
 Sample : K6088-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BQ8

Manual Integrations
 APPROVED

mohammad
 12/12/2019 11:32:58 AM

Quant Time: Dec 12 02:56:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 01:20:09 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2403	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	10502	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	6763	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	15792m	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	14233	0.40	ng/ul	0.00
20) Perylene-d12	23.27	264	14948	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	4085	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	11043	0.23	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	13.90	152	1121	0.030	ng/ul#	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

34 12/12/19