


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008943.D
Acq On : 12 Dec 2019 13:42
Operator : JU
Sample : PB125223BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK23

Manual Integrations
APPROVED

mohammad
12/13/2019 8:08:02 AM

Quant Time: Dec 12 14:28:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

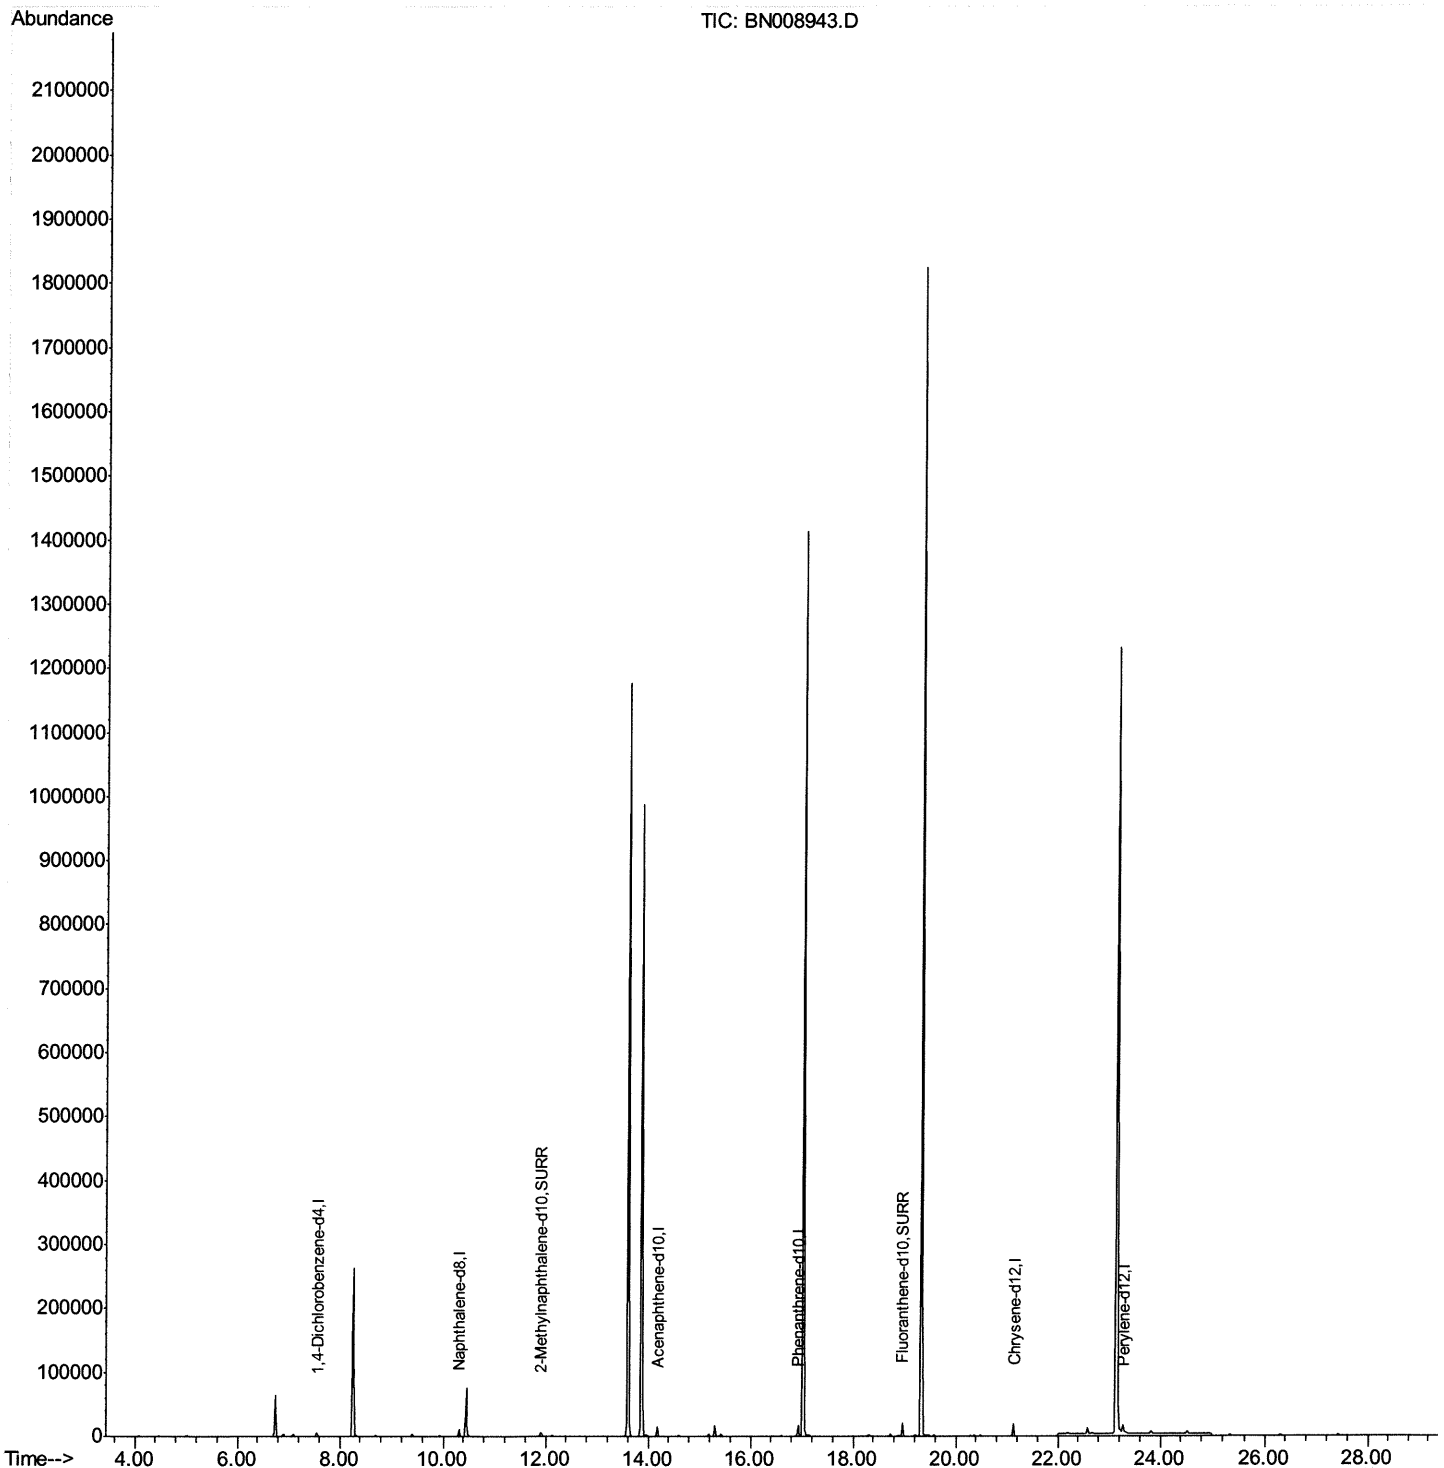

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008943.D
 Acq On : 12 Dec 2019 13:42
 Operator : JU
 Sample : PB125223BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK23

Manual Integrations
 APPROVED

mohammad
 12/13/2019 8:08:02 AM

Quant Time: Dec 12 14:26:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 00:49:42 2019
 Response via : Initial Calibration

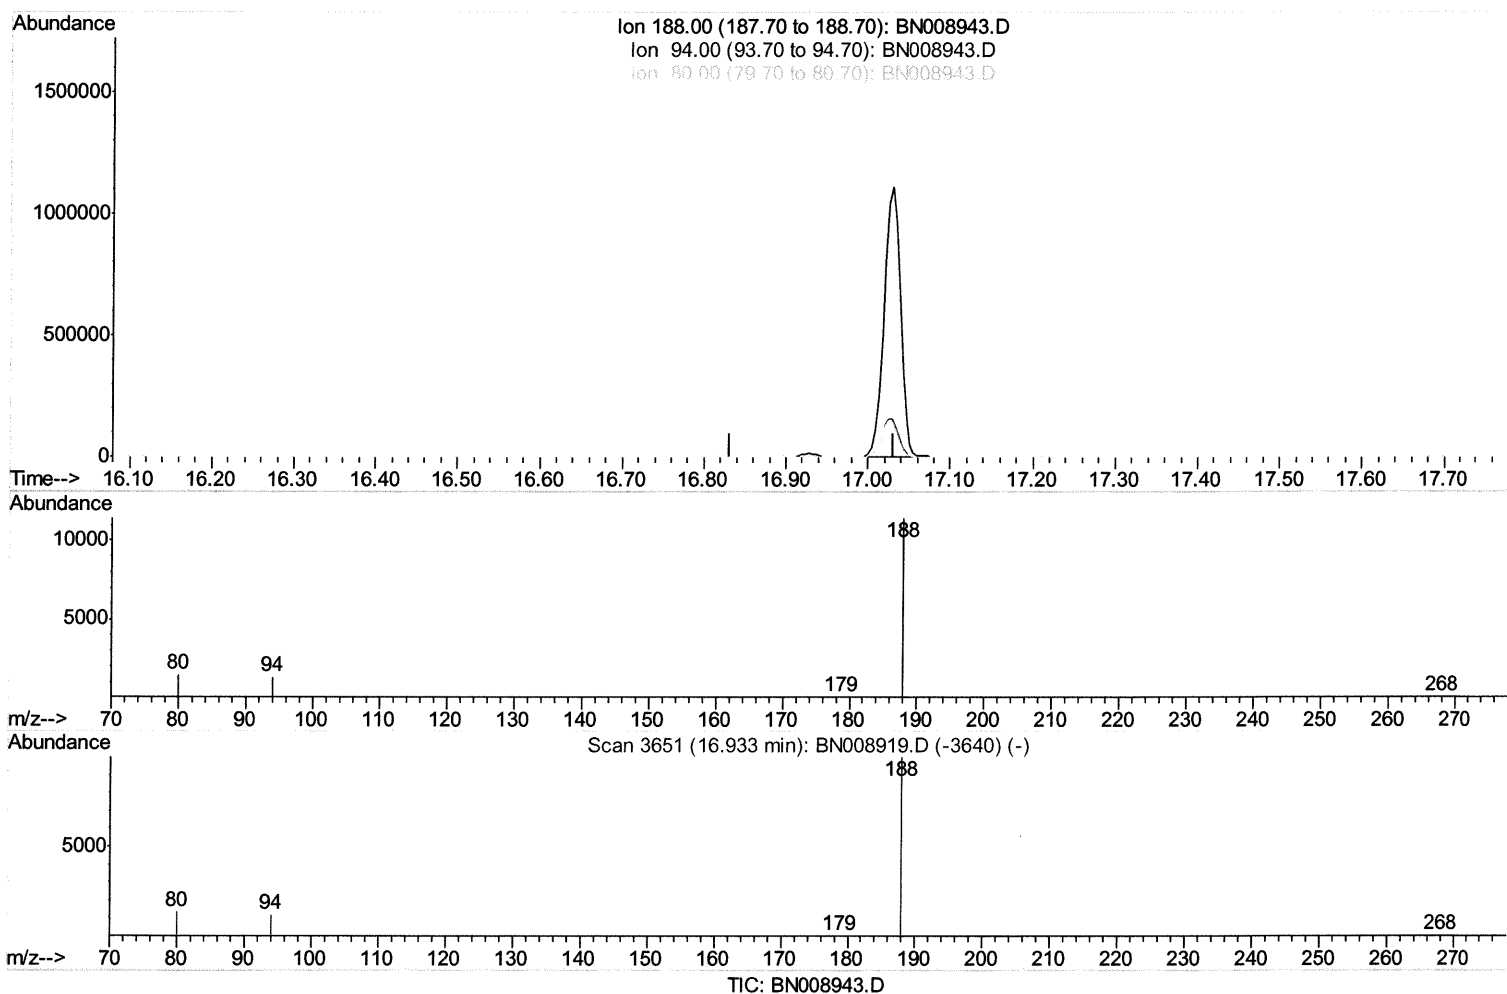

(10) Phenanthrene-d10 (I)

16.932min (-16.932) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
 Data File : BN008943.D
 Acq On : 12 Dec 2019 13:42
 Operator : JU
 Sample : PB125223BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK23

Manual Integrations
 APPROVED

mohammad
 12/13/2019 8:08:02 AM

Quant Time: Dec 12 14:26:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 00:49:42 2019
 Response via : Initial Calibration

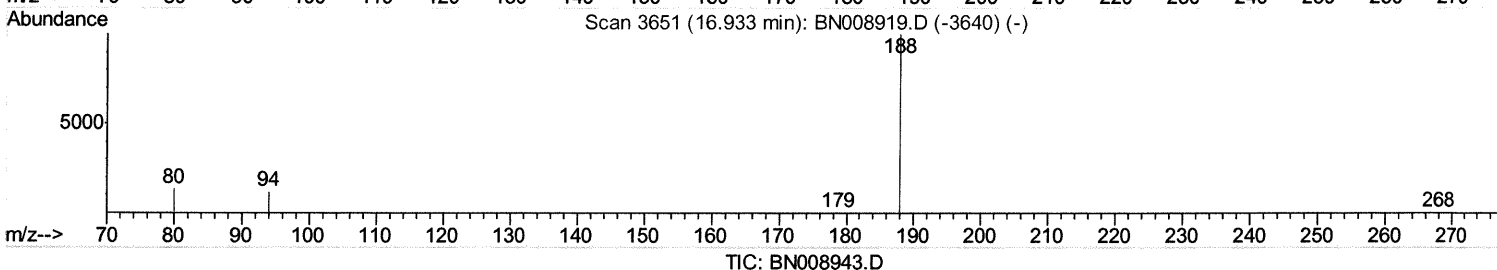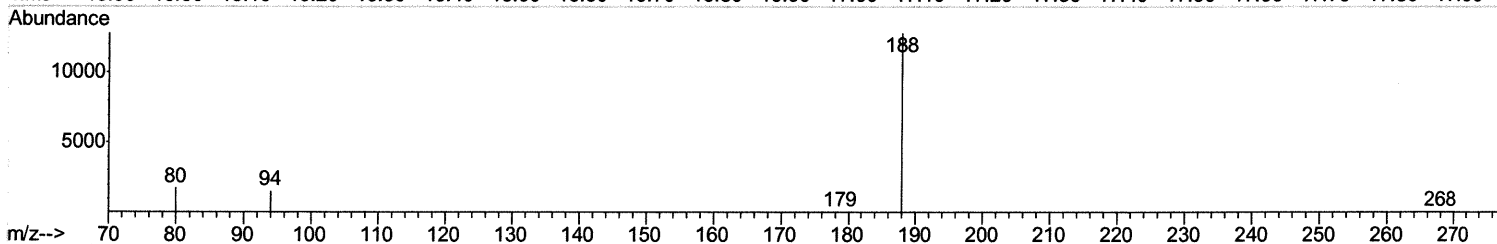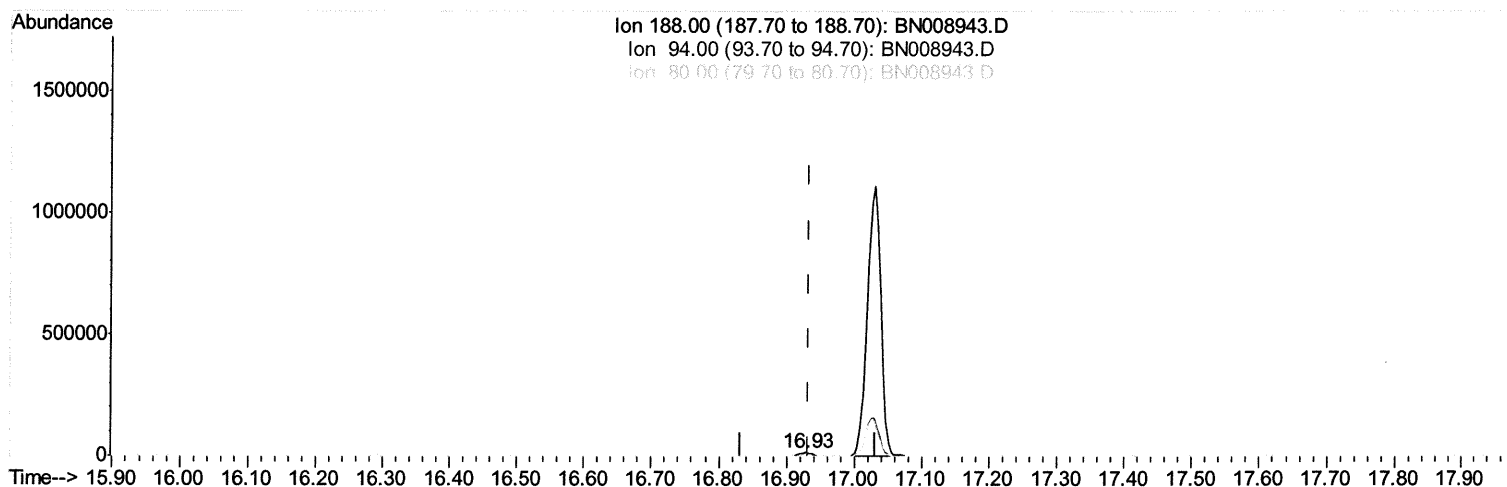

(10) Phenanthrene-d10 (I)

16.928min (-0.003) 0.40ng/ul m JU 12/12/19

response 17475

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.05
80.00	14.40	13.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121119\
Data File : BN008943.D
Acq On : 12 Dec 2019 13:42
Operator : JU
Sample : PB125223BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK23

Manual Integrations
APPROVED

mohammad
12/13/2019 8:08:02 AM

Quant Time: Dec 12 14:28:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2792	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	12196	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	7757	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	17475m	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	15914	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	16848	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.91	152	7923	0.40	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	21828	0.41	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2412/12/19