

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
 Data File : BN008954.D
 Acq On : 12 Dec 2019 20:14
 Operator : JU
 Sample : K6089-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BR0

Manual Integrations
 APPROVED

mohammad
 12/13/2019 9:08:01 AM

Quant Time: Dec 13 01:33:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 00:49:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	2721	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	12127	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	7860	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	17615	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	14456	0.40	ng/ul	0.00
20) Perylene-d12	23.27	264	13981	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	3771	0.19	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	11335	0.21	ng/ul	0.00
Target Compounds					Ovalue	
3) Naphthalene	10.36	128	10810	0.296	ng/ul	98
5) 2-Methylnaphthalene	11.98	142	10820	0.424	ng/ul	99
7) Acenaphthylene	13.90	152	18972	0.437	ng/ul	98
8) Acenaphthene	14.25	153	2724	0.084	ng/ul	96
9) Fluorene	15.24	166	8253	0.218	ng/ul#	92
12) Phenanthrene	16.97	178	195955	3.299	ng/ul	99
13) Anthracene	17.06	178	30324	0.540	ng/ul	99
15) Fluoranthene	18.99	202	424383	5.815	ng/ul	100
17) Pyrene	19.36	202	348089	6.002	ng/ul	97
18) Benzo(a)anthracene	21.11	228	179722	3.091	ng/ul	96
19) Chrysene	21.17	228	199668	3.497	ng/ul	97
21) Benzo(b)fluoranthene	22.64	252	239155m	4.148	ng/ul	
22) Benzo(k)fluoranthene	22.68	252	72605m	1.270	ng/ul	
23) Benzo(a)pyrene	23.18	252	151387m	2.798	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.38	276	99649	1.575	ng/ul#	90
25) Dibenzo(a,h)anthracene	25.38	278	29605	0.579	ng/ul#	90
26) Benzo(a,h,i)perylene	26.02	276	106122	2.005	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121119\
Data File : BN008954.D
Acq On : 12 Dec 2019 20:14
Operator : JU
Sample : K6089-12
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0BR0

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

Quant Time: Dec 13 01:33:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

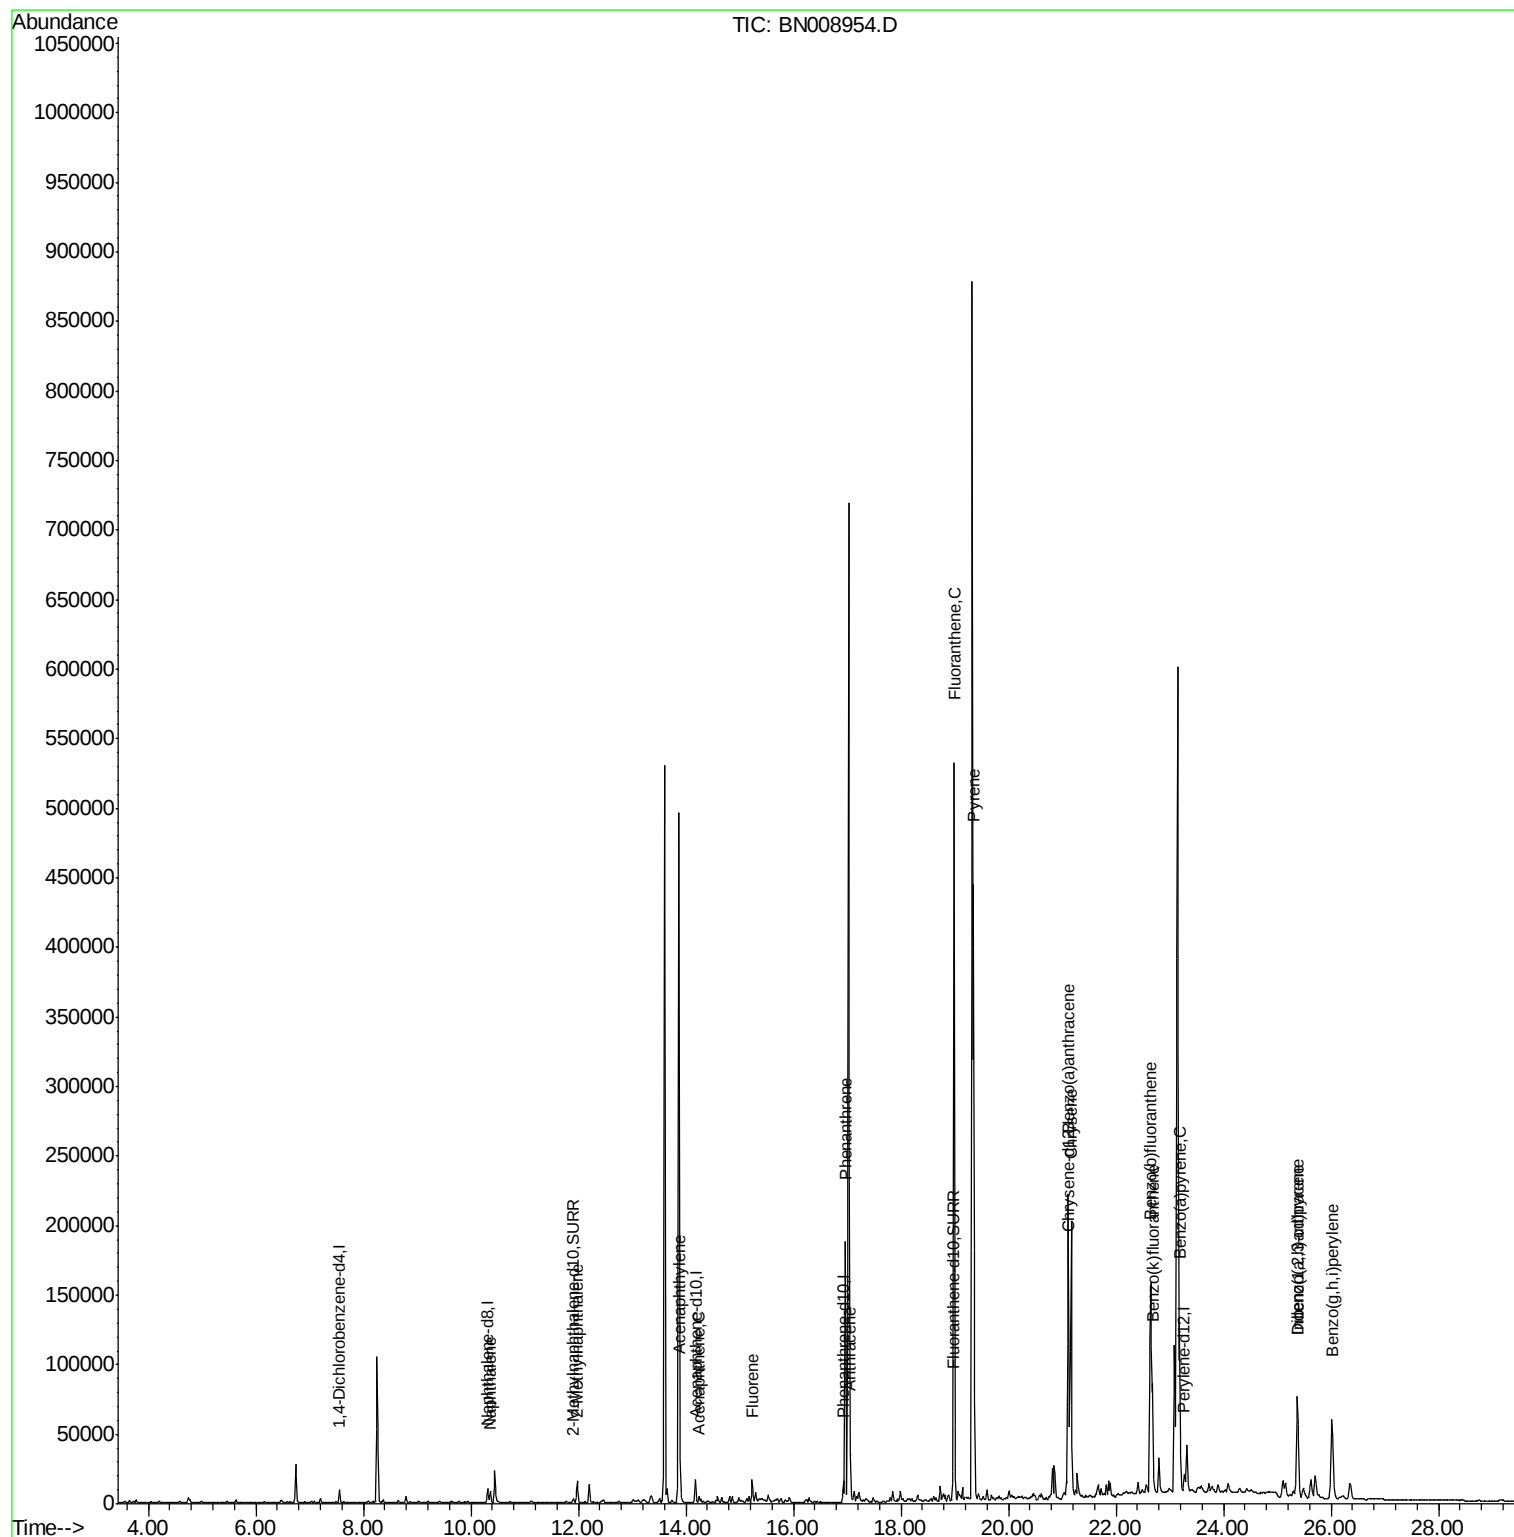

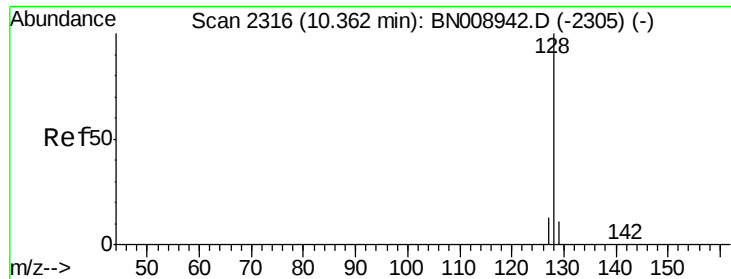

#3

Naphthalene

Concen: 0.296 ng/ul

RT: 10.36 min Scan# 2315

Delta R.T. -0.01 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Instrument :

BNA_N


ClientSampleId :

C0BR0




Tot Ion:128	Resp:	10810
Ion Ratio	Lower	Upper
128 100		
129 12.3	9.1	13.7
127 14.0	10.7	16.1

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

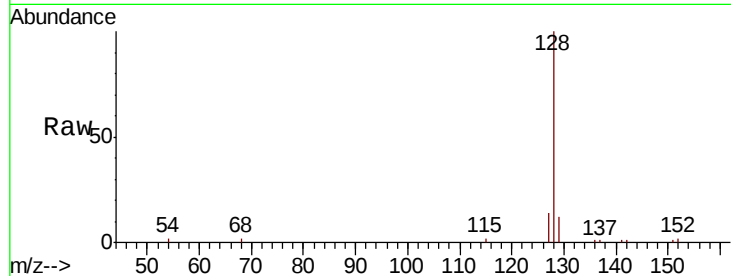

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

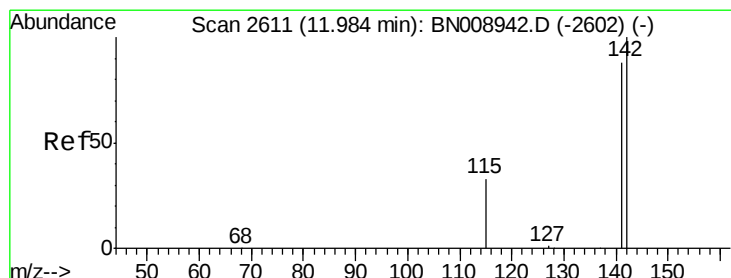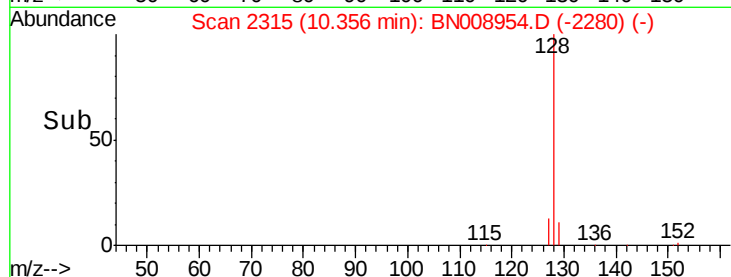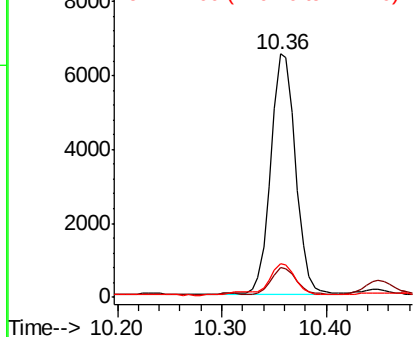

#5

2-Methylnaphthalene

Concen: 0.424 ng/ul


RT: 11.98 min Scan# 2610

Delta R.T. -0.01 min



Lab File: BN008954.D


Acq: 12 Dec 2019 20:14

Tgt Ion:142	Resp:	10820
Ion Ratio	Lower	Upper
142 100		
141 88.1	70.1	105.1

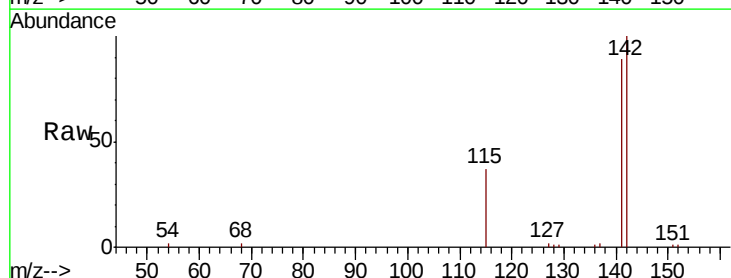

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

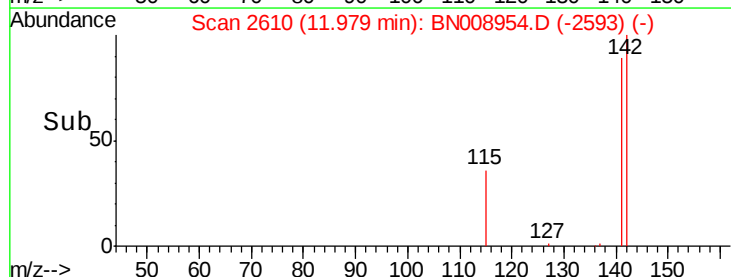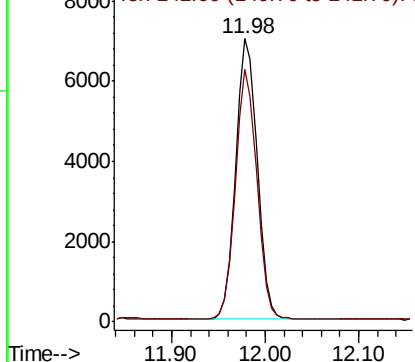

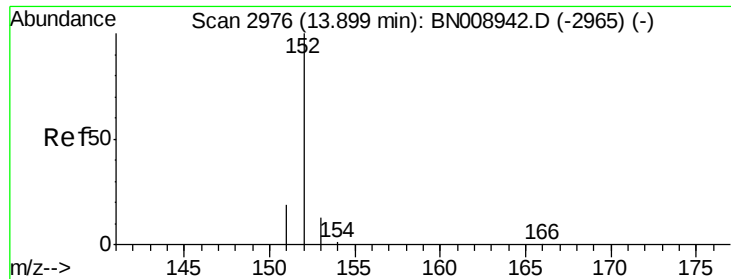

#7

Acenaphthylene

Concen: 0.437 ng/ul

RT: 13.90 min Scan# 2976

Delta R.T. -0.00 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Instrument :

BNA_N





ClientSampleId :

C0BR0

Tot Ion:	152	Resp:	18972
Ion Ratio	Lower	Upper	
152	100		
151	20.1	15.8	23.6
153	14.5	10.6	15.8

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

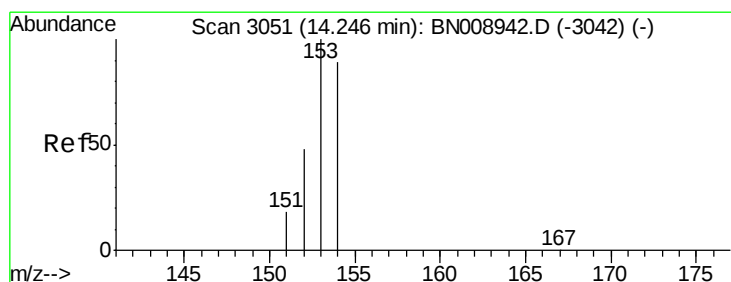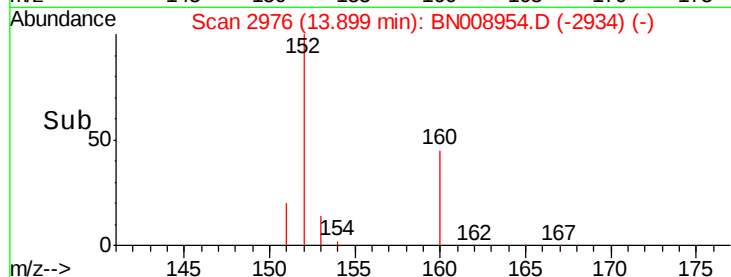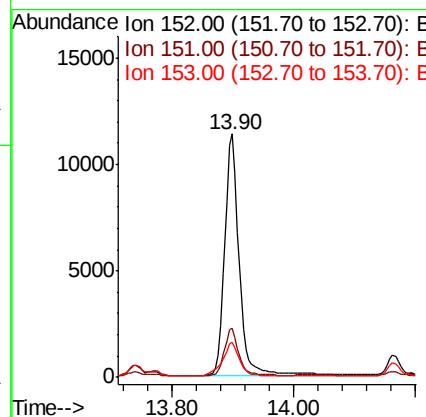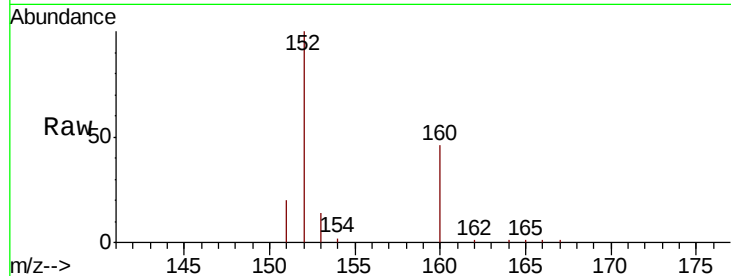

#8

Acenaphthene

Concen: 0.084 ng/ul




RT: 14.25 min Scan# 3051


Delta R.T. -0.00 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Tgt Ion:	153	Resp:	2724
Ion Ratio	Lower	Upper	
153	100		
152	54.1	38.6	58.0
154	89.8	70.6	105.8

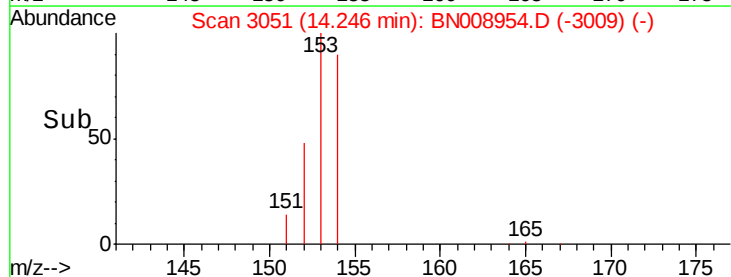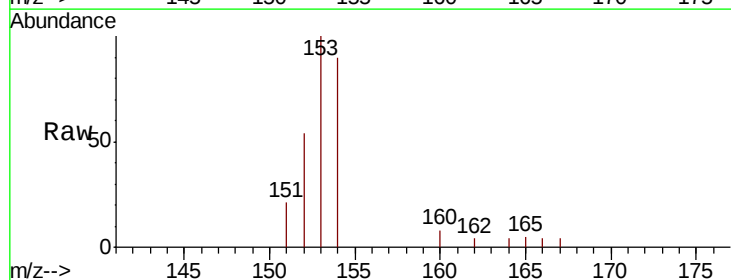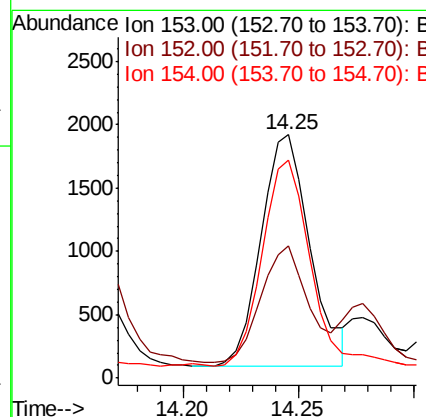

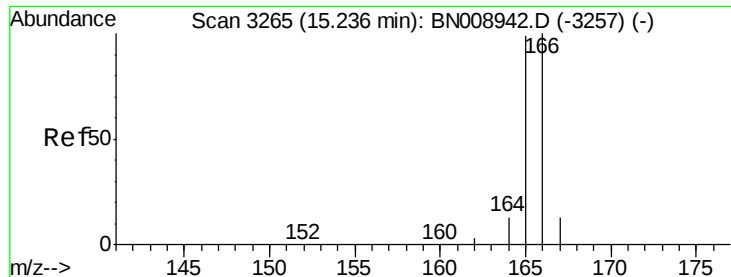

#9

Fluorene

Concen: 0.218 ng/ul

RT: 15.24 min Scan# 3265

Delta R.T. -0.00 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Instrument :

BNA_N





ClientSampleId :

C0BR0

Tot Ion:	166	Resp:	8253
Ion Ratio	Lower	Upper	
166	100		
165	100.6	77.7	116.5
167	28.8	11.1	16.7#

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

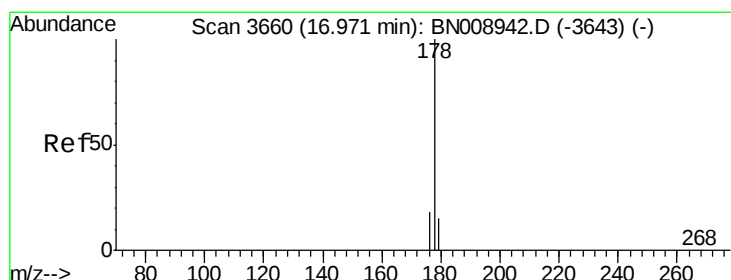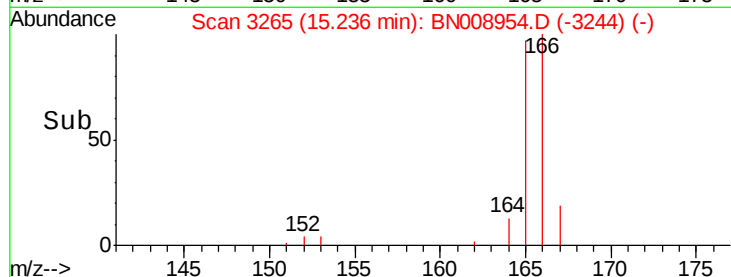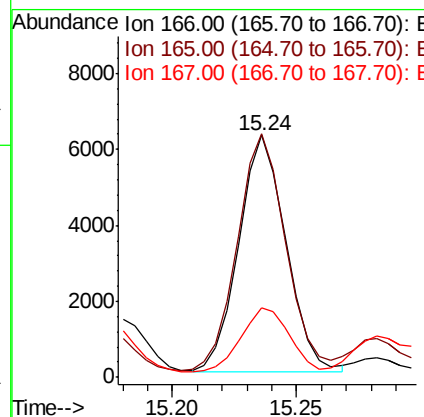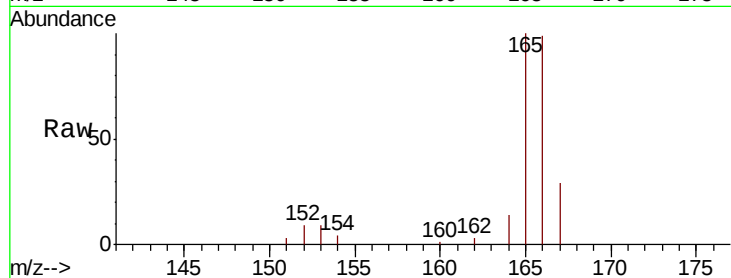

#12

Phenanthrene

Concen: 3.299 ng/ul




RT: 16.97 min Scan# 3659


Delta R.T. -0.00 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Tgt Ion:	178	Resp:	195955
Ion Ratio	Lower	Upper	
178	100		
179	15.4	12.6	18.8
176	18.6	15.3	22.9

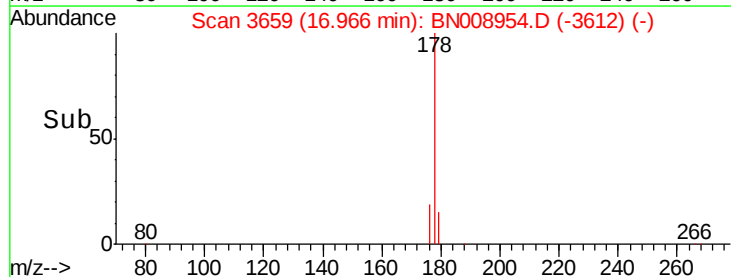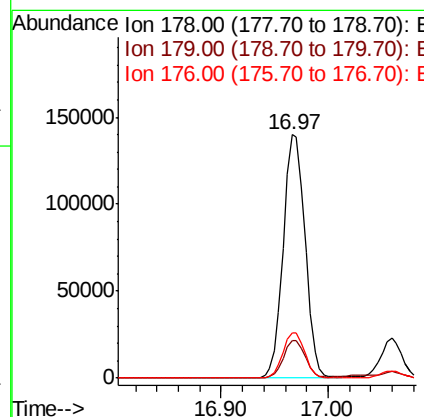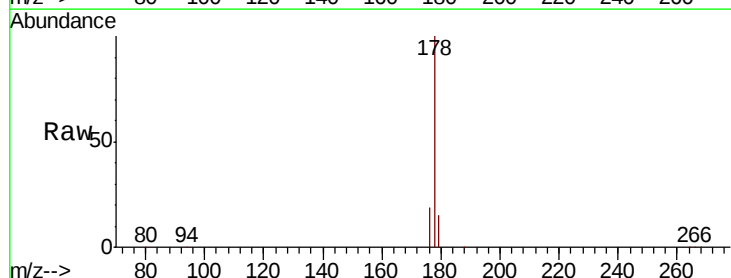

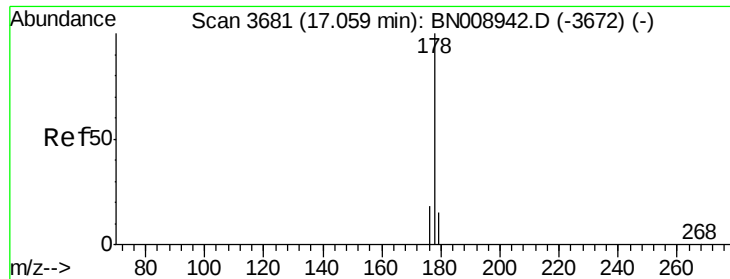





#13
 Anthracene
 Concen: 0.540 ng/ul
 RT: 17.06 min Scan# 3681
 Delta R.T. -0.00 min
 Lab File: BN008954.D
 Acq: 12 Dec 2019 20:14

Instrument :
 BNA_N
 ClientSampleId :
 C0BR0

Tot Ion	Ratio	Lower	Upper
178	100		
179	16.4	12.2	18.4
176	18.4	14.7	22.1




Manual Integrations
 APPROVED


mohammad
 12/13/2019 9:08:01 AM

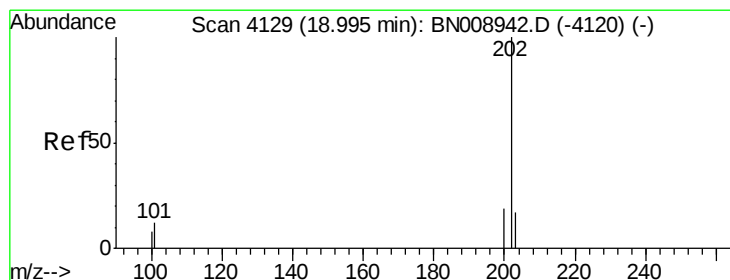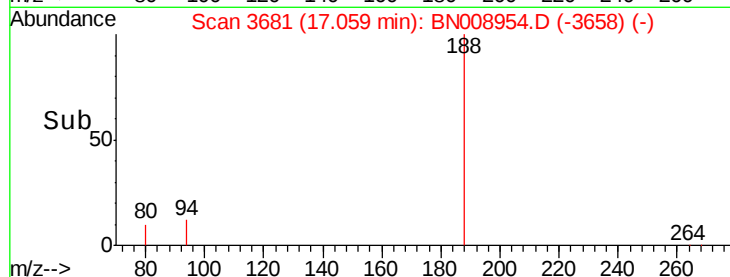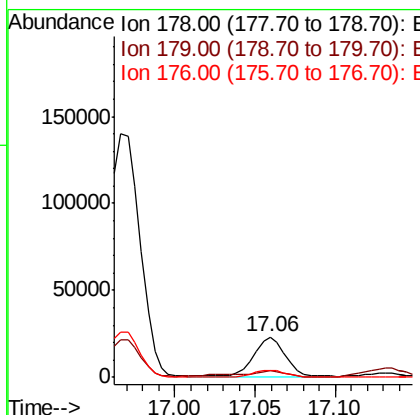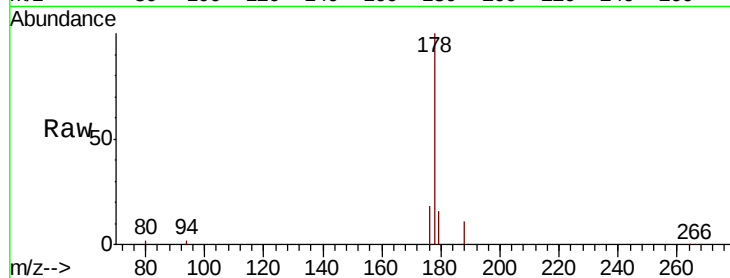

#15
 Fluoranthene
 Concen: 5.815 ng/ul
 RT: 18.99 min Scan# 4128
 Delta R.T. -0.00 min
 Lab File: BN008954.D
 Acq: 12 Dec 2019 20:14

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.4	0.0	32.4
100	9.2	0.0	29.2

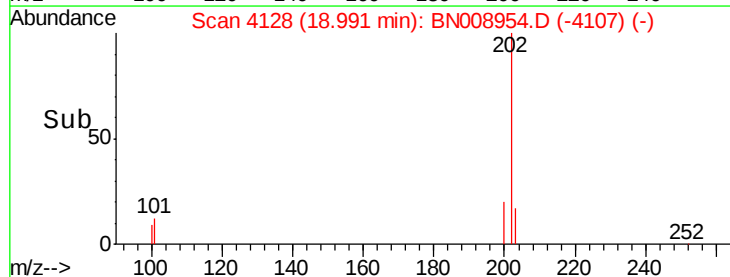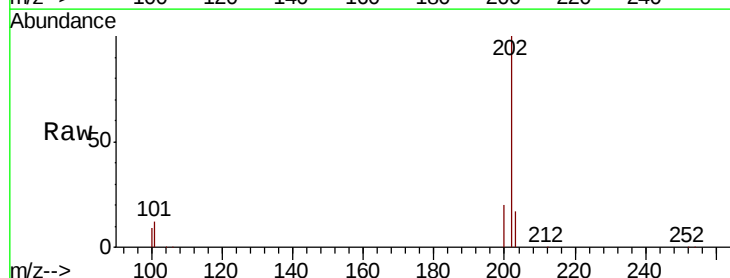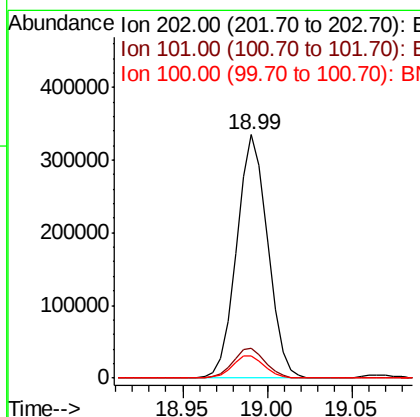

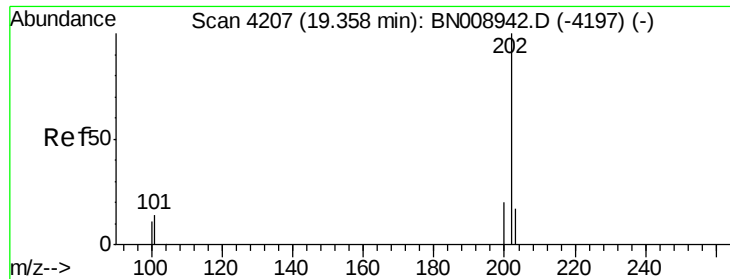





#17
Pvrene
Concen: 6.002 ng/ul
RT: 19.36 min Scan# 4207
Delta R.T. 0.00 min
Lab File: BN008954.D
Acq: 12 Dec 2019 20:14

Instrument :
BNA_N
ClientSampleId :
C0BR0

Tot Ion	Ratio	Lower	Upper
202	100		
101	13.8	12.2	18.4
100	11.0	9.5	14.3




Manual Integrations
APPROVED


mohammad
12/13/2019 9:08:01 AM

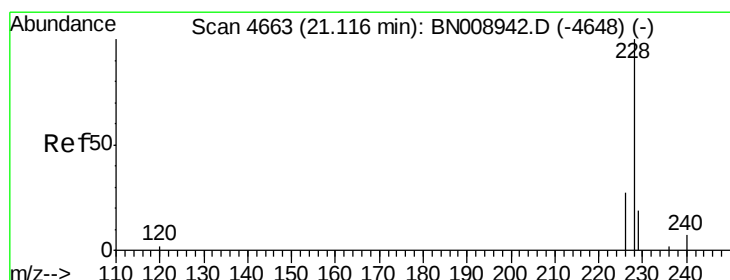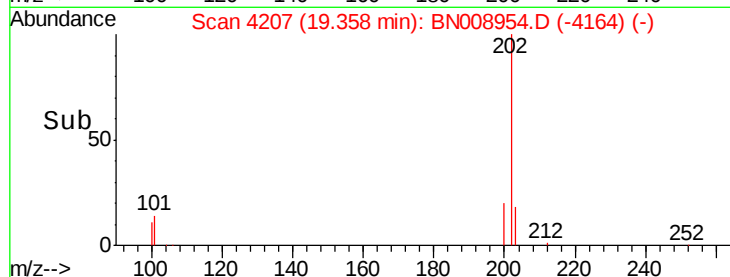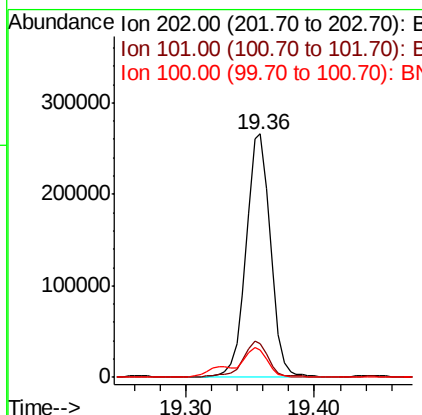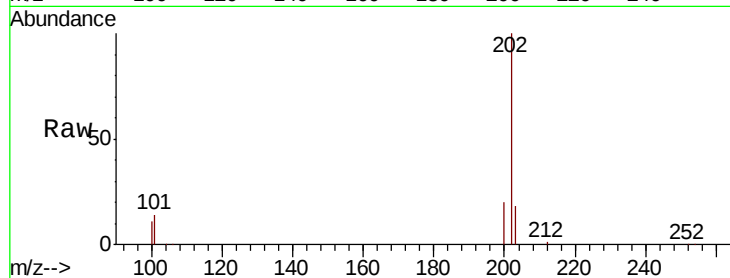

#18
Benzo(a)anthracene
Concen: 3.091 ng/ul
RT: 21.11 min Scan# 4662
Delta R.T. -0.01 min
Lab File: BN008954.D
Acq: 12 Dec 2019 20:14

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.8	15.7	23.5
226	28.7	21.5	32.3

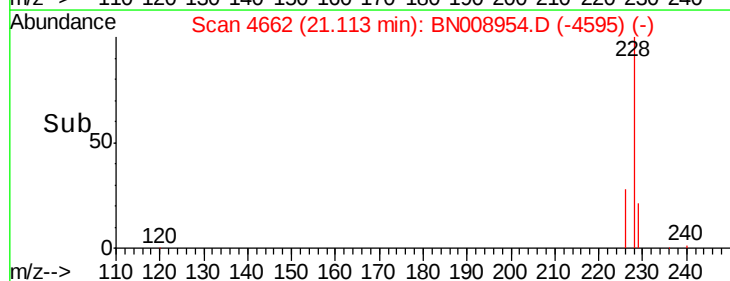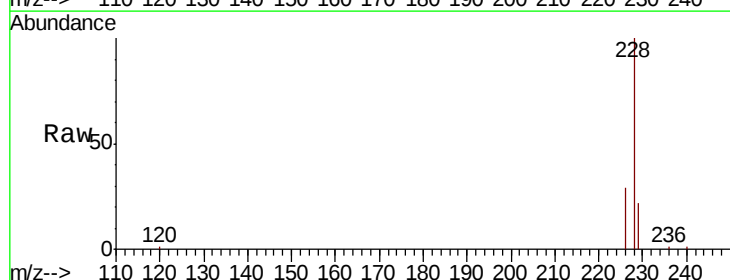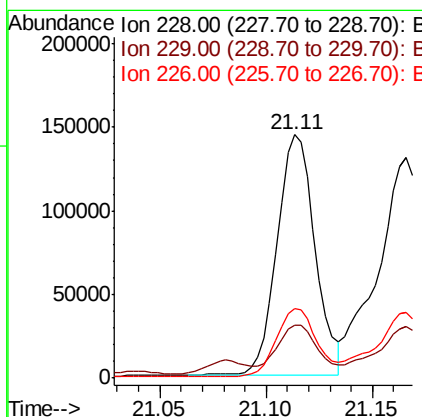

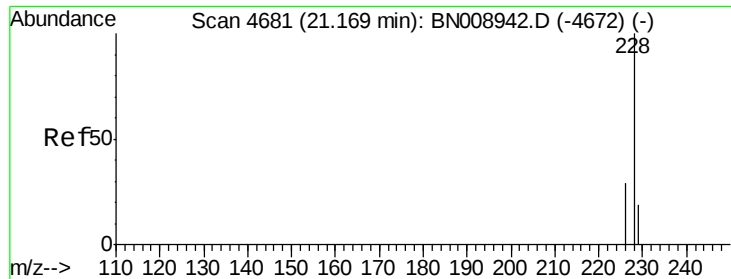

#19

Chrysene

Concen: 3.497 ng/ul

RT: 21.17 min Scan# 4680

Delta R.T. -0.01 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Instrument :

BNA_N





ClientSampleId :

C0BR0

Tot Ion:	228	Resp:	199668
Ion Ratio	Lower	Upper	
228	100		
226	29.7	23.8	35.6
229	23.2	15.6	23.4

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

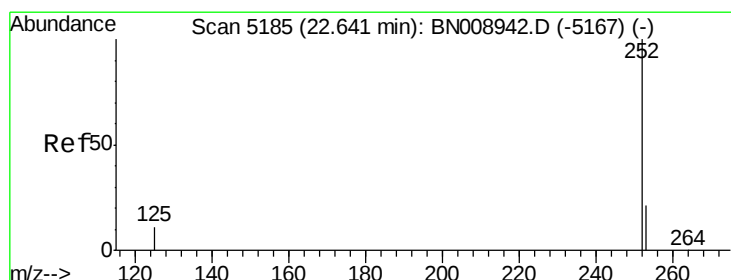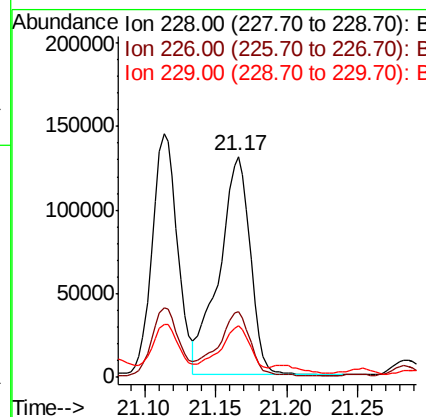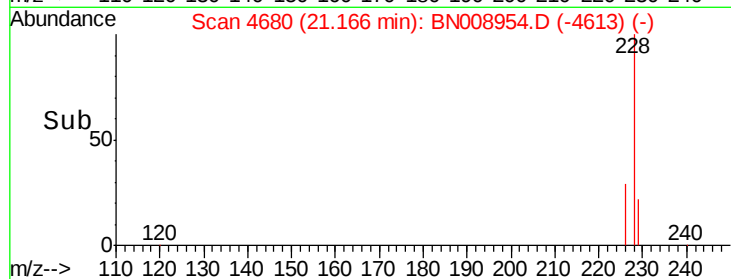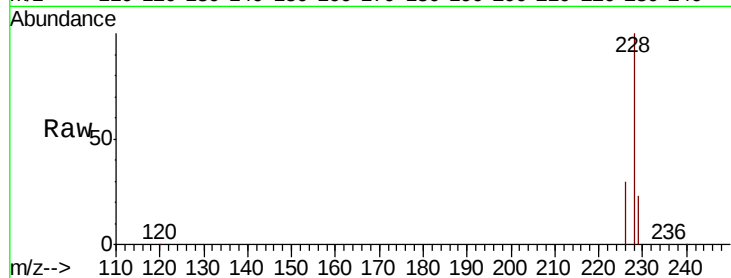

#21

Benzo(b)fluoranthene

Concen: 4.148 ng/ul m




RT: 22.64 min Scan# 5186


Delta R.T. -0.00 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Tgt Ion:	252	Resp:	239155
Ion Ratio	Lower	Upper	
252	100		
253	22.9	0.0	48.6
125	13.0	0.0	31.6

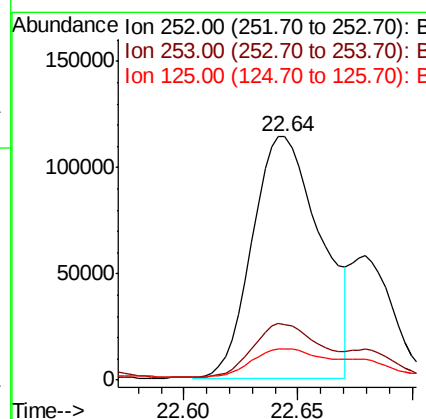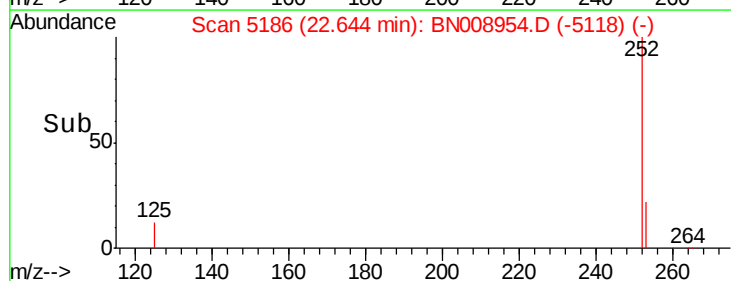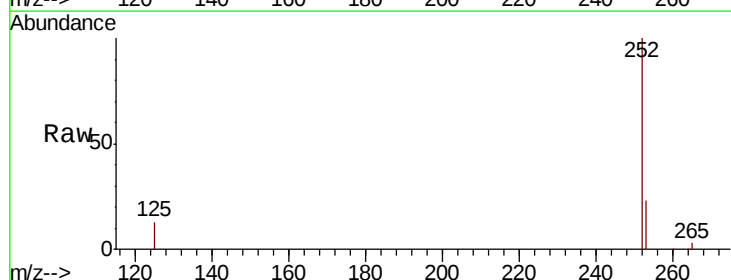

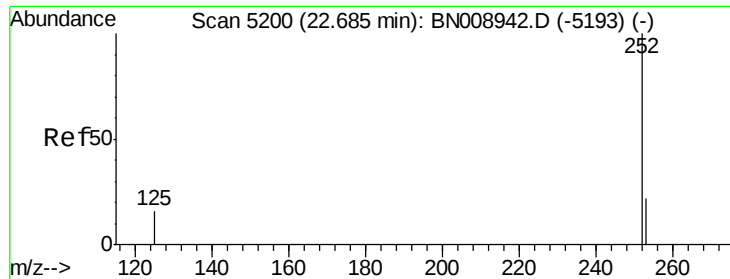

#22

Benzo(k)fluoranthene

Concen: 1.270 ng/ul m

RT: 22.68 min Scan# 5198

Delta R.T. -0.01 min

Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Instrument :

BNA_N


ClientSampleId :

C0BR0




Tot Ion:	252	Resp:	72605
Ion Ratio	Lower	Upper	
252	100		
253	24.8	19.6	29.4
125	16.4	13.8	20.6

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

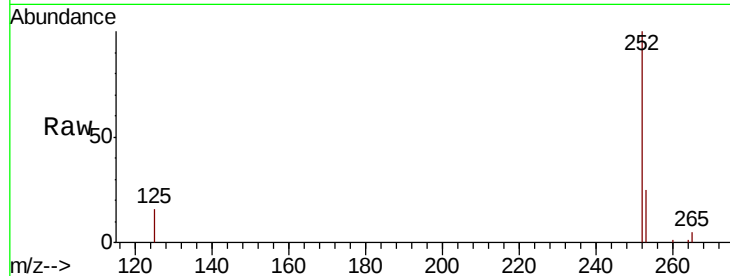

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

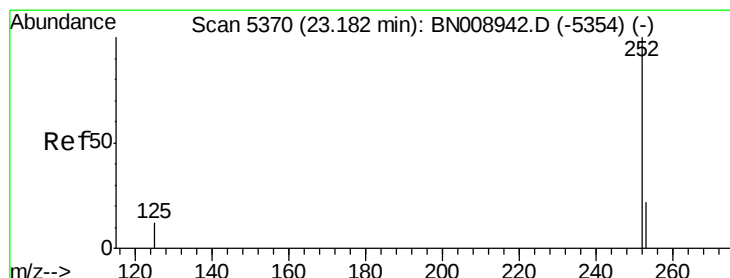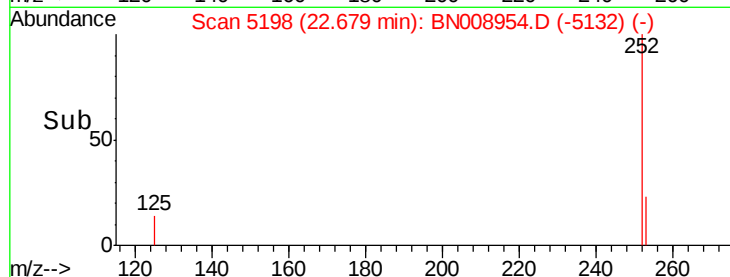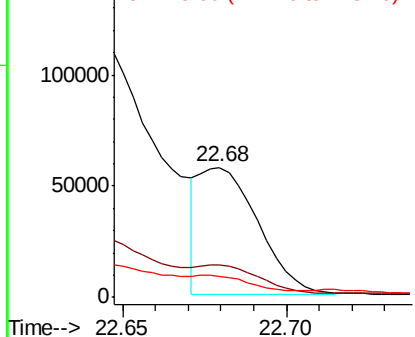

#23

Benzo(a)pyrene

Concen: 2.798 ng/ul m

RT: 23.18 min Scan# 5370




Delta R.T. -0.01 min


Lab File: BN008954.D

Acq: 12 Dec 2019 20:14

Tgt Ion:	252	Resp:	151387
Ion Ratio	Lower	Upper	
252	100		
253	23.2	19.9	29.9
125	13.6	14.6	22.0#

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

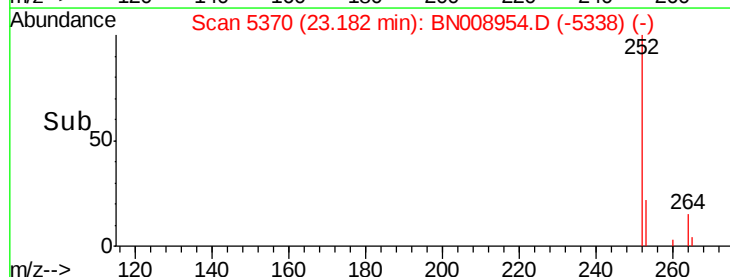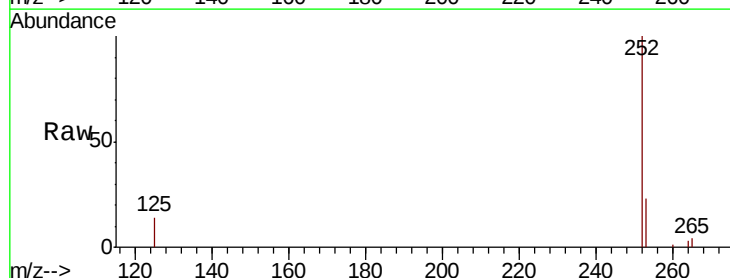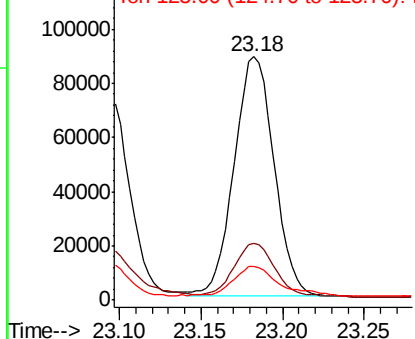

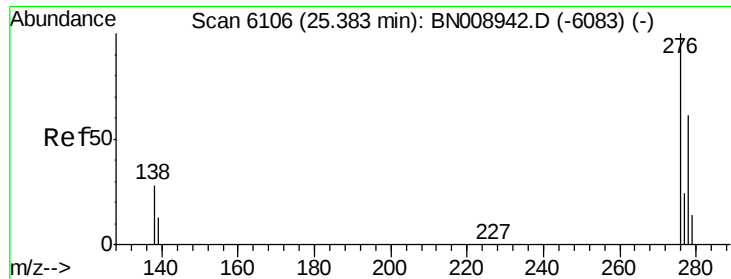





#24
Indeno(1,2,3-cd)pyrene
Concen: 1.575 ng/ul
RT: 25.38 min Scan# 6105
Delta R.T. -0.01 min
Lab File: BN008954.D
Acq: 12 Dec 2019 20:14

Instrument :
BNA_N
ClientSampleId :
C0BR0

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.5	23.8	35.6
227	0.2	0.2	0.2




Manual Integrations
APPROVED


mohammad
12/13/2019 9:08:01 AM

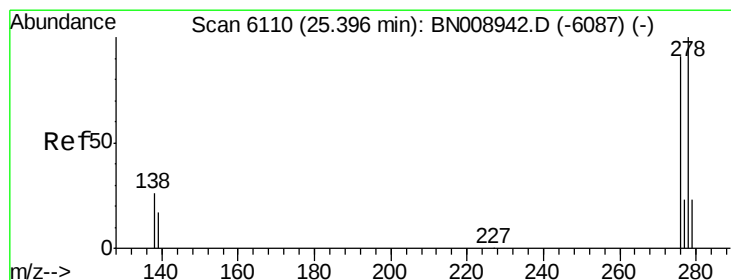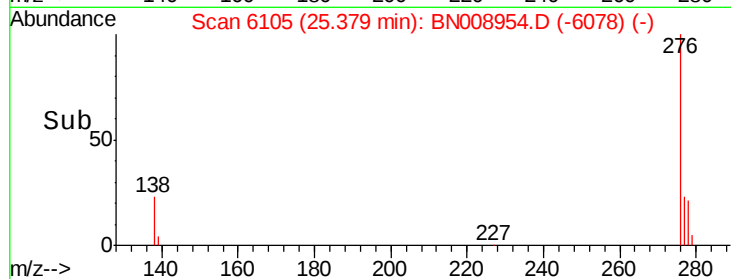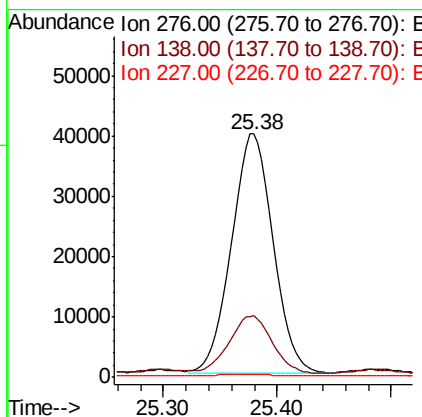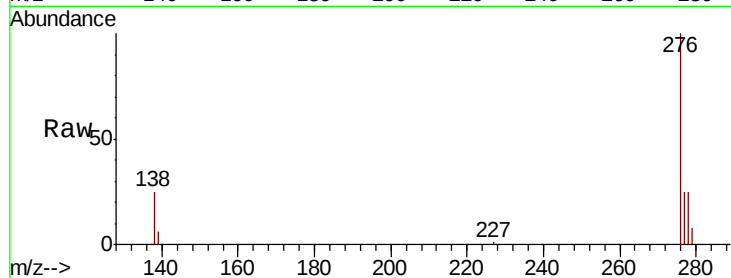

#25
Dibenzo(a,h)anthracene
Concen: 0.579 ng/ul
RT: 25.38 min Scan# 6106
Delta R.T. -0.02 min
Lab File: BN008954.D
Acq: 12 Dec 2019 20:14

Tgt Ion	Ratio	Lower	Upper
278	100		
139	24.8	17.4	26.0
279	32.6	20.5	30.7

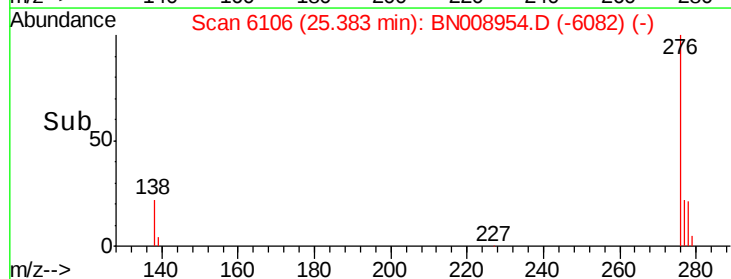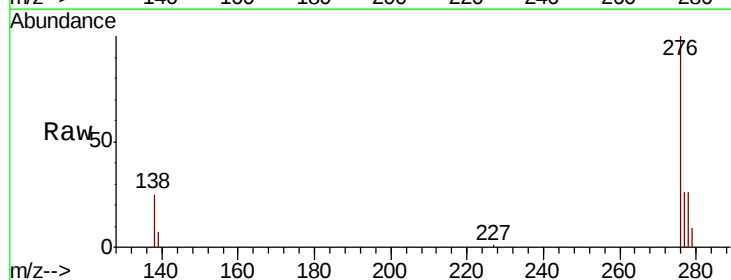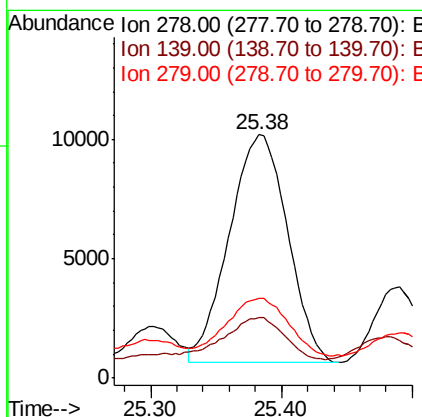

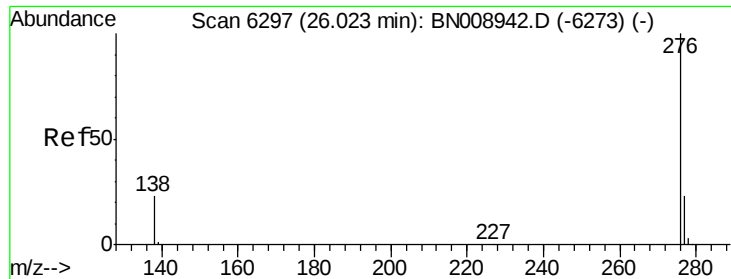

#26
Benzo(a,h,i)perylene
Concen: 2.005 ng/ul
RT: 26.02 min Scan# 6296
Delta R.T. -0.01 min
Lab File: BN008954.D
Acq: 12 Dec 2019 20:14

Instrument :
BNA_N
ClientSampleId :
C0BR0

Tot Ion	Ratio	Lower	Upper
276	100		
138	25.1	21.9	32.9
277	24.3	19.9	29.9

Manual Integrations
APPROVED

mohammad
12/13/2019 9:08:01 AM

