
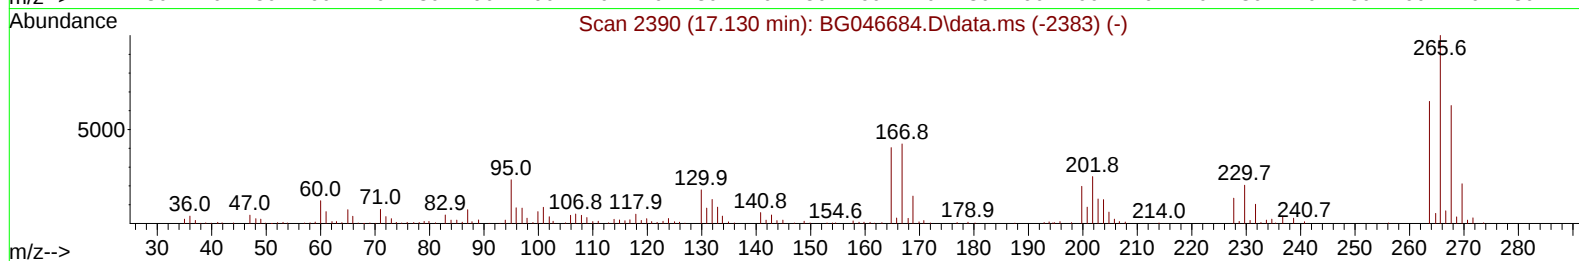
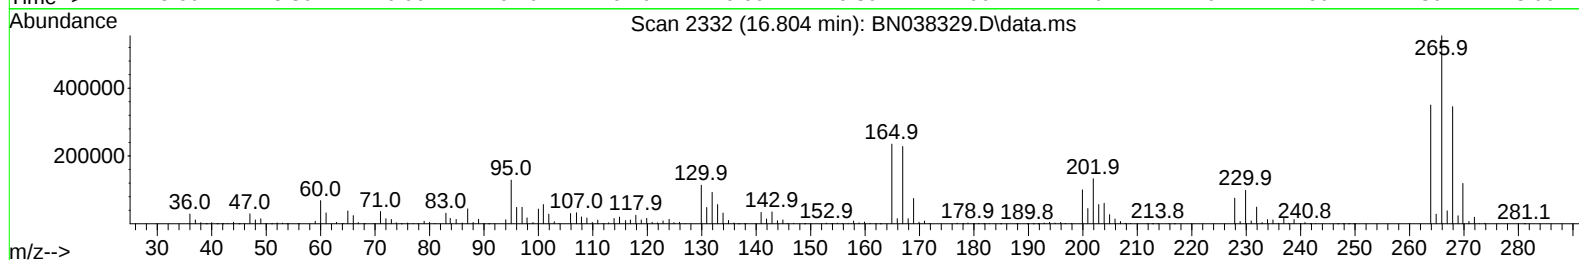


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038329.D
Acq On : 11 Dec 2025 23:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 03:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

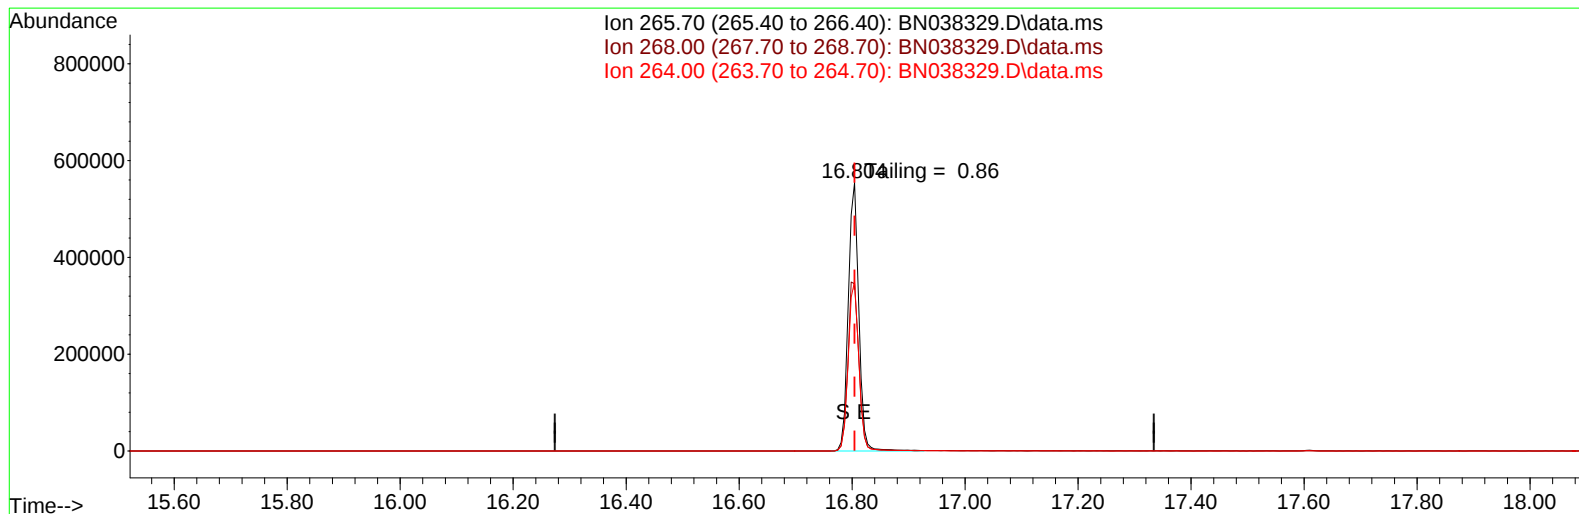

TIC: BN038329.D\data.ms

(70) Pentachlorophenol (C)




16.804min (0.000) 217492.83 ng

response 718575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.31
264.00	61.60	63.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121125\
Data File : BN038329.D
Acq On : 11 Dec 2025 23:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 03:10:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

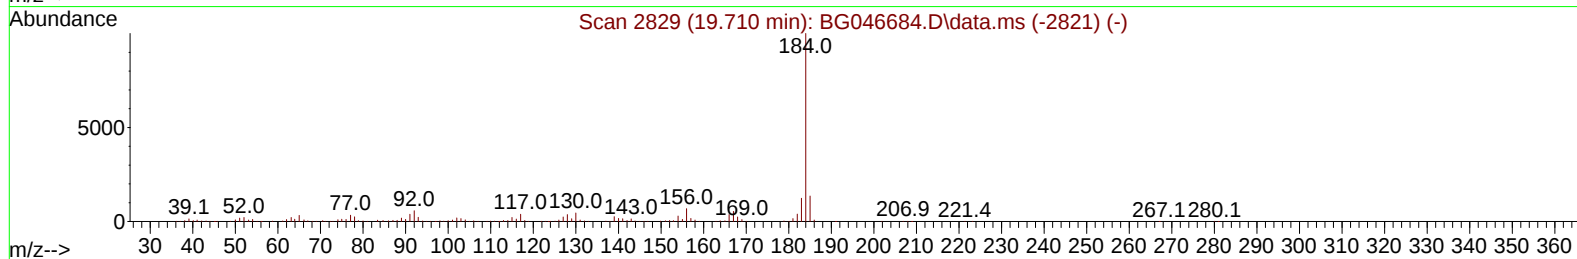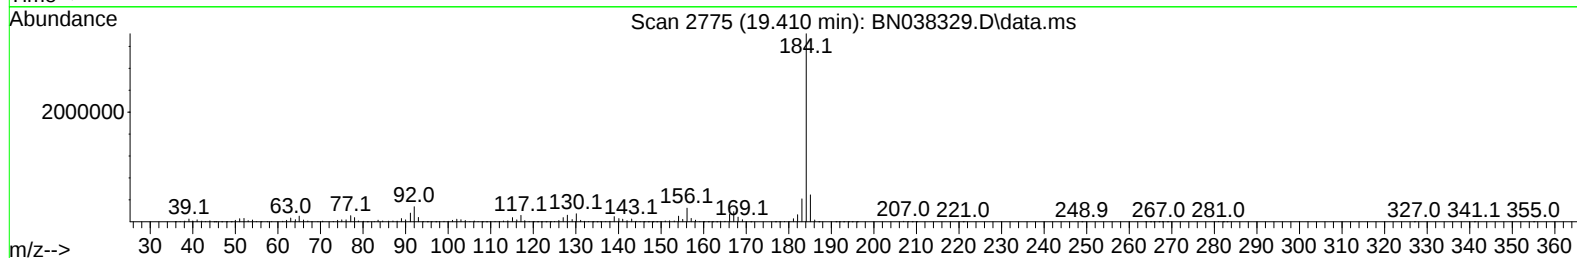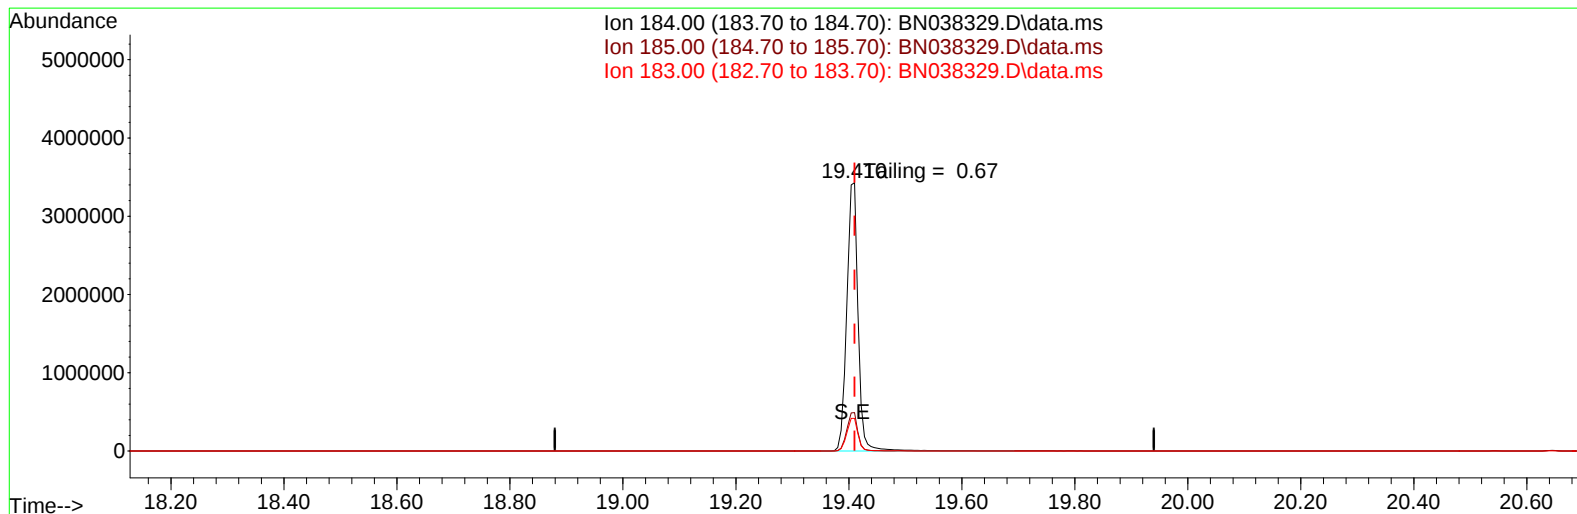

TIC: BN038329.D\data.ms

(77) Benzidine**19.410min (0.000) 4649.10 ng****response 4774950**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.32
183.00	13.20	12.17
0.00	0.00	0.00