


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121218\
Data File : BN003865.D
Acq On : 12 Dec 2018 23:29
Operator : JU/SJ
Sample : J6299-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F37

Manual Integrations
APPROVED

Sohil
12/13/2018 6:12:32 PM

Quant Time: Dec 13 12:28:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 04:12:26 2018
Response via : Initial Calibration

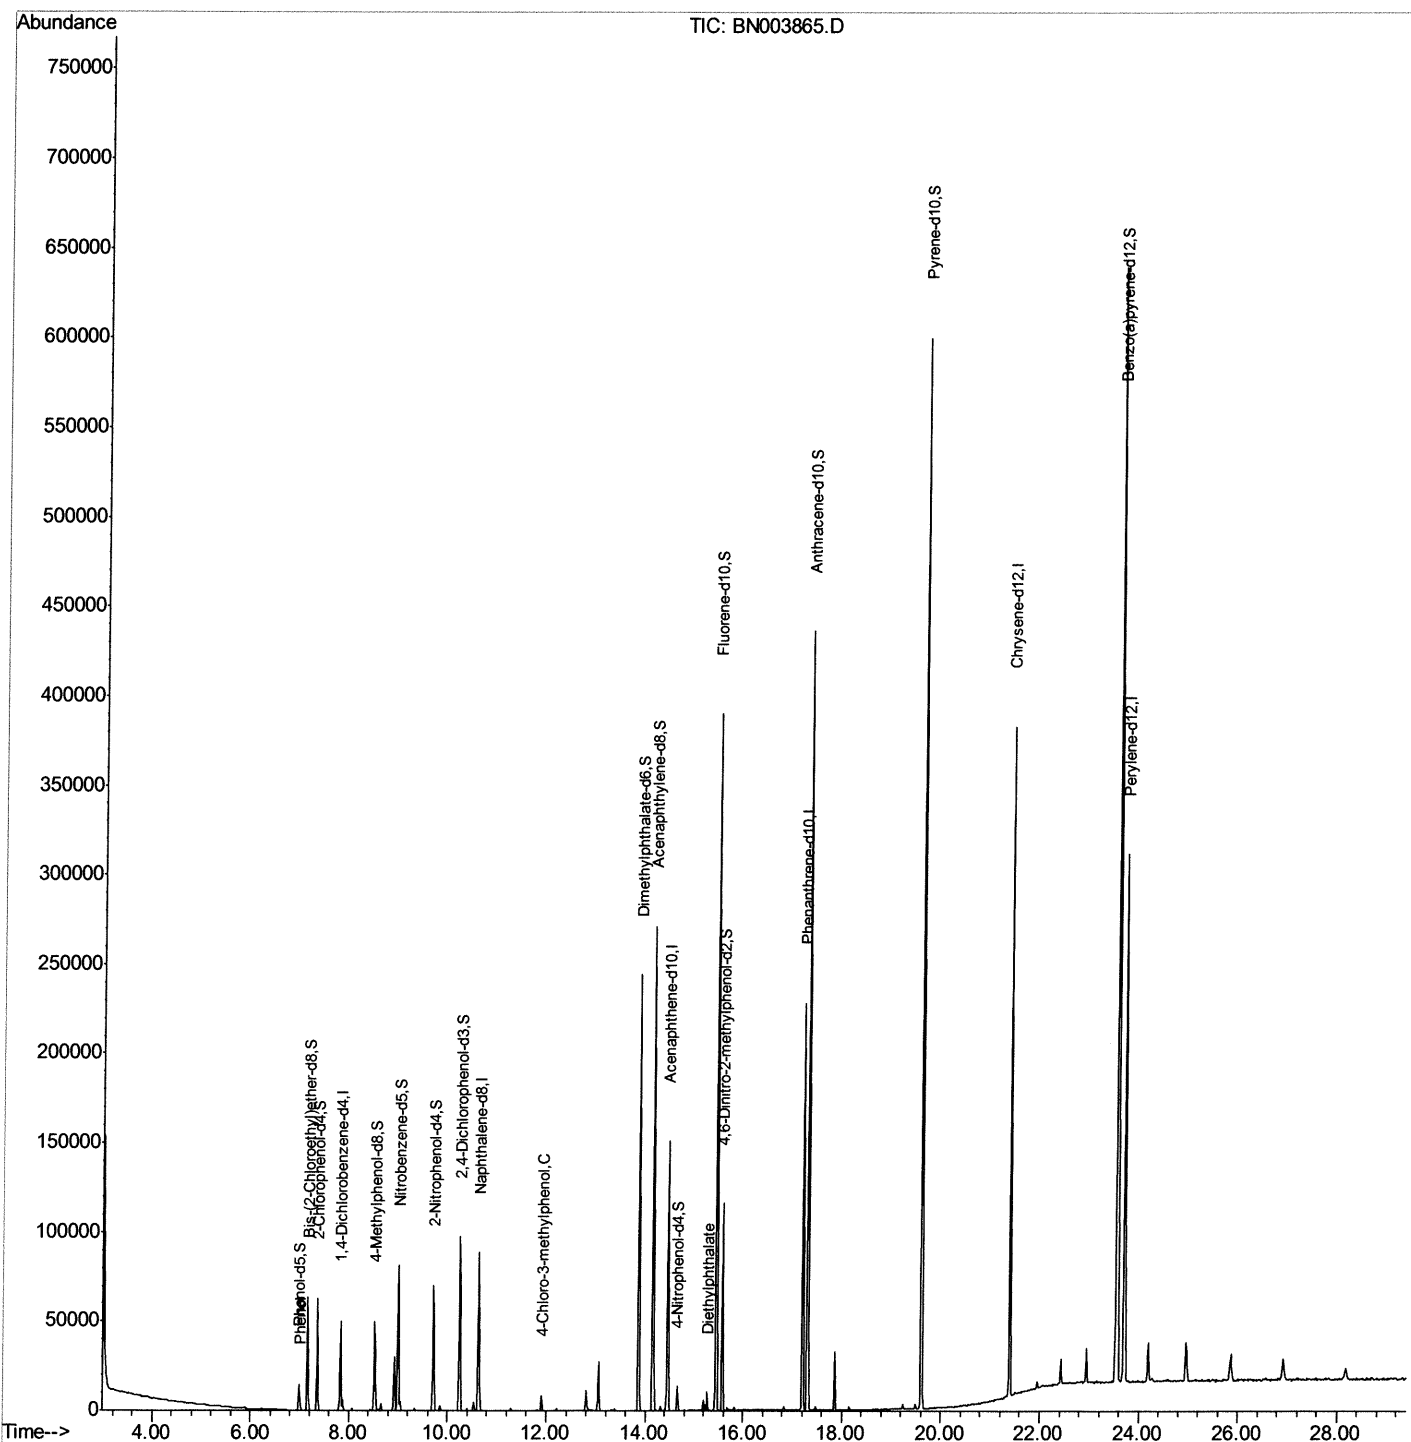

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121218\
 Data File : BN003865.D
 Acq On : 12 Dec 2018 23:29
 Operator : JU/SJ
 Sample : J6299-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F37

Manual Integrations
 APPROVED

Sohil
 12/13/2018 6:12:32 PM

Quant Time: Dec 13 05:54:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration

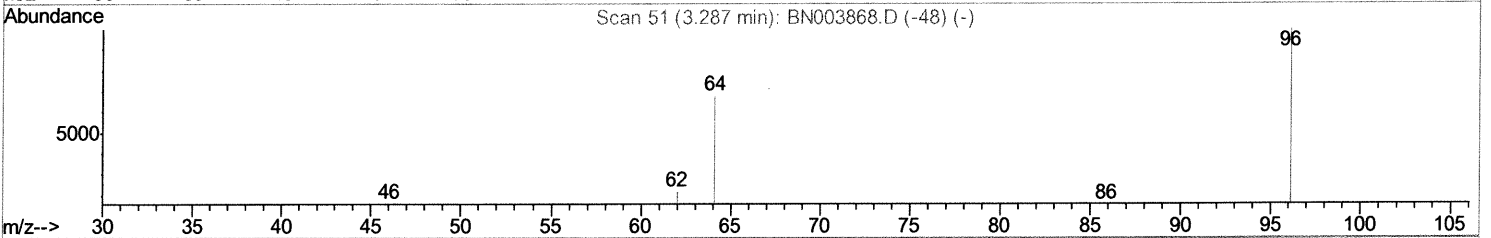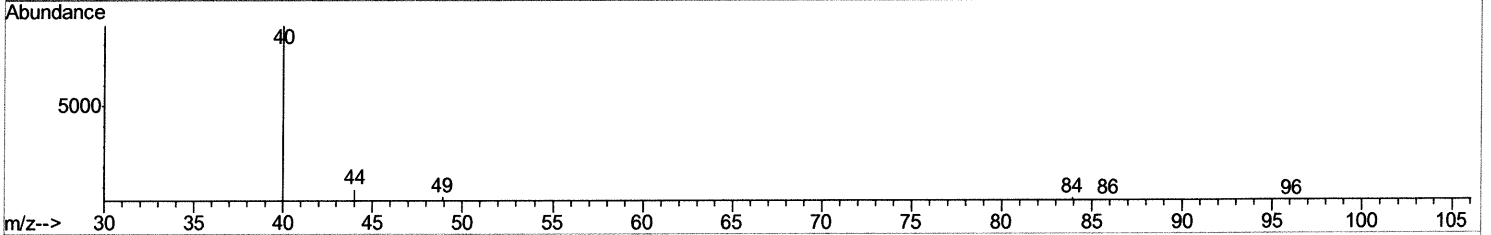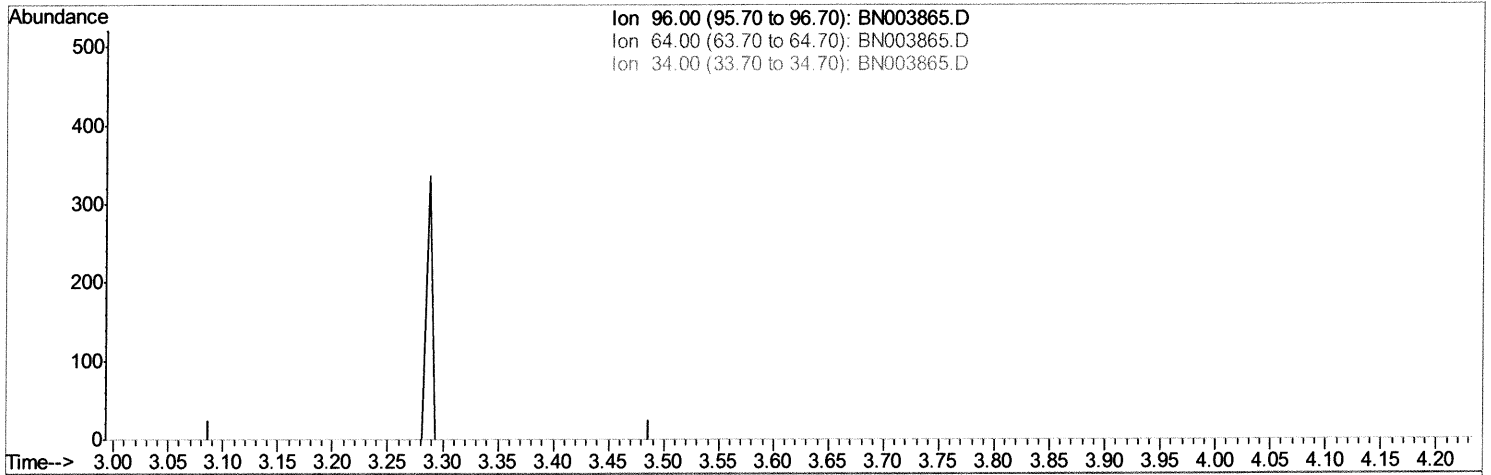

TIC: BN003865.D

(3) 1,4-Dioxane-d8 (S)

3.287min (-3.287) 0.00ng/uL

response 0

Ion	Exp%	Act%
96.00	100	0.00
64.00	66.10	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121218\
Data File : BN003865.D
Acq On : 12 Dec 2018 23:29
Operator : JU/SJ
Sample : J6299-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F37

Manual Integrations
APPROVED

Sohil
12/13/2018 6:12:32 PM

Quant Time: Dec 13 05:54:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 04:12:26 2018
Response via : Initial Calibration

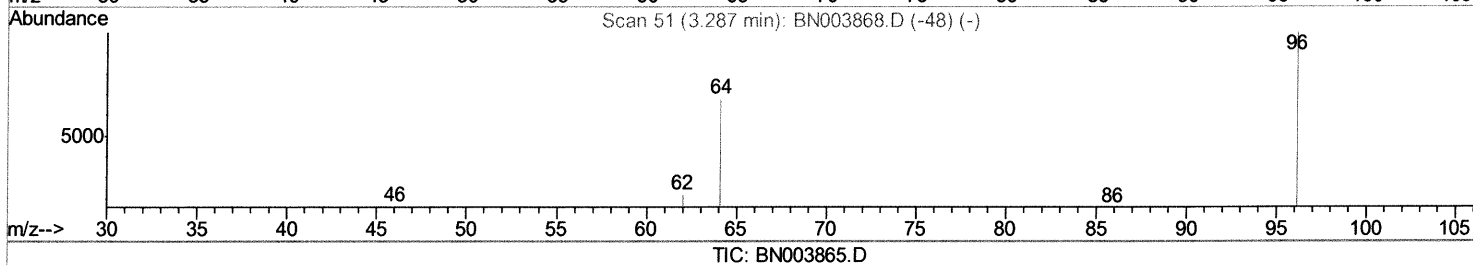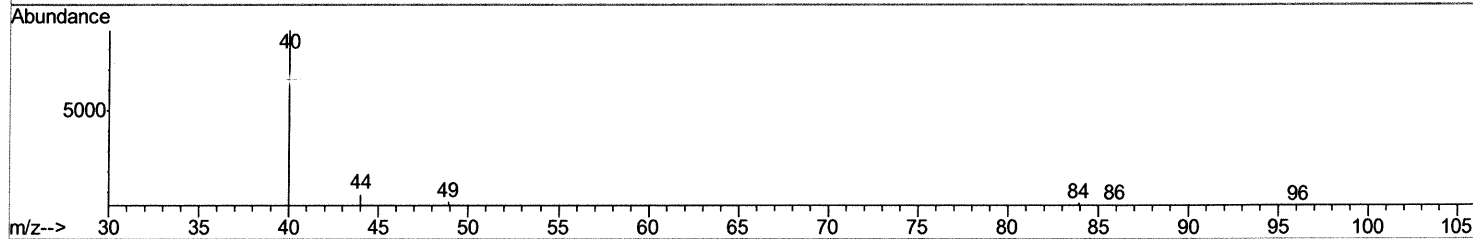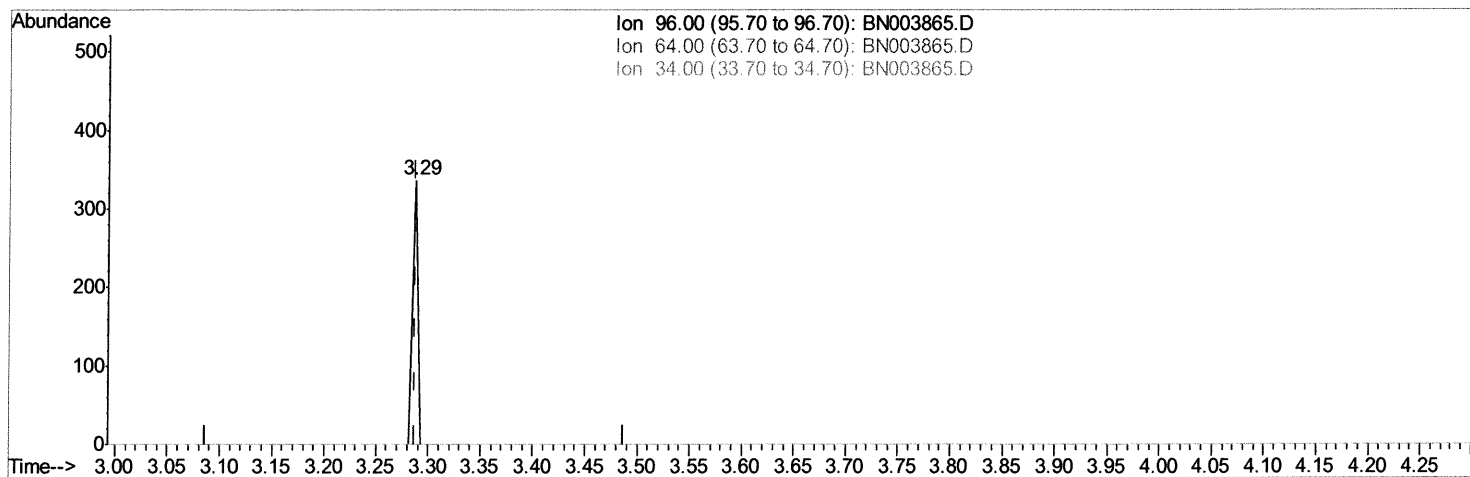

(3) 1,4-Dioxane-d8 (S)

3.287min (+0.000) 0.49ng/uL m> SJ 12/13/18

response 119

Ion	Exp%	Act%
96.00	100	100
64.00	66.10	0.00#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121218\
 Data File : BN003865.D
 Acq On : 12 Dec 2018 23:29
 Operator : JU/SJ
 Sample : J6299-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F37

Manual Integrations
 APPROVED

Sohil
 12/13/2018 6:12:32 PM

Quant Time: Dec 13 12:28:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	16036	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	79593	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	51886	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	131779	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	179287	20.00	ng/ul	0.00
85) Perylene-d12	23.70	264	222535	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	119m>	0.49	ng/uL	0.00
5) Phenol-d5	6.99	99	9959	6.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	29644	34.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	33014	26.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	20899	15.82	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	23017	36.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	25314	35.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	40562	30.96	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	169105	36.51	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	200820	36.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	5112	5.34	ng/ul	0.00
57) Fluorene-d10	15.46	176	149765	37.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	27562	29.04	ng/ul	0.00
70) Anthracene-d10	17.31	188	247666	37.19	ng/ul	0.00
78) Pyrene-d10	19.60	212	299777	37.38	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	460119	38.11	ng/ul	0.00

SD 12/13/18

Target Compounds

					Qvalue
6) Phenol	7.01	94	2062	1.296 ng/ul	96
33) 4-Chloro-3-methylphenol	11.90	107	4817	3.284 ng/ul	100
56) Diethylphthalate	15.27	149	6840	1.480 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed