

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121218\
 Data File : BN003855.D
 Acq On : 12 Dec 2018 17:39
 Operator : JU/SJ
 Sample : J6228-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E77

Quant Time: Dec 13 04:15:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	16895	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	83831	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	54459	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	135422	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	186746	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	228720	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	1410	5.46	ng/uL	0.00
5) Phenol-d5	6.99	99	43002	25.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	26616	29.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	35937	27.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	36854	26.48	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	19840	29.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	22502	29.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	37723	27.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	60243	46.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	156431	32.18	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	179397	31.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	26849	26.71	ng/ul	0.00
57) Fluorene-d10	15.46	176	134318	31.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	24065	24.67	ng/ul	0.00
70) Anthracene-d10	17.31	188	226909	33.16	ng/ul	0.00
78) Pyrene-d10	19.60	212	278653	33.36	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.57	264	417355	33.64	ng/ul	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.01	94	10415	6.212	ng/ul	97
44) Dimethylphthalate	13.92	163	54541	11.493	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121218\
 Data File : BN003855.D
 Acq On : 12 Dec 2018 17:39
 Operator : JU/SJ
 Sample : J6228-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E77

Quant Time: Dec 13 04:15:36 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration




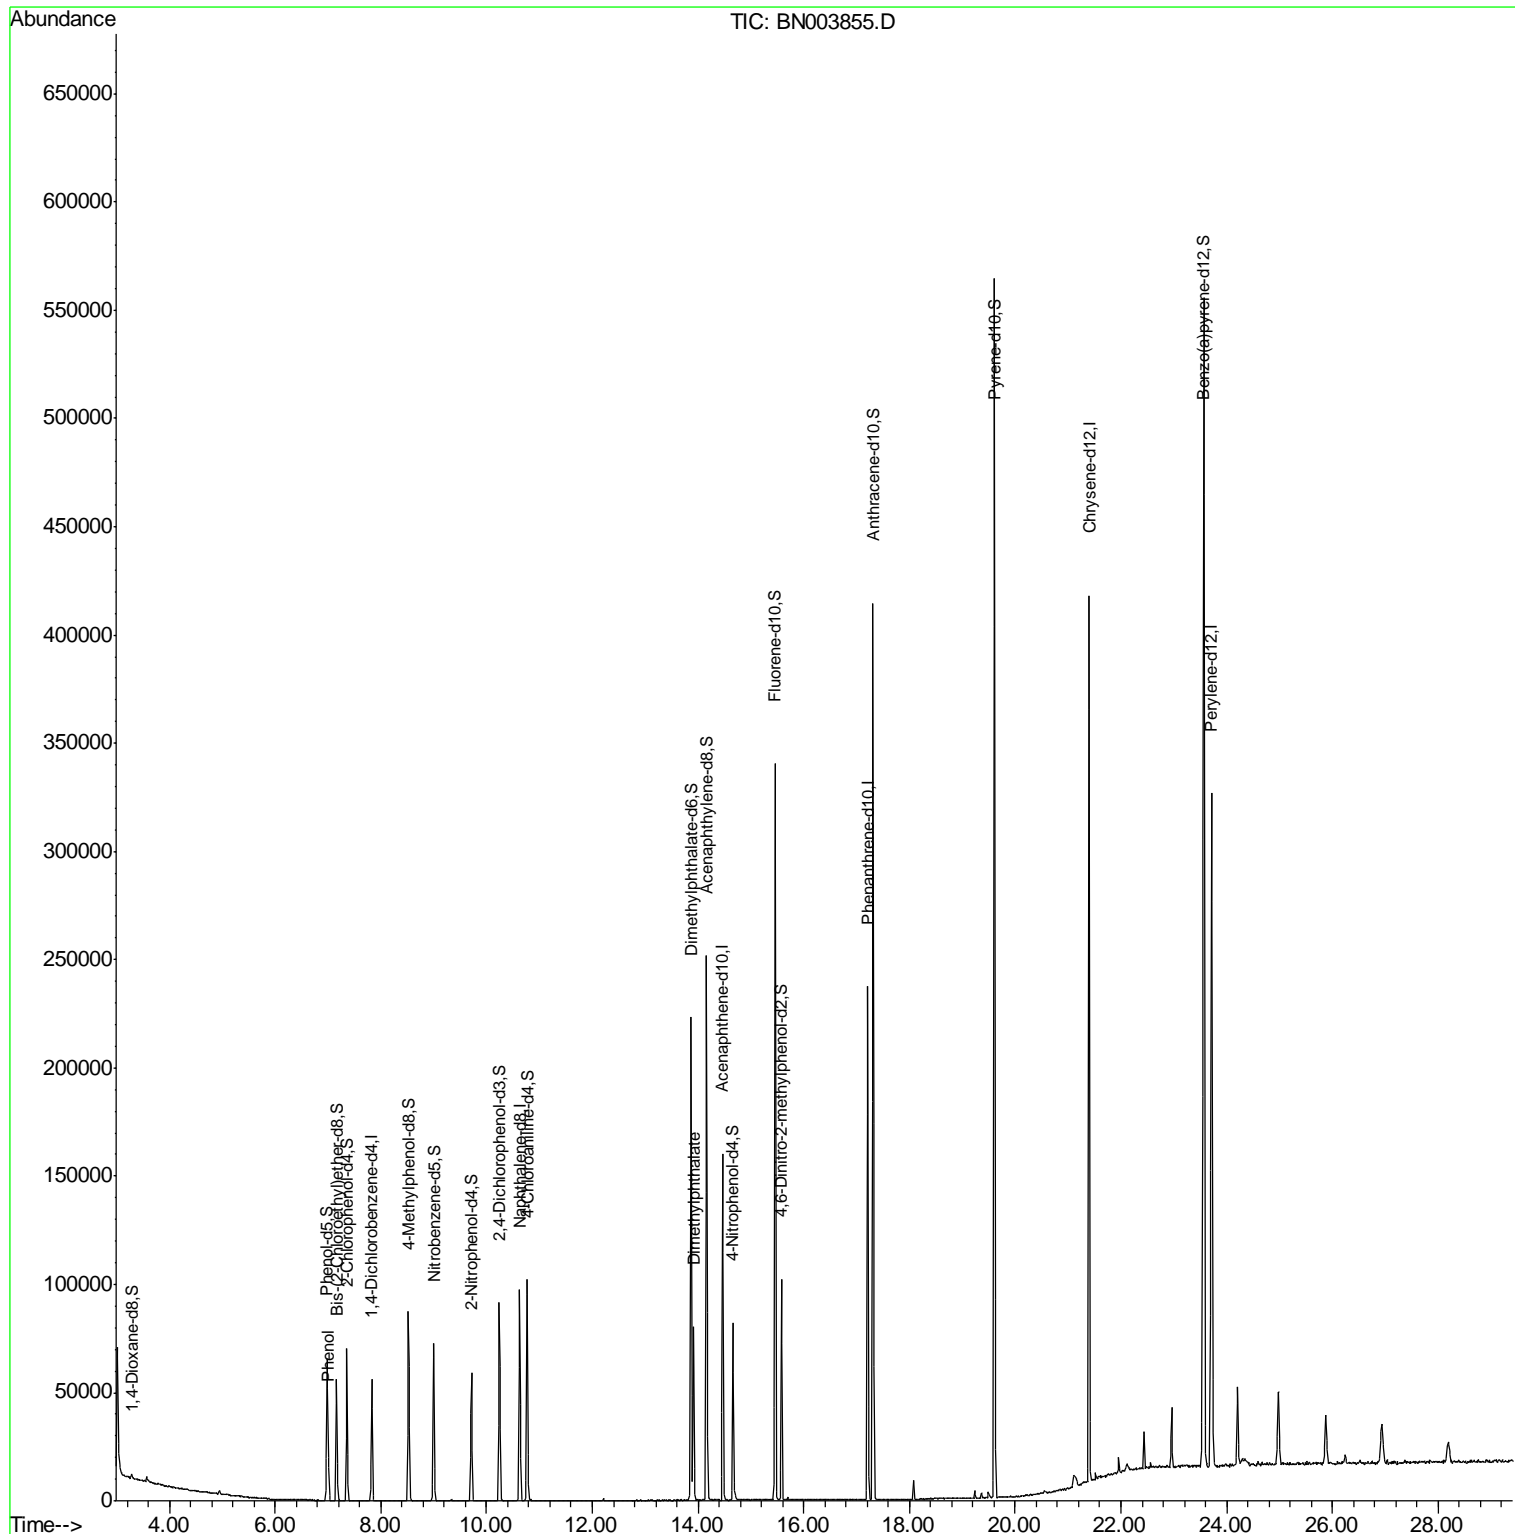


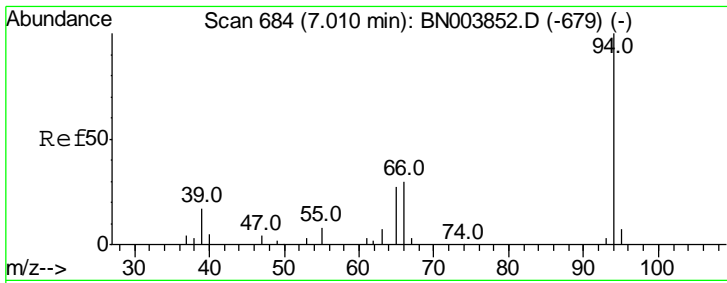

#6
 Phenol
 Concen: 6.212 ng/ul
 RT: 7.01 min Scan# 684
 Delta R.T. 0.00 min
 Lab File: BN003855.D
 Acq: 12 Dec 2018 17:39

Instrument :
 BNA_N
 ClientSampled :
 F9E77

Tgt Ion	Resp	Lower	Upper
94	10415		
65	27.6	21.2	31.8
66	35.4	26.9	40.3

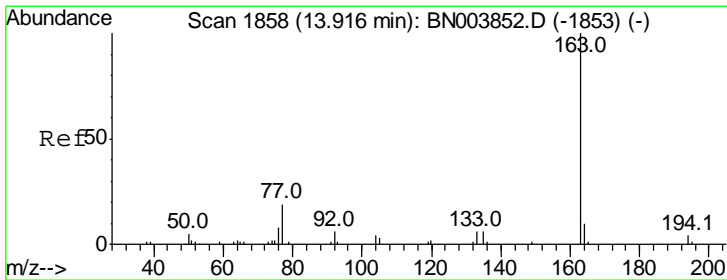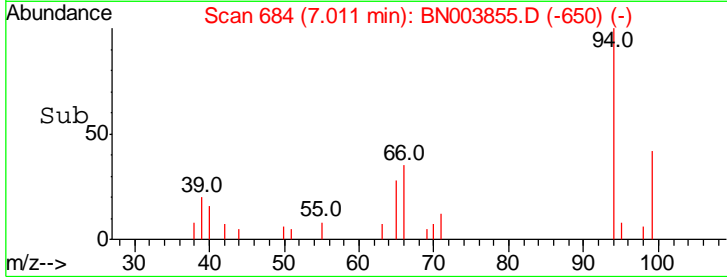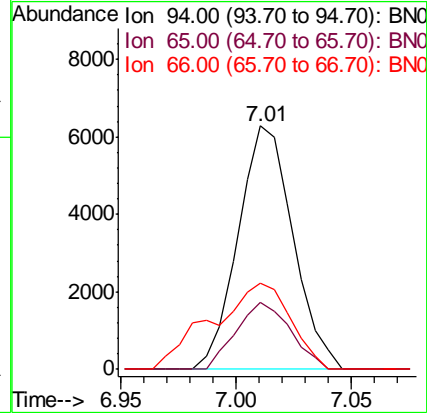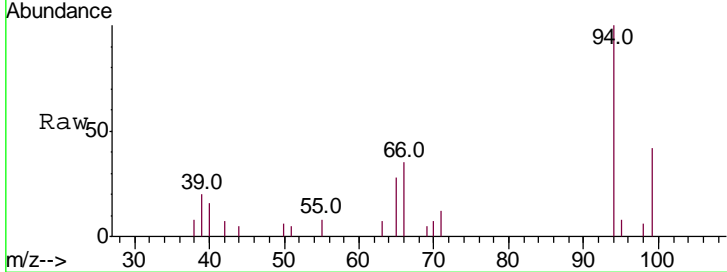

#44
 Dimethylphthalate
 Concen: 11.493 ng/ul
 RT: 13.92 min Scan# 1858
 Delta R.T. 0.00 min
 Lab File: BN003855.D
 Acq: 12 Dec 2018 17:39

Tgt Ion	Resp	Lower	Upper
163	54541		
194	4.3	3.4	5.0
164	10.6	7.9	11.9

