

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121218\
 Data File : BN003859.D
 Acq On : 12 Dec 2018 19:59
 Operator : JU/SJ
 Sample : J6228-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E89

Quant Time: Dec 13 04:16:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	20433	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	102009	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	65652	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	165926	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	219545	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	267985	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	1863	5.97	ng/uL	0.00
5) Phenol-d5	6.99	99	57881	28.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	35395	32.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	47987	30.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	49163	29.20	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	27548	34.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	31483	34.39	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	53182	31.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	82109	52.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	216969	37.02	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	252909	36.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	41459	34.22	ng/ul	0.00
57) Fluorene-d10	15.46	176	189025	37.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	36312	30.39	ng/ul	0.00
70) Anthracene-d10	17.31	188	312680	37.29	ng/ul	0.00
78) Pyrene-d10	19.60	212	384797	39.18	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	568294	39.09	ng/ul	0.00
Target Compounds						
6) Phenol	7.01	94	14788	7.293	ng/ul	98
44) Dimethylphthalate	13.92	163	74139	12.959	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121218\
Data File : BN003859.D
Acq On : 12 Dec 2018 19:59
Operator : JU/SJ
Sample : J6228-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E89

Quant Time: Dec 13 04:16:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 04:12:26 2018
Response via : Initial Calibration

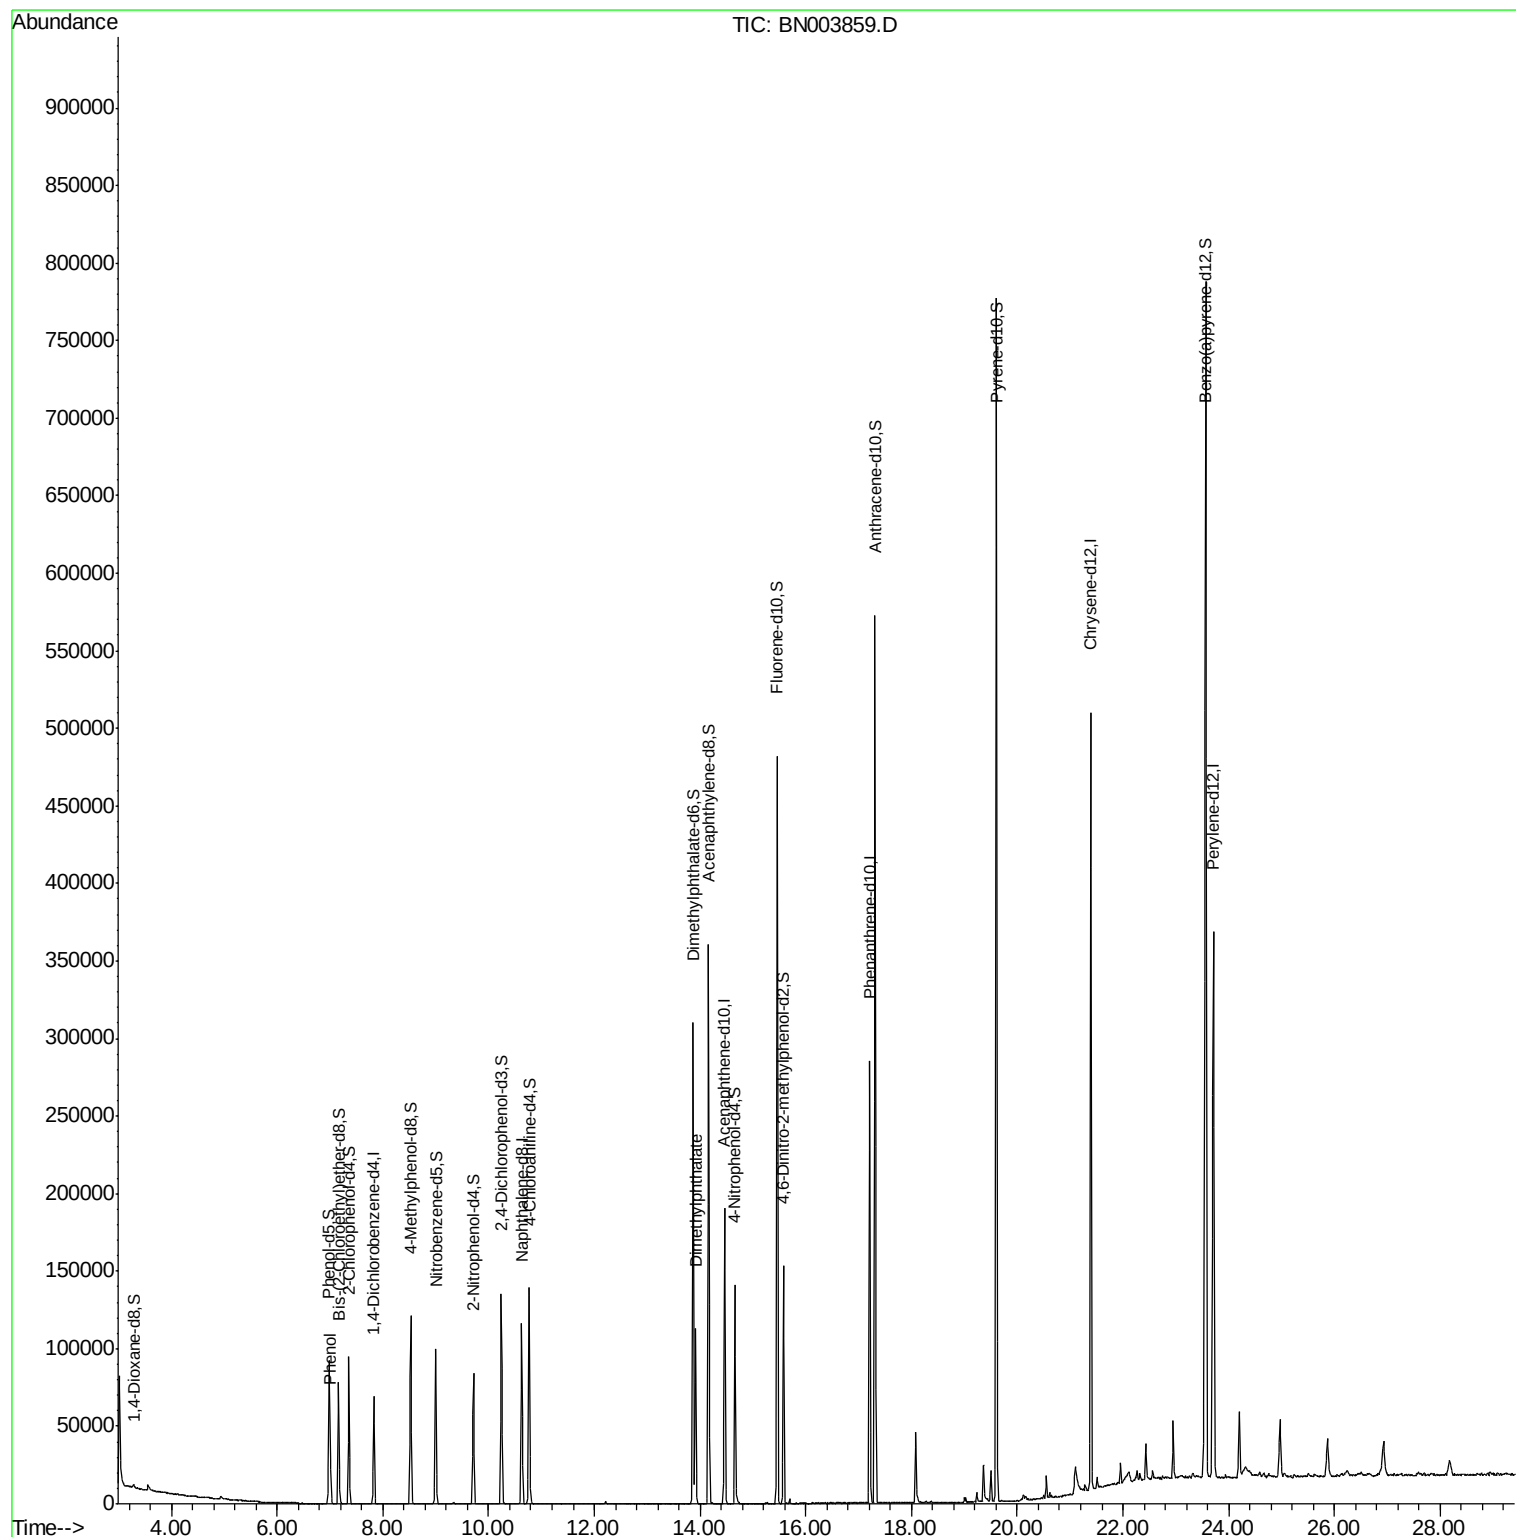

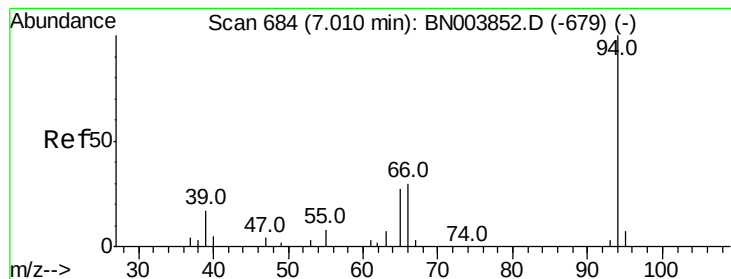

#6

Phenol

Concen: 7.293 ng/ul

RT: 7.01 min Scan# 684

Delta R.T. 0.00 min

Lab File: BN003859.D

Acq: 12 Dec 2018 19:59

Instrument :

BNA_N

ClientSampleId :

F9E89





Tot Ion: 94 Resp: 14788

Ion Ratio Lower Upper

94 100

65 26.6 21.2 31.8

66 35.2 26.9 40.3

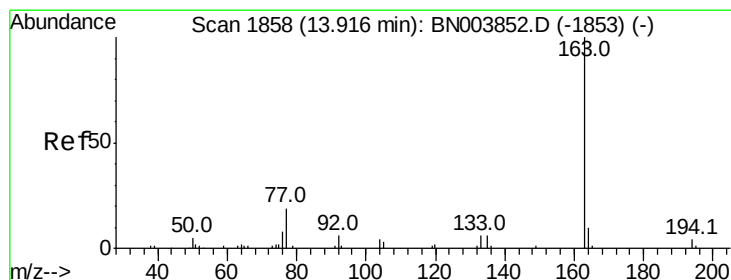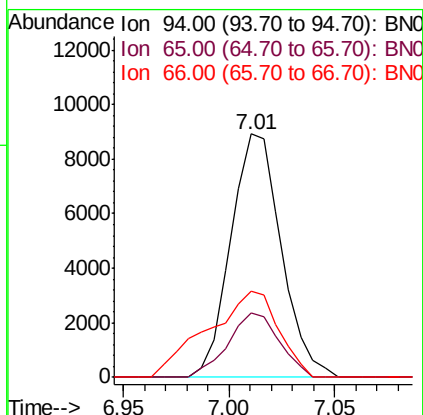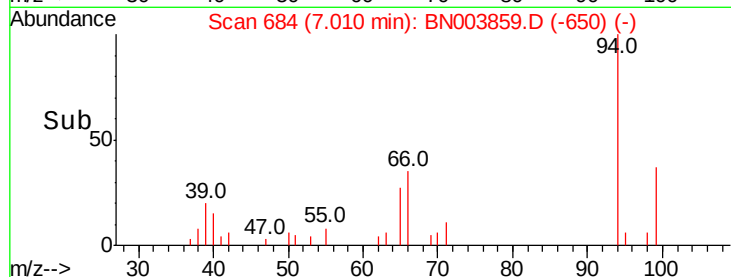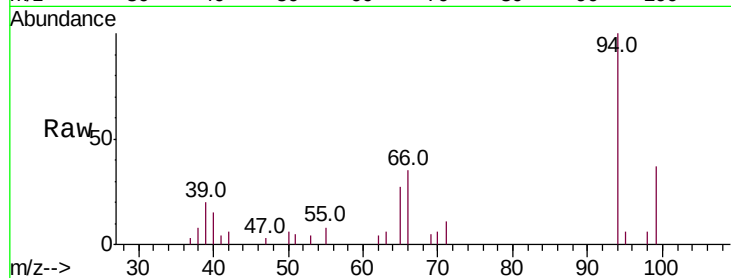

#44

Dimethylphthalate

Concen: 12.959 ng/ul

RT: 13.92 min Scan# 1858

Delta R.T. 0.00 min

Lab File: BN003859.D

Acq: 12 Dec 2018 19:59

Tgt Ion:163 Resp: 74139

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.4 7.9 11.9

