

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121218\
 Data File : BN003865.D
 Acq On : 12 Dec 2018 23:29
 Operator : JU/SJ
 Sample : J6299-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F37

Manual Integrations
 APPROVED

Sohil
 12/13/2018 6:12:32 PM

Quant Time: Dec 13 12:28:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 13 04:12:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	16036	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	79593	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	51886	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	131779	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	179287	20.00	ng/ul	0.00
85) Perylene-d12	23.70	264	222535	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	119m	0.49	ng/uL	0.00
5) Phenol-d5	6.99	99	9959	6.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	29644	34.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	33014	26.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	20899	15.82	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	23017	36.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	25314	35.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	40562	30.96	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.87	166	169105	36.51	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	200820	36.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	5112	5.34	ng/ul	0.00
57) Fluorene-d10	15.46	176	149765	37.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	27562	29.04	ng/ul	0.00
70) Anthracene-d10	17.31	188	247666	37.19	ng/ul	0.00
78) Pyrene-d10	19.60	212	299777	37.38	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	460119	38.11	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.01	94	2062	1.296 ng/ul	96
33) 4-Chloro-3-methylphenol	11.90	107	4817	3.284 ng/ul	100
56) Diethylphthalate	15.27	149	6840	1.480 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121218\
Data File : BN003865.D
Acq On : 12 Dec 2018 23:29
Operator : JU/SJ
Sample : J6299-10
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F9F37

Quant Time: Dec 13 12:28:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 04:12:26 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/13/2018 6:12:32 PM

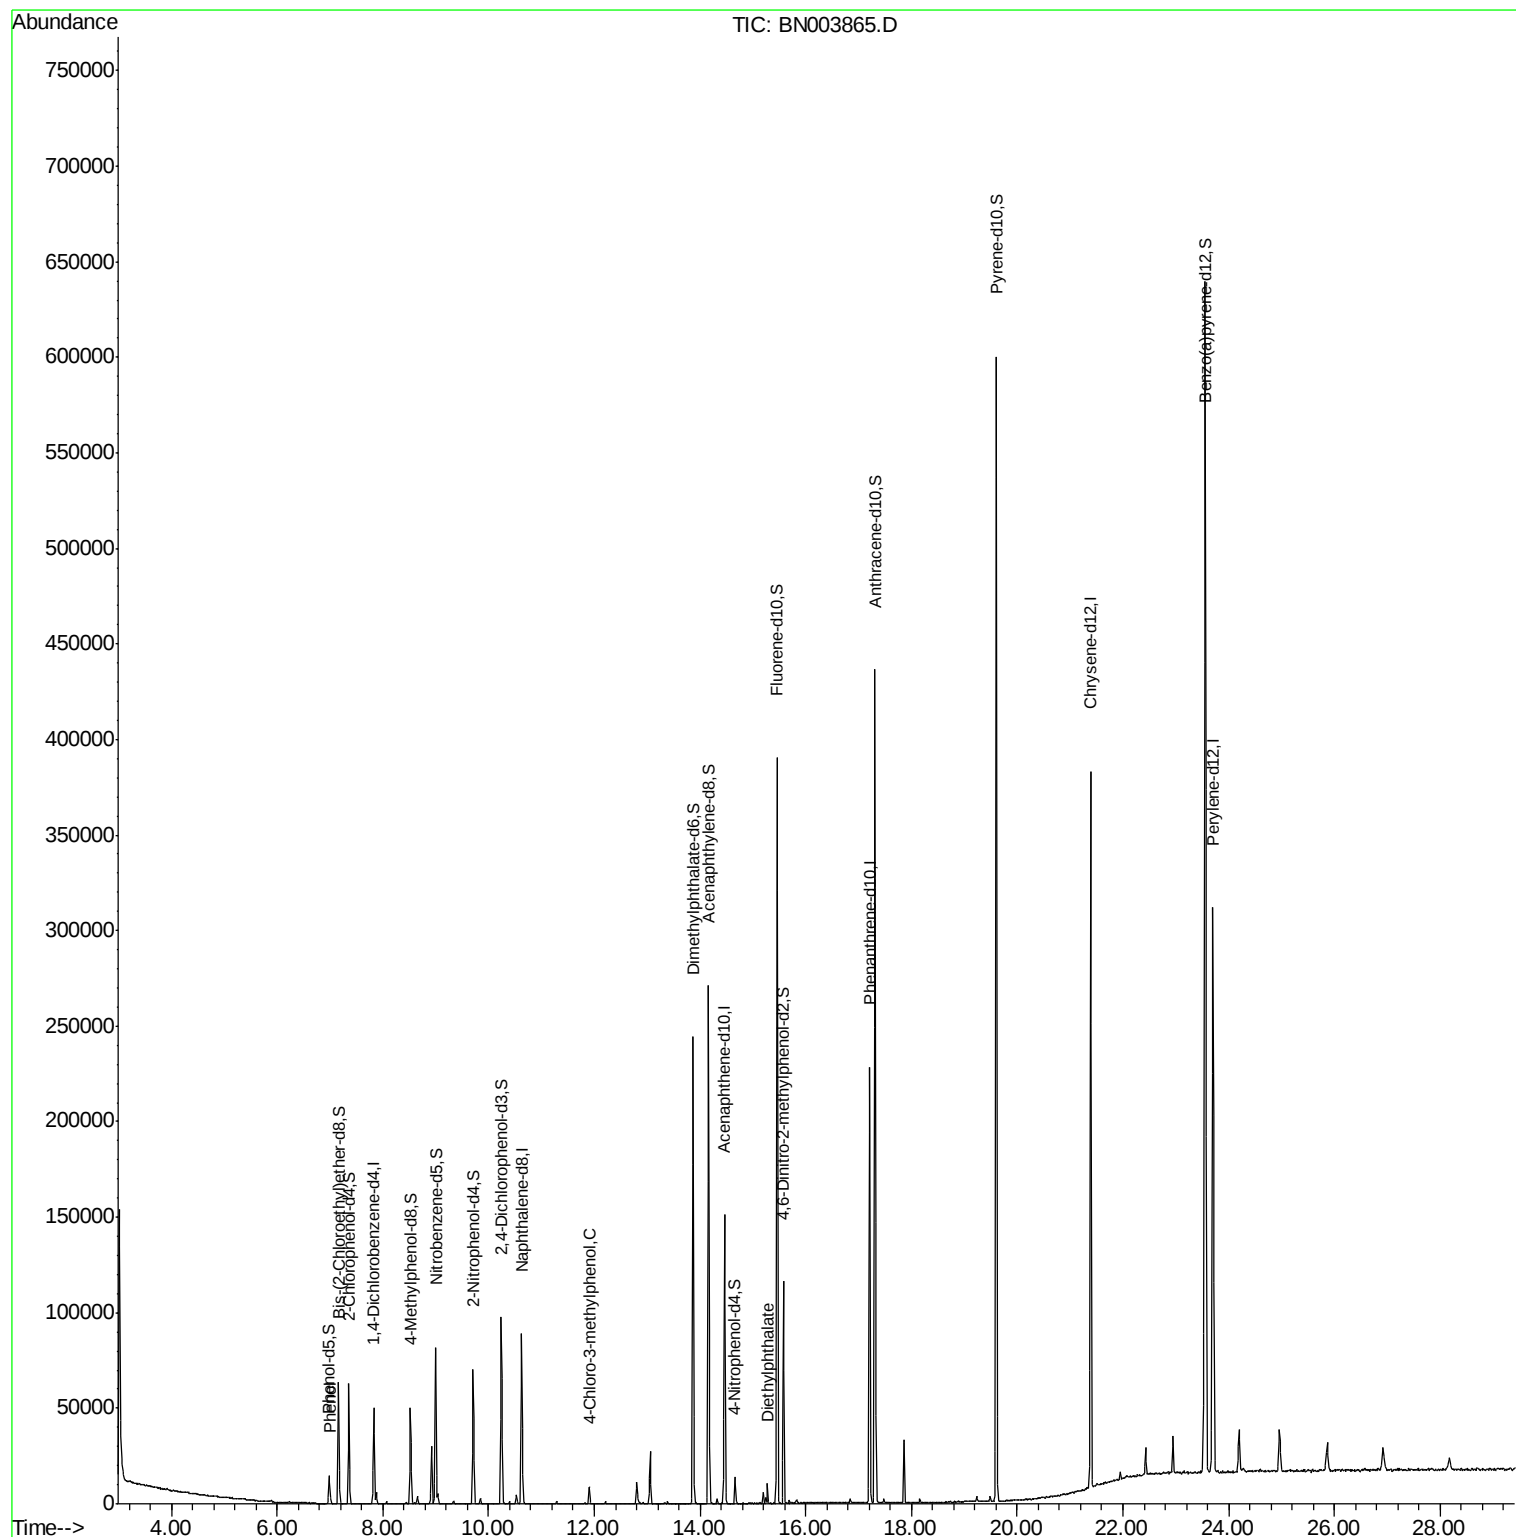

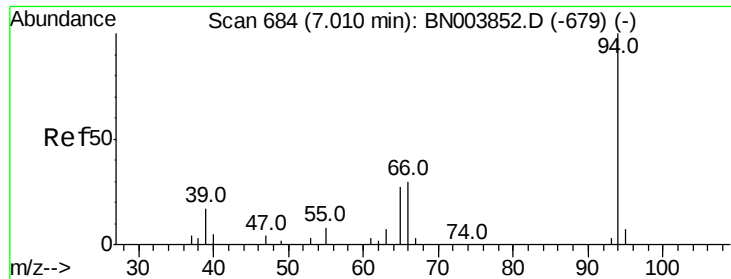

#6

Phenol

Concen: 1.296 ng/ul

RT: 7.01 min Scan# 684

Delta R.T. 0.00 min

Lab File: BN003865.D

Acq: 12 Dec 2018 23:29

Instrument :

BNA_N

ClientSampled :

F9F37

Tot Ion: 94 Resp: 2062

Ion Ratio Lower Upper

94 100

65 27.2 21.2 31.8



66 37.4 26.9 40.3

Manual Integrations

APPROVED

Sohil



12/13/2018 6:12:32 PM

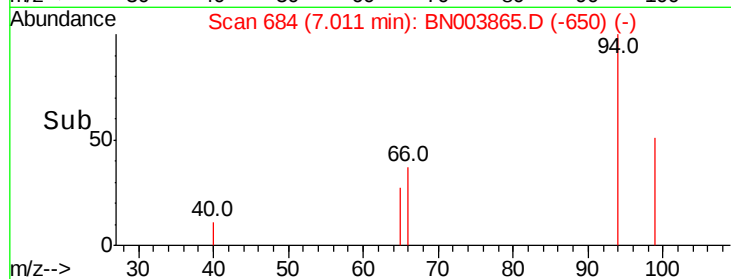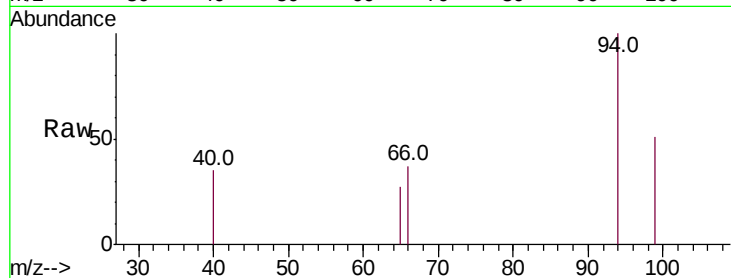

Abundance Ion 94.00 (93.70 to 94.70): BN003865.D (-650) (-)

Ion 65.00 (64.70 to 65.70): BN003865.D (-650) (-)

Ion 66.00 (65.70 to 66.70): BN003865.D (-650) (-)

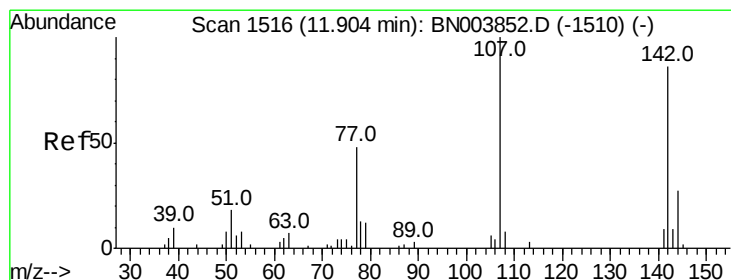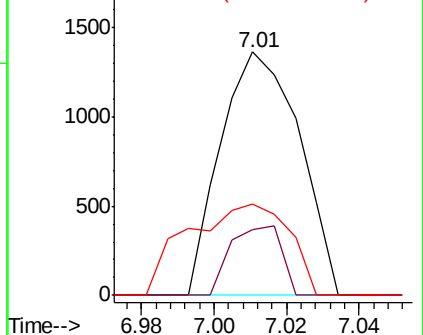

#33

4-Chloro-3-methylphenol

Concen: 3.284 ng/ul

RT: 11.90 min Scan# 1516

Delta R.T. 0.00 min

Lab File: BN003865.D

Acq: 12 Dec 2018 23:29



Tgt Ion: 107 Resp: 4817

Ion Ratio Lower Upper

107 100

144 26.3 21.1 31.7


142 81.7 65.0 97.4

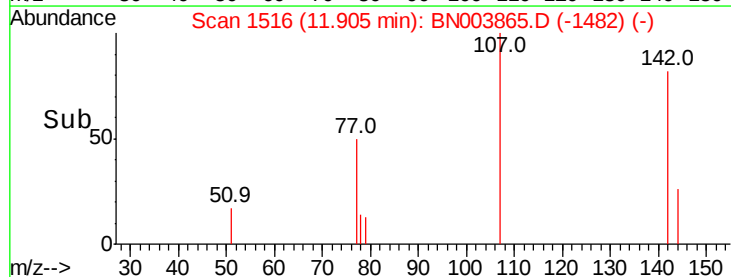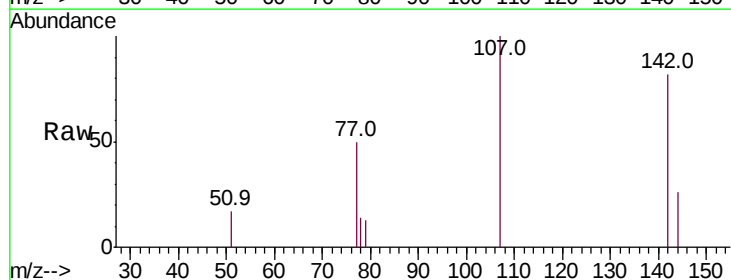


Abundance Ion 107.00 (106.70 to 107.70): BN003865.D (-1482) (-)

Ion 144.00 (143.70 to 144.70): BN003865.D (-1482) (-)

Ion 142.00 (141.70 to 142.70): BN003865.D (-1482) (-)

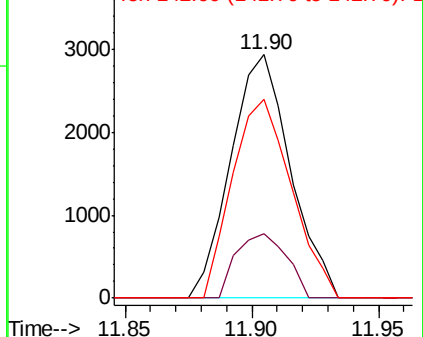

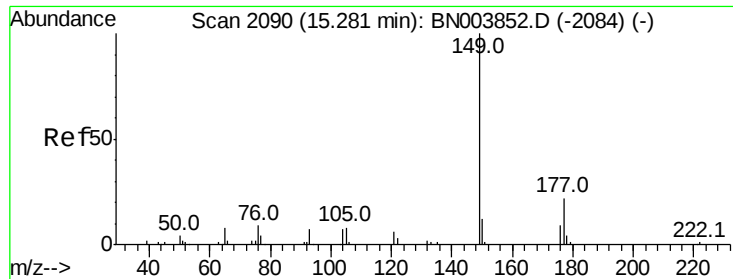


#56
 Diethylphthalate
 Concen: 1.480 ng/ul
 RT: 15.27 min Scan# 2089
 Delta R.T. -0.01 min
 Lab File: BN003865.D
 Acq: 12 Dec 2018 23:29

Instrument :
 BNA_N
 ClientSampleId :
 F9F37

Tot Ion	Ratio	Lower	Upper
149	100		
177	22.4	17.8	26.6
150	11.3	10.2	15.2

Manual Integrations
 APPROVED

Sohil
 12/13/2018 6:12:32 PM

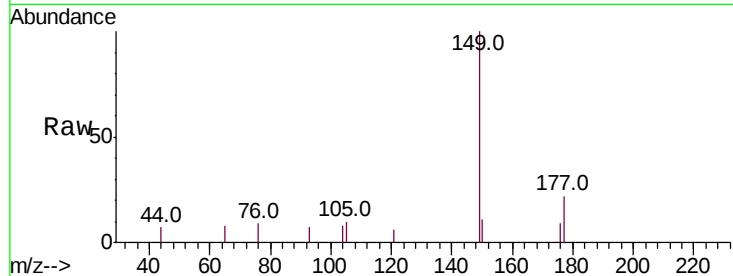

Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

