


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121218\
 Data File : BN003844.D
 Acq On : 12 Dec 2018 10:02
 Operator : JU/SJ
 Sample : DFTPP66
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP66

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Dec 13 06:00:44 2018

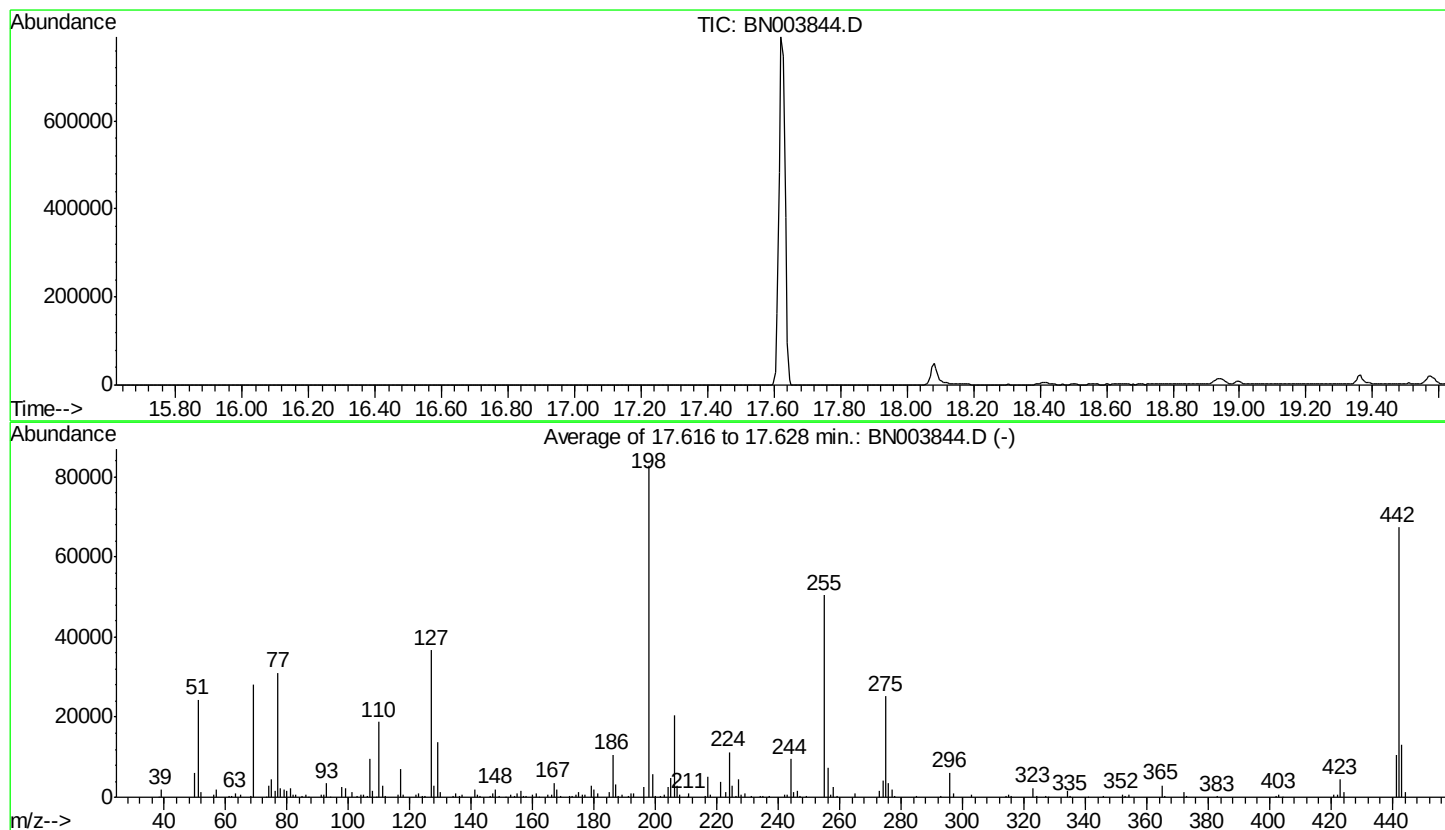

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	24368	PASS
68	69	0.00	2	1.4	388	PASS
69	198	0.00	100	33.9	28053	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.4	36762	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82840	PASS
199	198	5	9	6.8	5614	PASS
275	198	10	60	30.4	25192	PASS
365	198	1	100	3.6	2988	PASS
441	198	0.01	100	12.8	10610	PASS
442	198	50	100	81.3	67333	PASS
443	442	15	24	19.5	13142	PASS

m/z	Abundance
44.00	1006.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

m/z	Abundance
39.00	1661.0
44.00	875.0
50.00	5198.0
51.00	20928.0
52.00	1130.0
56.00	684.0
57.00	1585.0
61.00	308.0
62.00	365.0
63.00	873.0
65.00	453.0
69.00	23888.0
74.00	2183.0
75.00	3703.0
76.00	1318.0
77.00	25792.0
78.00	1869.0
79.00	1700.0
80.00	1340.0
81.00	1766.0
81.90	428.0
83.00	460.0
85.00	325.0
86.00	582.0
91.00	425.0
92.00	529.0
93.00	2813.0
98.00	2186.0
99.00	1832.0
101.00	997.0
103.00	379.0
103.90	672.0
105.00	601.0
107.00	7555.0
108.00	1276.0
110.00	15242.0
111.00	2181.0
116.00	429.0
117.00	5694.0
117.90	464.0
121.90	553.0
123.00	773.0
123.90	392.0
124.90	350.0
127.00	28656.0
128.00	2258.0
129.00	10592.0
130.00	930.0
134.00	316.0
135.00	965.0
136.00	329.0
137.00	487.0
141.00	1471.0
142.00	417.0
142.90	349.0
147.00	708.0
148.00	1484.0
148.90	367.0
152.90	471.0
153.90	374.0
155.00	750.0
156.00	1141.0
159.90	472.0
161.00	692.0
165.00	516.0
165.90	435.0
167.00	2733.0
168.00	1685.0
172.90	356.0
174.00	622.0
175.00	1043.0
176.00	363.0
176.90	551.0
179.00	2018.0
180.00	1547.0
181.00	783.0
185.00	921.0
186.00	7769.0
187.00	2414.0
188.90	451.0
192.00	650.0
193.00	721.0
196.00	1665.0
198.00	60544.0
199.00	4353.0
199.90	354.0
202.90	388.0
204.00	1993.0
205.00	3426.0
206.00	14744.0
207.00	2299.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

208.00	448.0
210.90	633.0
216.00	333.0
217.00	3688.0
218.00	486.0
221.00	2608.0
223.00	872.0
224.00	7998.0
225.10	2210.0
226.00	303.0
227.00	3222.0
228.00	477.0
229.00	748.0
237.00	357.0
242.10	403.0
243.00	536.0
244.00	6519.0
245.00	924.0
246.00	1180.0
255.00	34768.0
256.00	5360.0
257.00	491.0
258.00	1825.0
258.90	358.0
265.00	757.0
273.00	952.0
274.00	2675.0
275.00	17192.0
276.00	2319.0
277.00	1280.0
292.90	331.0
296.00	4095.0
296.90	637.0
303.10	489.0
315.00	419.0
323.00	1317.0
334.00	885.0
335.00	307.0
352.10	398.0
354.00	478.0
365.00	1821.0
366.00	309.0
372.00	794.0
403.00	427.0
421.00	366.0
422.00	405.0
423.10	2501.0
424.00	790.0
441.10	5931.0
442.10	37064.0
443.10	7349.0
444.00	747.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

m/z	Abundance
38.00	329.0
39.00	2198.0
44.00	913.0
50.00	7376.0
51.00	28824.0
52.00	1468.0
56.00	960.0
57.00	2153.0
61.00	399.0
61.90	472.0
63.00	1205.0
65.00	597.0
68.20	643.0
69.00	33176.0
73.00	301.0
74.00	3379.0
75.00	5139.0
76.10	1685.0
77.10	37152.0
78.00	2520.0
79.00	2365.0
80.00	1849.0
81.00	2607.0
82.00	671.0
83.00	634.0
85.00	515.0
85.90	729.0
86.90	380.0
91.00	642.0
92.00	707.0
93.00	4121.0
94.00	350.0
98.00	3093.0
99.00	2605.0
101.00	1509.0
103.00	560.0
103.90	971.0
105.00	793.0
106.00	354.0
107.00	11462.0
108.00	1888.0
109.10	400.0
110.00	22104.0
111.00	3417.0
111.90	463.0
116.00	669.0
117.00	8401.0
118.00	612.0
122.00	756.0
123.00	1268.0
123.90	558.0
124.90	510.0
127.00	43752.0
128.00	3300.0
129.00	16672.0
130.00	1336.0
133.90	470.0
135.00	1233.0
136.00	515.0
137.00	781.0
141.00	2103.0
142.00	644.0
143.00	459.0
146.00	413.0
147.00	1126.0
148.00	2355.0
149.00	563.0
151.00	301.0
153.00	675.0
154.00	491.0
155.00	1220.0
156.00	1684.0
157.10	395.0
157.90	421.0
160.00	657.0
161.00	992.0
161.90	323.0
164.90	872.0
166.00	618.0
167.00	4242.0
168.00	2158.0
169.00	378.0
172.00	425.0
173.00	494.0
174.00	847.0
175.00	1679.0
176.00	530.0
176.90	743.0
179.00	3304.0
180.00	2188.0
181.00	1049.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

185.00	1631.0
186.00	12760.0
187.00	3631.0
187.90	379.0
189.00	766.0
191.10	369.0
191.90	1109.0
193.00	1183.0
196.00	2952.0
198.00	97640.0
199.00	6649.0
200.00	474.0
201.50	596.0
203.00	689.0
204.00	3234.0
205.00	5492.0
206.00	24448.0
207.00	3555.0
208.00	770.0
210.90	945.0
216.10	498.0
217.00	6142.0
218.00	766.0
221.00	4291.0
223.00	1378.0
224.00	13280.0
225.00	3482.0
226.00	407.0
227.00	5196.0
228.00	733.0
229.00	1265.0
231.00	554.0
234.00	329.0
235.00	433.0
237.00	547.0
242.00	767.0
243.10	753.0
244.00	11347.0
245.00	1592.0
246.00	2066.0
246.90	433.0
249.00	418.0
255.00	58960.0
256.00	8809.0
257.00	787.0
258.00	3160.0
259.00	488.0
265.00	1338.0
273.00	1880.0
274.00	4749.0
275.00	29232.0
276.00	4131.0
277.00	2190.0
278.00	380.0
285.00	434.0
293.00	593.0
296.00	7277.0
297.00	1116.0
303.00	921.0
314.00	452.0
315.00	825.0
316.00	479.0
323.00	2639.0
324.00	512.0
327.00	491.0
334.00	1685.0
335.10	495.0
345.90	519.0
352.00	777.0
353.00	569.0
354.00	881.0
365.00	3376.0
366.00	430.0
372.00	1347.0
373.00	408.0
382.90	380.0
402.00	554.0
403.00	942.0
421.00	646.0
422.00	721.0
423.10	4710.0
424.00	1292.0
441.10	12066.0
442.10	73752.0
443.10	14911.0
444.10	1458.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

m/z	Abundance
39.00	1835.0
44.00	872.0
50.00	5913.0
51.00	23352.0
52.00	1173.0
55.90	789.0
57.00	1711.0
61.00	327.0
62.00	386.0
63.00	1000.0
65.00	559.0
68.10	522.0
69.00	27096.0
74.00	2663.0
75.00	4259.0
76.00	1405.0
77.00	30496.0
78.00	2114.0
79.00	2056.0
80.00	1578.0
81.00	2161.0
81.90	559.0
83.00	568.0
85.00	399.0
85.90	566.0
91.00	527.0
92.00	624.0
93.00	3365.0
98.00	2670.0
99.00	2196.0
101.00	1188.0
102.90	401.0
104.00	752.0
105.00	746.0
106.10	309.0
107.00	9478.0
108.00	1438.0
110.00	19144.0
111.00	2763.0
112.00	333.0
116.00	600.0
117.00	7441.0
118.00	551.0
121.90	677.0
123.00	1067.0
123.90	442.0
124.90	413.0
127.00	37880.0
128.00	2792.0
129.00	14196.0
130.00	1207.0
133.90	405.0
135.00	1180.0
136.00	479.0
137.00	570.0
141.00	1869.0
142.00	588.0
143.00	405.0
146.00	309.0
147.00	980.0
148.00	2031.0
148.90	480.0
152.90	589.0
154.00	461.0
155.00	1156.0
156.00	1599.0
156.90	347.0
157.90	384.0
160.00	551.0
161.00	825.0
164.90	770.0
166.10	657.0
167.00	3609.0
168.00	1863.0
168.90	334.0
172.00	314.0
173.00	464.0
174.00	750.0
175.00	1554.0
176.00	587.0
176.90	741.0
179.00	3092.0
180.00	2115.0
181.00	949.0
185.00	1430.0
186.00	11509.0
187.00	3331.0
188.00	415.0
189.00	653.0
191.00	357.0
191.90	944.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66

193.00	1049.0
196.00	2737.0
198.00	90336.0
199.00	5842.0
199.90	431.0
201.40	476.0
203.00	573.0
204.00	2885.0
205.00	5112.0
206.00	22712.0
207.00	3183.0
208.00	731.0
210.30	424.0
210.90	883.0
216.00	452.0
217.00	5651.0
218.00	707.0
221.00	4229.0
223.00	1403.0
224.00	12685.0
225.00	3300.0
226.10	391.0
227.00	5135.0
228.00	722.0
229.00	1089.0
231.00	488.0
234.00	352.0
235.00	392.0
237.00	499.0
242.00	773.0
243.10	764.0
244.00	10836.0
245.00	1356.0
246.00	2023.0
247.00	416.0
249.00	432.0
255.00	57552.0
256.00	8298.0
257.00	649.0
258.00	3043.0
259.00	528.0
265.00	1199.0
273.00	1743.0
274.00	4712.0
275.00	29152.0
276.00	3878.0
277.00	2231.0
278.00	422.0
285.00	413.0
293.00	520.0
296.00	7341.0
297.00	1037.0
303.00	928.0
314.00	396.0
315.00	897.0
316.00	528.0
323.00	2951.0
324.00	508.0
327.00	529.0
327.90	309.0
334.00	1853.0
335.00	462.0
341.00	373.0
345.90	607.0
352.00	922.0
353.00	659.0
354.00	942.0
365.00	3767.0
366.00	527.0
372.00	1704.0
373.00	420.0
383.00	507.0
402.00	661.0
403.00	923.0
404.00	425.0
421.00	738.0
422.00	770.0
423.10	5848.0
424.10	1366.0
441.10	13834.0
442.10	91184.0
443.10	17168.0
444.10	1641.0

Instrument :
BNA_N
ClientSampleId :
DFTPP66