
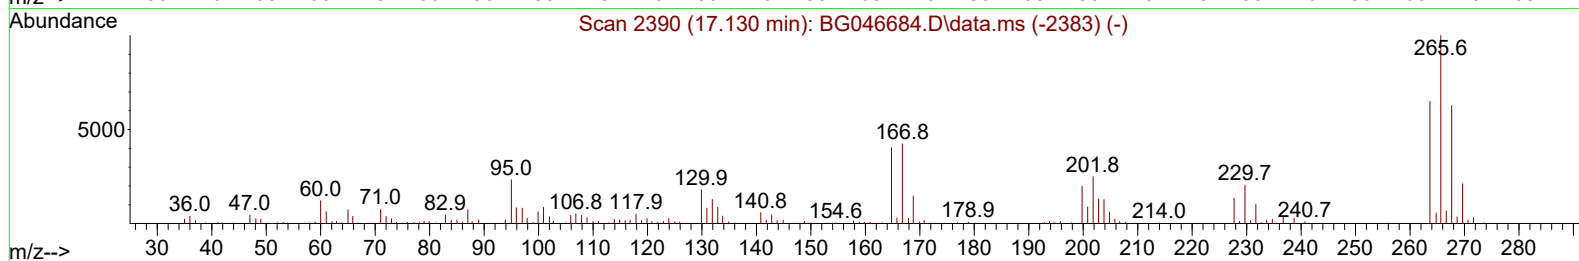
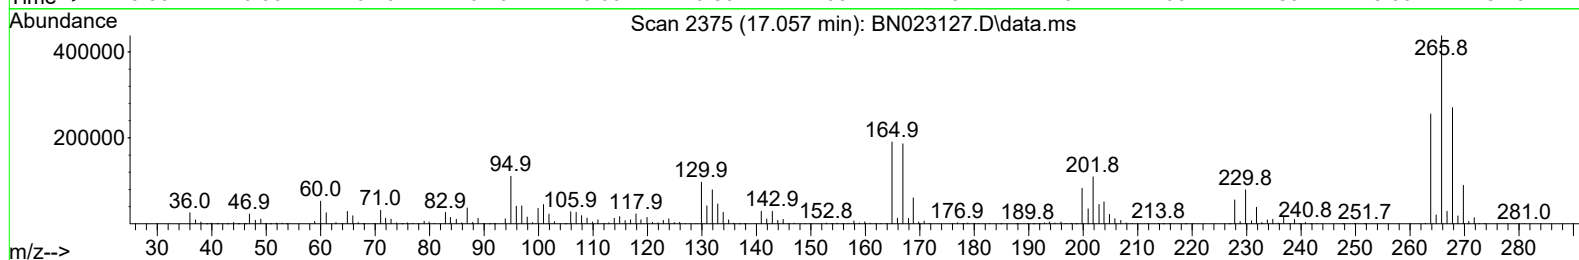


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023127.D
 Acq On : 12 Dec 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:04:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 08:04:03 2022
 Response via : Initial Calibration

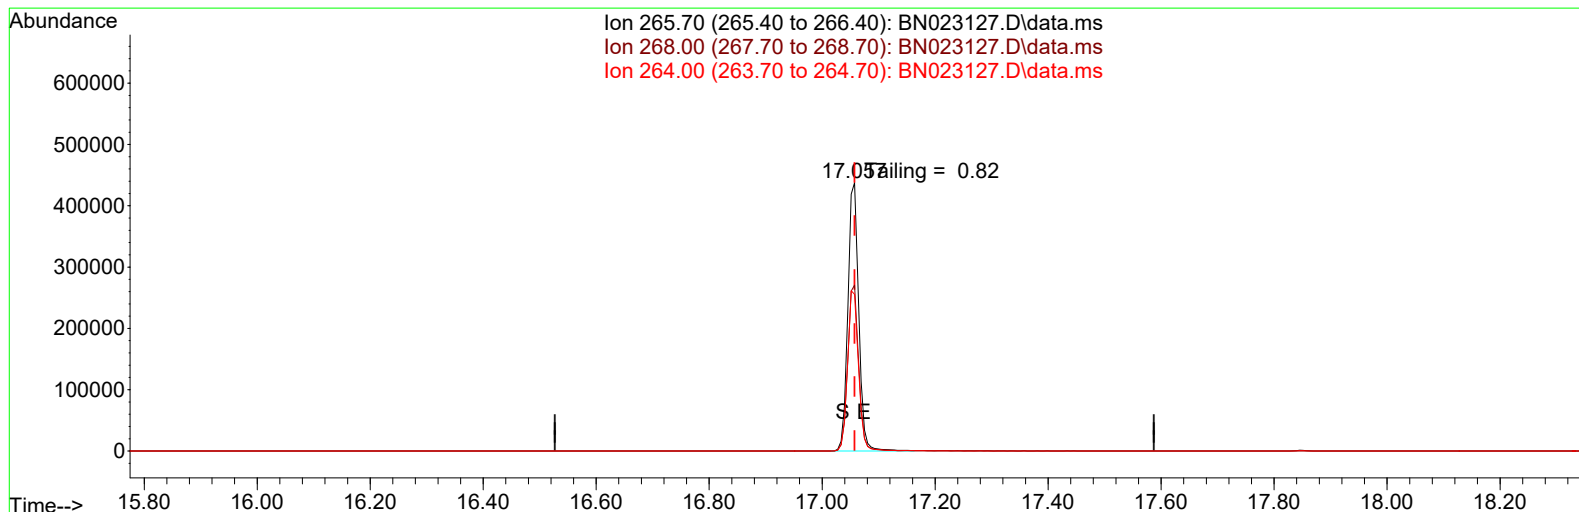

TIC: BN023127.D\data.ms

(70) Pentachlorophenol (C)




17.057min (0.000) 22440.85 ng

response 583805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.83
264.00	61.60	58.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023127.D
 Acq On : 12 Dec 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:04:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 08:04:03 2022
 Response via : Initial Calibration

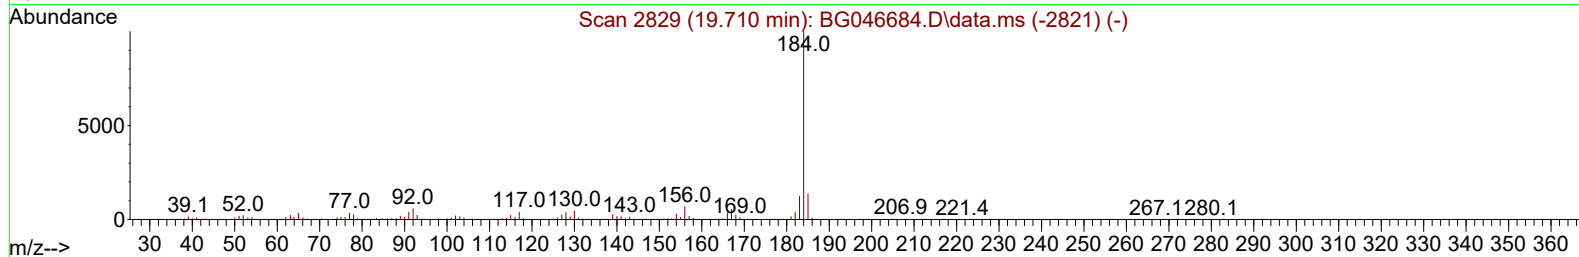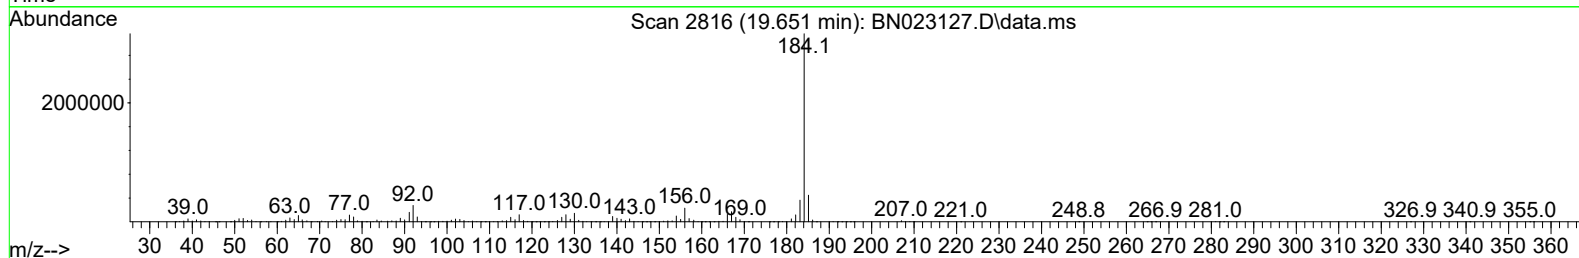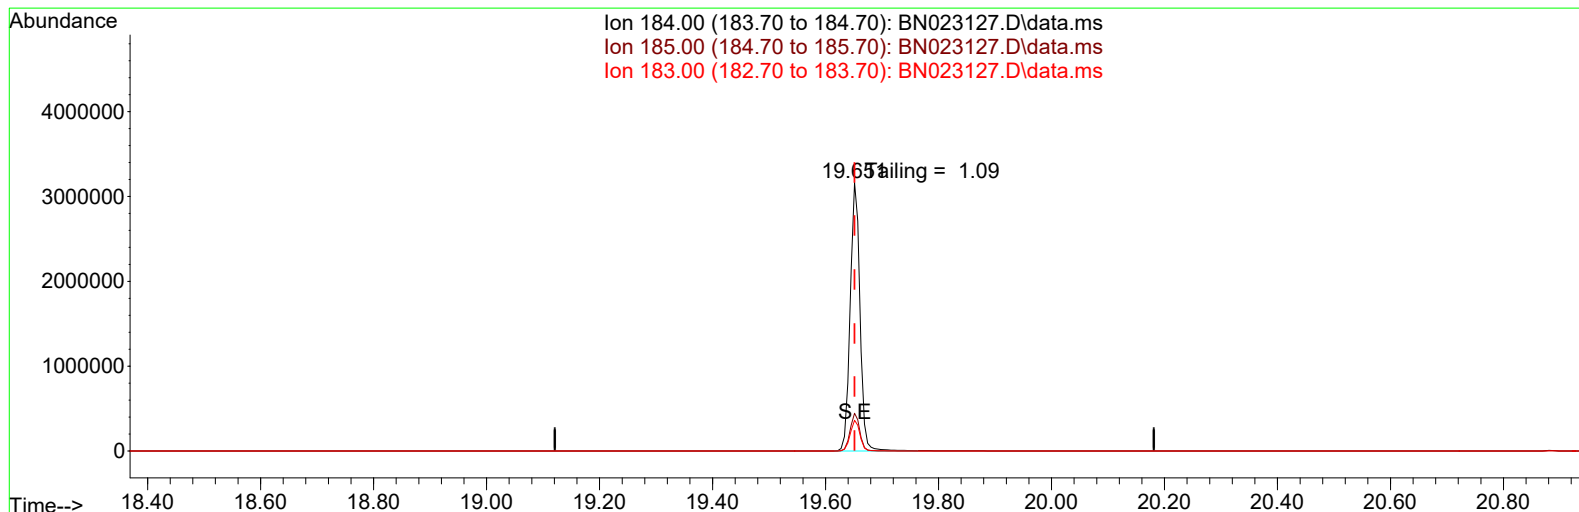

TIC: BN023127.D\data.ms

(77) Benzidine

19.651min (0.000) 0.00 ng

response 3841322

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.48
0.00	0.00	0.00