
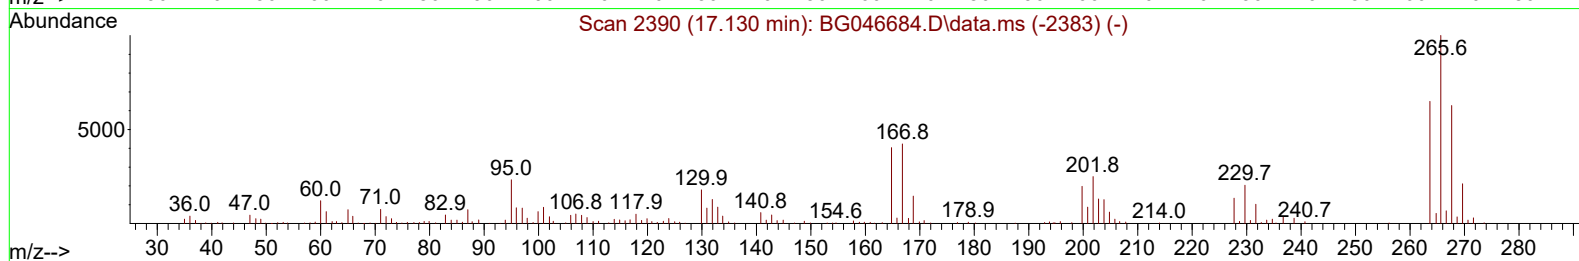
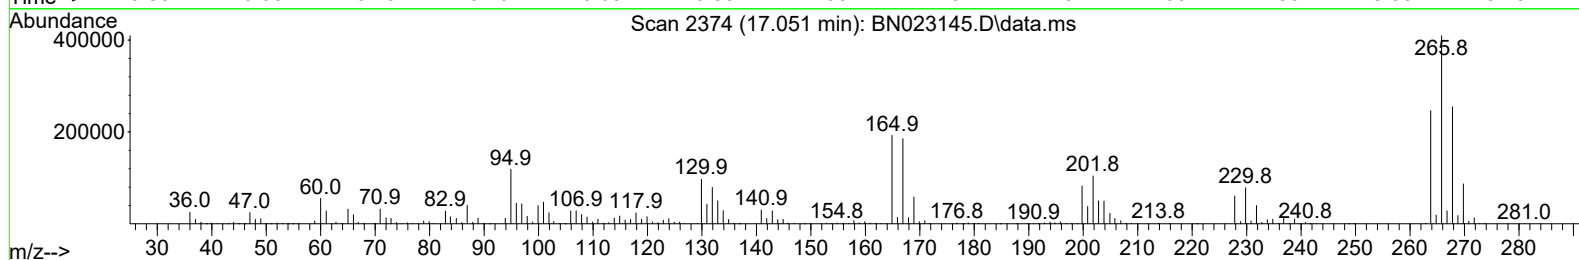


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
Data File : BN023145.D
Acq On : 12 Dec 2022 21:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:05:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 08:04:03 2022
Response via : Initial Calibration

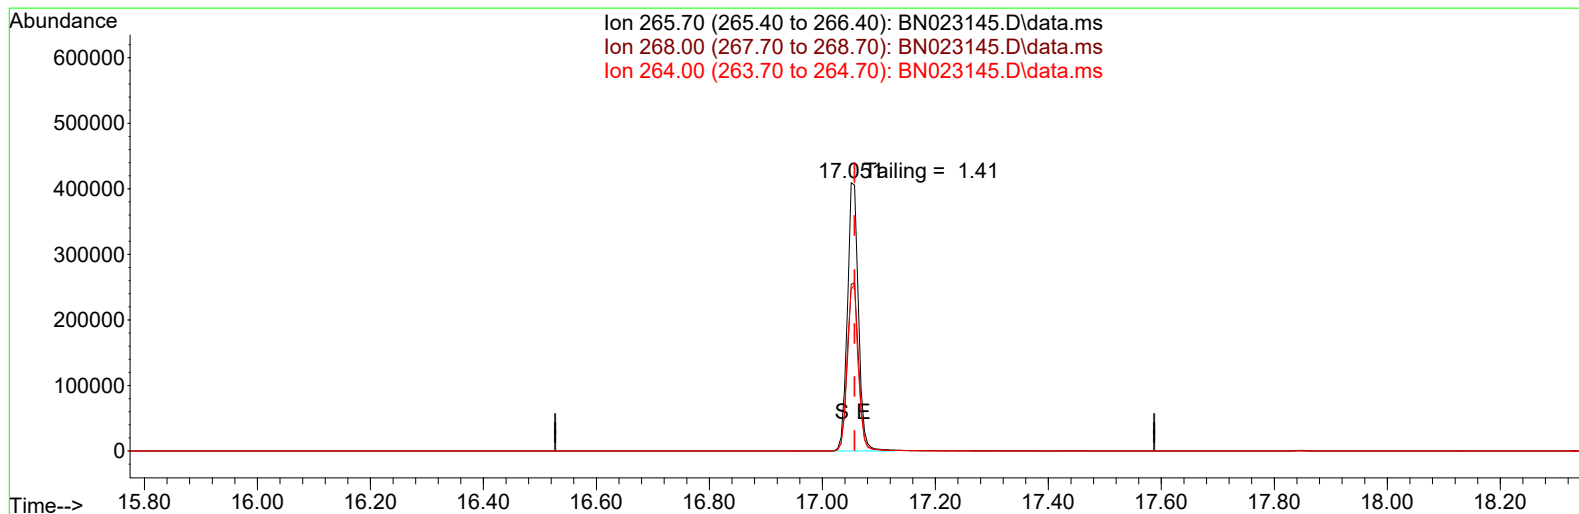

TIC: BN023145.D\data.ms

(70) Pentachlorophenol (C)




17.051min (-0.006) 21747.15 ng

response 558249

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.21
264.00	61.60	60.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
Data File : BN023145.D
Acq On : 12 Dec 2022 21:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 08:05:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 08:04:03 2022
Response via : Initial Calibration

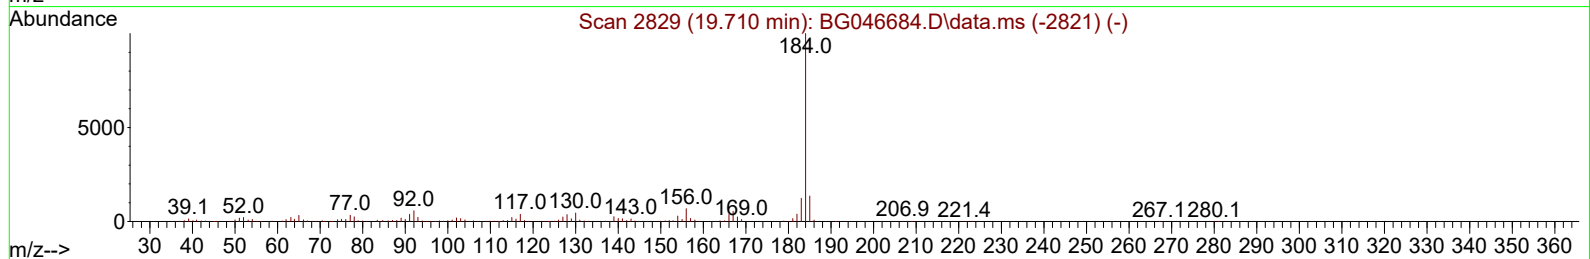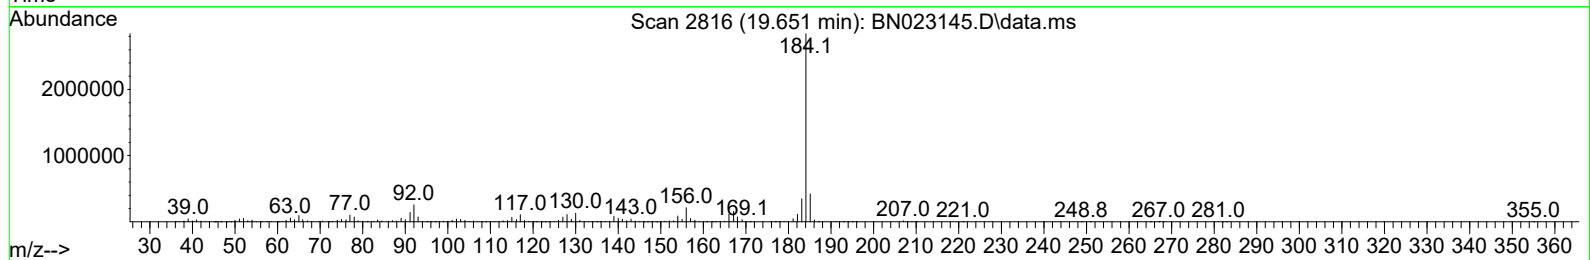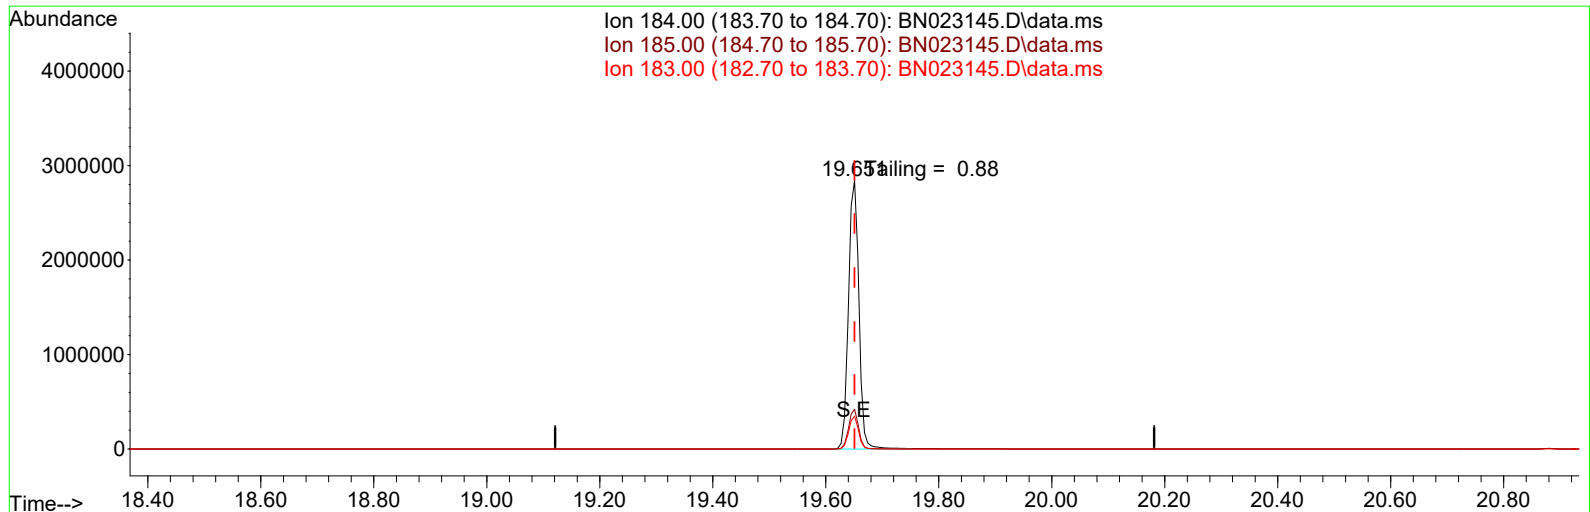

TIC: BN023145.D\data.ms

(77) Benzidine

19.651min (-0.000) 0.00 ng

response 3659736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.83
183.00	13.20	12.28
0.00	0.00	0.00