

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023130.D
 Acq On : 12 Dec 2022 11:51
 Operator : CG/JU
 Sample : PB149511BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB149511BL

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/13/2022
 Supervised By :mohammad ahmed 12/14/2022

Quant Time: Dec 12 15:45:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 12 05:18:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.021	152	6810	0.400	ng	0.00
7) Naphthalene-d8	10.840	136	19394	0.400	ng	# 0.00
13) Acenaphthene-d10	14.666	164	9431	0.400	ng	0.01
19) Phenanthrene-d10	17.402	188	20898	0.400	ng	# 0.00
29) Chrysene-d12	21.589	240	14860	0.400	ng	# 0.00
35) Perylene-d12	24.053	264	11864	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.551	112	5481	0.432	ng	0.00
5) Phenol-d6	7.168	99	6673	0.414	ng	0.00
8) Nitrobenzene-d5	9.185	82	4099m	0.321	ng	0.00
11) 2-Methylnaphthalene-d10	12.424	152	9100	0.277	ng	0.00
14) 2,4,6-Tribromophenol	16.148	330	1245	0.364	ng	0.00
15) 2-Fluorobiphenyl	13.287	172	12877	0.342	ng	0.00
27) Fluoranthene-d10	19.435	212	14475	0.296	ng	0.00
31) Terphenyl-d14	20.031	244	9065	0.376	ng	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
Data File : BN023130.D
Acq On : 12 Dec 2022 11:51
Operator : CG/JU
Sample : PB149511BL
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PB149511BL

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022


Quant Time: Dec 12 15:45:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 05:18:26 2022
Response via : Initial Calibration

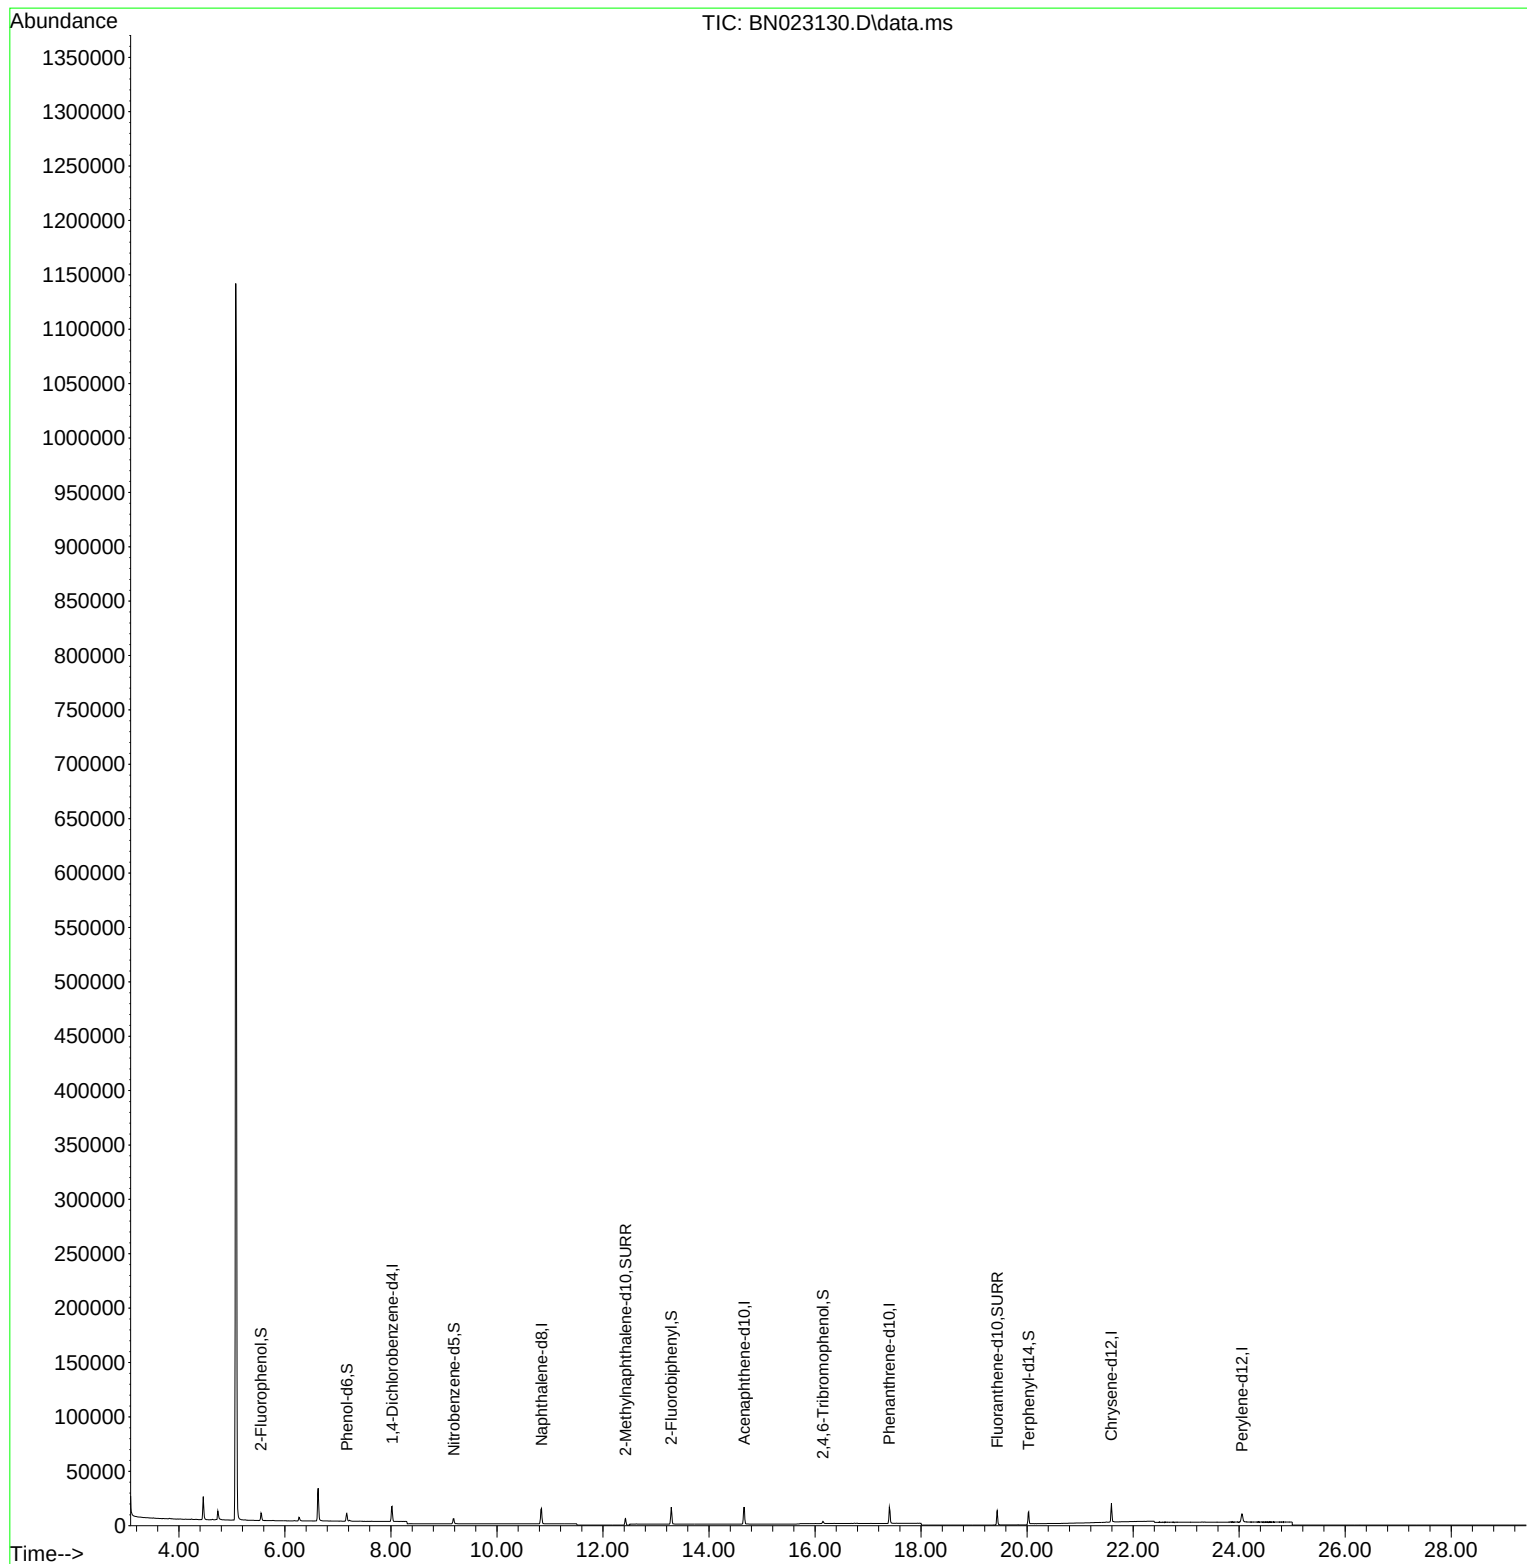

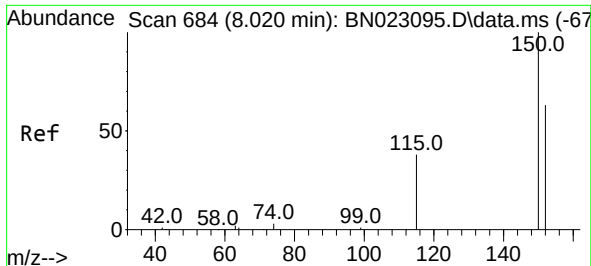

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.021 min Scan# 684
Delta R.T. -0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51




Instrument :
BNA_N
ClientSampleId :
PB149511BL

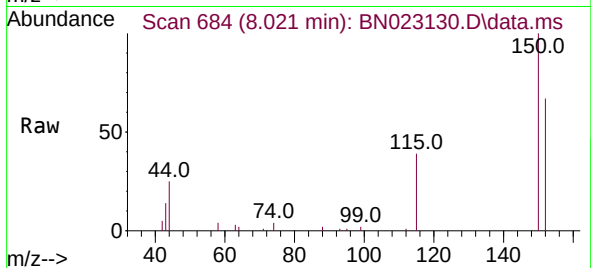

Tgt Ion:152 Resp: 6810
Ion Ratio Lower Upper
152 100
150 150.2 125.6 188.4
115 58.0 49.0 73.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

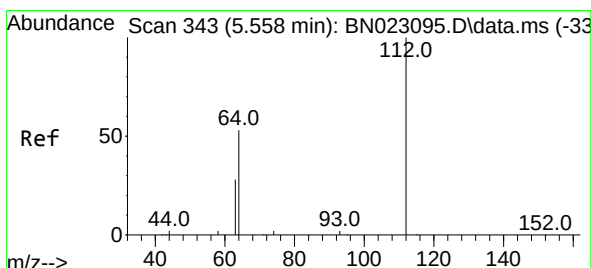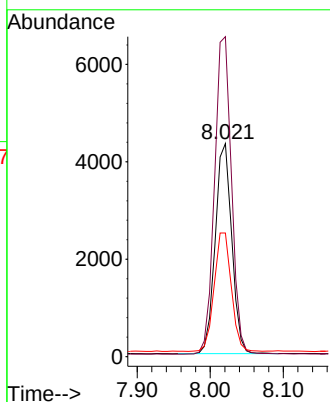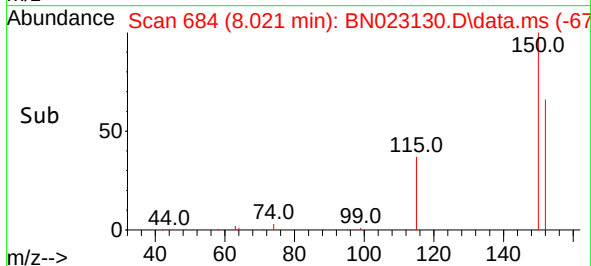

#4
2-Fluorophenol
Concen: 0.432 ng
RT: 5.551 min Scan# 342
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51


Tgt Ion:112 Resp: 5481
Ion Ratio Lower Upper
112 100
64 55.7 44.4 66.6
63 29.2 23.7 35.5

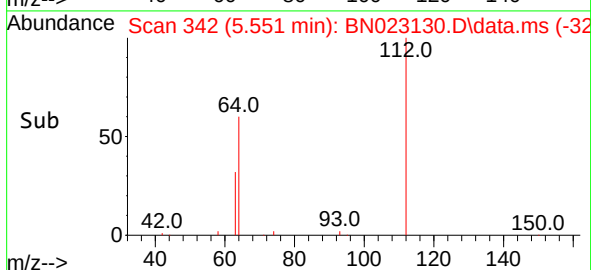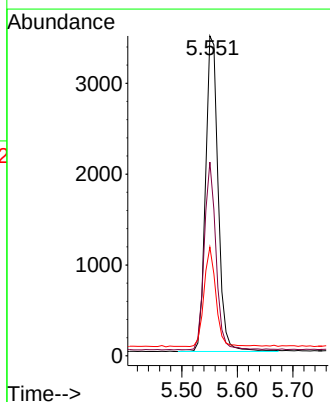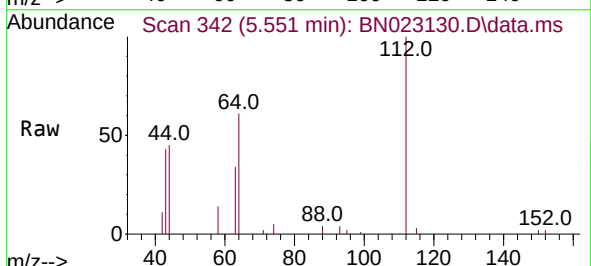

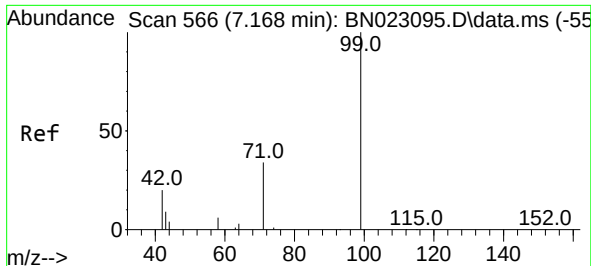

#5
Phenol-d6
Concen: 0.414 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51




Instrument :
BNA_N
ClientSampleId :
PB149511BL

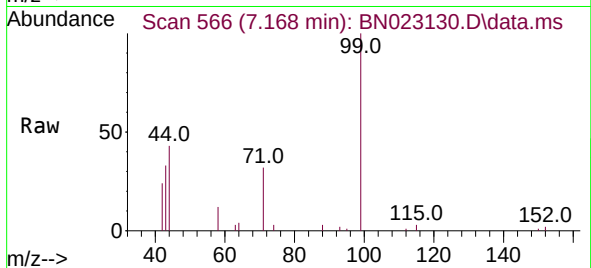

Tgt Ion: 99 Resp: 6673
Ion Ratio Lower Upper
99 100
42 19.5 16.3 24.5
71 33.1 26.5 39.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

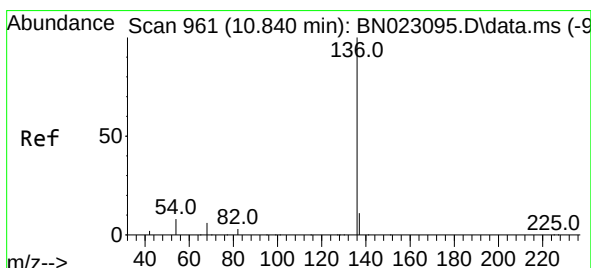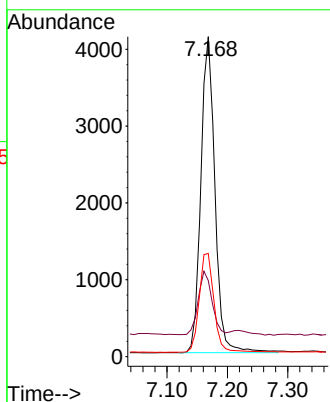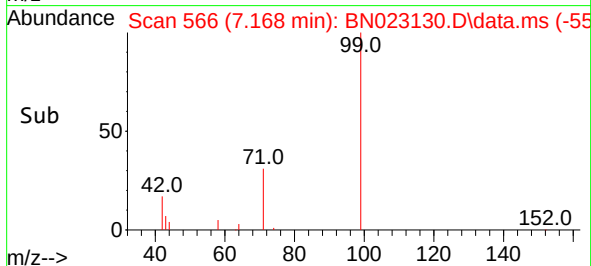

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.840 min Scan# 961
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51


Tgt Ion:136 Resp: 19394
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.4
54 6.4 6.5 9.7#
68 5.6 5.4 8.2

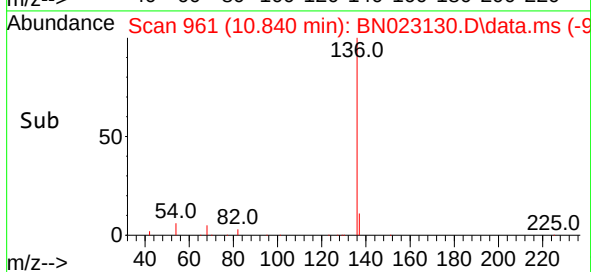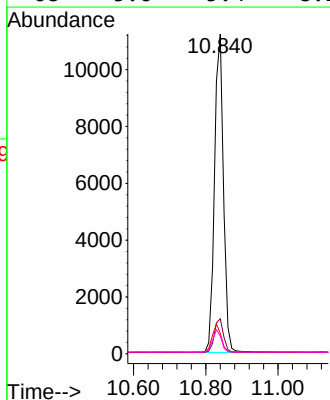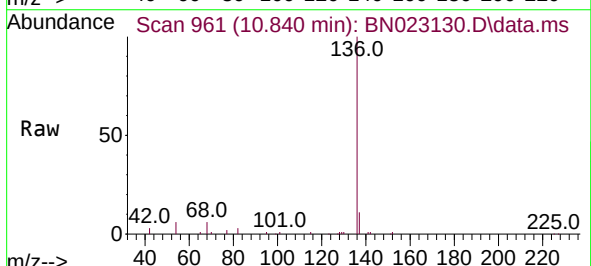

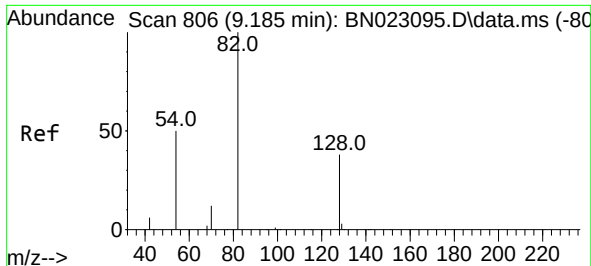

#8
Nitrobenzene-d5
Concen: 0.321 ng m
RT: 9.185 min Scan# 806
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51




Instrument :
BNA_N
ClientSampleId :
PB149511BL

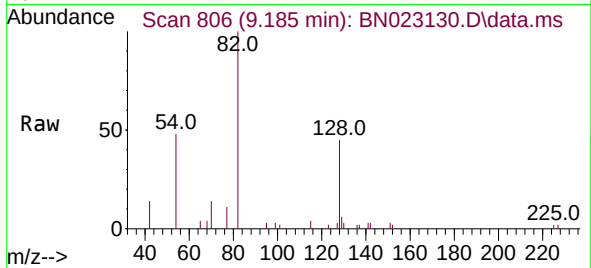


Tgt Ion: 82 Resp: 4099
Ion Ratio Lower Upper
82 100
128 44.8 31.4 47.2
54 47.6 41.0 61.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

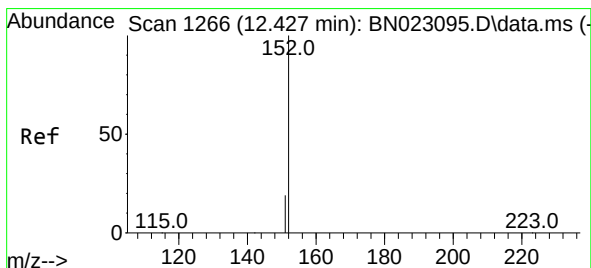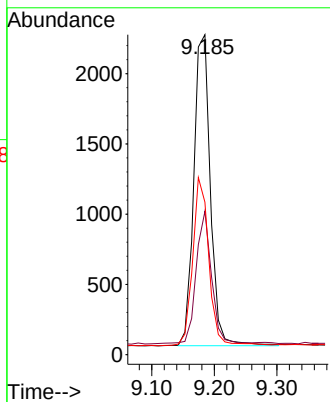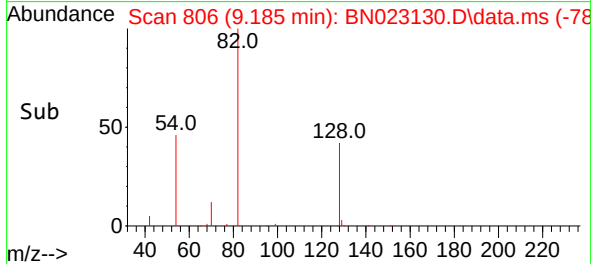


#11
2-Methylnaphthalene-d10
Concen: 0.277 ng
RT: 12.424 min Scan# 1265
Delta R.T. 0.004 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51

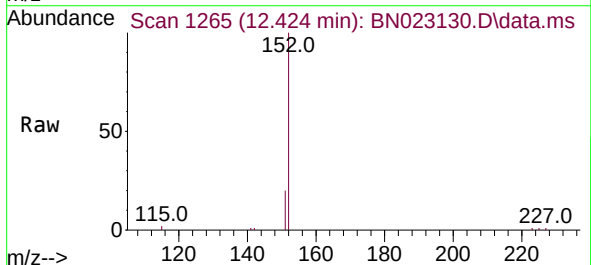


Tgt Ion:152 Resp: 9100
Ion Ratio Lower Upper
152 100
151 21.7 15.1 22.7

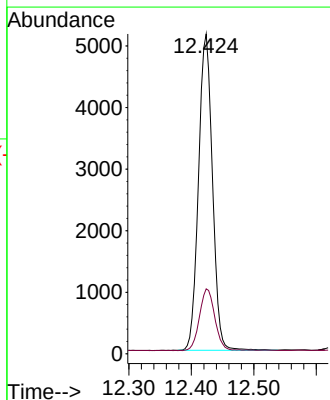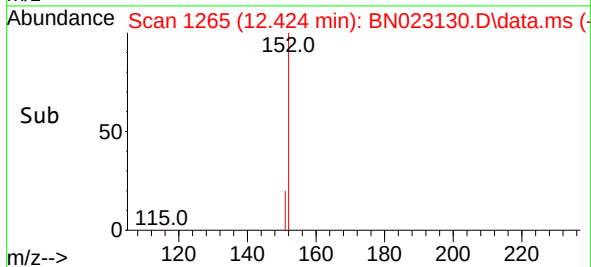

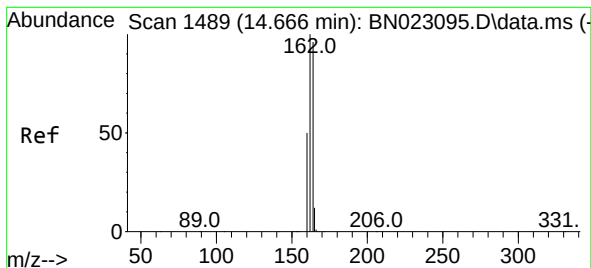

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.666 min Scan# 1489
Delta R.T. 0.011 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51




Instrument :
BNA_N
ClientSampleId :
PB149511BL

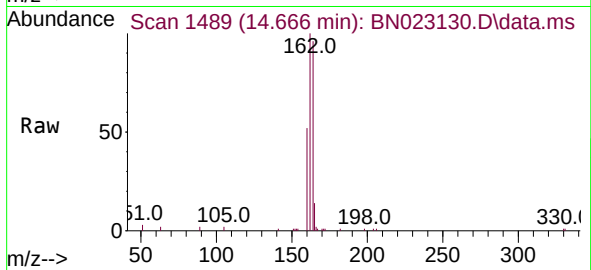


Tgt Ion:164 Resp: 943
Ion Ratio Lower Upper
164 100
162 104.0 83.4 125.0
160 53.7 41.8 62.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

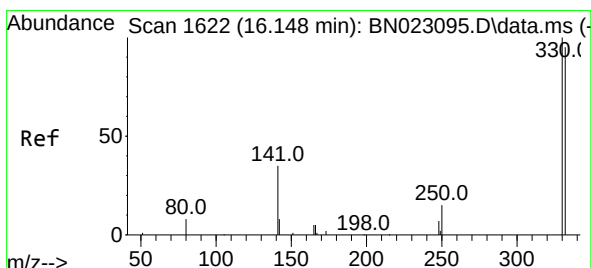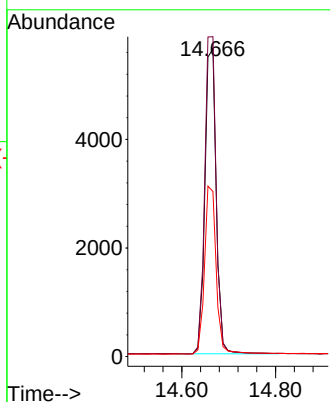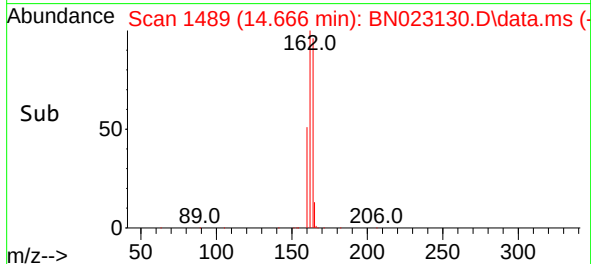


#14
2,4,6-Tribromophenol
Concen: 0.364 ng
RT: 16.148 min Scan# 1622
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51

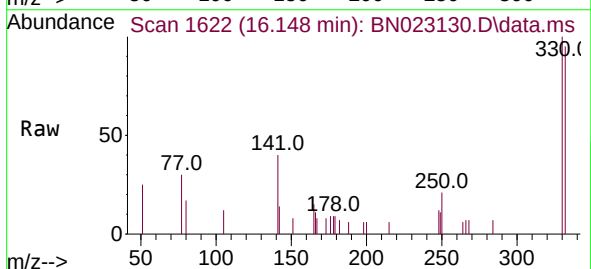

Tgt Ion:330 Resp: 1245
Ion Ratio Lower Upper
330 100
332 96.6 77.3 115.9
141 42.6 33.5 50.3

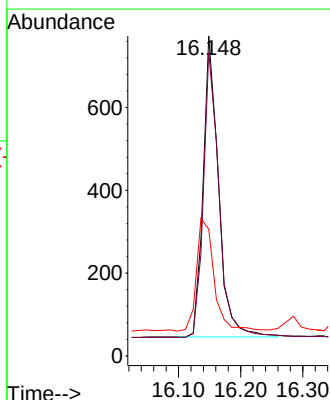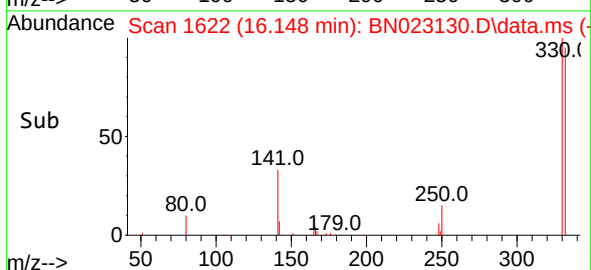

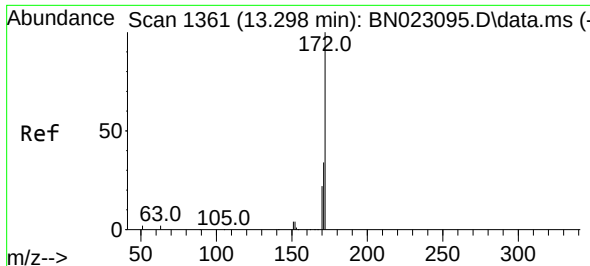

#15
2-Fluorobiphenyl
Concen: 0.342 ng
RT: 13.287 min Scan# 1361
Delta R.T. -0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51

Instrument :

BNA_N





ClientSampleId :

PB149511BL

Tgt Ion:172 Resp: 1287
Ion Ratio Lower Upper
172 100
171 35.7 27.4 41.0
170 24.9 17.9 26.9




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

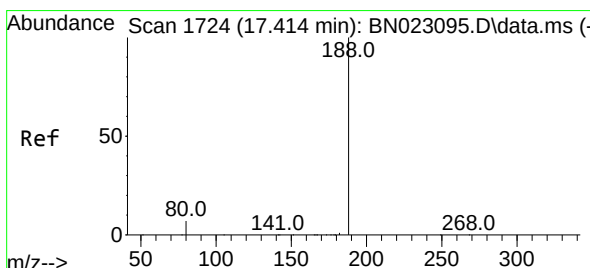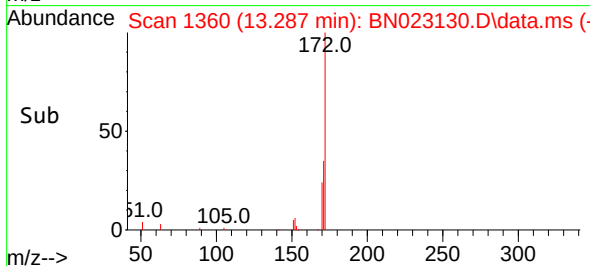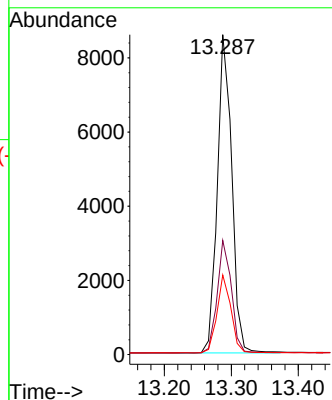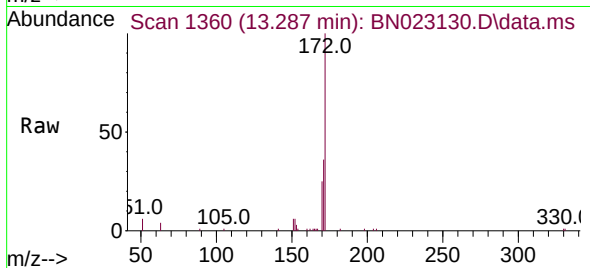

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.402 min Scan# 1723
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51


Tgt Ion:188 Resp: 20898
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 15.5 6.1 9.1#

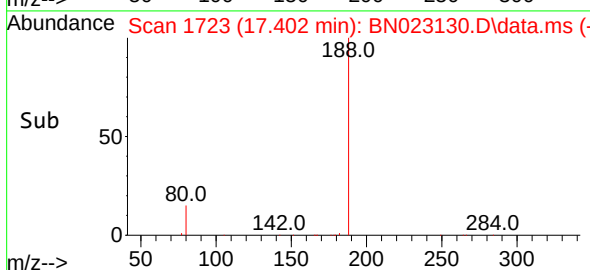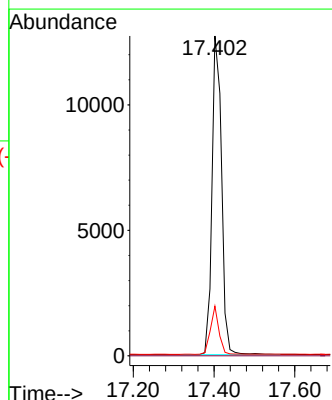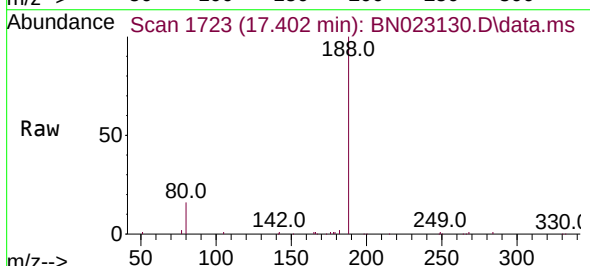

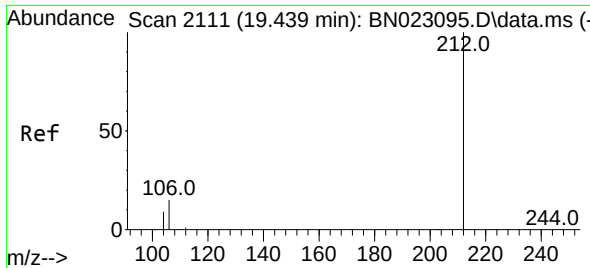

#27
Fluoranthene-d10
Concen: 0.296 ng
RT: 19.435 min Scan# 2111
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51




Instrument :
BNA_N
ClientSampleId :
PB149511BL

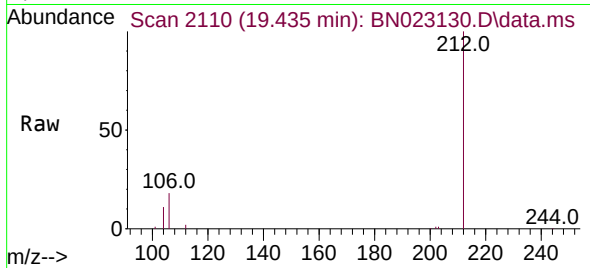


Tgt Ion:212 Resp: 14475
Ion Ratio Lower Upper
212 100
106 17.6 13.0 19.4
104 9.9 7.5 11.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

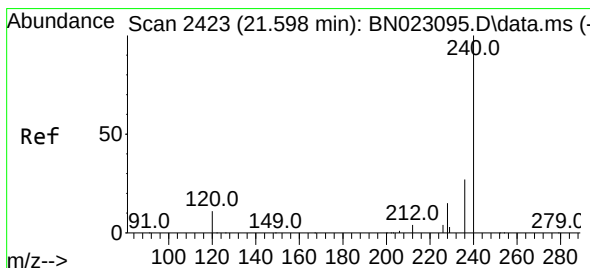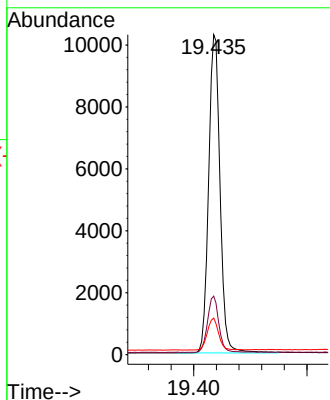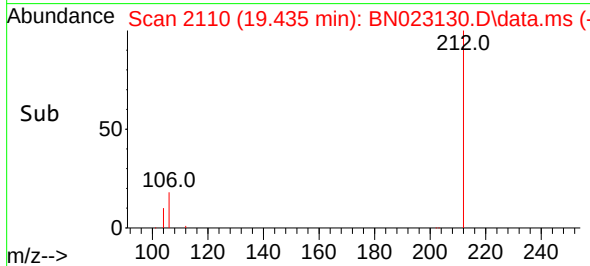


#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.589 min Scan# 2422
Delta R.T. 0.000 min
Lab File: BN023130.D
Acq: 12 Dec 2022 11:51

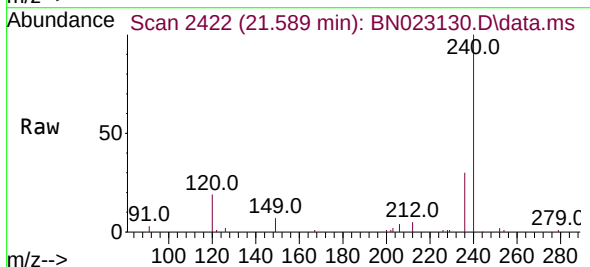


Tgt Ion:240 Resp: 14860
Ion Ratio Lower Upper
240 100
120 19.4 10.1 15.1#
236 29.6 22.2 33.4

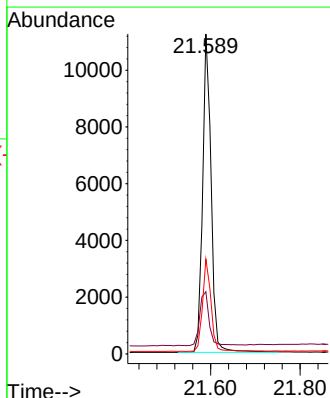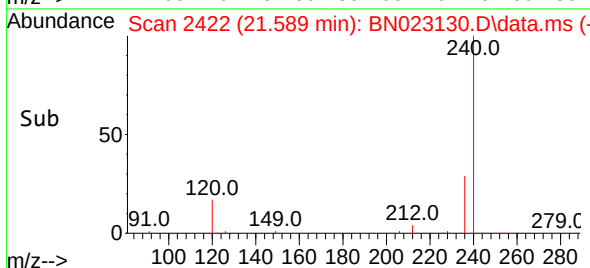

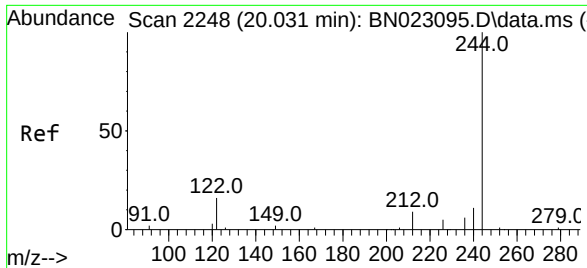

#31
 Terphenyl-d14
 Concen: 0.376 ng
 RT: 20.031 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN023130.D
 Acq: 12 Dec 2022 11:51




Instrument :
 BNA_N
 ClientSampleId :
 PB149511BL

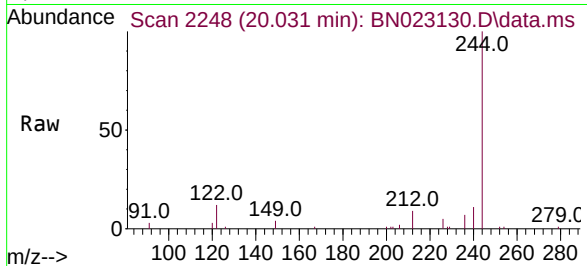


Tgt Ion:244 Resp: 9065
 Ion Ratio Lower Upper
 244 100
 212 8.8 7.6 11.4
 122 12.0 12.6 18.8

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/13/2022
 Supervised By :mohammad ahmed 12/14/2022

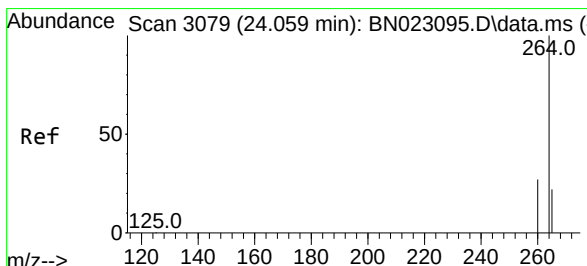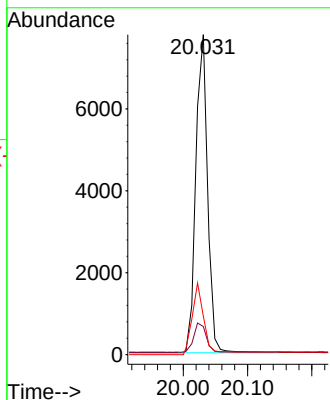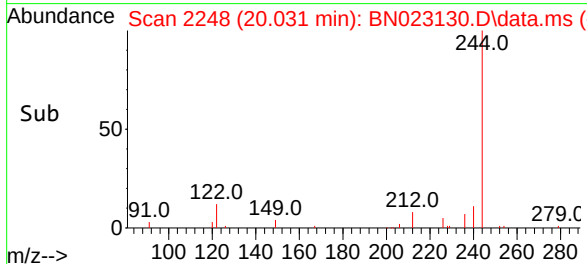

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.053 min Scan# 3077
 Delta R.T. 0.003 min
 Lab File: BN023130.D
 Acq: 12 Dec 2022 11:51

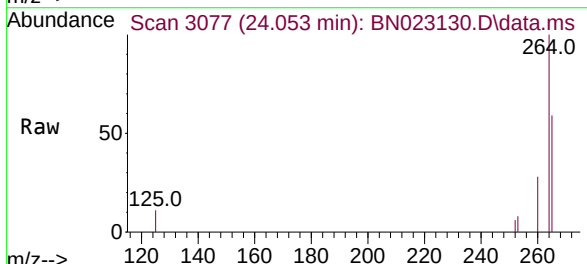

Tgt Ion:264 Resp: 11864
 Ion Ratio Lower Upper
 264 100
 260 27.6 21.7 32.5
 265 58.7 43.2 64.8

