


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023127.D
 Acq On : 12 Dec 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 12 05:18:26 2022

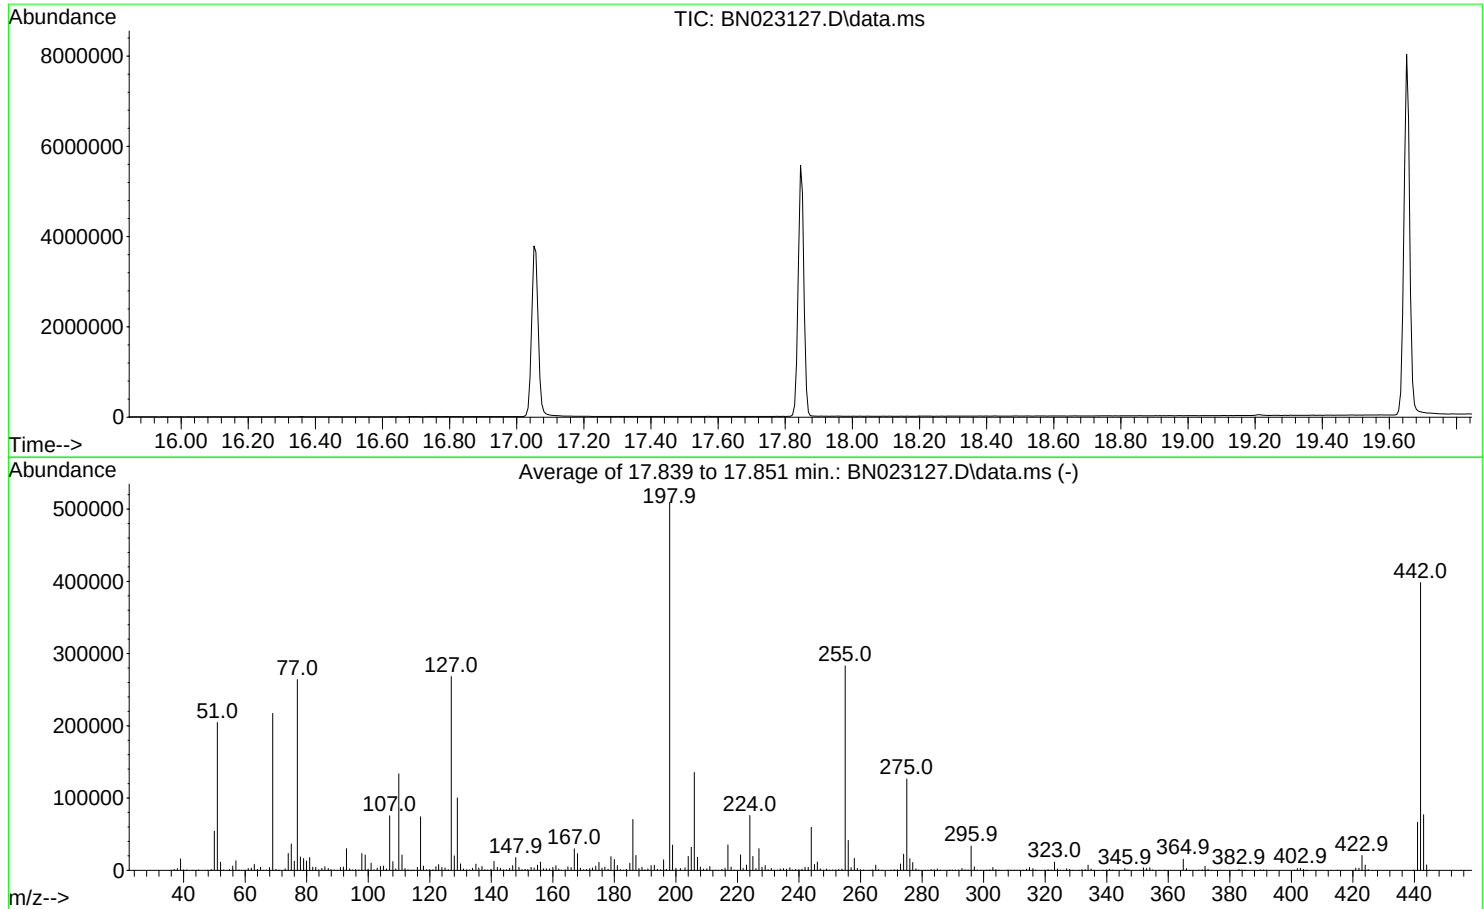




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	204587	PASS
68	69	0.00	2	1.7	3684	PASS
69	198	0.00	100	42.6	217173	PASS
70	69	0.00	2	0.5	1188	PASS
127	198	10	80	52.7	268203	PASS
197	198	0.00	2	0.2	999	PASS
198	198	100	100	100.0	509248	PASS
199	198	5	9	6.8	34813	PASS
275	198	10	60	24.8	126408	PASS
365	198	1	100	3.0	15371	PASS
441	198	0.01	100	13.1	66523	PASS
442	442	50	100	100.0	398357	PASS
443	442	15	24	19.3	76896	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023127.D
 Acq On : 12 Dec 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 13 08:04:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 08:04:03 2022
 Response via : Initial Calibration

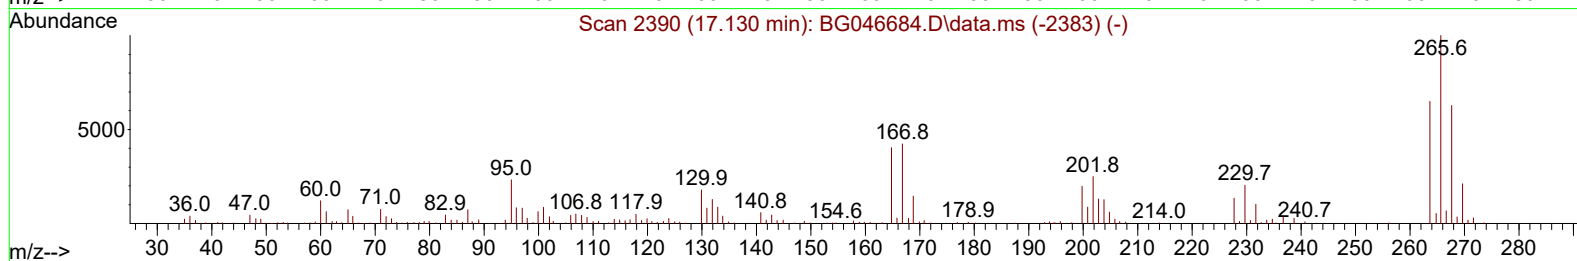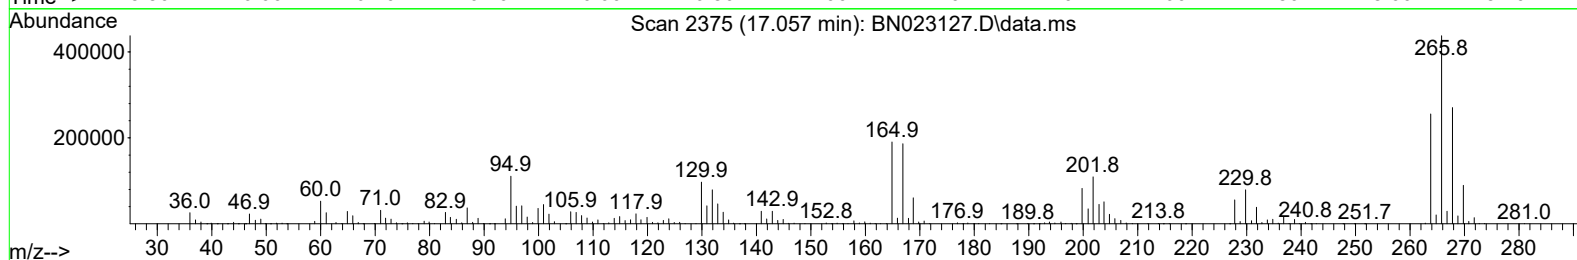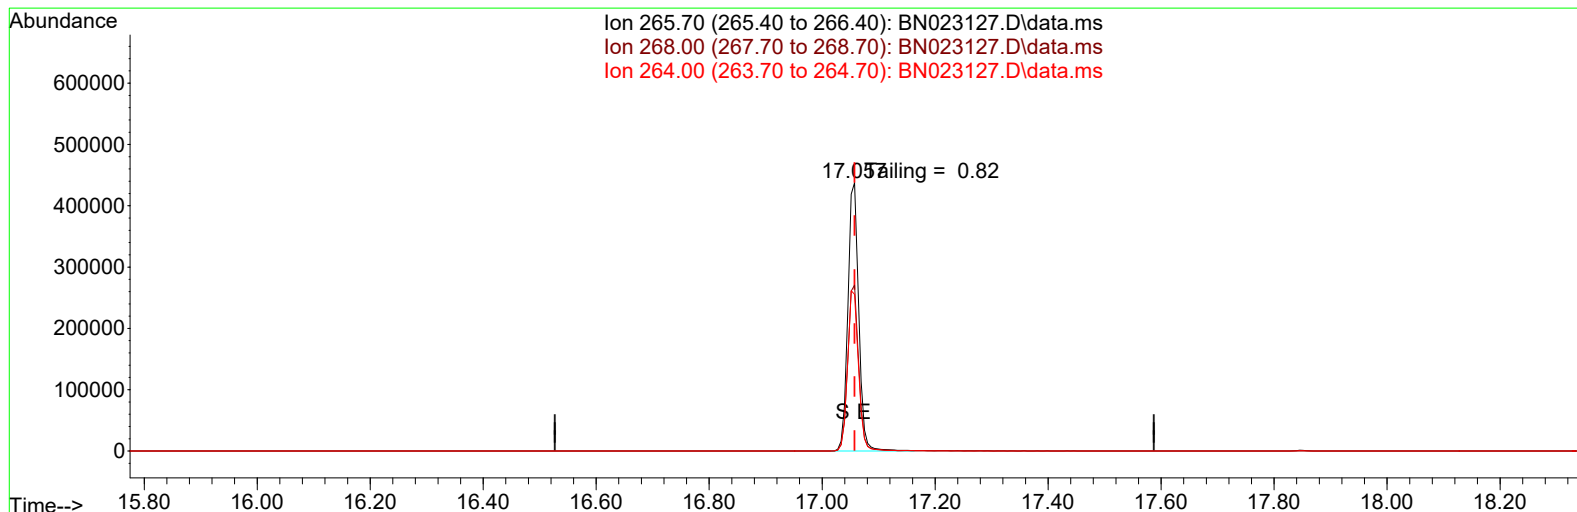

TIC: BN023127.D\data.ms

(70) Pentachlorophenol (C)

17.057min (0.000) 22440.85 ng




response 583805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.83
264.00	61.60	58.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023127.D
 Acq On : 12 Dec 2022 09:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 13 08:04:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 08:04:03 2022
 Response via : Initial Calibration

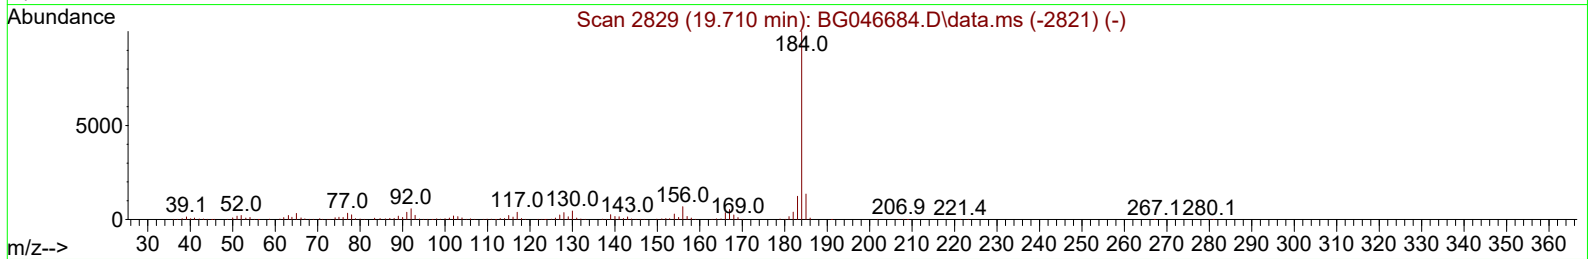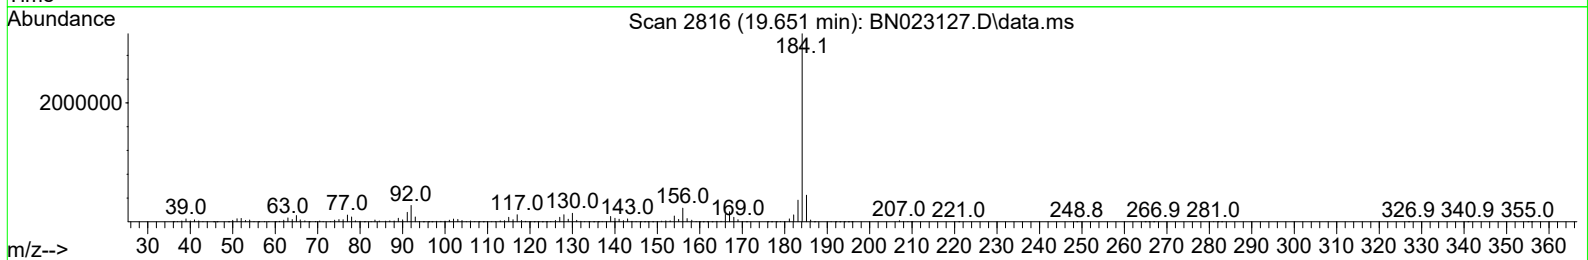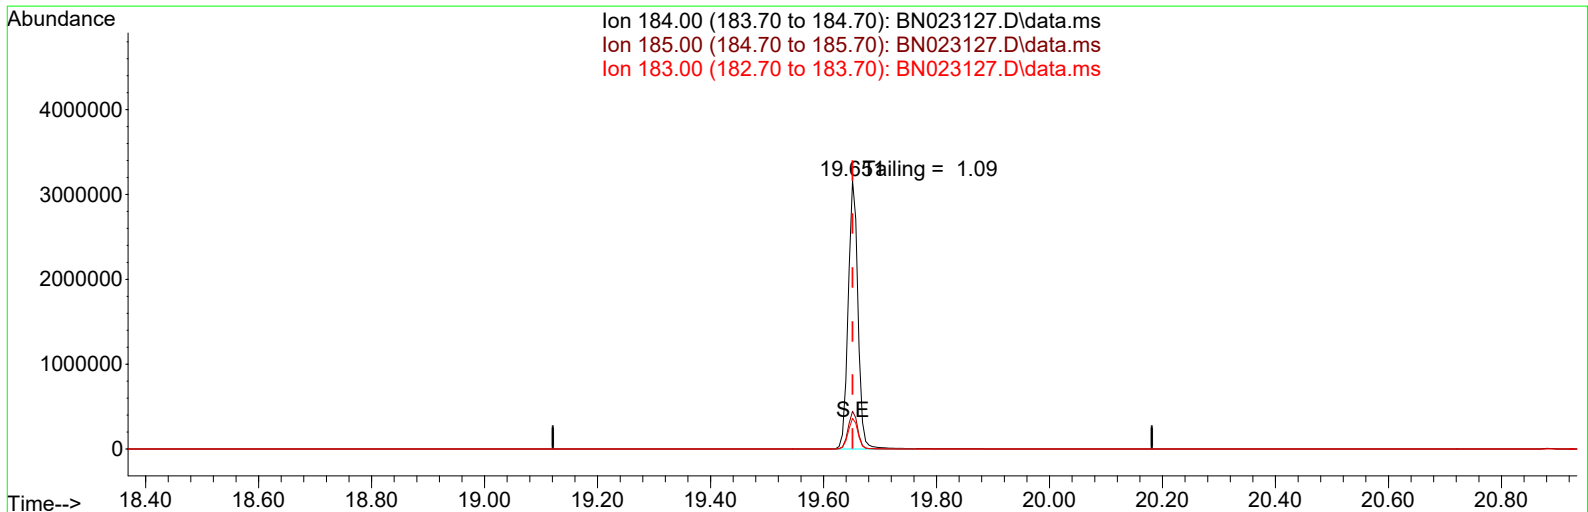

TIC: BN023127.D\data.ms

(77) Benzidine

19.651min (0.000) 0.00 ng

response 3841322

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2022	BNA_N	<u>BN023127.D</u>
Compound Name	Response	Retention Time
DDT	1706917	20.886
DDD	13310	20.498
DDE	402	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13712	1720629	0.80

Instrument :
BNA_N
ClientSampleId :
DFTPP