


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
 Data File : BN023145.D
 Acq On : 12 Dec 2022 21:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 12 05:18:26 2022

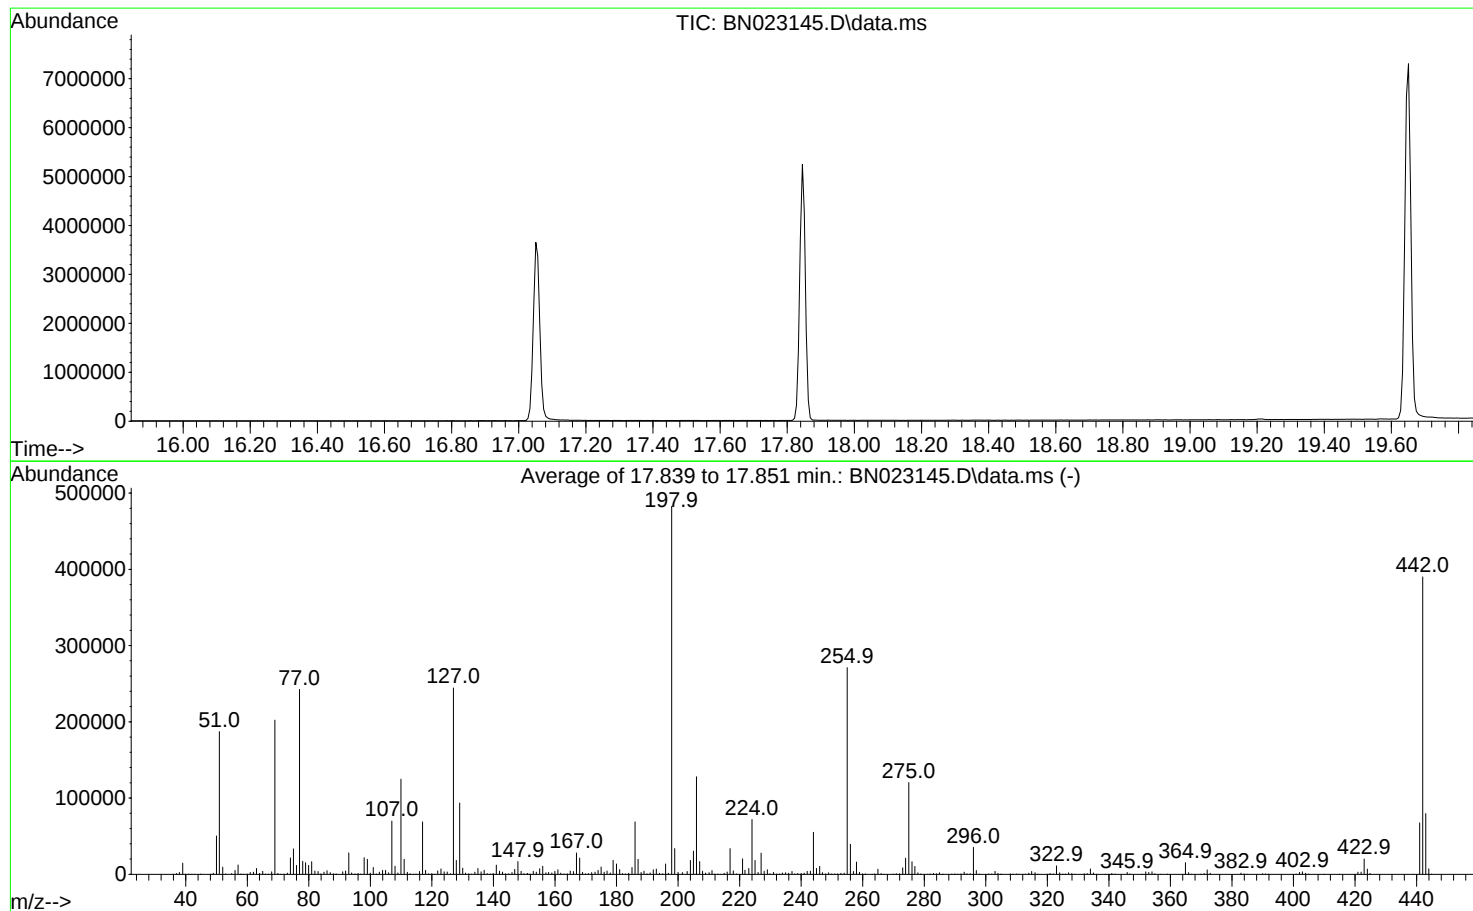




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	187107	PASS
68	69	0.00	2	1.7	3347	PASS
69	198	0.00	100	41.9	202133	PASS
70	69	0.00	2	0.6	1175	PASS
127	198	10	80	50.7	244395	PASS
197	198	0.00	2	0.3	1374	PASS
198	198	100	100	100.0	482496	PASS
199	198	5	9	7.0	33736	PASS
275	198	10	60	25.0	120400	PASS
365	198	1	100	3.1	15121	PASS
441	198	0.01	100	14.0	67432	PASS
442	442	50	100	100.0	390101	PASS
443	442	15	24	20.4	79669	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
Data File : BN023145.D
Acq On : 12 Dec 2022 21:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 13 08:05:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 08:04:03 2022
Response via : Initial Calibration

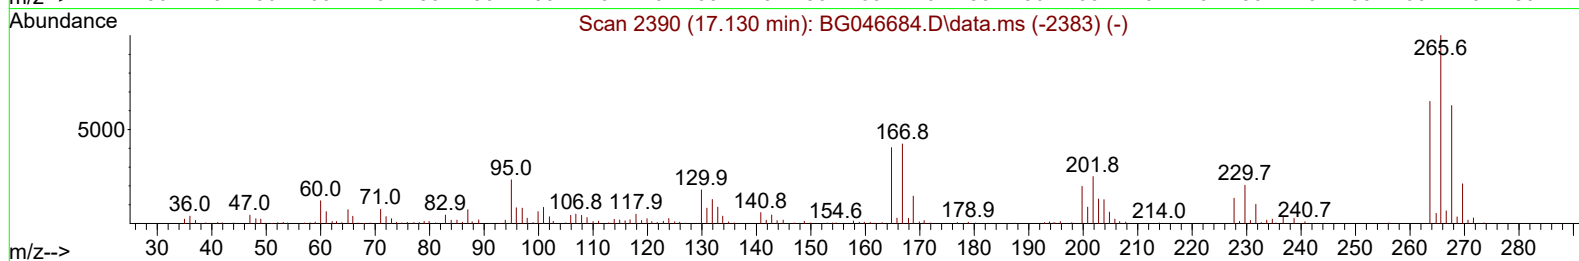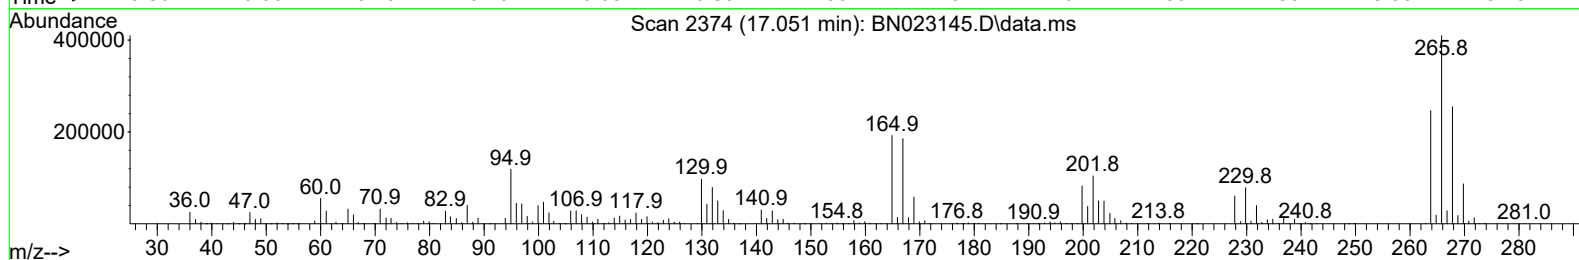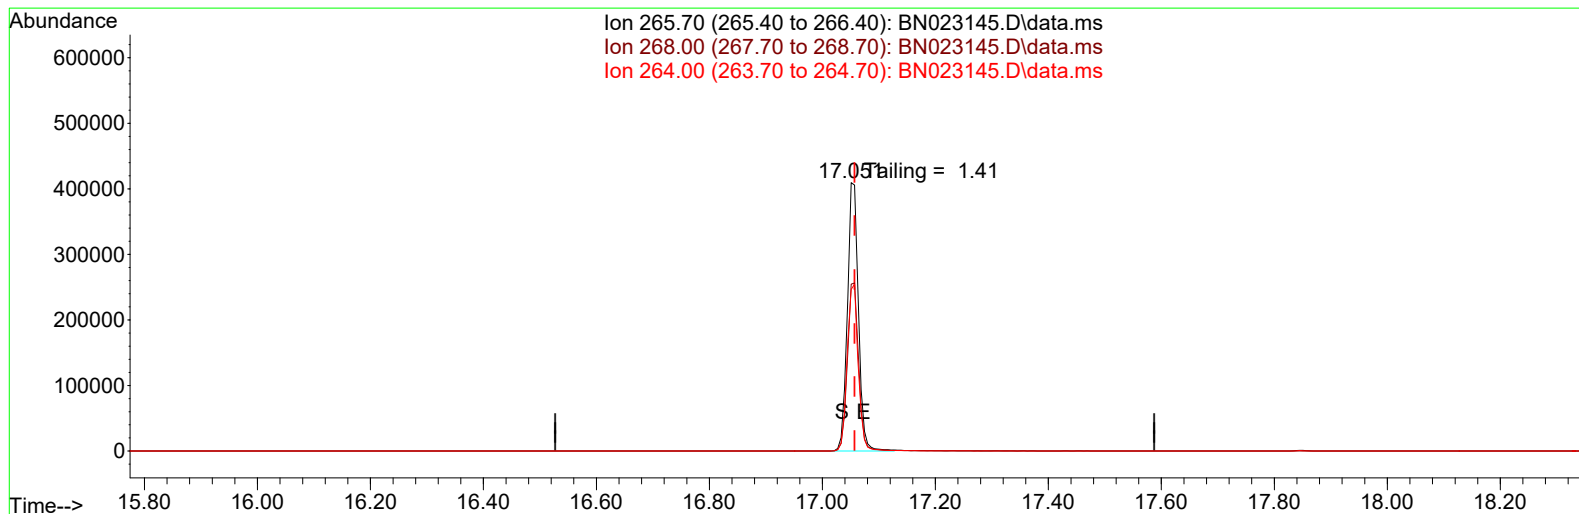

TIC: BN023145.D\data.ms

(70) Pentachlorophenol (C)

17.051min (-0.006) 21747.15 ng




response 558249

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.21
264.00	61.60	60.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121222\
Data File : BN023145.D
Acq On : 12 Dec 2022 21:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 13 08:05:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 08:04:03 2022
Response via : Initial Calibration

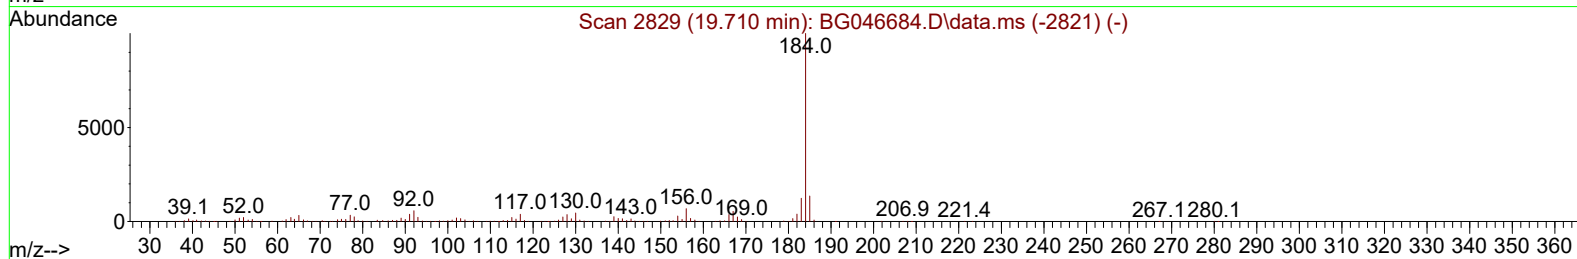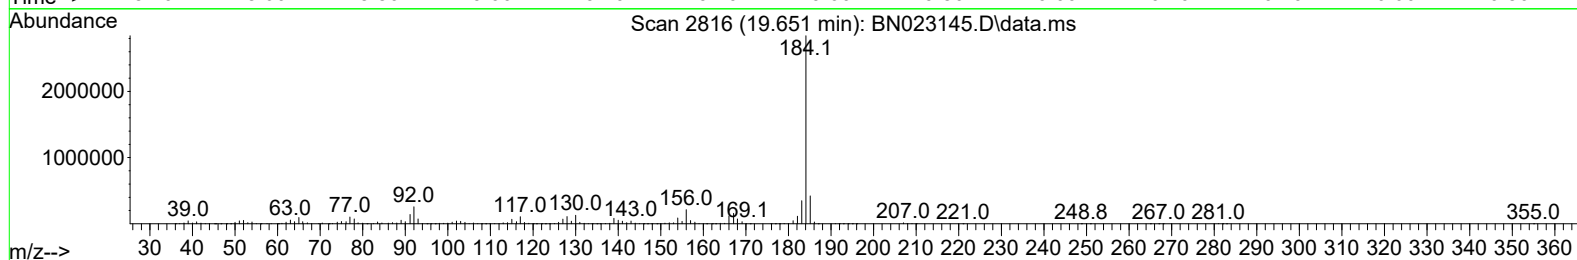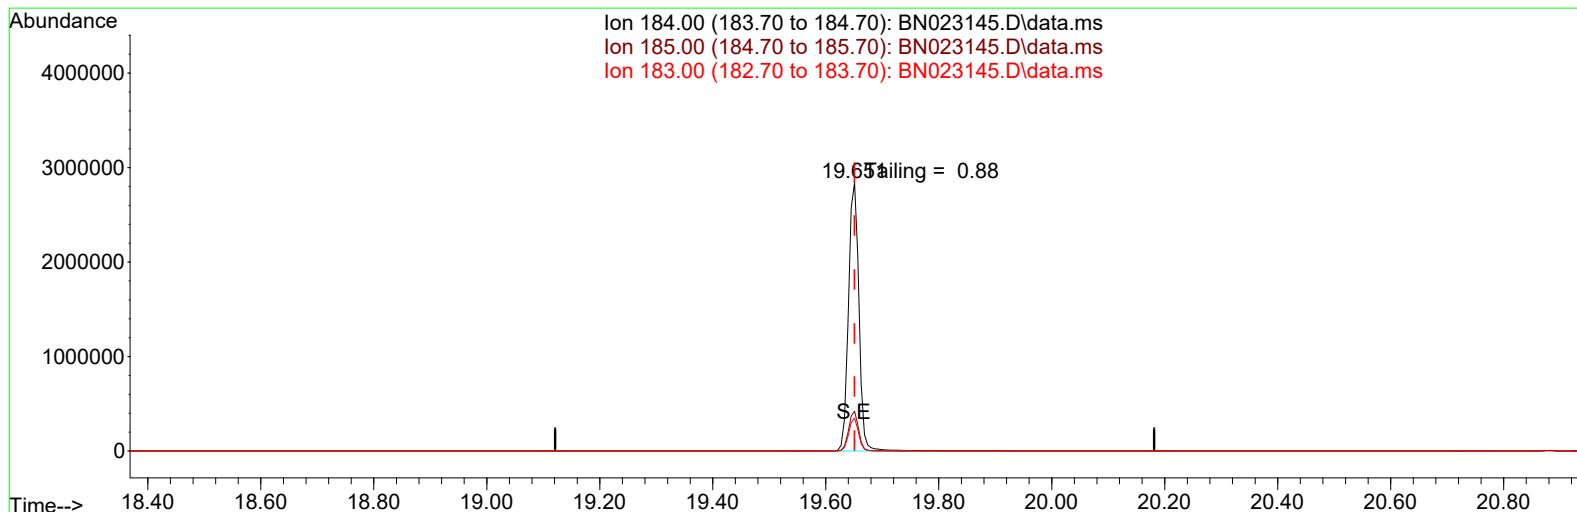

TIC: BN023145.D\data.ms

(77) Benzidine

19.651min (-0.000) 0.00 ng

response 3659736

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.83
183.00	13.20	12.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2022	BNA_N	<u>BN023145.D</u>
Compound Name	Response	Retention Time
DDT	1567235	20.88
DDD	40149	20.439
DDE	692	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40841	1608076	2.54

Instrument :
BNA_N
ClientSampleId :
DFTPP