
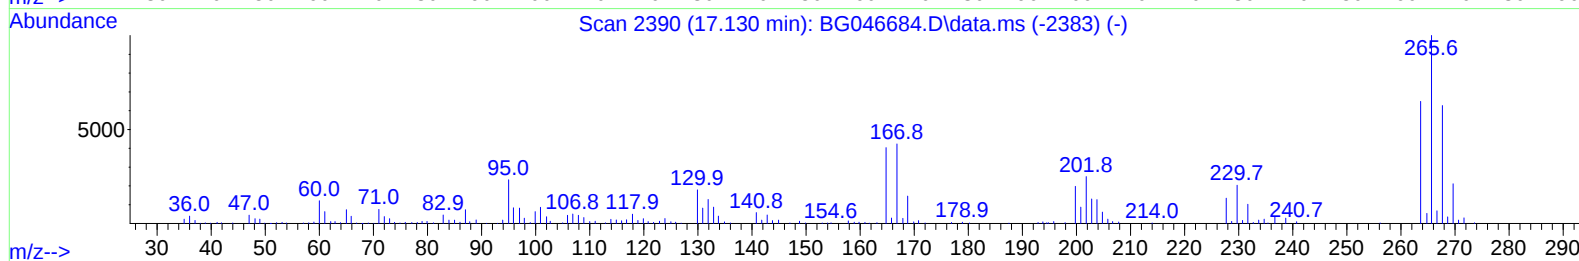
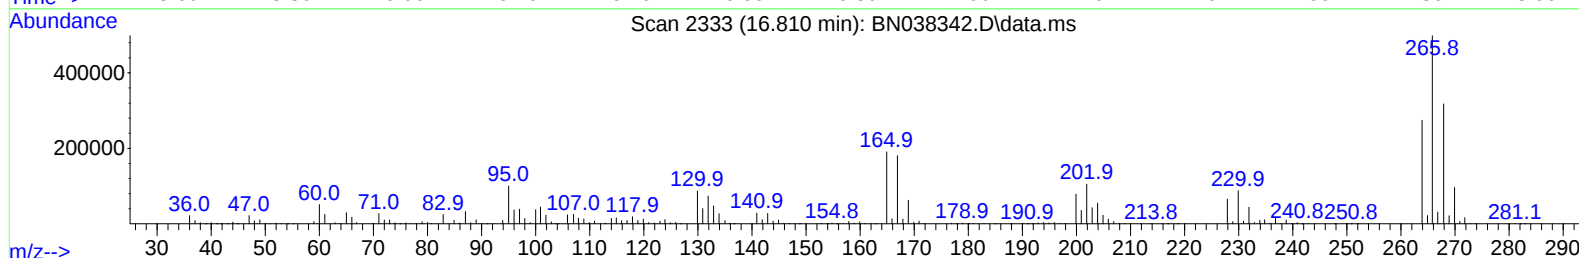


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121225\  
Data File : BN038342.D  
Acq On : 12 Dec 2025 08:45  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 10:08:50 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 12 03:10:04 2025  
Response via : Initial Calibration

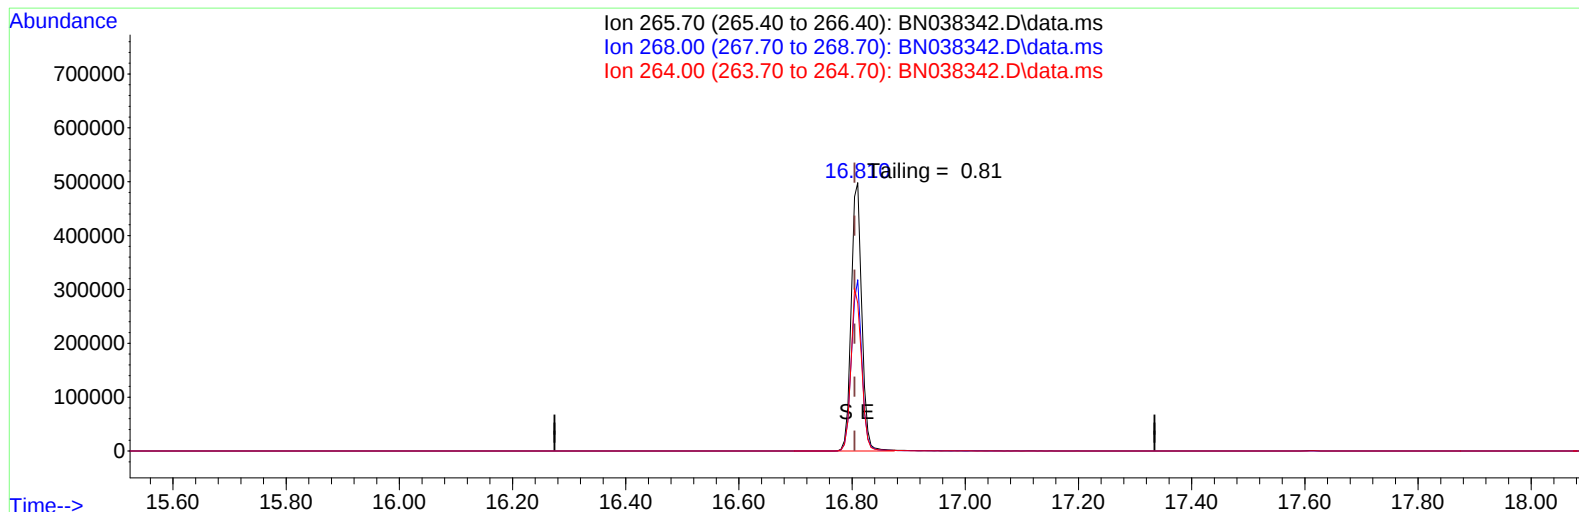

TIC: BN038342.D\data.ms

**(70) Pentachlorophenol (C)**




**16.810min (+ 0.006) 224665.32 ng**

**response 648827**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.78  |
| 264.00 | 61.60  | 55.06  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121225\  
Data File : BN038342.D  
Acq On : 12 Dec 2025 08:45  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 10:08:50 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 12 03:10:04 2025  
Response via : Initial Calibration

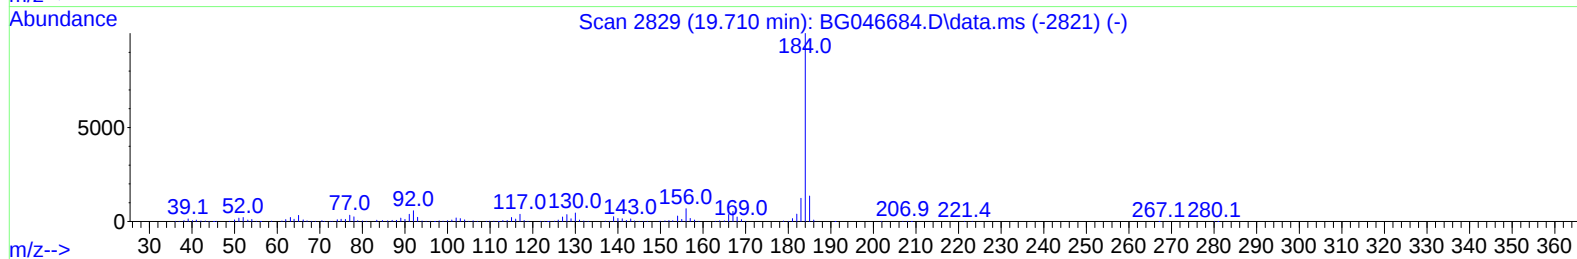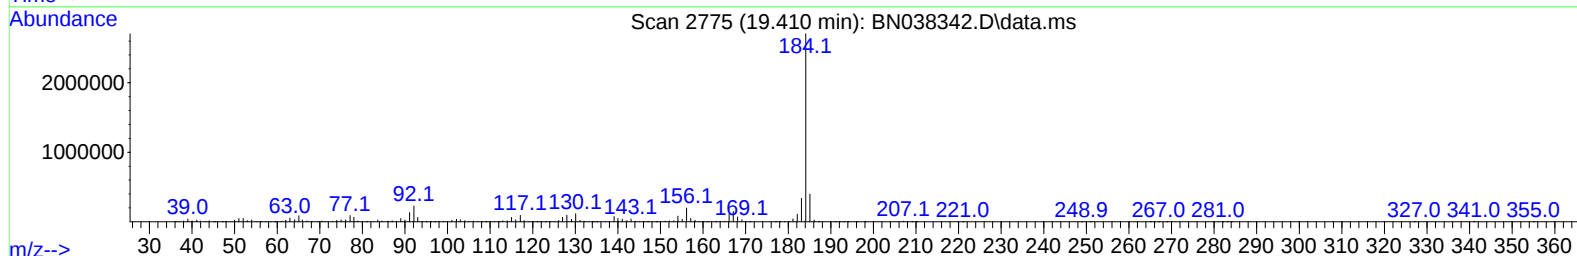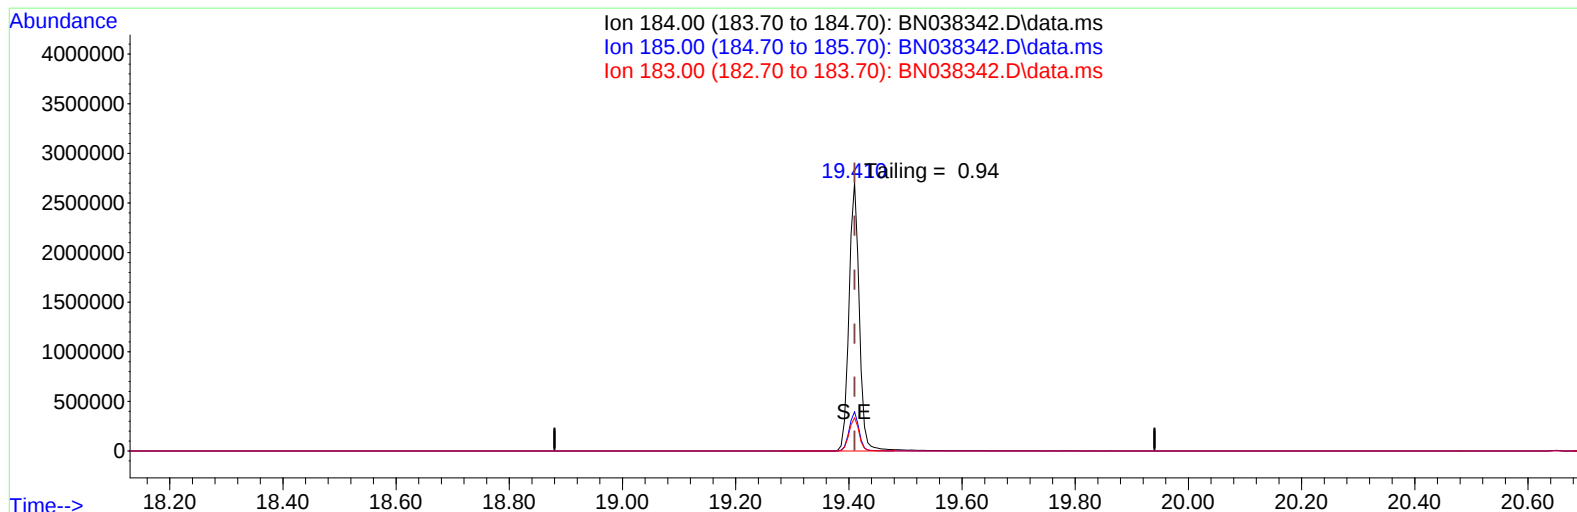

TIC: BN038342.D\data.ms

**(77) Benzidine****19.410min ( 0.000) 4688.42 ng m****response 3400755**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.67  |
| 183.00 | 13.20  | 12.40  |
| 0.00   | 0.00   | 0.00   |