
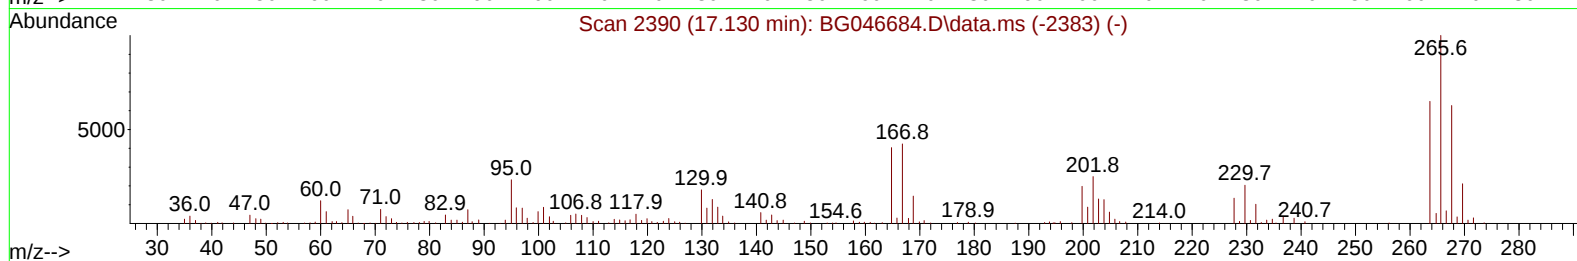
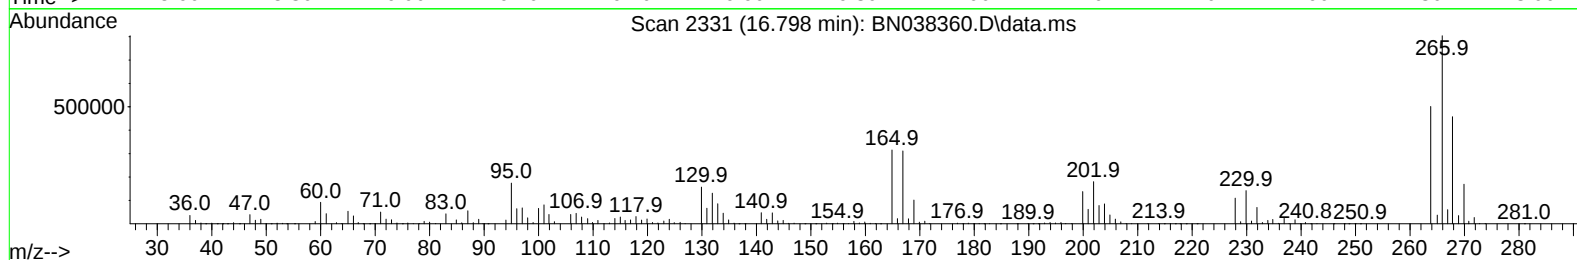


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038360.D
Acq On : 12 Dec 2025 21:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 07:57:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

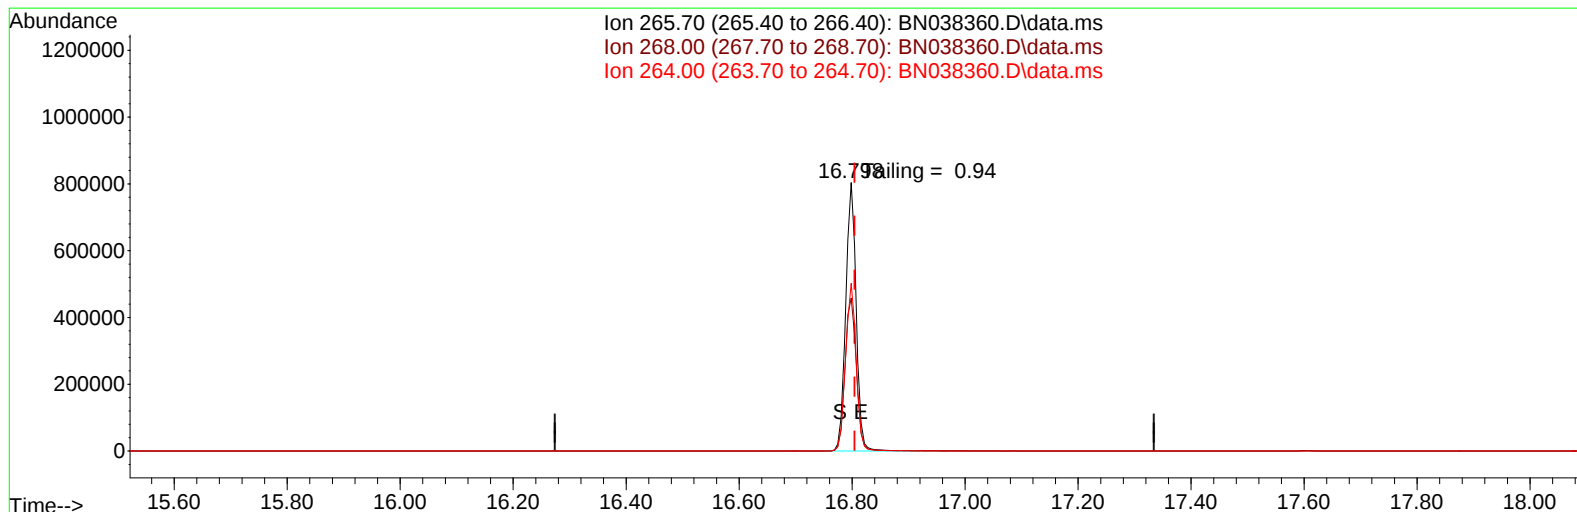

TIC: BN038360.D\data.ms

(70) Pentachlorophenol (C)




16.798min (-0.006) 226726.49 ng

response 1028431

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.98
264.00	61.60	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038360.D
Acq On : 12 Dec 2025 21:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 07:57:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

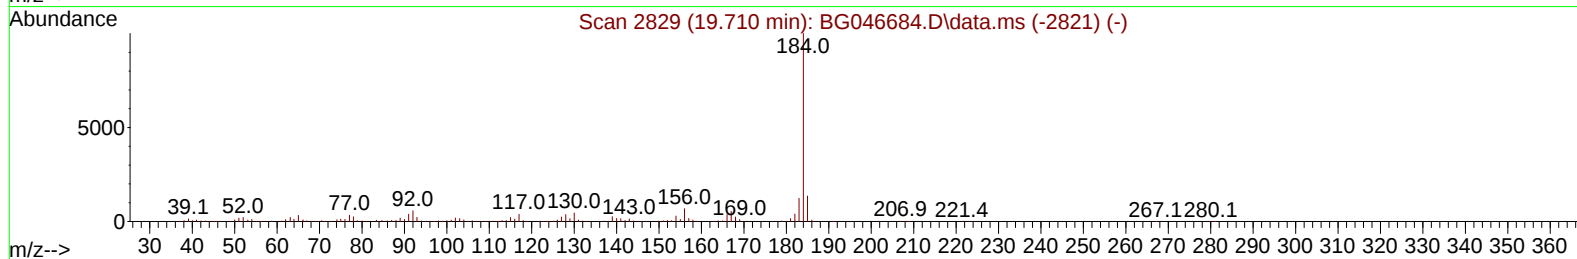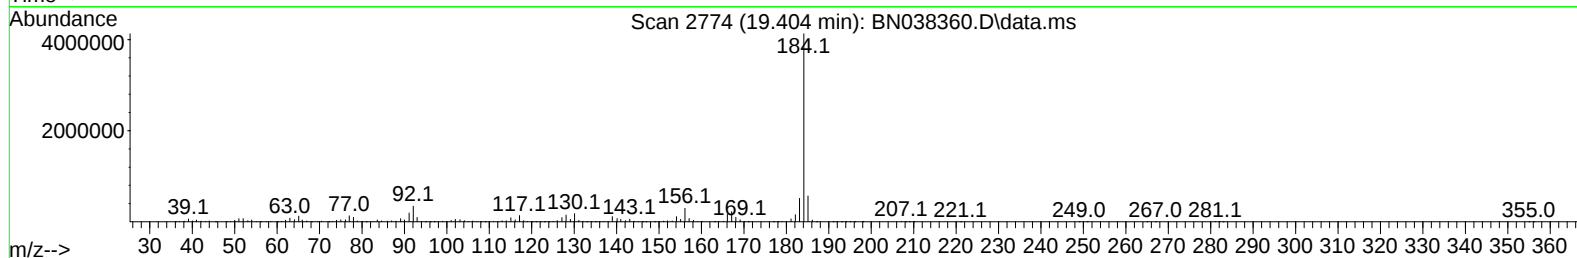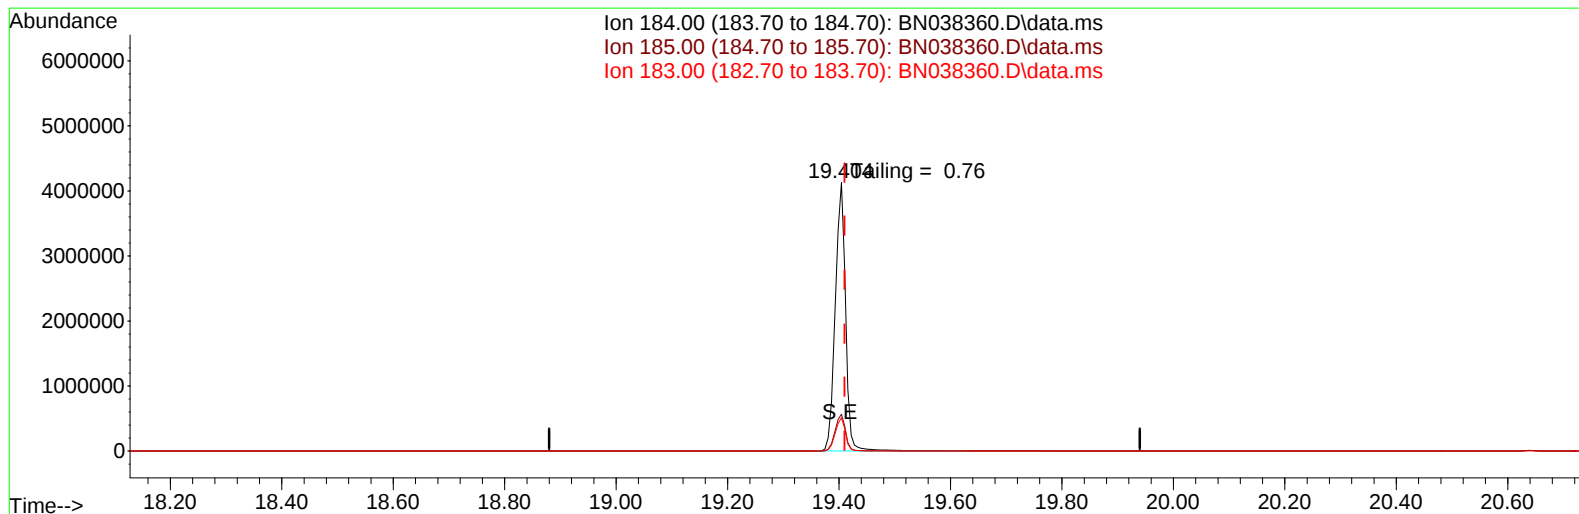

TIC: BN038360.D\data.ms

(77) Benzidine**19.404min (-0.006) 4504.77 ng****response 5342548**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	12.42
0.00	0.00	0.00