

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
 Data File : BN038369.D
 Acq On : 13 Dec 2025 03:03
 Operator : RC/JU
 Sample : Q3839-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAN3

Quant Time: Dec 13 06:06:39 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 13:56:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.717	152	5370	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	13907	0.400	ng	#-0.01
13) Acenaphthene-d10	14.388	164	6961	0.400	ng	-0.01
19) Phenanthrene-d10	17.136	188	12016	0.400	ng	#-0.01
29) Chrysene-d12	21.331	240	9585	0.400	ng	0.00
35) Perylene-d12	23.622	264	10050	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	3437	0.257	ng	0.00
5) Phenol-d6	6.887	99	3802	0.239	ng	0.00
8) Nitrobenzene-d5	8.875	82	2791	0.238	ng	0.00
11) 2-Methylnaphthalene-d10	12.121	152	4097	0.209	ng	0.00
14) 2,4,6-Tribromophenol	15.883	330	972	0.315	ng	-0.01
15) 2-Fluorobiphenyl	13.009	172	8444	0.252	ng	0.00
27) Fluoranthene-d10	19.178	212	5556	0.187	ng	0.00
31) Terphenyl-d14	19.782	244	4663	0.218	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.196	88	190	0.031	ng	# 76
9) Naphthalene	10.573	128	1229	0.030	ng	# 80
12) 2-Methylnaphthalene	12.197	142	655	0.025	ng	# 87
25) Phenanthrene	17.186	178	2160	0.052	ng	97
28) Fluoranthene	19.211	202	2412	0.054	ng	# 93
30) Pyrene	19.573	202	1628	0.035	ng	# 95
33) Chrysene	21.367	228	1143	0.028	ng	# 75
34) Bis(2-ethylhexyl)phtha...	21.259	149	1037	0.051	ng	# 91
37) Benzo(b)fluoranthene	22.932	252	1190	0.026	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038369.D
Acq On : 13 Dec 2025 03:03
Operator : RC/JU
Sample : Q3839-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN3

Quant Time: Dec 13 06:06:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 13:56:50 2025
Response via : Initial Calibration




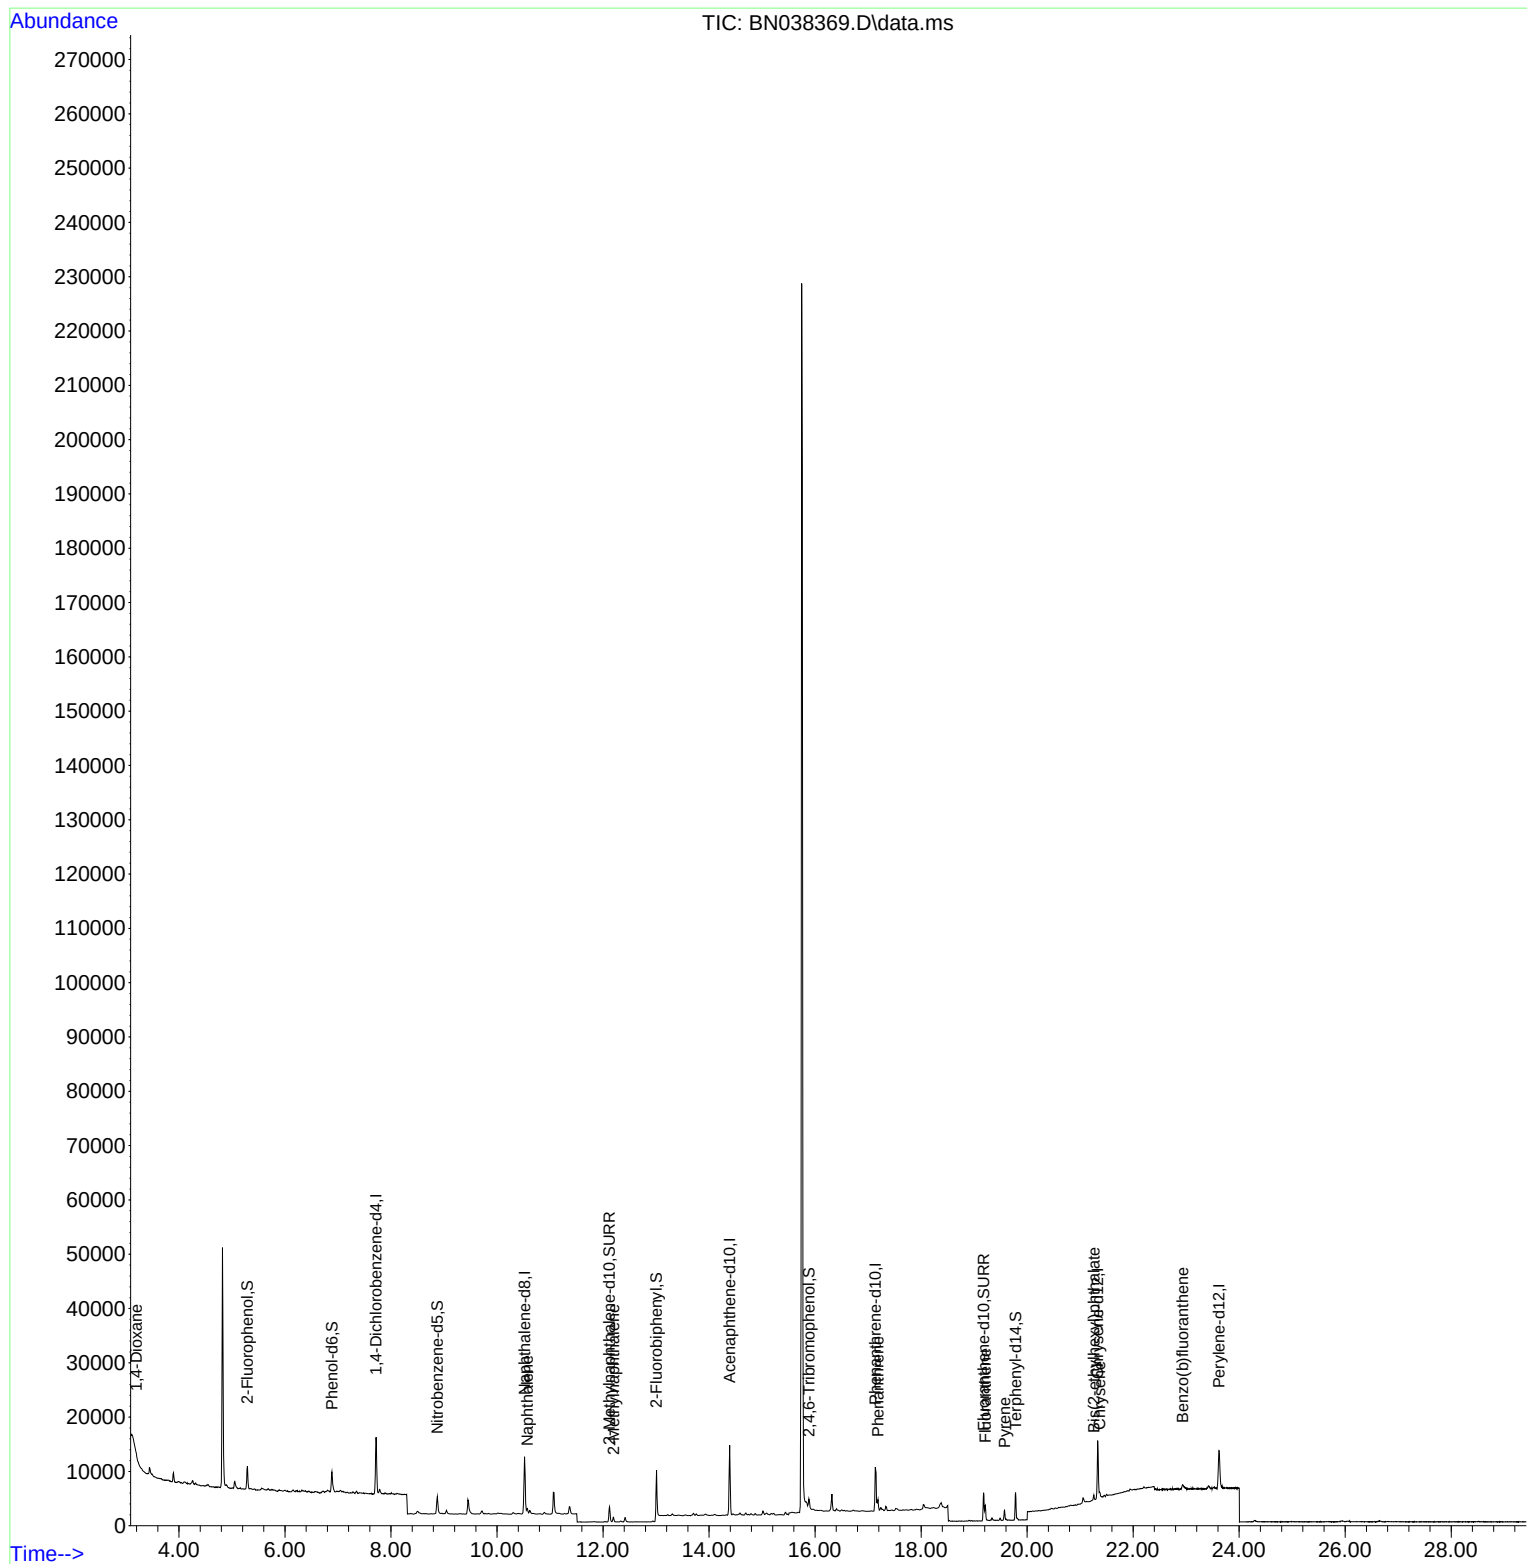


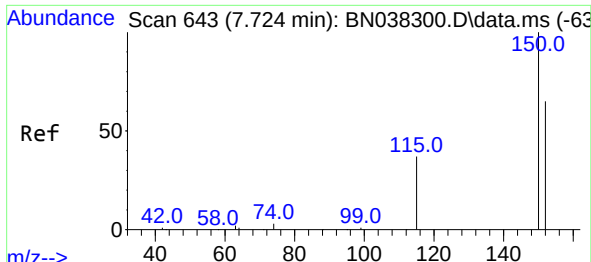

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.717 min Scan# 64
Delta R.T. -0.007 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:152 Resp: 5370
Ion Ratio Lower Upper
152 100
150 153.1 122.4 183.6
115 61.0 47.3 70.9

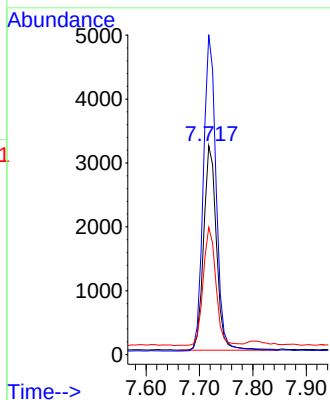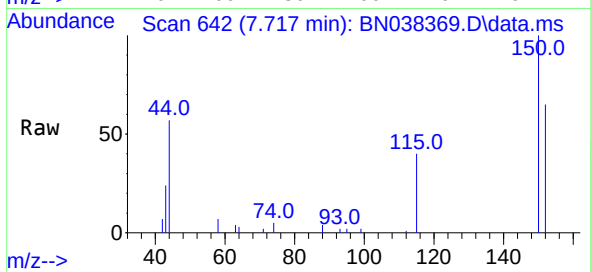

#2
1,4-Dioxane
Concen: 0.031 ng
RT: 3.196 min Scan# 16
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion: 88 Resp: 190
Ion Ratio Lower Upper
88 100
43 0.0 24.9 37.3#
58 66.8 61.4 92.0


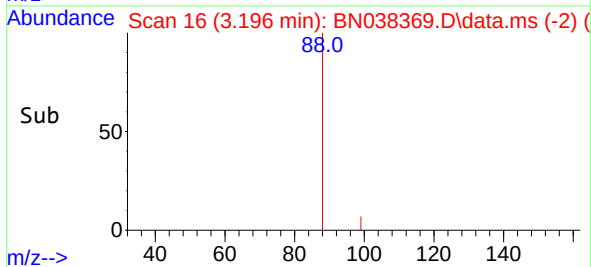
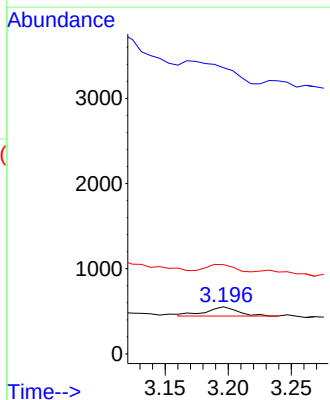
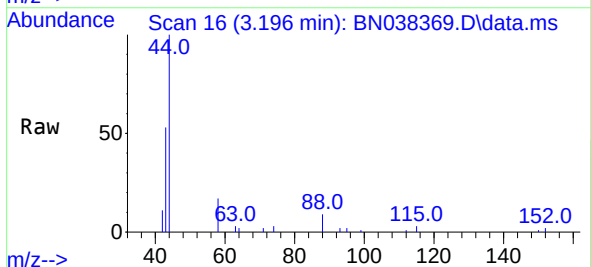




#4
2-Fluorophenol
Concen: 0.257 ng
RT: 5.291 min Scan# 306
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:112 Resp: 3437
Ion Ratio Lower Upper
112 100
64 58.3 44.4 66.6
63 31.0 23.4 35.0



#5
Phenol-d6
Concen: 0.239 ng
RT: 6.887 min Scan# 527
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion: 99 Resp: 3802
Ion Ratio Lower Upper
99 100
42 19.9 16.5 24.7
71 32.0 24.9 37.3

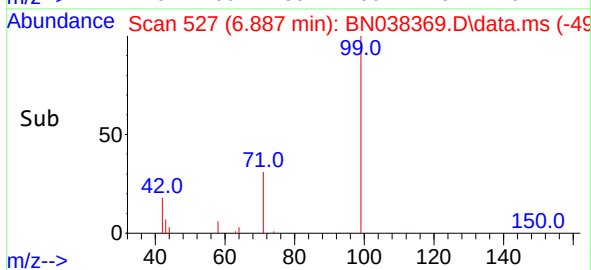







#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Instrument :
BNA_N
ClientSampleId :
C0AN3

Tgt Ion:136 Resp: 13907




Ion	Ratio	Lower	Upper
136	100		
137	11.8	9.1	13.7
54	9.5	5.2	7.8#
68	7.0	4.1	6.1#

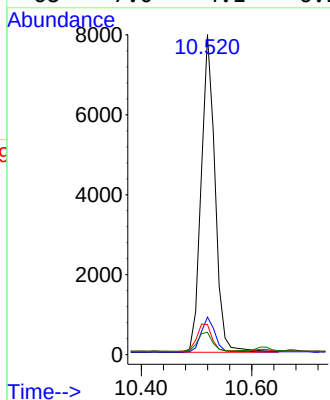


#8
Nitrobenzene-d5
Concen: 0.238 ng
RT: 8.875 min Scan# 777
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion: 82 Resp: 2791

Ion	Ratio	Lower	Upper
82	100		
128	48.7	34.0	51.0
54	54.6	44.4	66.6


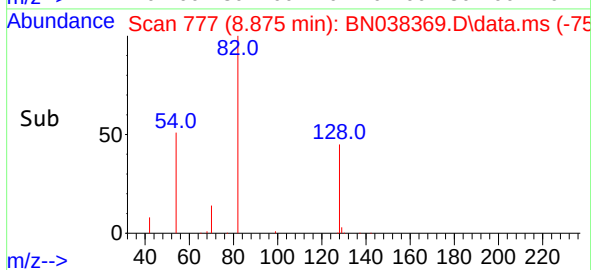
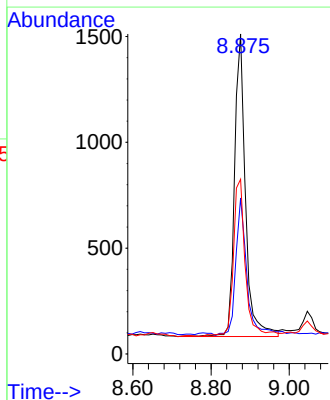



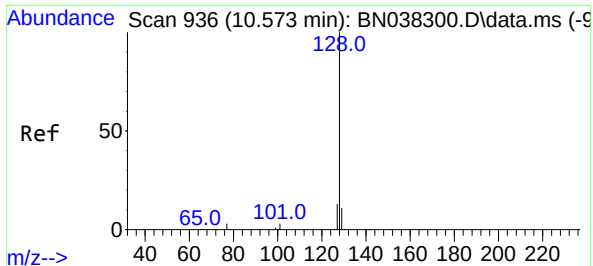

#9
Naphthalene
Concen: 0.030 ng
RT: 10.573 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:128 Resp: 1229
Ion Ratio Lower Upper
128 100
129 21.0 9.1 13.7#
127 19.6 10.9 16.3#

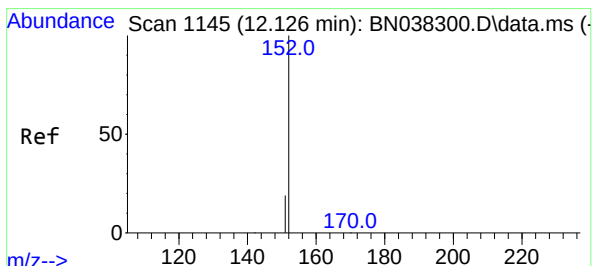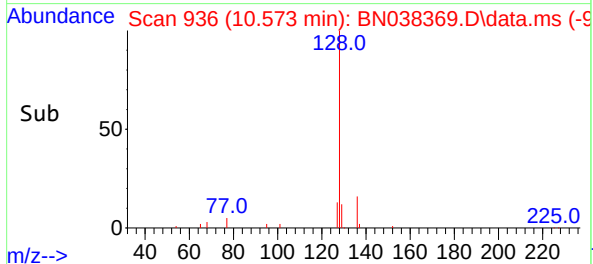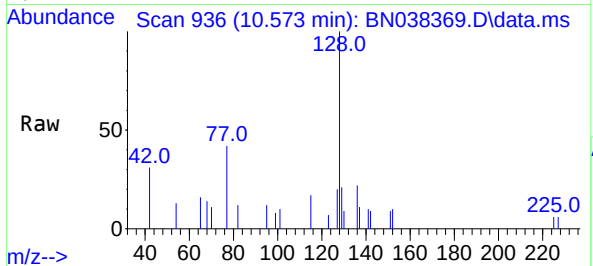

#11
2-Methylnaphthalene-d10
Concen: 0.209 ng
RT: 12.121 min Scan# 1144
Delta R.T. -0.005 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:152 Resp: 4097
Ion Ratio Lower Upper
152 100
151 20.6 17.0 25.6


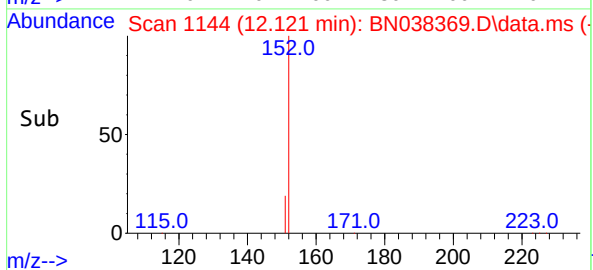

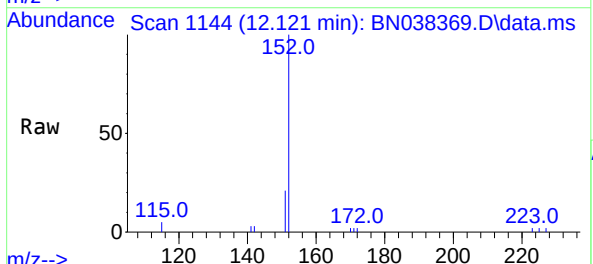




#12
2-Methylnaphthalene
Concen: 0.025 ng
RT: 12.197 min Scan# 1159
Delta R.T. -0.005 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:142 Resp: 655
Ion Ratio Lower Upper
142 100
141 94.1 71.4 107.2
115 55.1 28.4 42.6#

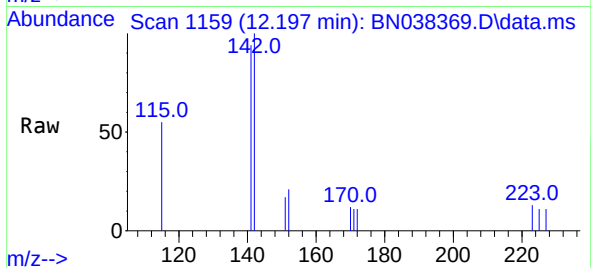

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.388 min Scan# 1448
Delta R.T. -0.011 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:164 Resp: 6961
Ion Ratio Lower Upper
164 100
162 104.3 86.2 129.4
160 52.4 44.6 67.0


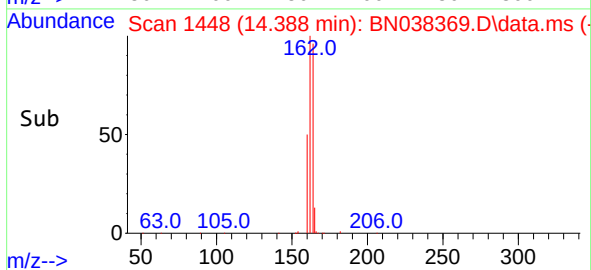






#14
2,4,6-Tribromophenol
Concen: 0.315 ng
RT: 15.883 min Scan# 1583
Delta R.T. -0.012 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:330 Resp: 972
Ion Ratio Lower Upper
330 100
332 96.5 75.8 113.6
141 39.7 31.8 47.8

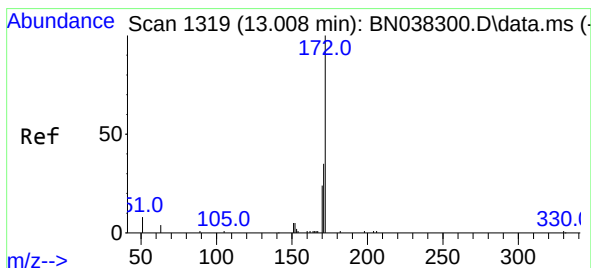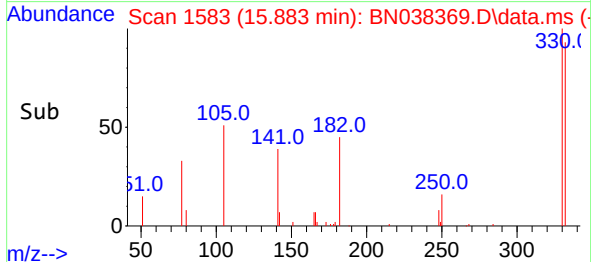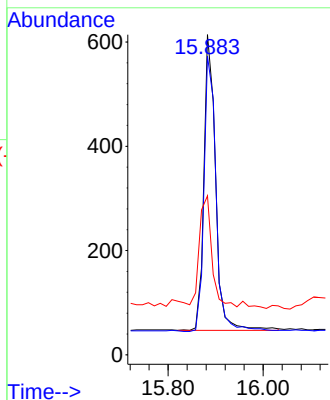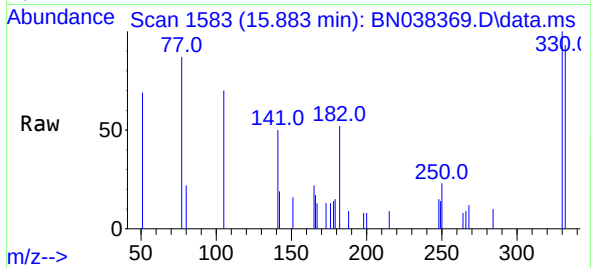

#15
2-Fluorobiphenyl
Concen: 0.252 ng
RT: 13.009 min Scan# 1319
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:172 Resp: 8444
Ion Ratio Lower Upper
172 100
171 35.5 28.6 42.8
170 23.9 19.3 28.9


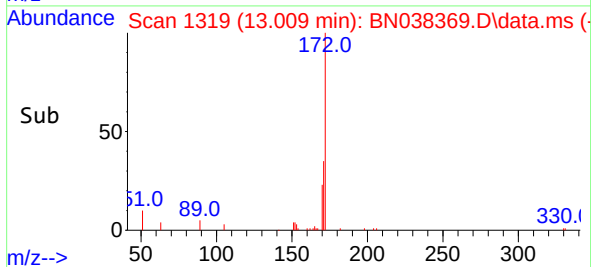
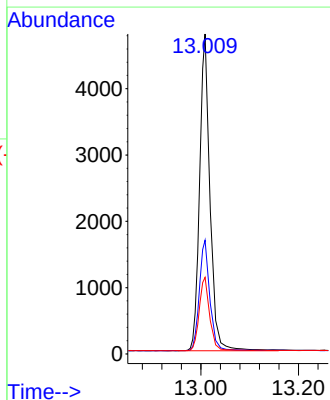
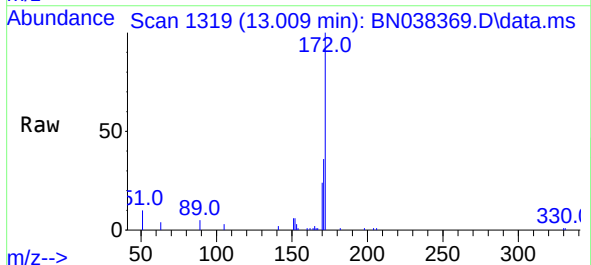




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.136 min Scan# 1684
Delta R.T. -0.012 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:188 Resp: 12016
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 17.4 7.4 11.0#

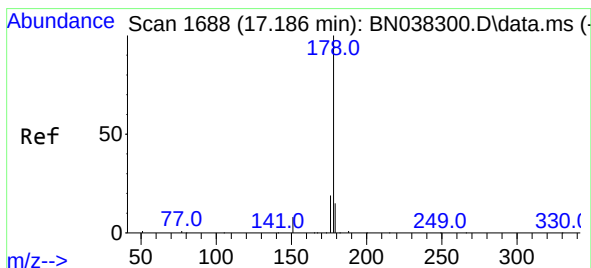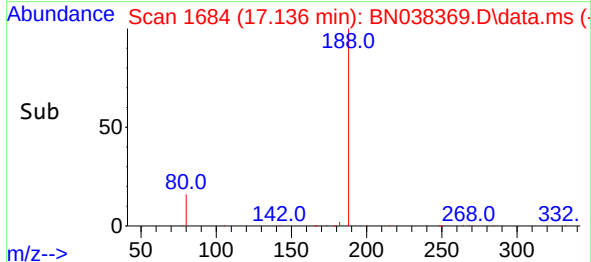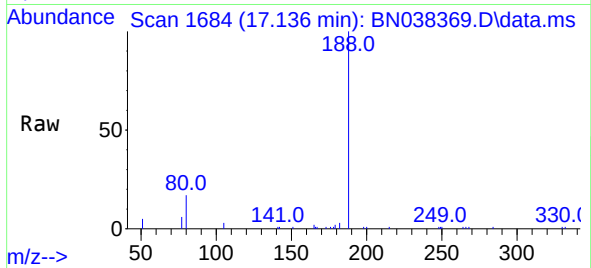

#25
Phenanthrene
Concen: 0.052 ng
RT: 17.186 min Scan# 1688
Delta R.T. 0.000 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:178 Resp: 2160
Ion Ratio Lower Upper
178 100
176 19.6 15.5 23.3
179 17.9 12.2 18.2


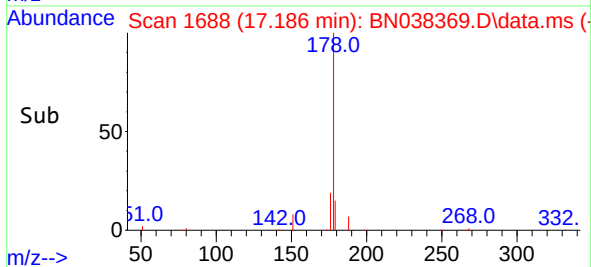

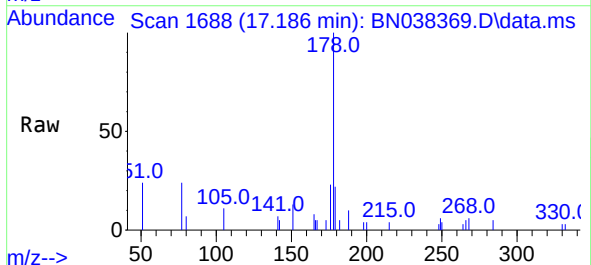




#27
Fluoranthene-d10
Concen: 0.187 ng
RT: 19.178 min Scan# 1938
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:212 Resp: 5556
Ion Ratio Lower Upper
212 100
106 18.2 13.7 20.5
104 10.4 7.8 11.8

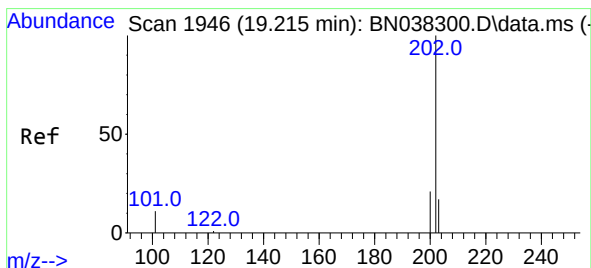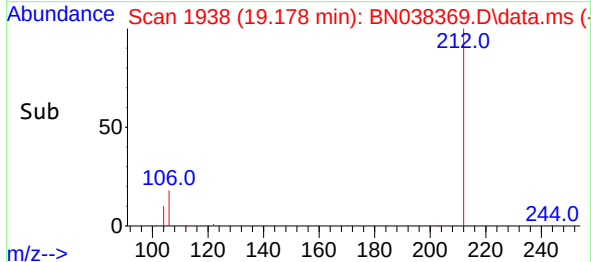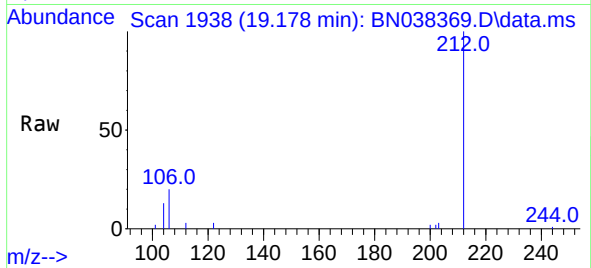

#28
Fluoranthene
Concen: 0.054 ng
RT: 19.211 min Scan# 1945
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:202 Resp: 2412
Ion Ratio Lower Upper
202 100
101 16.0 9.6 14.4#
203 18.7 13.5 20.3


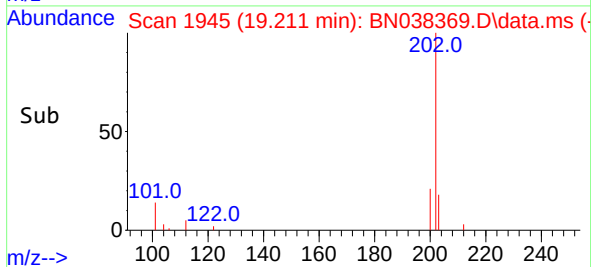

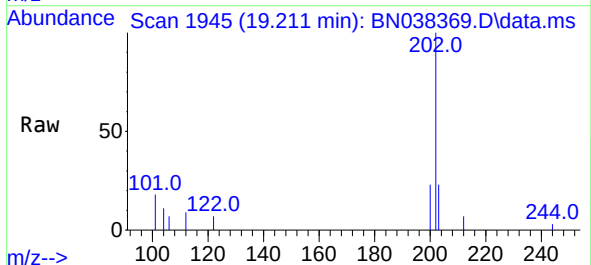




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.331 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:240 Resp: 9585
Ion Ratio Lower Upper
240 100
120 22.0 15.4 23.2
236 30.4 23.9 35.9



#30
Pyrene
Concen: 0.035 ng
RT: 19.573 min Scan# 2023
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03


Tgt Ion:202 Resp: 1628
Ion Ratio Lower Upper
202 100
200 21.4 16.9 25.3
203 22.0 14.2 21.2#

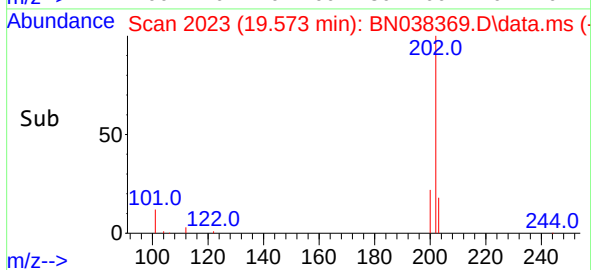






#31
Terphenyl-d14
Concen: 0.218 ng
RT: 19.782 min Scan# 2068
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Instrument :
BNA_N
ClientSampleId :
COAN3



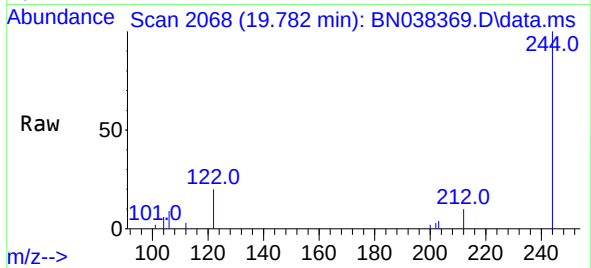



Tgt Ion:244 Resp: 4663
Ion Ratio Lower Upper
244 100
212 10.4 7.9 11.9
122 20.0 15.0 22.6

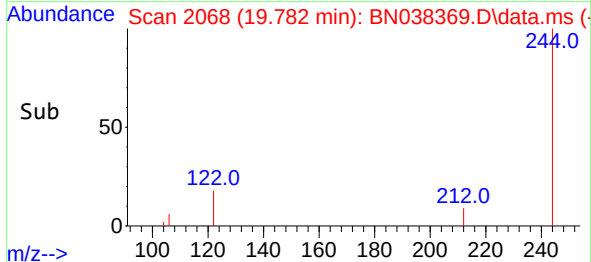

#33
Chrysene
Concen: 0.028 ng
RT: 21.367 min Scan# 2268
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:228 Resp: 1143
Ion Ratio Lower Upper
228 100
226 40.4 25.0 37.4#
229 36.3 15.5 23.3#


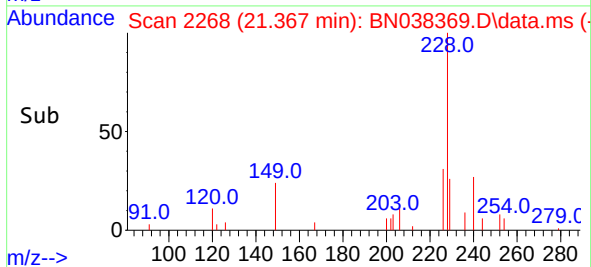

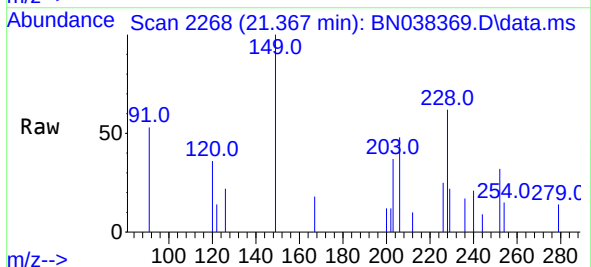


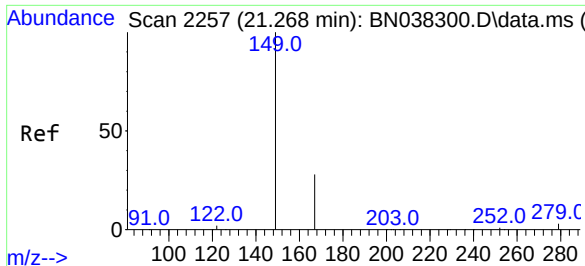

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.051 ng
RT: 21.259 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03




Instrument :
BNA_N
ClientSampleId :
COAN3


Tgt Ion:149 Resp: 1037
Ion Ratio Lower Upper
149 100
167 21.8 21.4 32.0
279 4.9 2.4 3.6#

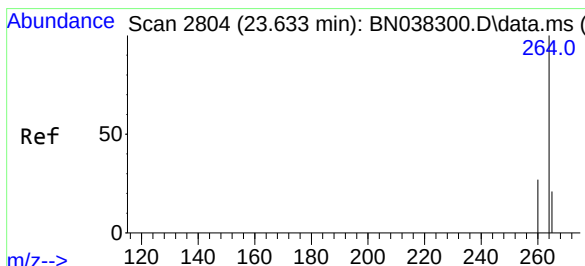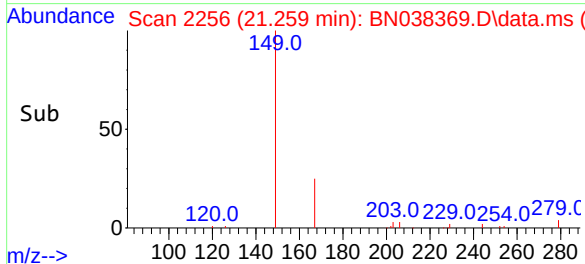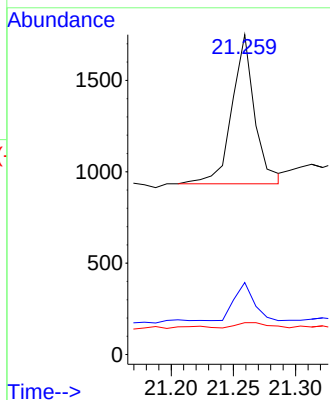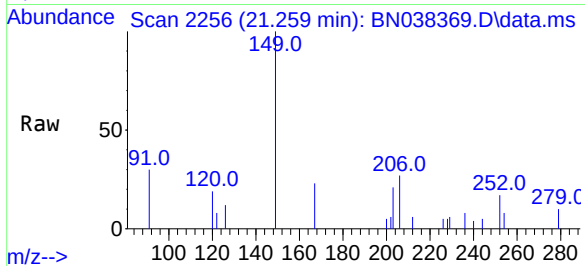

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.622 min Scan# 2800
Delta R.T. -0.012 min
Lab File: BN038369.D
Acq: 13 Dec 2025 03:03

Tgt Ion:264 Resp: 10050
Ion Ratio Lower Upper
264 100
260 27.4 22.2 33.2
265 110.0 80.2 120.2

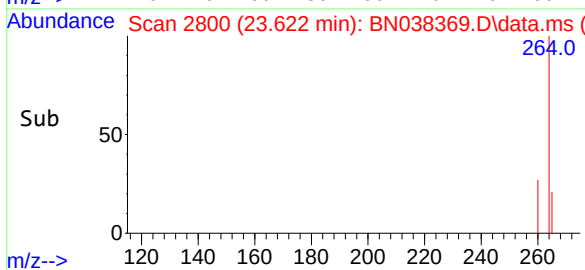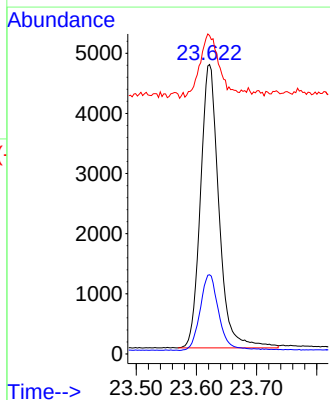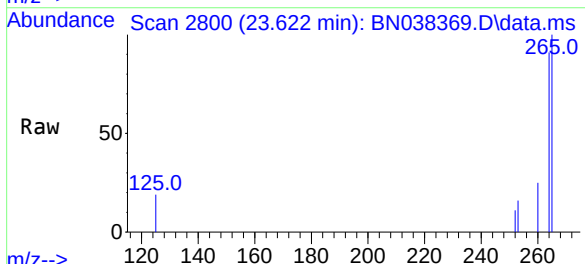

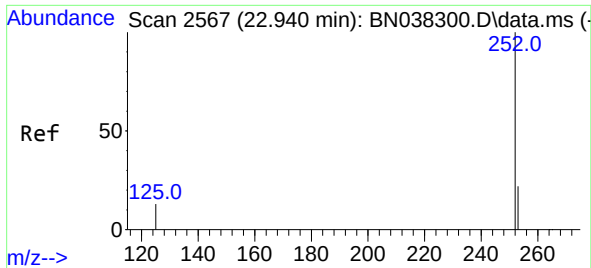

#37

Benzo(b)fluoranthene

Concen: 0.026 ng

RT: 22.932 min Scan# 21

Delta R.T. -0.014 min

Lab File: BN038369.D


Acq: 13 Dec 2025 03:03

Instrument :

BNA_N

ClientSampleId :

C0AN3

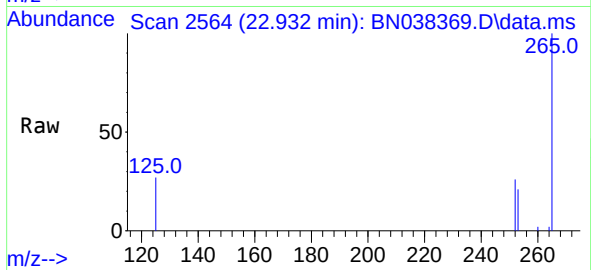

Tgt Ion:252 Resp: 1190

Ion Ratio Lower Upper

252 100

253 83.5 21.1 31.7#

125 104.9 16.4 24.6#

