


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038342.D
Acq On : 12 Dec 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

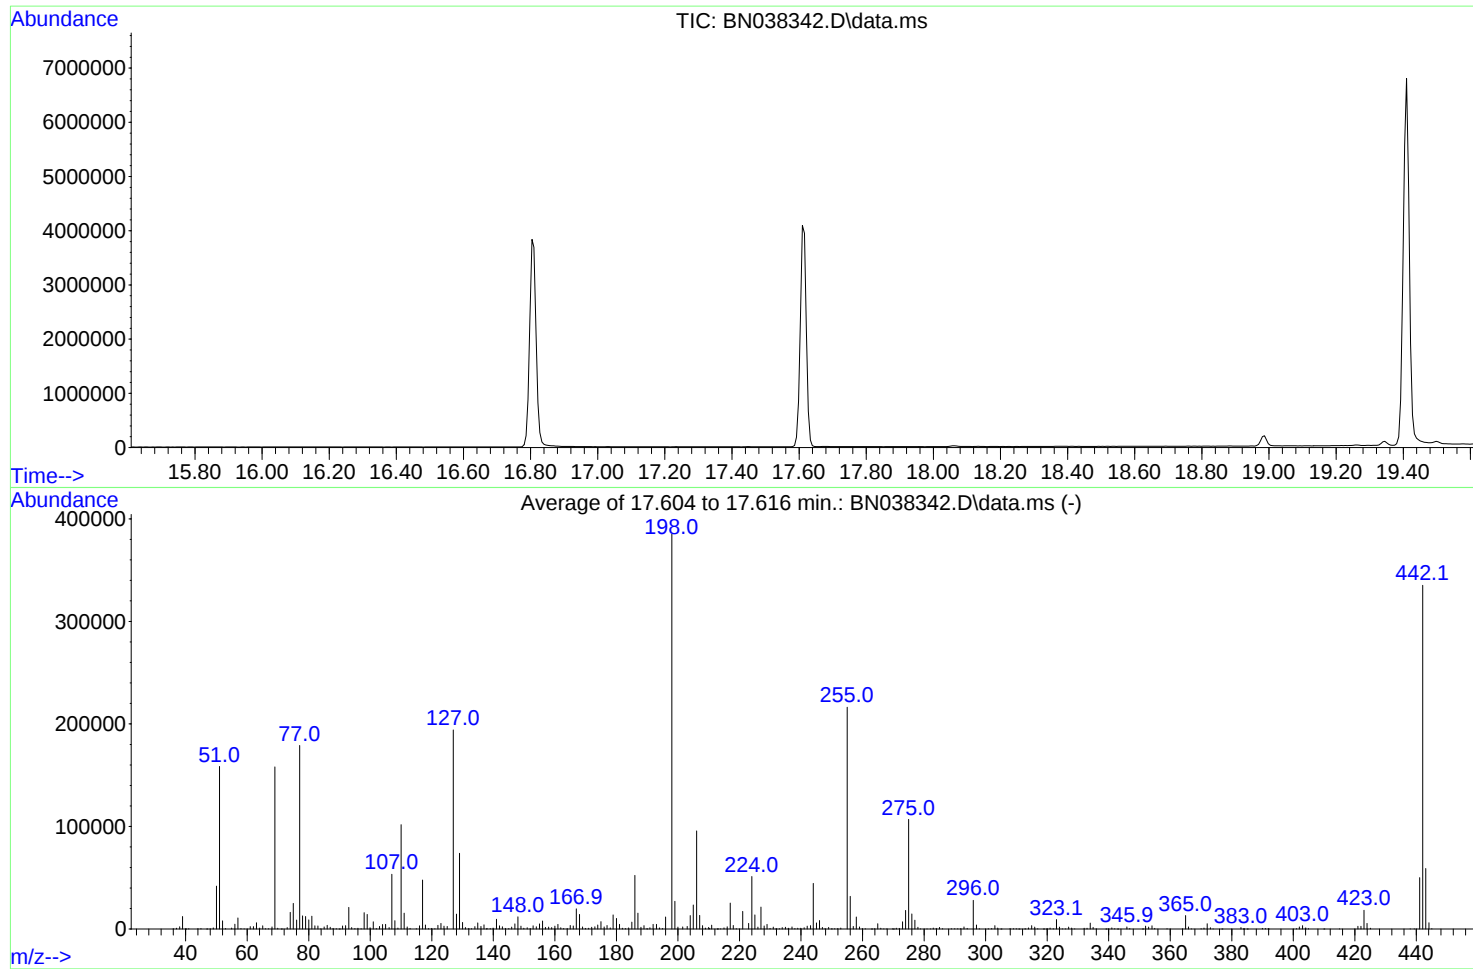

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.3	2072	PASS
69	69	100	100	100.0	158144	PASS
70	69	0.00	2	0.5	777	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	385088	PASS
199	198	5	9	7.0	26973	PASS
365	198	1	100	3.4	13061	PASS
441	443	0.01	150	85.0	50136	PASS
442	442	100	100	100.0	335232	PASS
443	442	15	24	17.6	58984	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/12/2025	BNA_N	<u>BN038342.D</u>
Compound Name	Response	Retention Time
DDT	1615063	20.651
DDD	69905	20.21
DDE	2480	19.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
72385	1687448	4.29

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038342.D
Acq On : 12 Dec 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 10:08:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

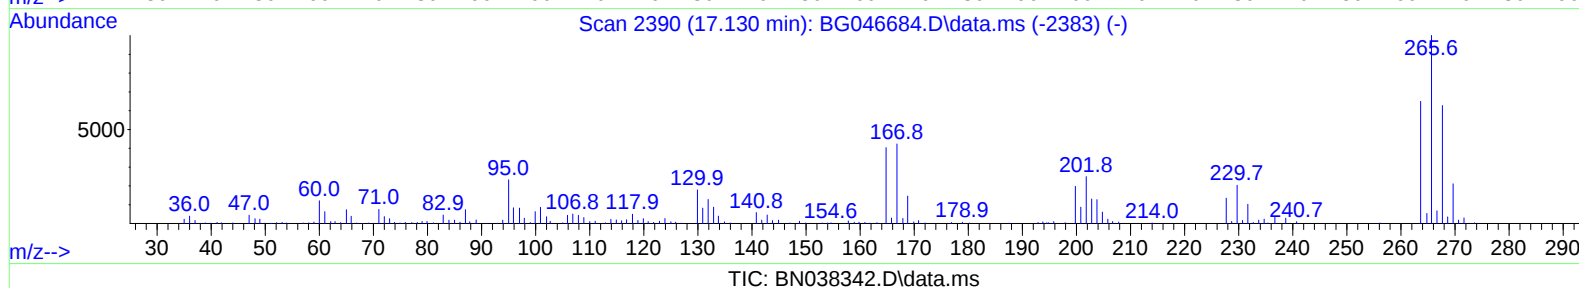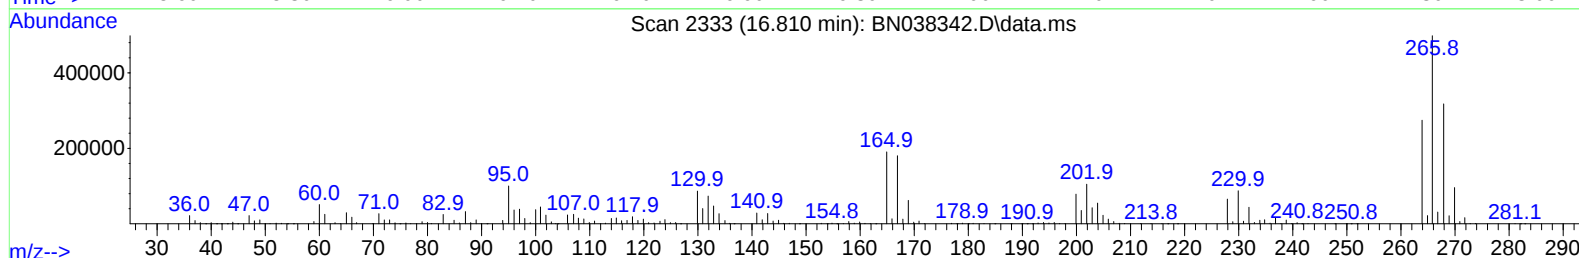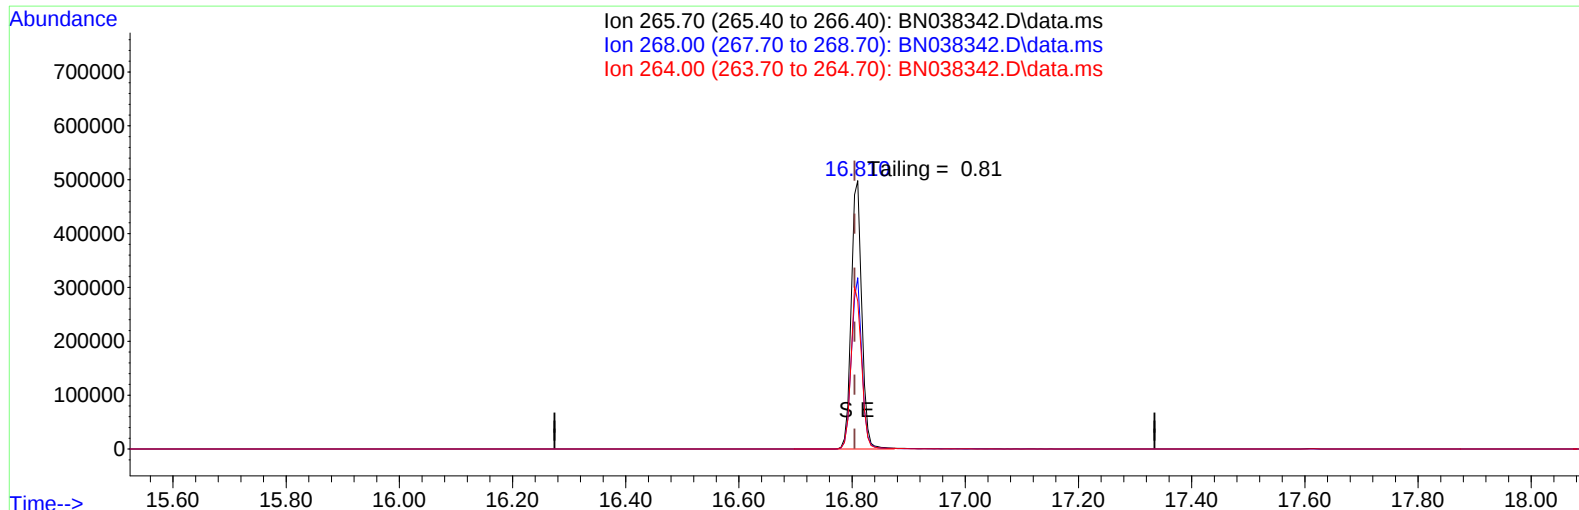

TIC: BN038342.D\data.ms

(70) Pentachlorophenol (C)

16.810min (+ 0.006) 224665.32 ng




response 648827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.78
264.00	61.60	55.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038342.D
Acq On : 12 Dec 2025 08:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 10:08:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

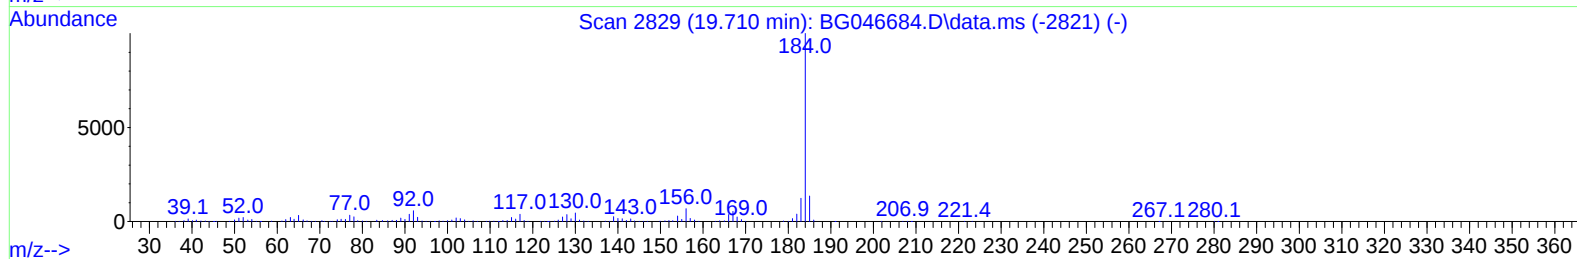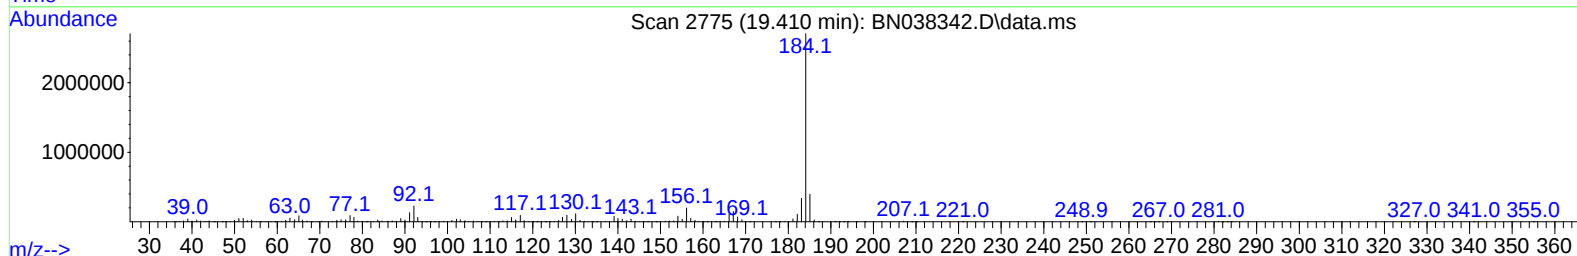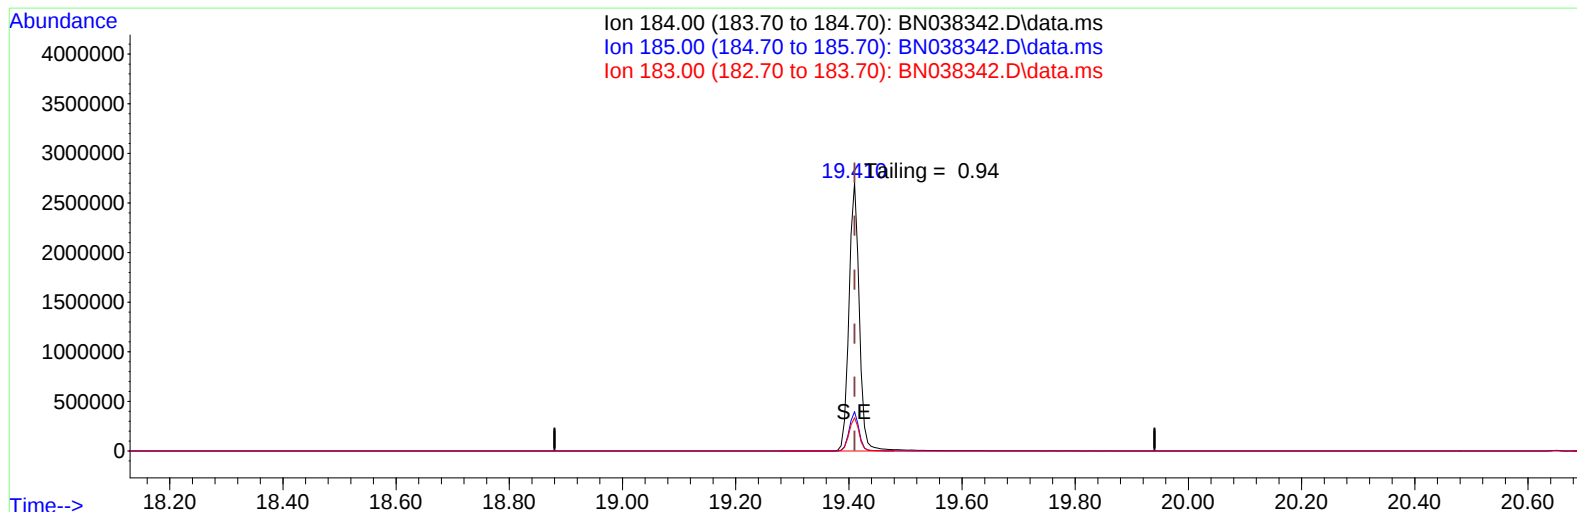

TIC: BN038342.D\data.ms

(77) Benzidine

19.410min (0.000) 4688.42 ng m

response 3400755

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.67
183.00	13.20	12.40
0.00	0.00	0.00