


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038360.D
Acq On : 12 Dec 2025 21:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

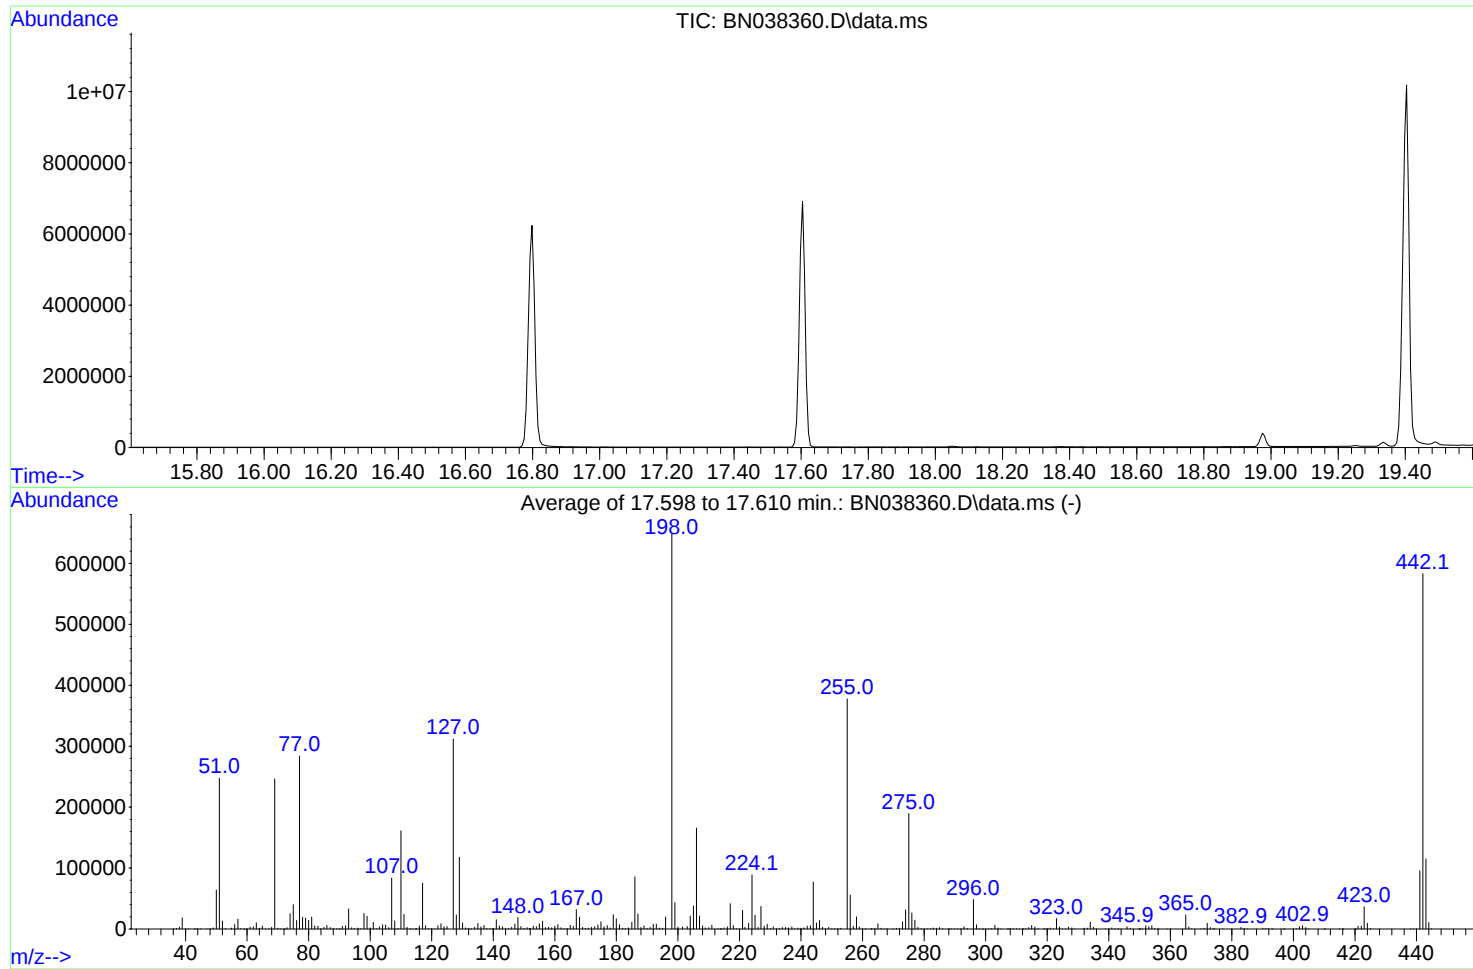

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.2	2975	PASS
69	69	100	100	100.0	246443	PASS
70	69	0.00	2	0.5	1338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	647957	PASS
199	198	5	9	6.7	43389	PASS
365	198	1	100	3.6	23237	PASS
441	443	0.01	150	83.2	95712	PASS
442	442	100	100	100.0	583104	PASS
443	442	15	24	19.7	115069	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/12/2025	BNA_N	<u>BN038360.D</u>
Compound Name	Response	Retention Time
DDT	2548182	20.639
DDD	41130	20.198
DDE	1498	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
42628	2590810	1.65

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038360.D
Acq On : 12 Dec 2025 21:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 07:57:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

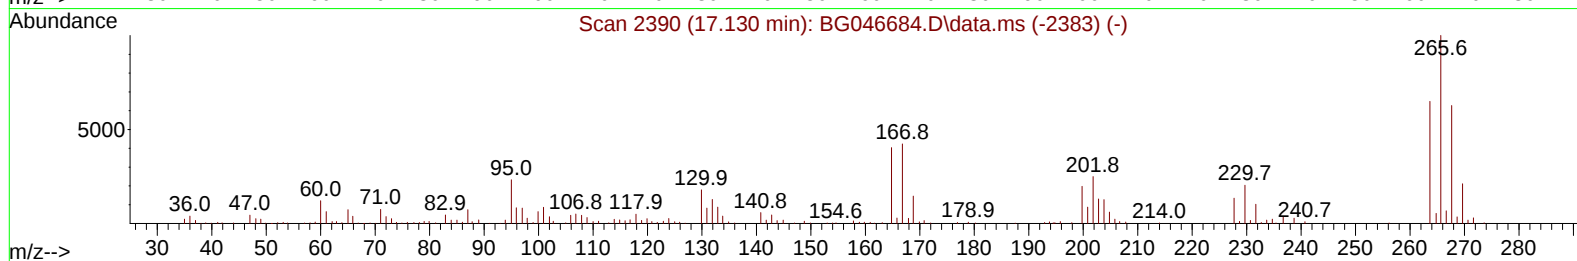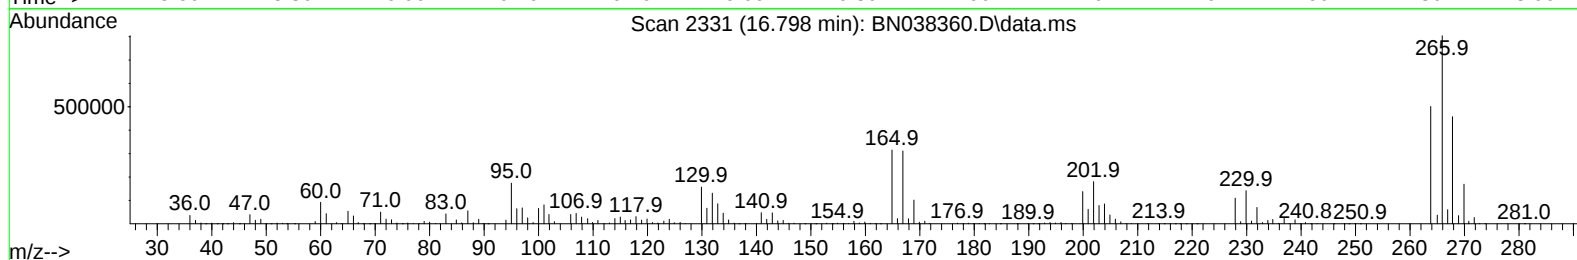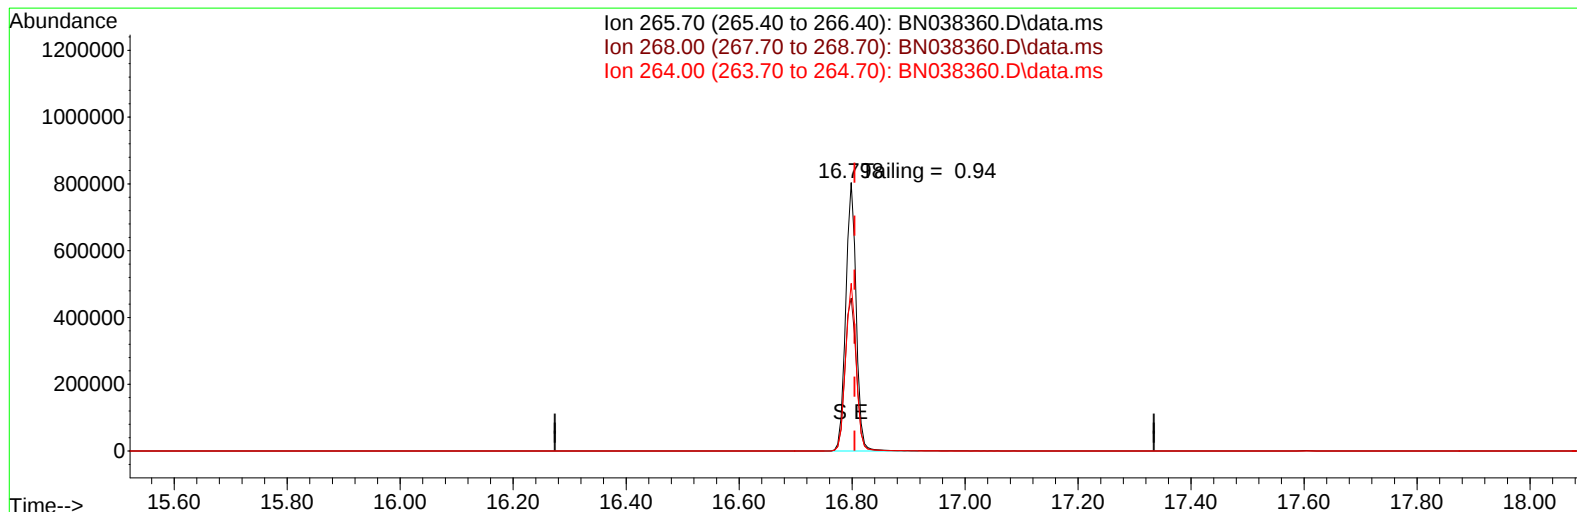

TIC: BN038360.D\data.ms

(70) Pentachlorophenol (C)

16.798min (-0.006) 226726.49 ng




response 1028431

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.98
264.00	61.60	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038360.D
Acq On : 12 Dec 2025 21:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 07:57:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

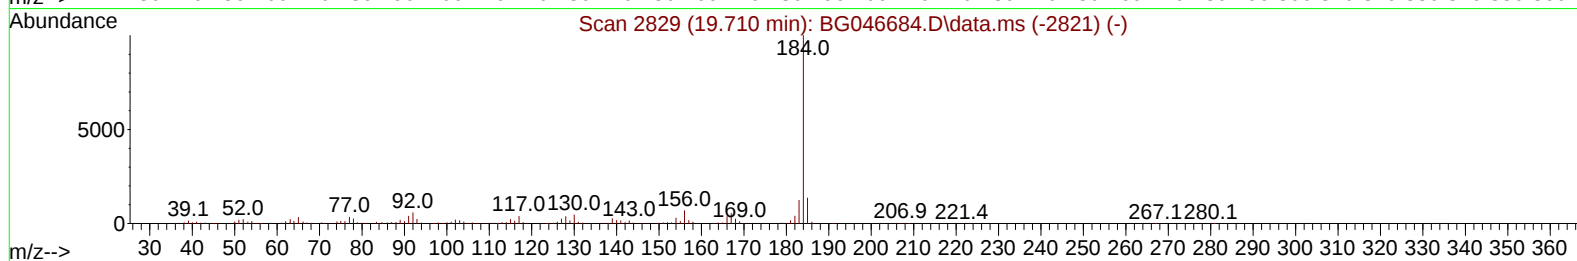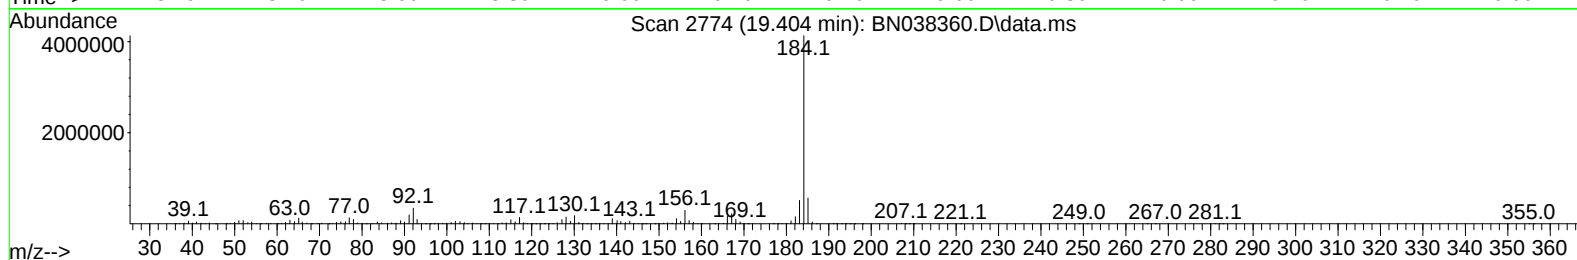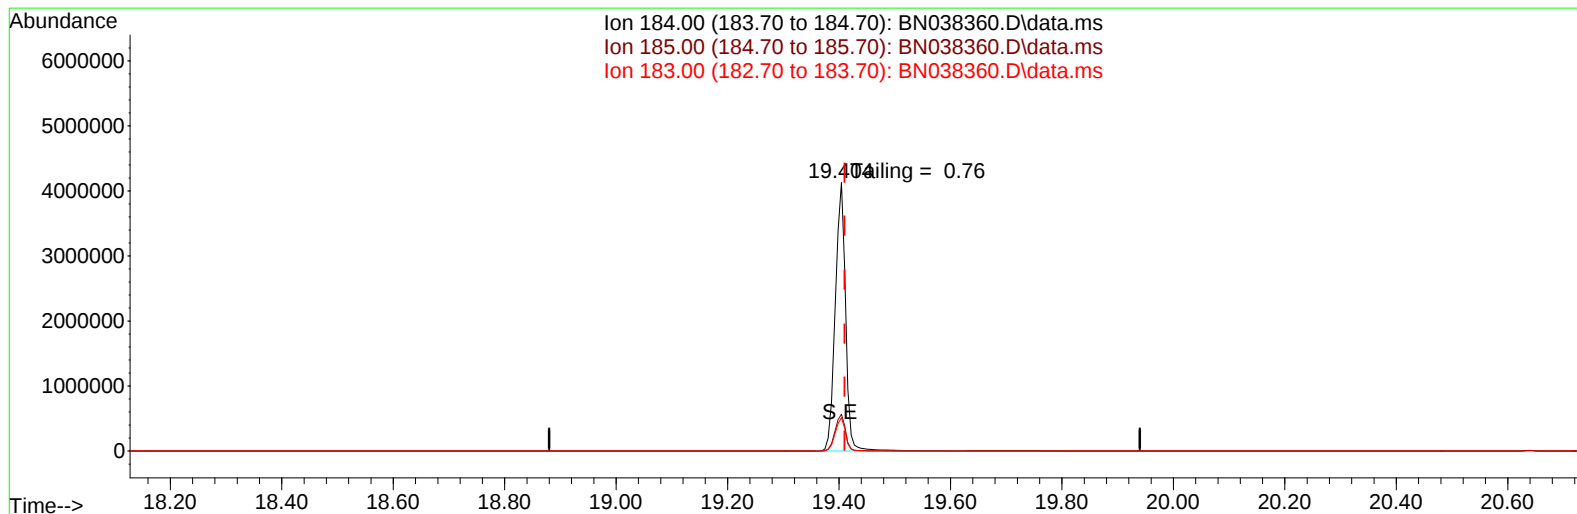

TIC: BN038360.D\data.ms

(77) Benzidine

19.404min (-0.006) 4504.77 ng

response 5342548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	12.42
0.00	0.00	0.00