


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038379.D
Acq On : 13 Dec 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

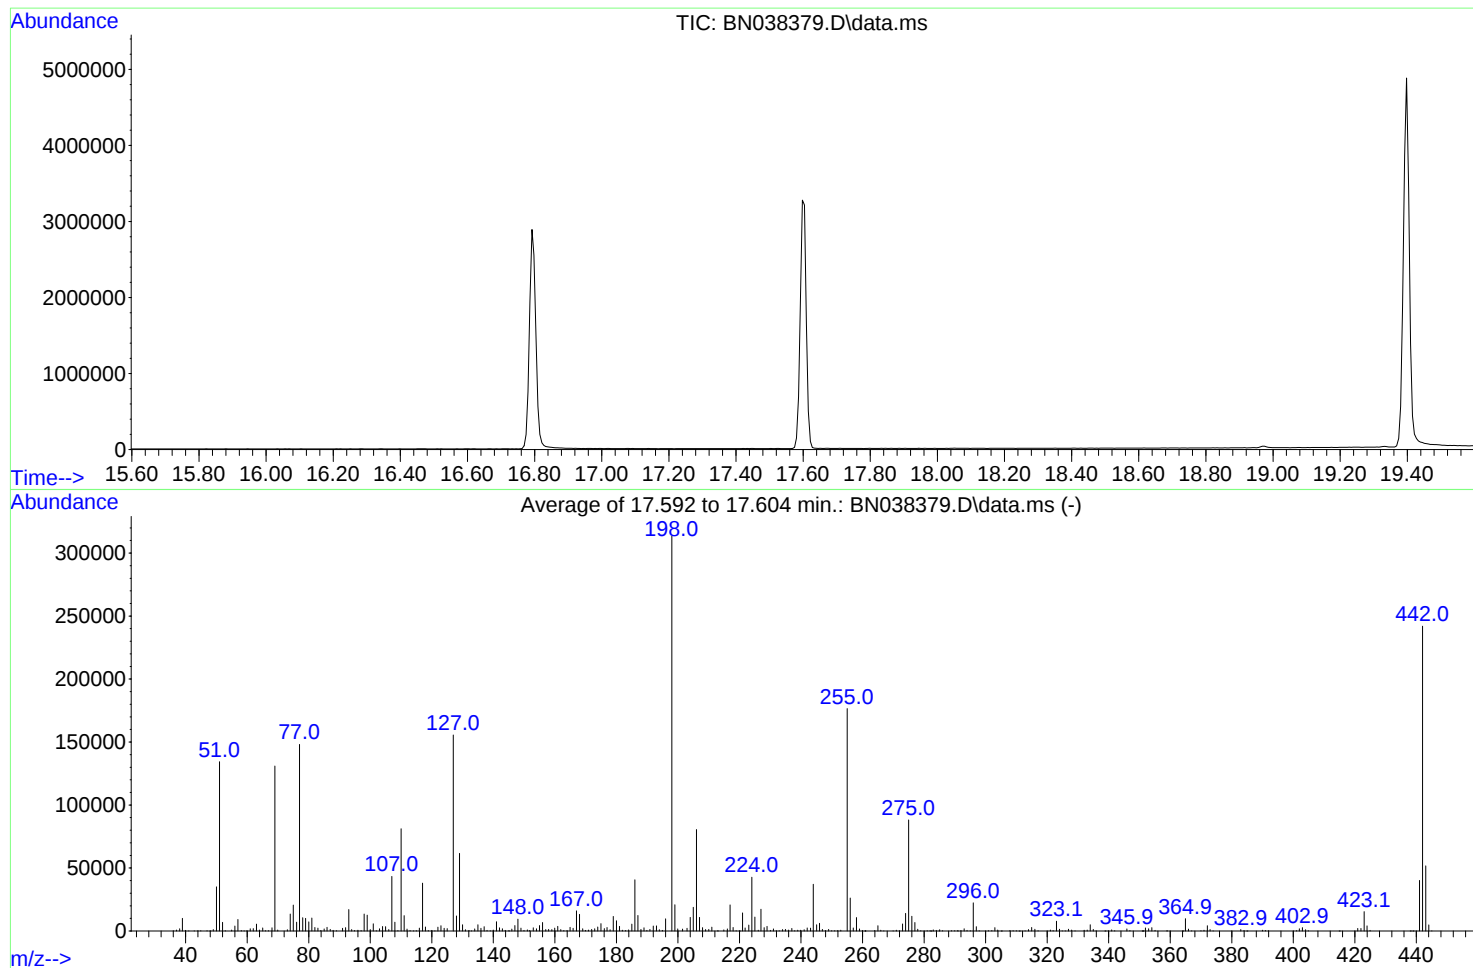

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	2551	PASS
69	69	100	100	100.0	130904	PASS
70	69	0.00	2	0.6	765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	313429	PASS
199	198	5	9	6.7	20870	PASS
365	198	1	100	3.1	9849	PASS
441	443	0.01	150	77.8	40200	PASS
442	442	100	100	100.0	241947	PASS
443	442	15	24	21.4	51701	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/12/2025	BNA_N	<u>BN038379.D</u>
Compound Name	Response	Retention Time
DDT	1156836	20.639
DDD	48129	20.198
DDE	1489	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
49618	1206454	4.11




S

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038379.D
Acq On : 13 Dec 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 08:16:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

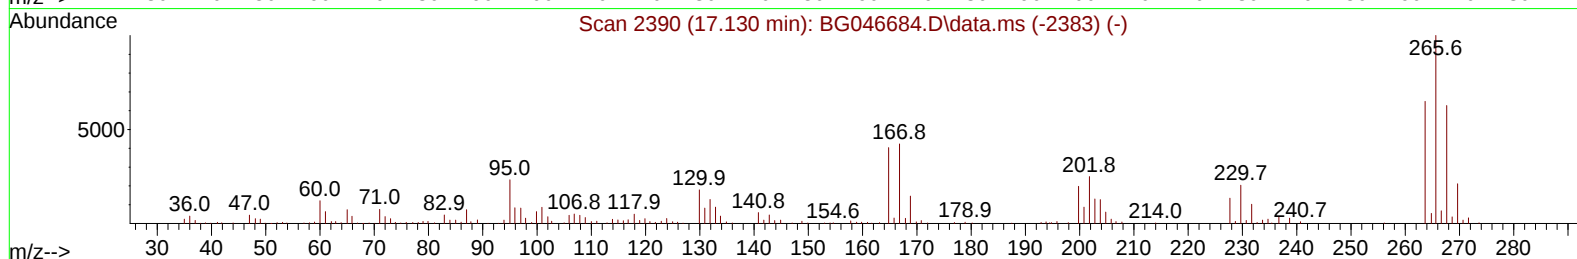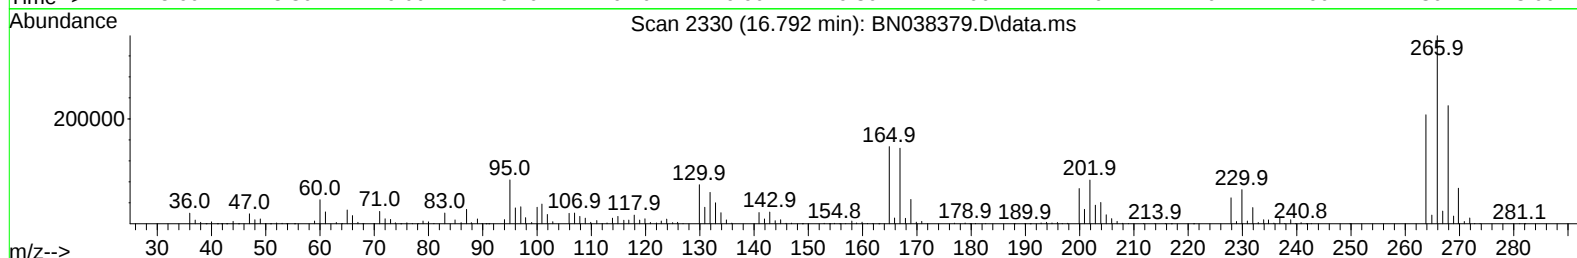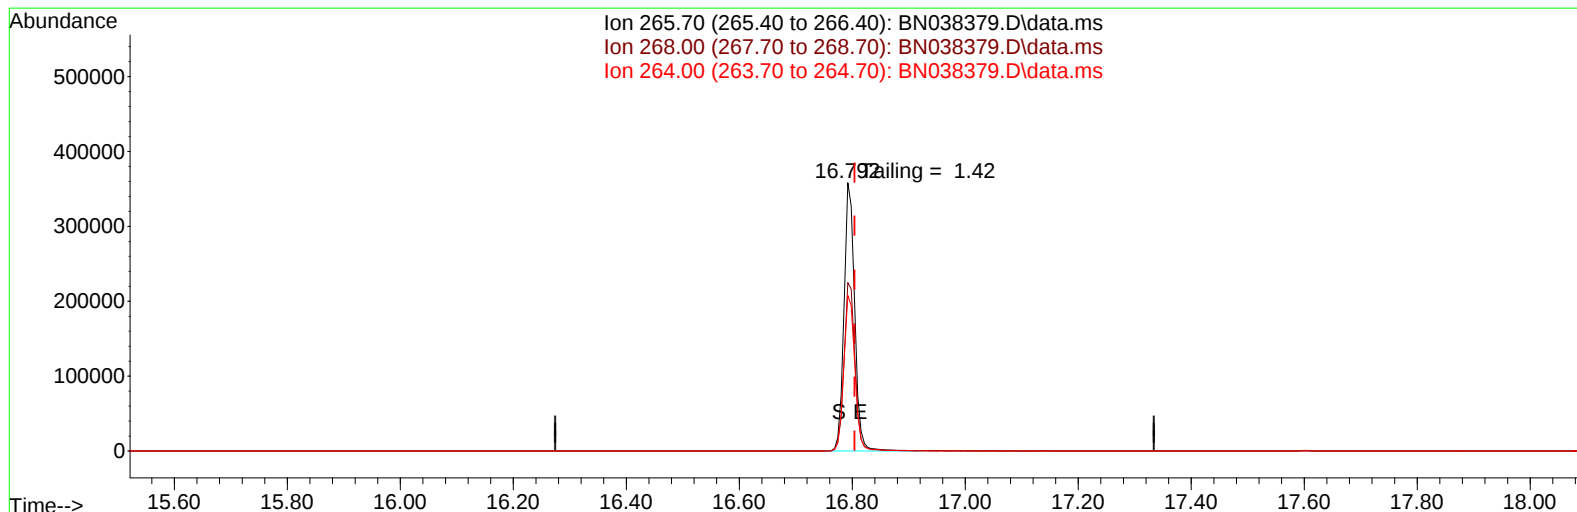

TIC: BN038379.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.012) 205733.08 ng




response 468217

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.80
264.00	61.60	57.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121225\
Data File : BN038379.D
Acq On : 13 Dec 2025 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 08:16:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

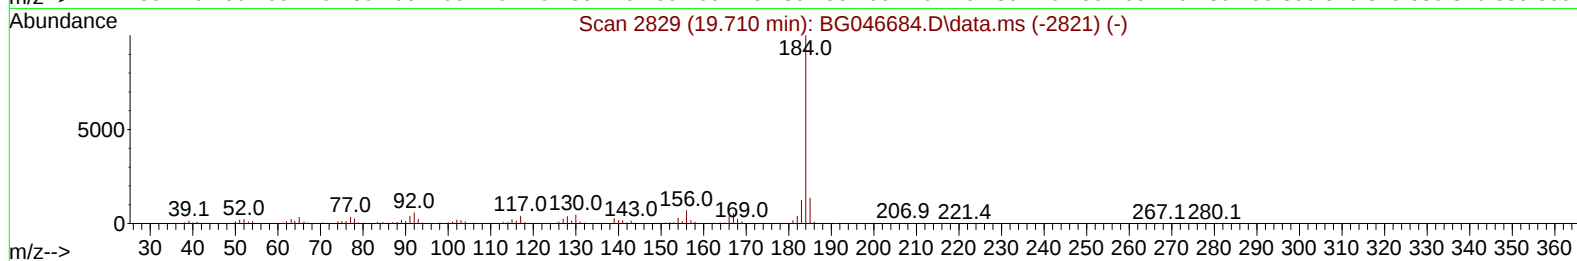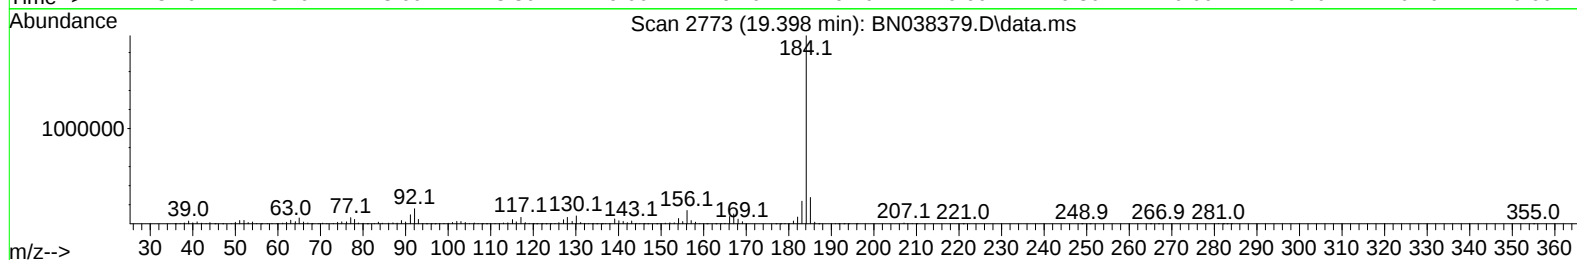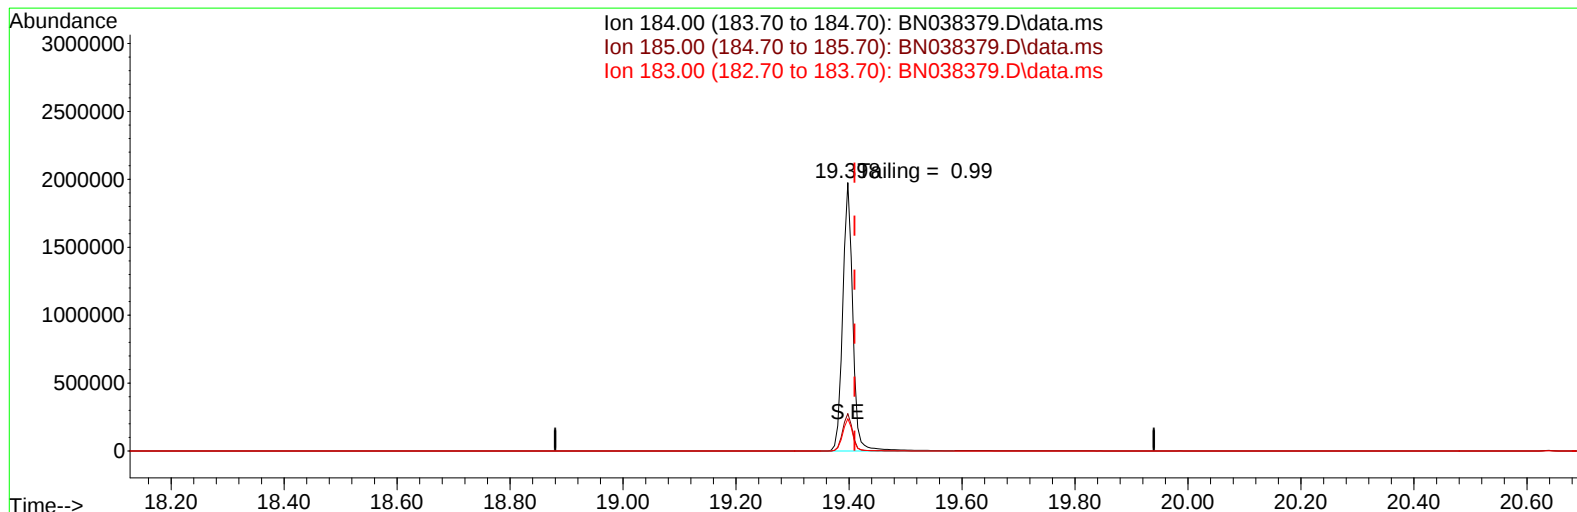

TIC: BN038379.D\data.ms

(77) Benzidine

19.398min (-0.012) 4902.30 ng

response 2430839

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	12.03
0.00	0.00	0.00