

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121318\
 Data File : BN003918.D
 Acq On : 14 Dec 2018 07:00
 Operator : JU/SJ
 Sample : J6299-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F39

Quant Time: Dec 14 14:18:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 14 04:33:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	23143	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	122283	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	81239	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	206940	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	303084	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	360848	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	1645	4.65	ng/uL	0.00
5) Phenol-d5	6.99	99	11770	5.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	33222	26.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	38797	21.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	25059	13.14	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	27727	28.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	31586	28.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	53043	26.35	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	199327	27.49	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	254041	29.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	6823	4.55	ng/ul	0.00
57) Fluorene-d10	15.46	176	185493	29.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	26004	17.45	ng/ul	0.00
70) Anthracene-d10	17.31	188	316939	30.31	ng/ul	0.00
78) Pyrene-d10	19.60	212	390993	28.84	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	602378	30.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
56) Diethylphthalate	15.27	149	8399	1.160	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121318\
Data File : BN003918.D
Acq On : 14 Dec 2018 07:00
Operator : JU/SJ
Sample : J6299-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F39

Quant Time: Dec 14 14:18:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 14 04:33:02 2018
Response via : Initial Calibration

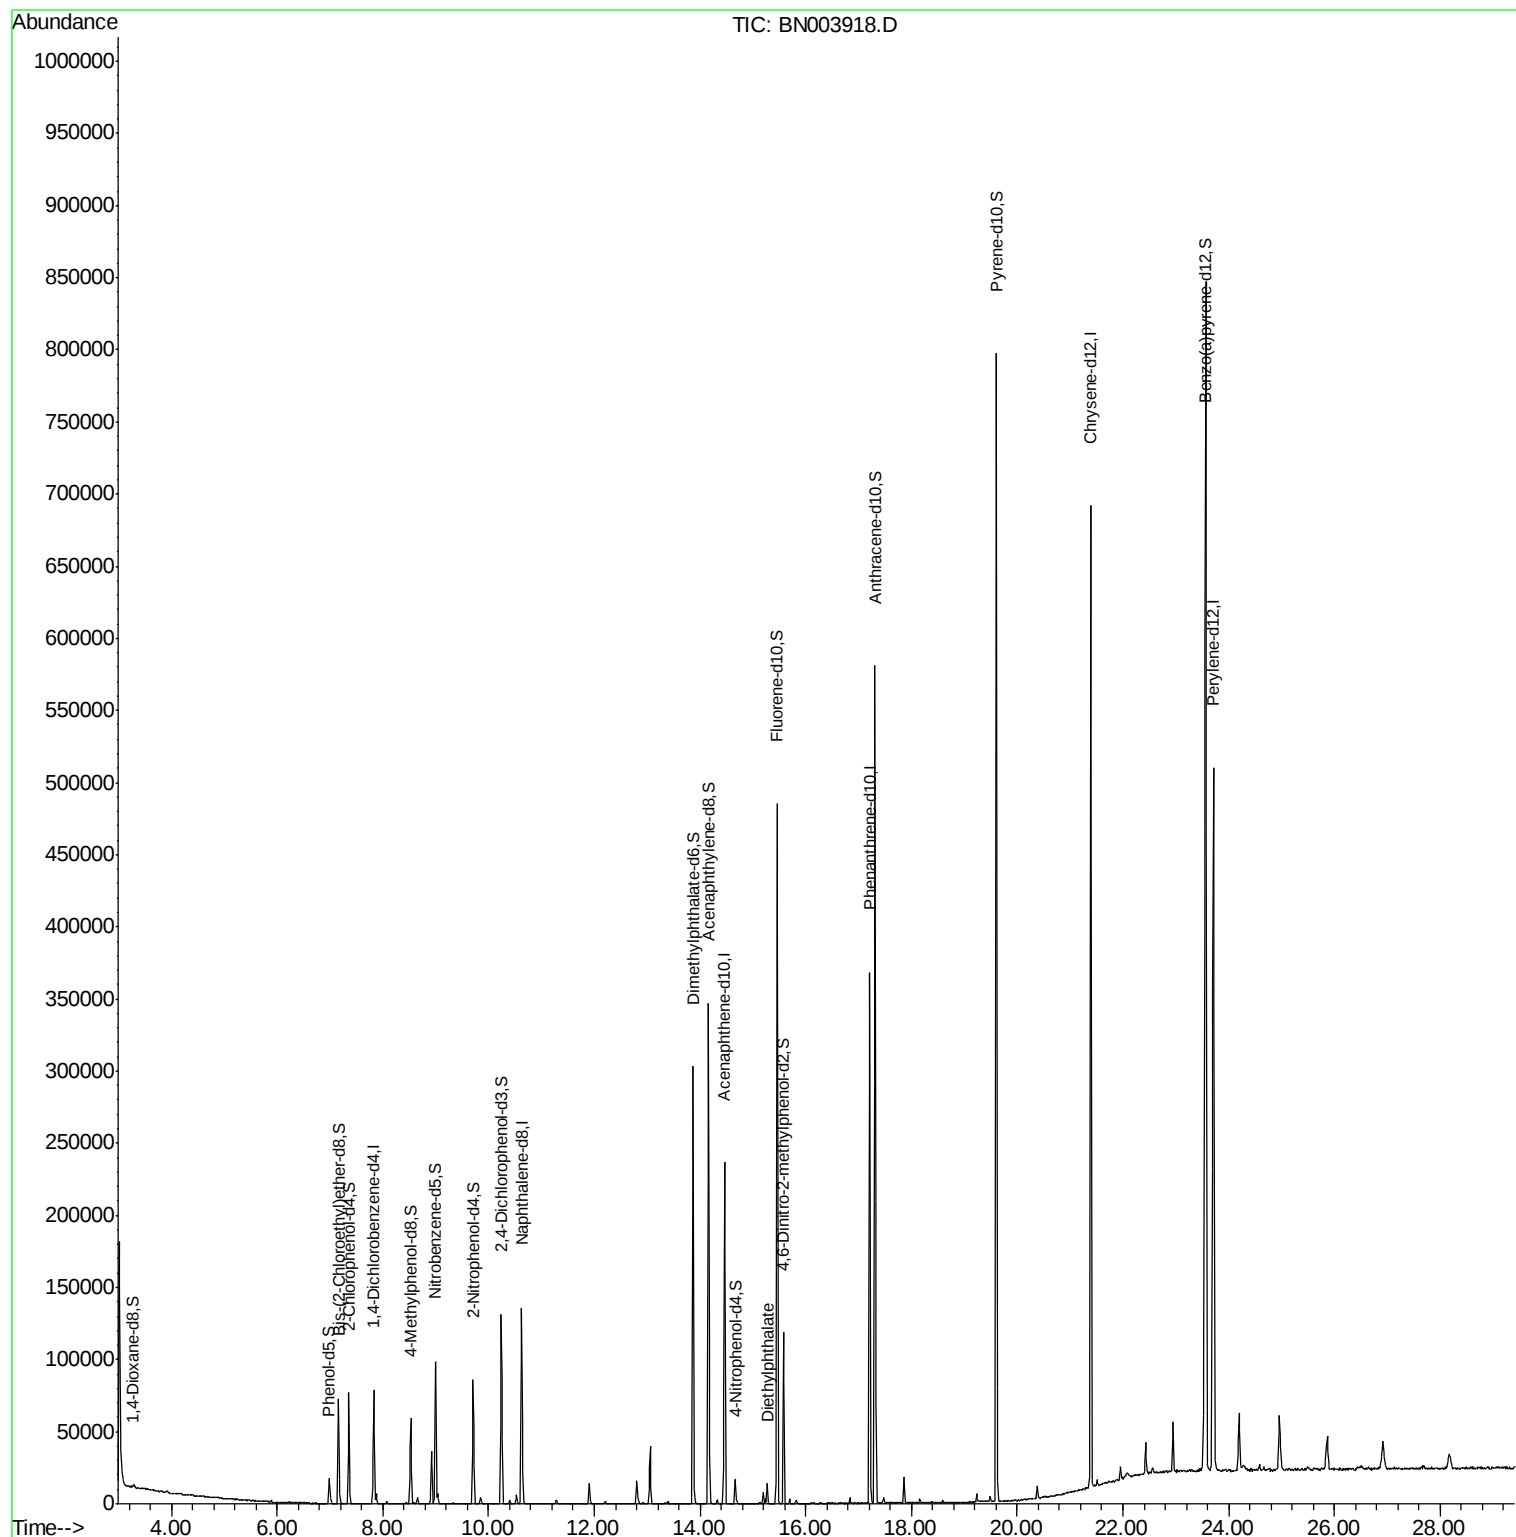

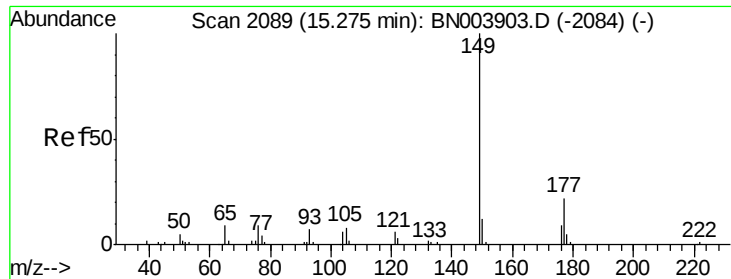

#56

Diethylphthalate

Concen: 1.160 ng/ul

RT: 15.27 min Scan# 2089

Delta R.T. 0.00 min

Lab File: BN003918.D


Acq: 14 Dec 2018 07:00

Instrument :

BNA_N

ClientSampleId :

F9F39

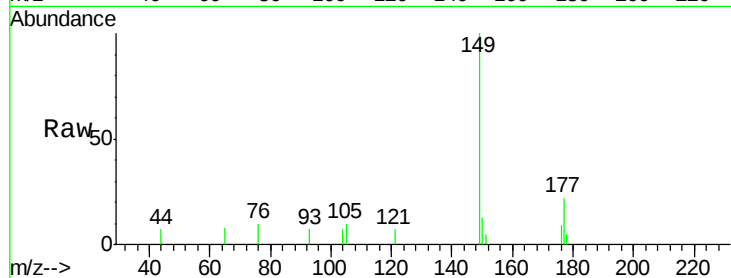


Tgt Ion:149 Resp: 8399

Ion Ratio Lower Upper

149 100

177 22.3 17.8 26.6

150 13.2 10.2 15.2

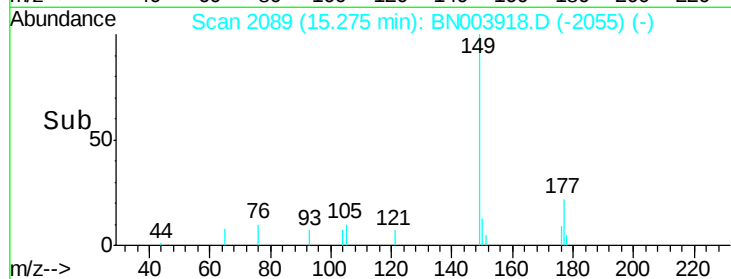

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

